
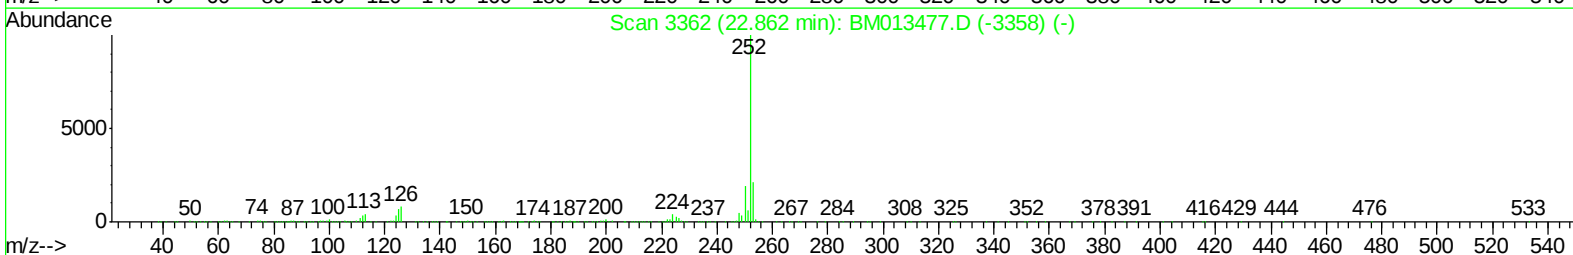
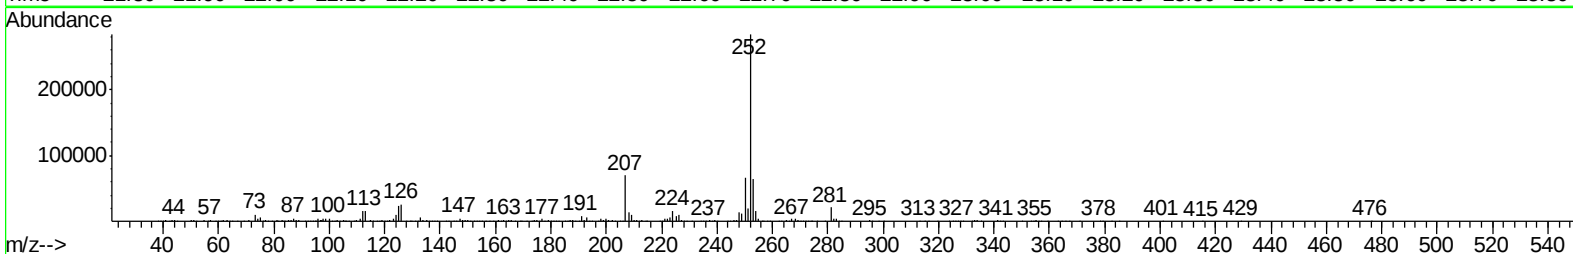


Data File : BM013486.D
Acq On : 16 Dec 2017 20:44
Operator : SJ/JU
Sample : I6776-06DL 30X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Dec 18 03:15:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

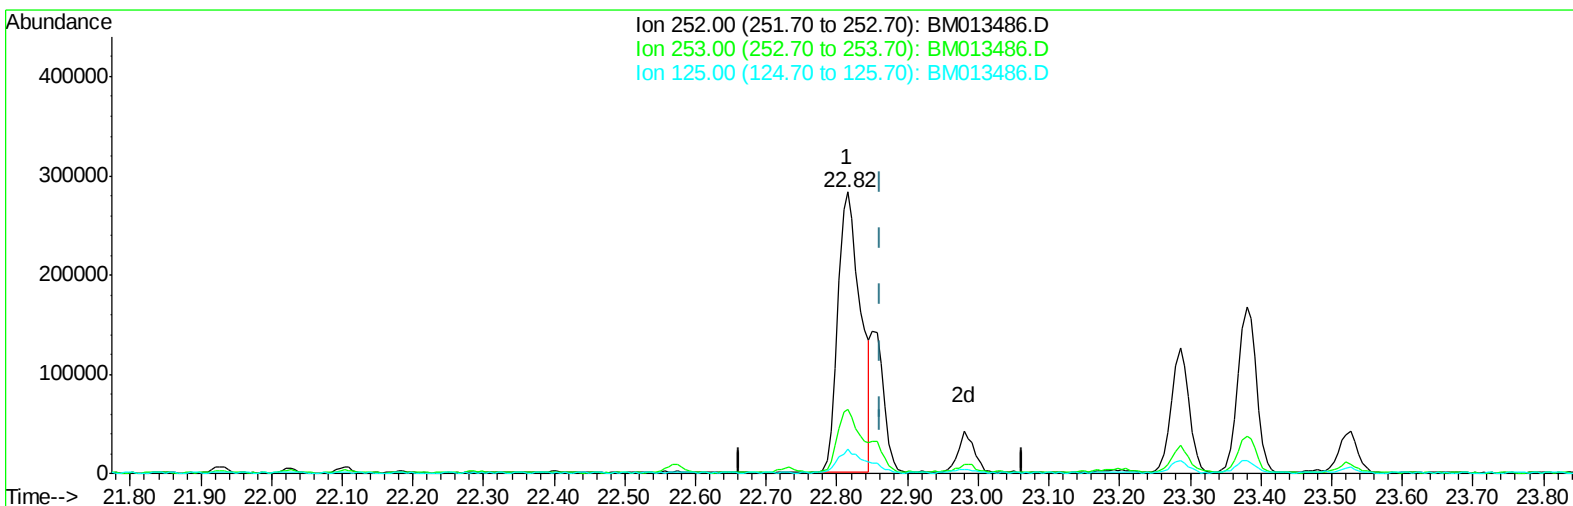

TIC: BM013486.D

(86) Benzo(k)fluoranthene

22.815min (-0.047) 12.03ng/ul

response 634387

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.77
125.00	4.30	8.48#
0.00	0.00	0.00