
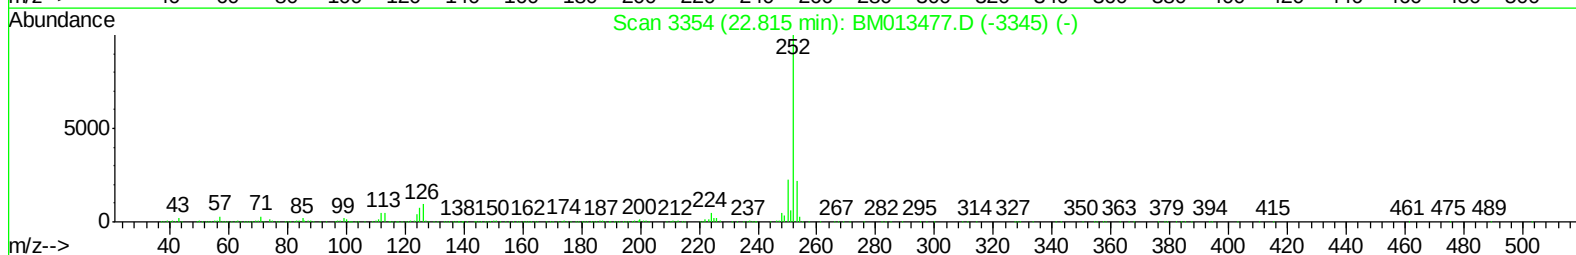
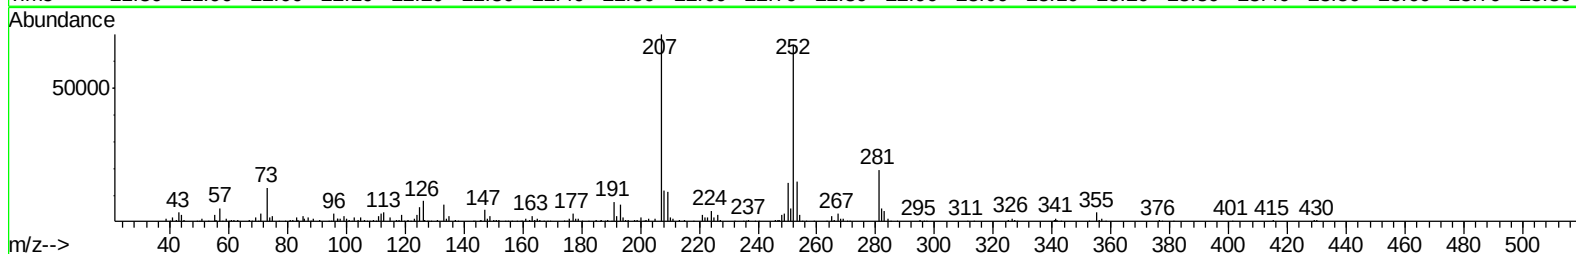


Data File : BM013487.D
Acq On : 16 Dec 2017 21:20
Operator : SJ/JU
Sample : I6778-15DL 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Quant Time: Dec 18 03:15:51 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 18 03:13:05 2017
Response via : Initial Calibration

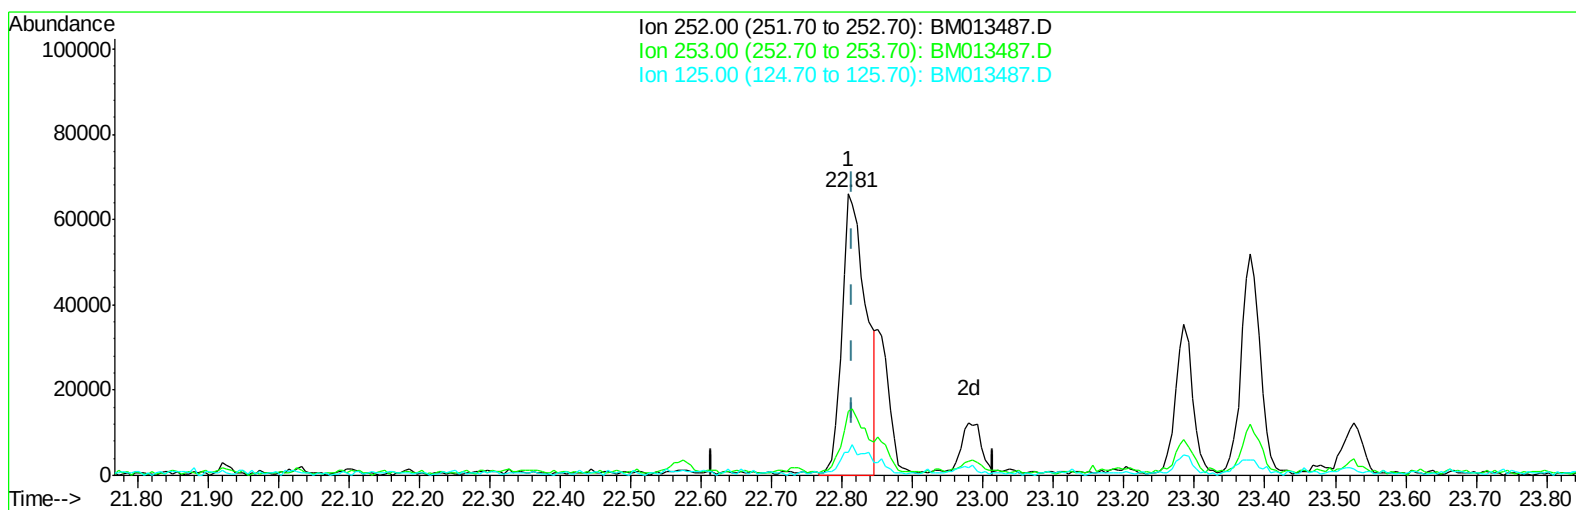

TIC: BM013487.D

(85) Benzo(b)fluoranthene

22.809min (-0.006) 2.70ng/ul m

response 154631

Ion	Exp%	Act%
252.00	100	100
253.00	22.40	22.56
125.00	4.50	8.36#
0.00	0.00	0.00