

Data File : BM013451.D
Acq On : 15 Dec 2017 22:44
Operator : SJ/JU
Sample : I6775-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A12

Quant Time: Dec 16 00:24:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	228258	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	970870	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	582417	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1355758	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1366976	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	1065521	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	24146	5.24	ng/uL	0.00
5) Phenol-d5	6.86	99	887417	44.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	322242	28.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	737853	47.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	477442	28.30	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	328339	42.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	265732	32.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	494717	29.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	650595	41.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1550149	29.91	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1958353	30.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	184396	20.48	ng/ul	0.00
57) Fluorene-d10	15.32	176	1331105	29.86	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	127584	14.96	ng/ul	0.00
70) Anthracene-d10	17.17	188	2131469	31.39	ng/ul	0.00
76) Pyrene-d10	19.47	212	2397463	35.20	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	1740197	32.06	ng/ul	0.00

Target Compounds

						Qvalue
6) Phenol	6.88	94	70843	3.63	ng/ul#	88
28) Naphthalene	10.50	128	64396	1.29	ng/ul#	93
40) 1,1'-Biphenyl	13.15	154	369437	7.51	ng/ul	99
44) Dimethylphthalate	13.78	163	297574	6.00	ng/ul	100
49) Acenaphthene	14.39	153	1997819	49.55	ng/ul	98
53) Dibenzofuran	14.72	168	2112243	35.49	ng/ul	99
58) Fluorene	15.37	166	1777444	36.10	ng/ul	98
60) 4-Nitroaniline	15.37	138	20600	1.93	ng/ul#	12
68) Pentachlorophenol	16.72	266	11094	1.09	ng/ul	96
69) Phenanthrene	17.12	178	6141988	79.74	ng/ul	99
71) Anthracene	17.20	178	1304465	16.57	ng/ul	99
72) Carbazole	17.47	167	424460	6.27	ng/ul	98
74) Fluoranthene	19.13	202	5814045	61.60	ng/ul#	92
77) Pyrene	19.50	202	3888208	46.82	ng/ul#	90
80) Benzo(a)anthracene	21.24	228	781482	9.01	ng/ul	98
82) Chrysene	21.30	228	726866	9.03	ng/ul	98
85) Benzo(b)fluoranthene	22.82	252	307885	4.29	ng/ul#	98
86) Benzo(k)fluoranthene	22.86	252	102022	1.51	ng/ul#	95
88) Benzo(a)pyrene	23.39	252	164923	2.56	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM013451.D

Acq On : 15 Dec 2017 22:44

Operator : SJ/JU

Sample : I6775-09

Misc :

ALS Vial : 8 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

F9A12


Quant Time: Dec 16 00:24:03 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Dec 16 00:23:08 2017

Response via : Initial Calibration

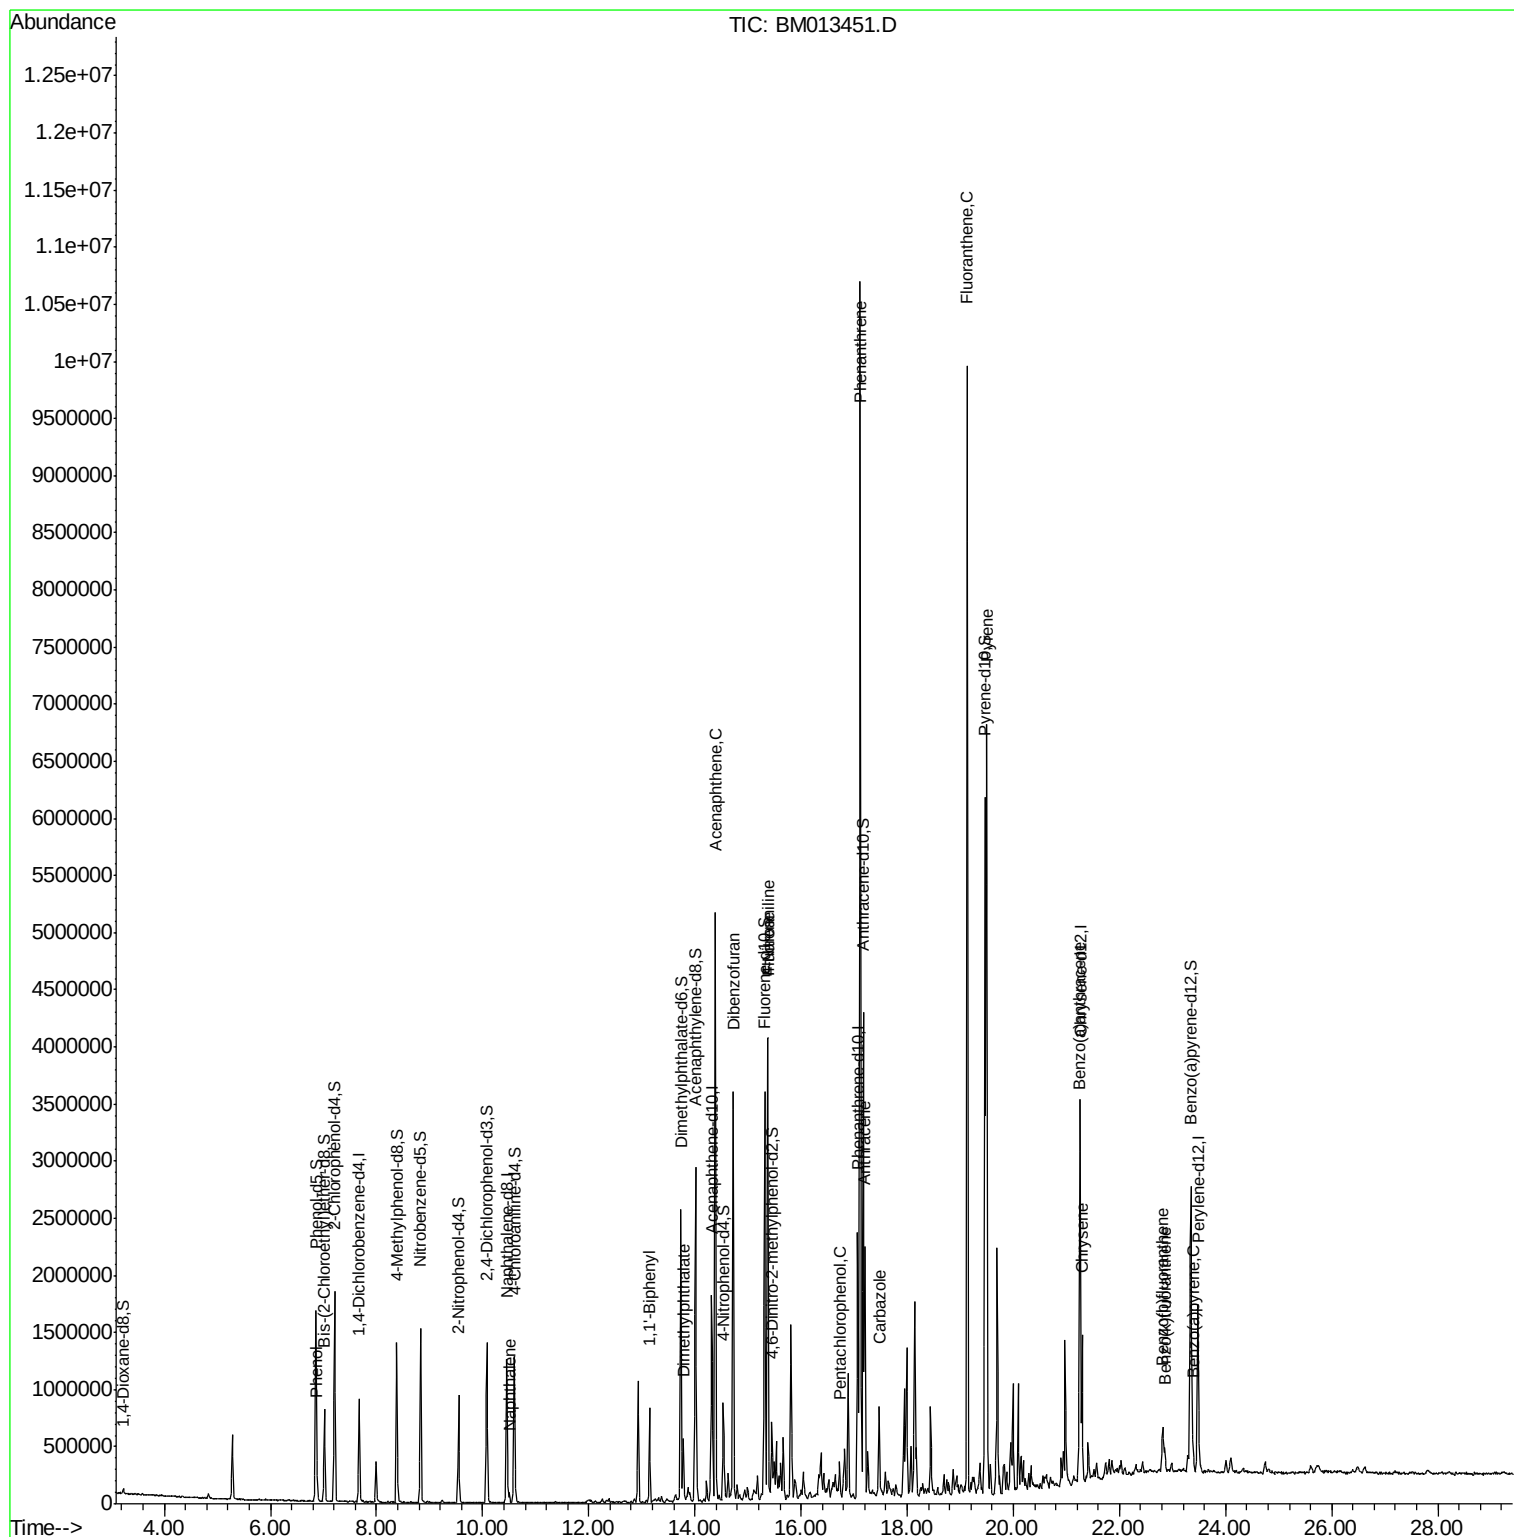

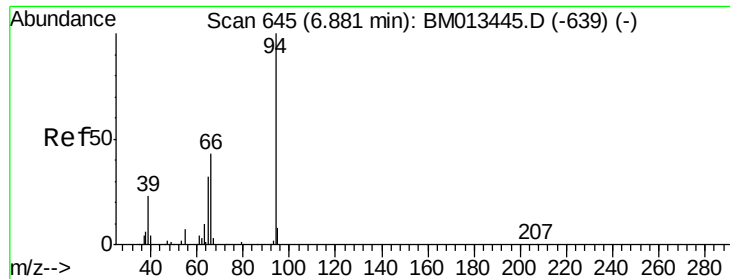

#6

Phenol

Concen: 3.63 ng/ul

RT: 6.88 min Scan# 645

Delta R.T. -0.00 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12





Tgt Ion: 94 Resp: 70843

Ion Ratio Lower Upper

94 100

65 35.5 28.2 42.4

66 45.1 47.2 70.8#

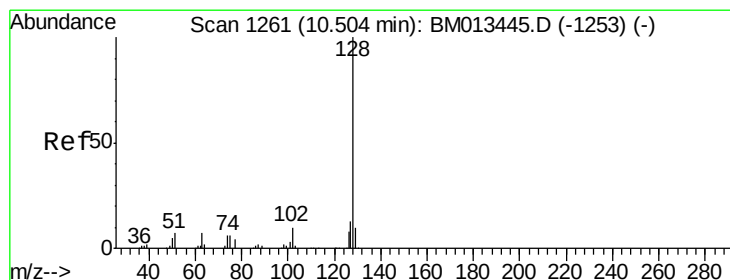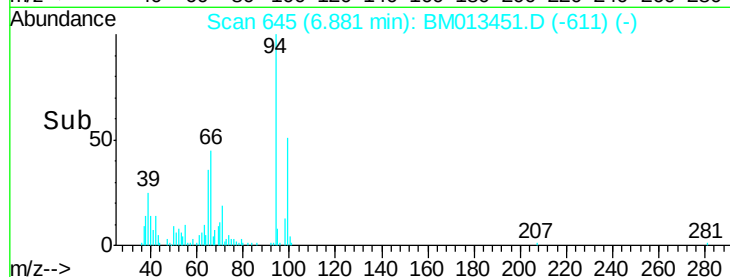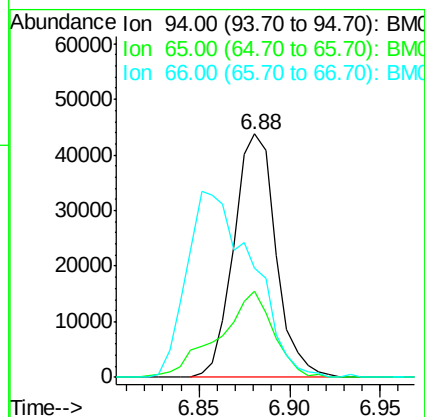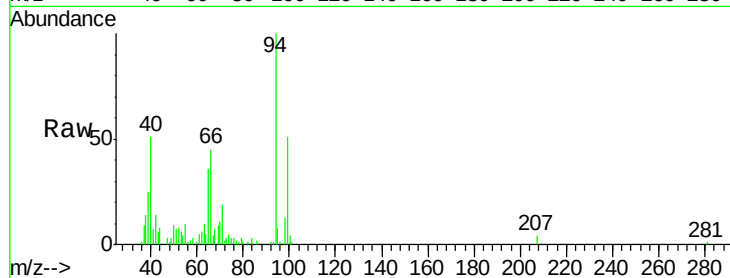

#28

Naphthalene

Concen: 1.29 ng/ul

RT: 10.50 min Scan# 1261

Delta R.T. -0.00 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44




Tgt Ion: 128 Resp: 64396


Ion Ratio Lower Upper

128 100

129 8.4 8.8 13.2#

127 10.1 10.6 16.0#


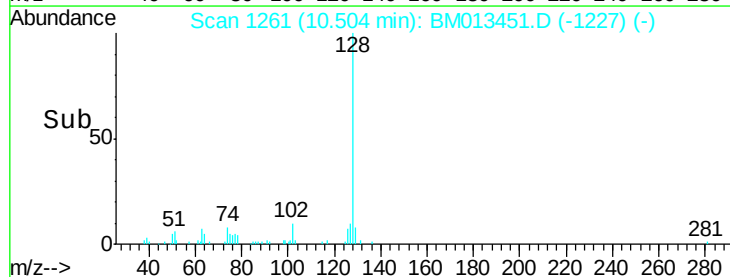
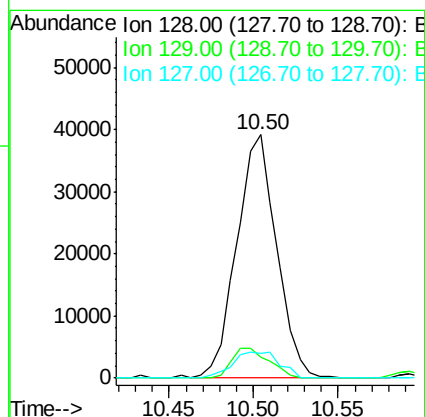
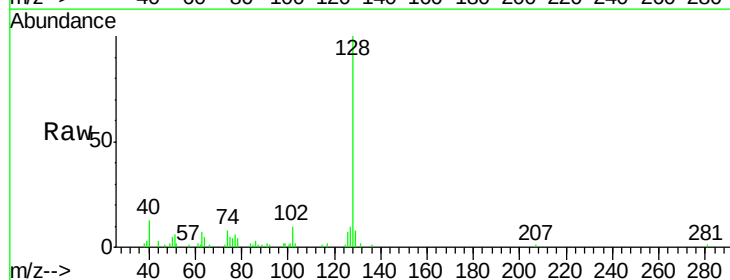


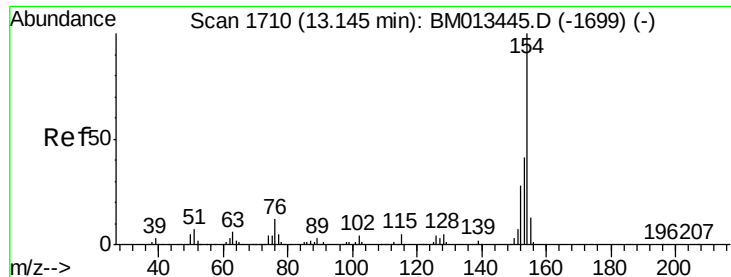

#40
1,1'-Biphenyl
Concen: 7.51 ng/ul
RT: 13.15 min Scan# 1710
Delta R.T. -0.00 min
Lab File: BM013451.D
Acq: 15 Dec 2017 22:44




Instrument :
BNA_M
ClientSampleId :
F9A12


Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.1	32.6	48.8
76	11.4	8.5	12.7

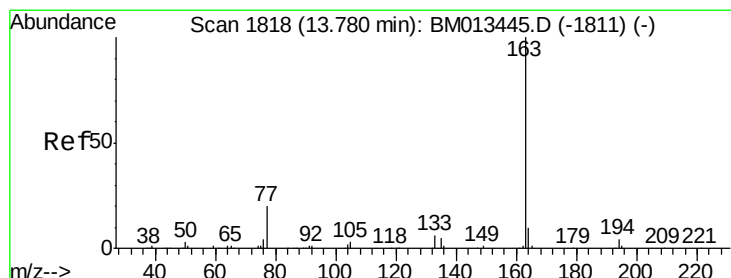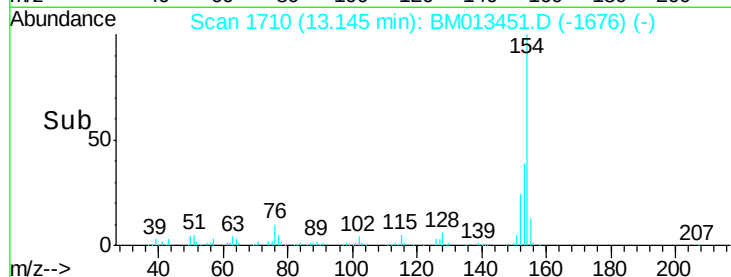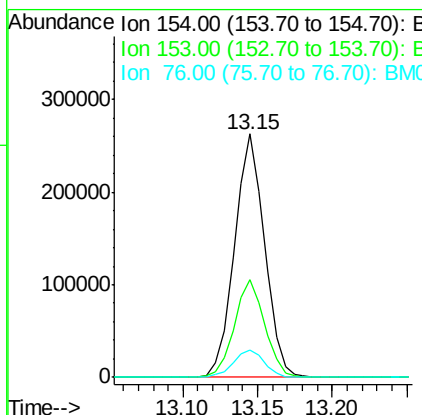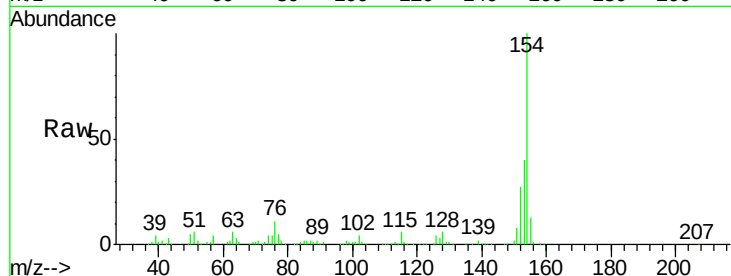

#44
Dimethylphthalate
Concen: 6.00 ng/ul
RT: 13.78 min Scan# 1818
Delta R.T. -0.00 min
Lab File: BM013451.D
Acq: 15 Dec 2017 22:44

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.5	5.3
164	10.2	8.2	12.4

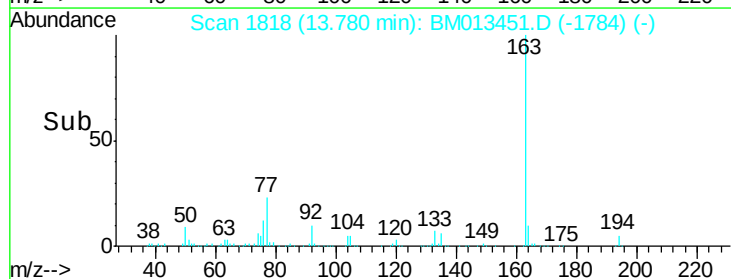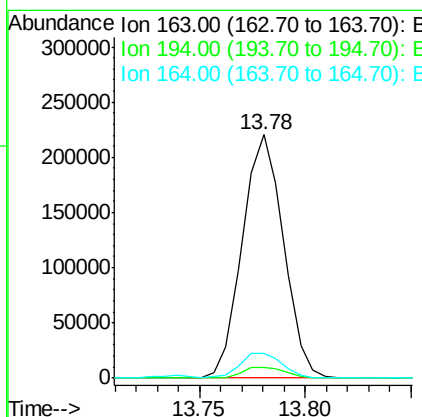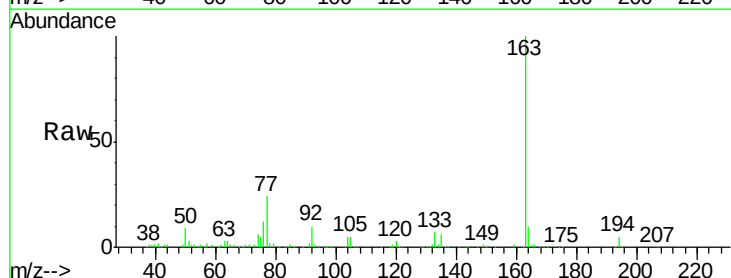

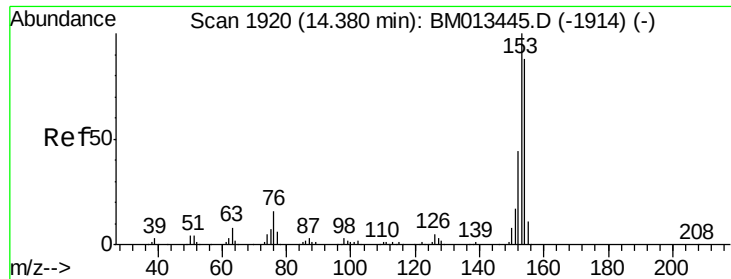

#49

Acenaphthene

Concen: 49.55 ng/ul

RT: 14.39 min Scan# 1921

Delta R.T. 0.01 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12


Tgt Ion:153 Resp: 1997819

Ion Ratio Lower Upper

153 100

152 45.2 37.6 56.4




154 88.8 70.4 105.6

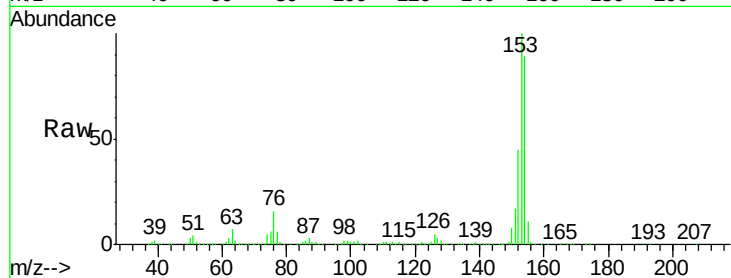

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

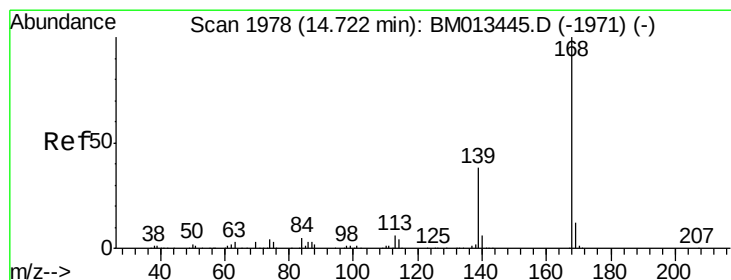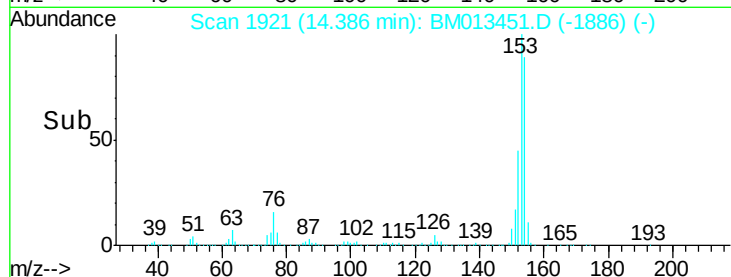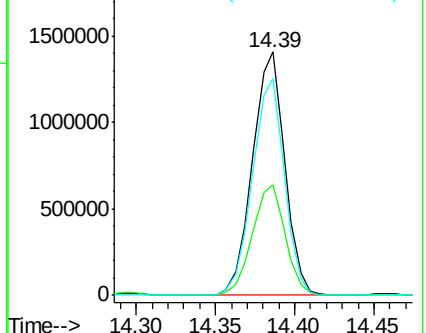

#53

Dibenzofuran

Concen: 35.49 ng/ul

RT: 14.72 min Scan# 1978

Delta R.T. -0.00 min

Lab File: BM013451.D


Acq: 15 Dec 2017 22:44

Tgt Ion:168 Resp: 2112243

Ion Ratio Lower Upper



168 100


139 37.6 30.8 46.2

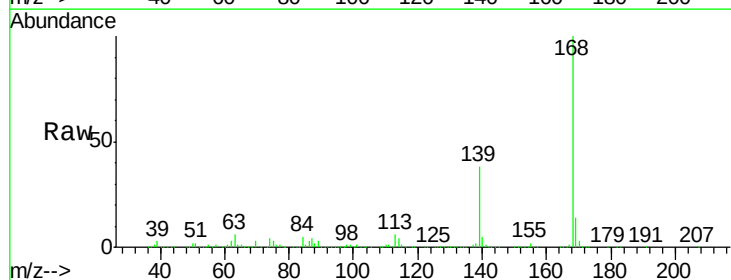

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

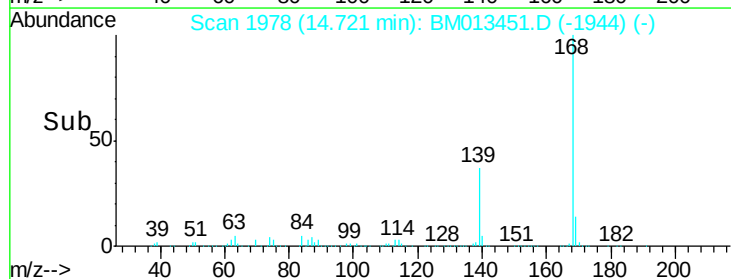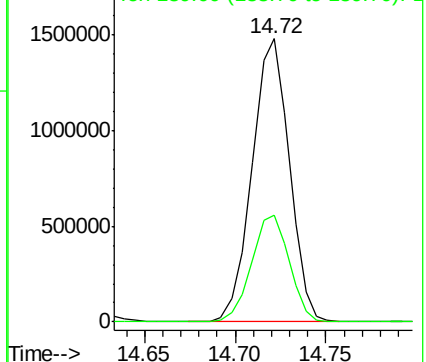

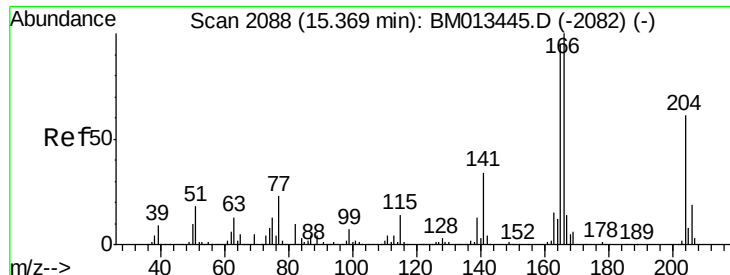

#58

Fluorene

Concen: 36.10 ng/ul

RT: 15.37 min Scan# 2089

Delta R.T. 0.01 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12


Tgt Ion:166 Resp: 1777444

Ion Ratio Lower Upper

166 100

165 95.8 77.9 116.9




167 14.0 10.6 16.0

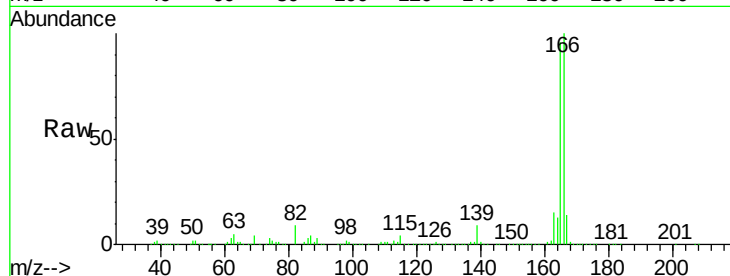

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

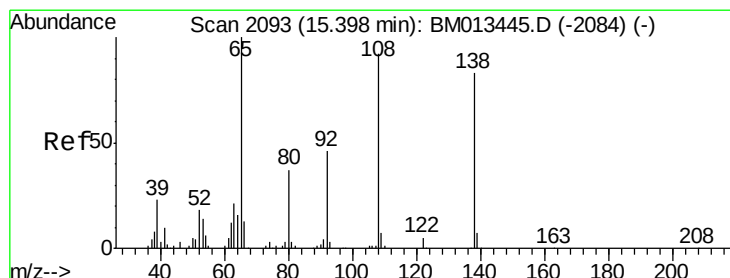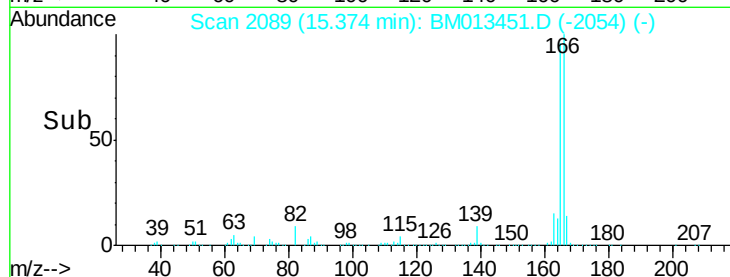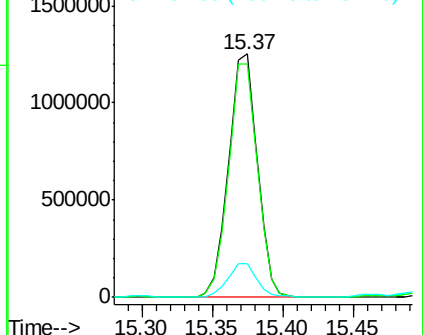

#60

4-Nitroaniline

Concen: 1.93 ng/ul

RT: 15.37 min Scan# 2089

Delta R.T. -0.02 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44


Tgt Ion:138 Resp: 20600

Ion Ratio Lower Upper

138 100

92 0.0 40.0 60.0#



108 4.5 80.0 120.0#

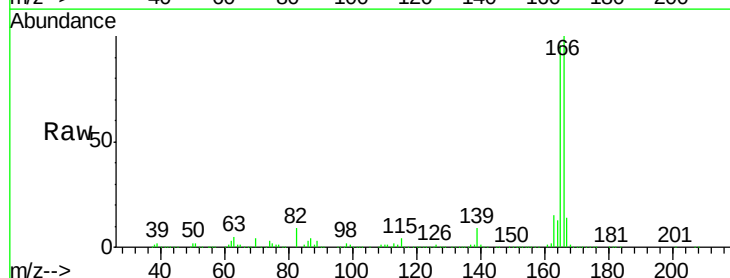


Abundance Ion 138.00 (137.70 to 138.70): E

Ion 92.00 (91.70 to 92.70): BM0

Ion 108.00 (107.70 to 108.70): E

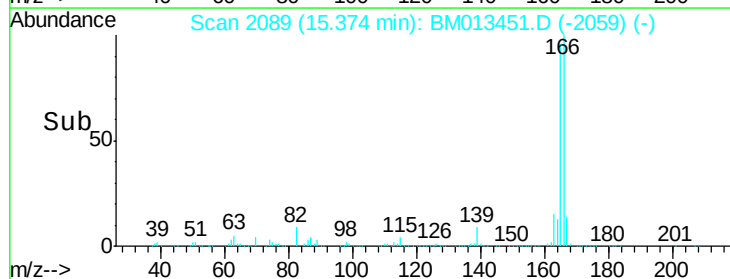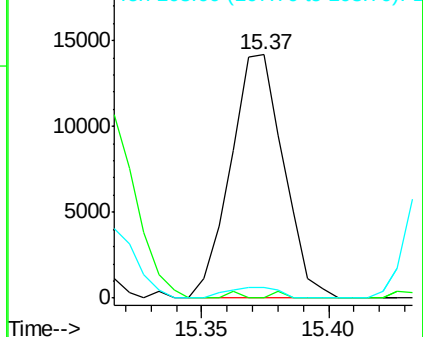


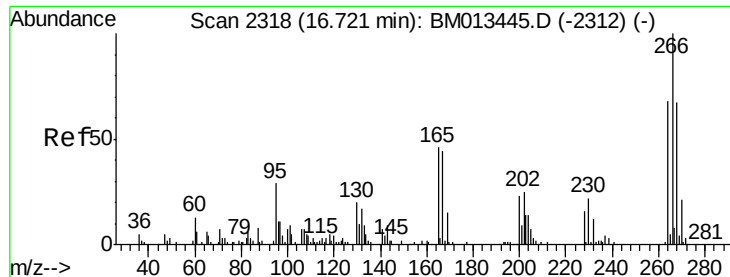




#68
 Pentachlorophenol
 Concen: 1.09 ng/ul
 RT: 16.72 min Scan# 2318
 Delta R.T. -0.00 min
 Lab File: BM013451.D
 Acq: 15 Dec 2017 22:44

Instrument :
 BNA_M
 ClientSampleId :
 F9A12

Tgt Ion:266 Resp: 11094
 Ion Ratio Lower Upper
 266 100
 264 56.3 49.3 73.9
 268 66.7 52.6 78.8

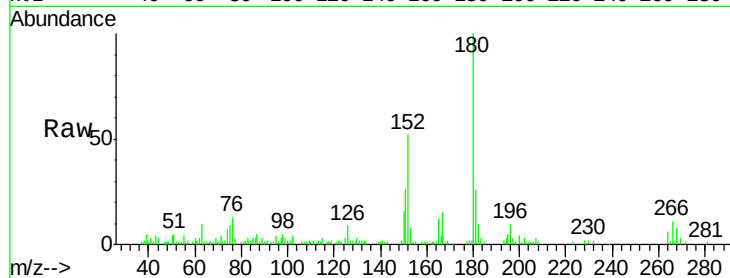


Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

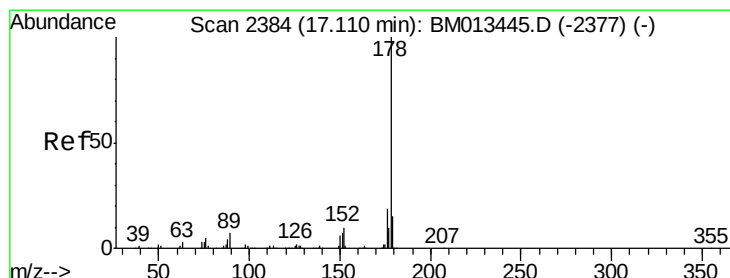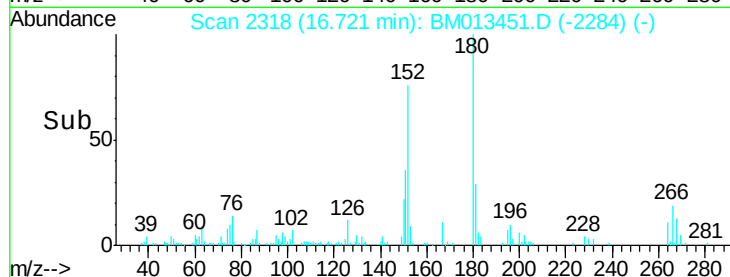
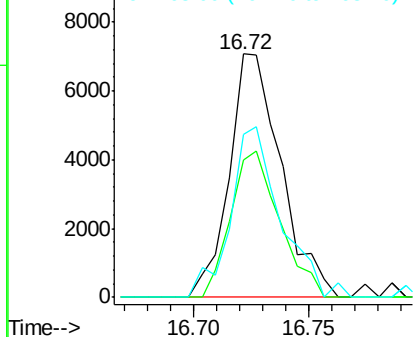



#69
 Phenanthrene
 Concen: 79.74 ng/ul
 RT: 17.12 min Scan# 2385
 Delta R.T. 0.01 min
 Lab File: BM013451.D
 Acq: 15 Dec 2017 22:44

Tgt Ion:178 Resp: 6141988
 Ion Ratio Lower Upper
 178 100
 179 15.4 12.6 19.0
 176 18.3 14.9 22.3

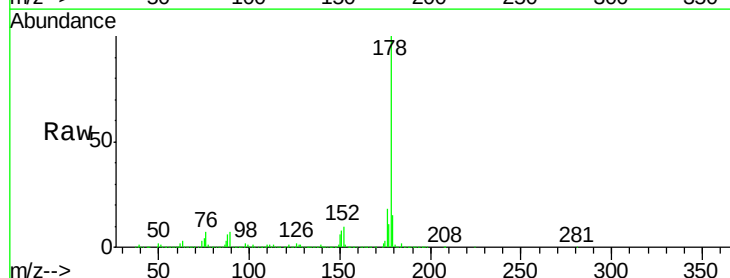

Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

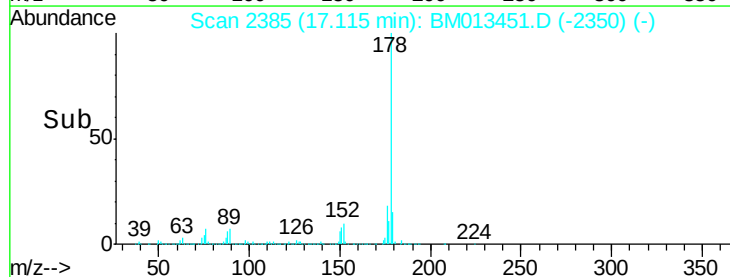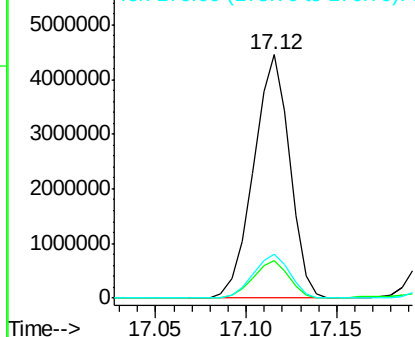


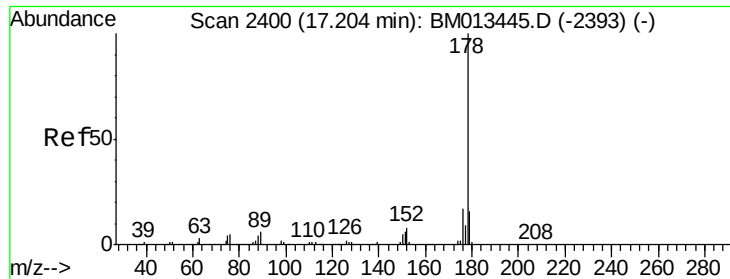




#71
 Anthracene
 Concen: 16.57 ng/ul
 RT: 17.20 min Scan# 2400
 Delta R.T. -0.00 min
 Lab File: BM013451.D
 Acq: 15 Dec 2017 22:44

Instrument :
 BNA_M
 ClientSampleID :
 F9A12

Tgt Ion:178 Resp: 1304465
 Ion Ratio Lower Upper
 178 100
 179 15.4 11.7 17.5
 176 17.7 14.6 21.8

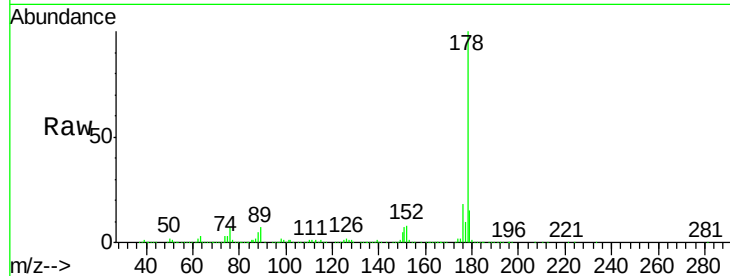


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

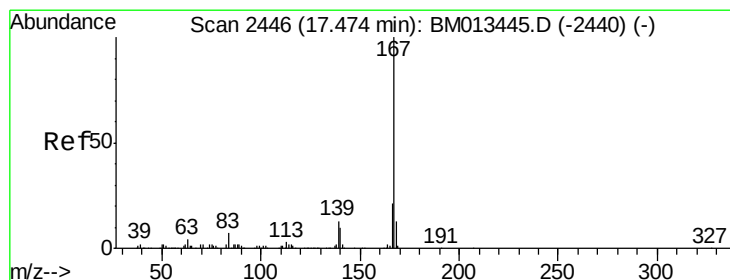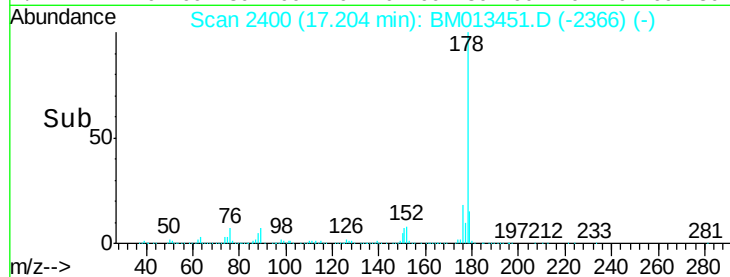
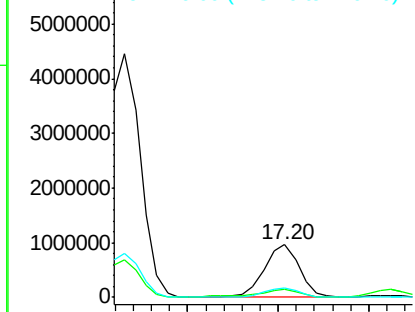



#72
 Carbazole
 Concen: 6.27 ng/ul
 RT: 17.47 min Scan# 2446
 Delta R.T. -0.00 min
 Lab File: BM013451.D
 Acq: 15 Dec 2017 22:44

Tgt Ion:167 Resp: 424460
 Ion Ratio Lower Upper
 167 100
 166 22.3 17.1 25.7
 139 11.9 10.0 15.0

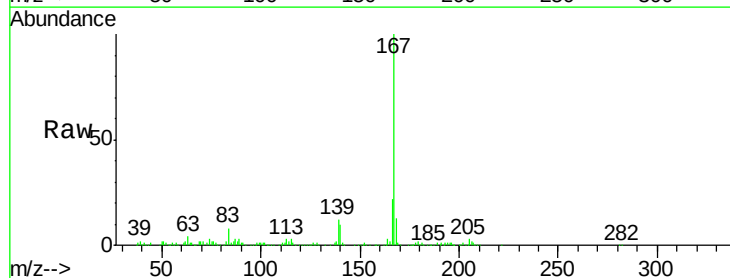

Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E

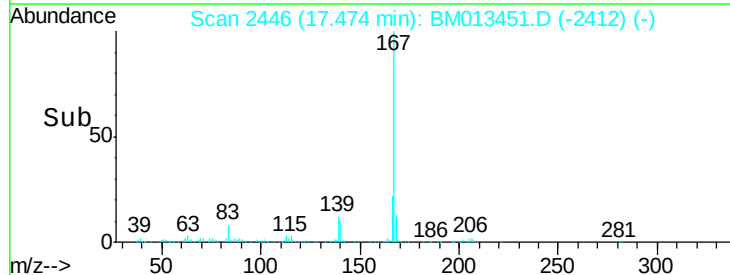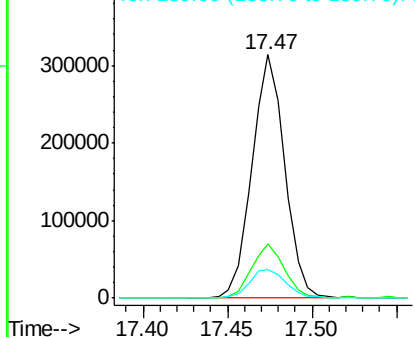

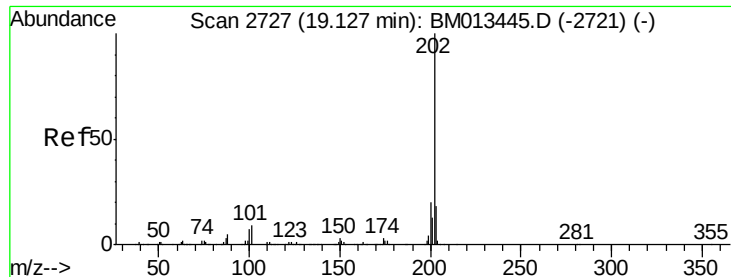

#74

Fluoranthene

Concen: 61.60 ng/ul

RT: 19.13 min Scan# 2728

Delta R.T. 0.01 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12


Tgt Ion:202 Resp: 5814045

Ion Ratio Lower Upper

202 100

101 8.6 4.6 7.0#




100 6.8 3.4 5.2#

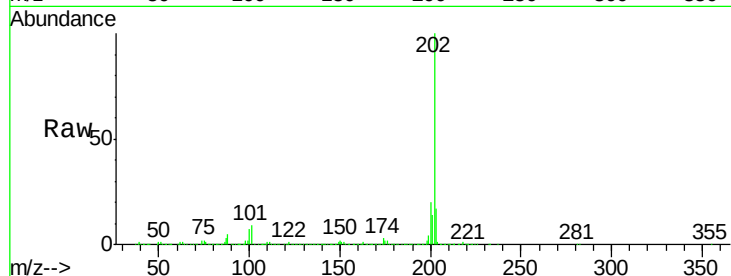

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

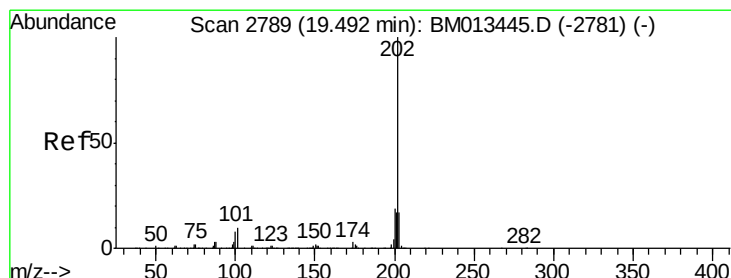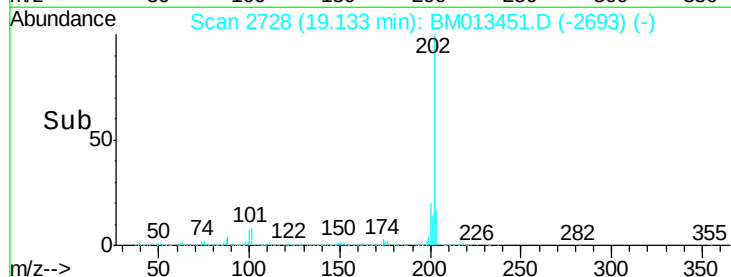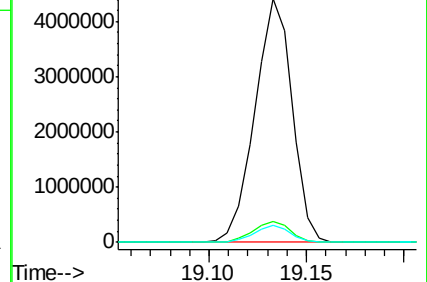

#77

Pyrene

Concen: 46.82 ng/ul

RT: 19.50 min Scan# 2790

Delta R.T. 0.01 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44


Tgt Ion:202 Resp: 3888208

Ion Ratio Lower Upper

202 100

101 10.4 5.1 7.7#



100 8.6 4.9 7.3#

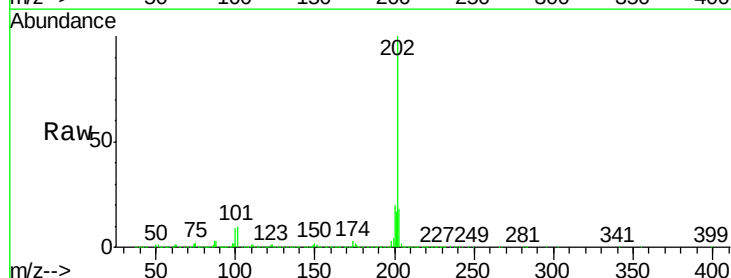


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

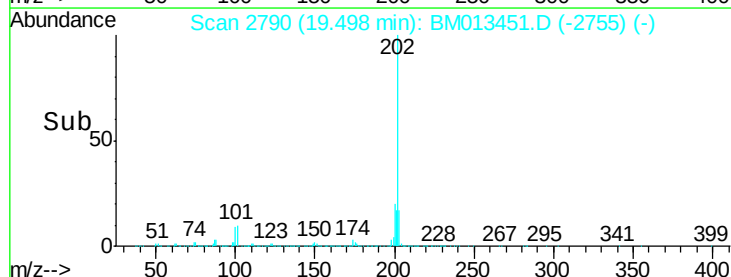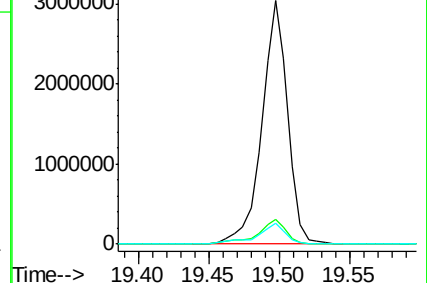

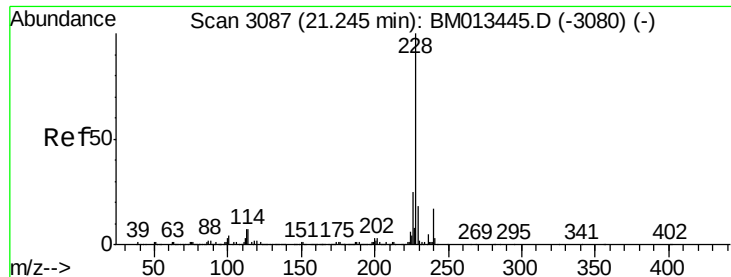

#80

Benzo(a)anthracene

Concen: 9.01 ng/ul

RT: 21.24 min Scan# 3087

Delta R.T. -0.00 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12


Tgt Ion:228 Resp: 781482

Ion Ratio Lower Upper




228 100

229 20.8 15.4 23.0

226 26.0 21.4 32.0

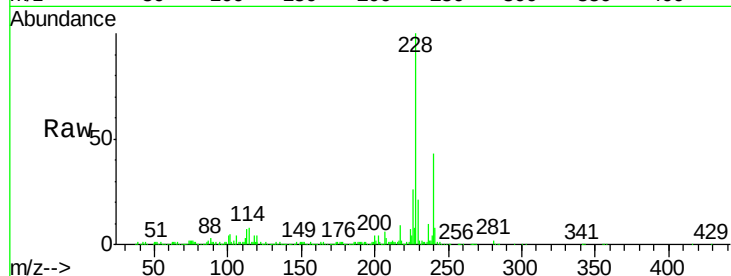

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

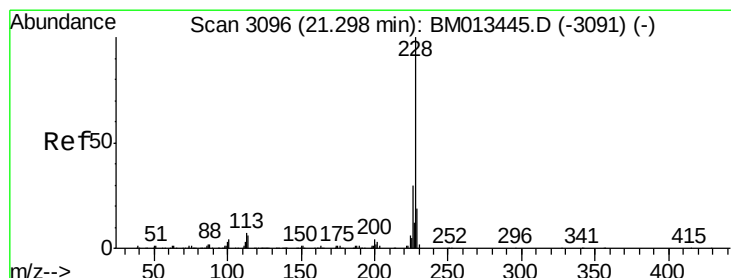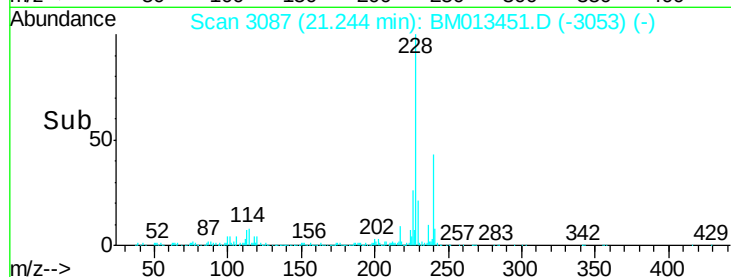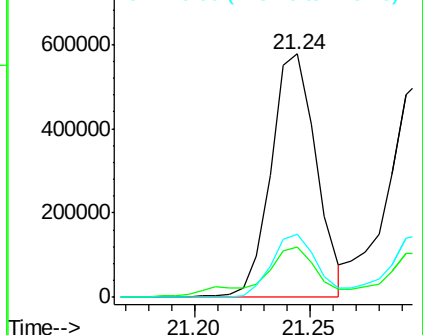

#82

Chrysene

Concen: 9.03 ng/ul

RT: 21.30 min Scan# 3096

Delta R.T. -0.00 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44


Tgt Ion:228 Resp: 726866

Ion Ratio Lower Upper



228 100


226 27.9 23.4 35.2

229 19.9 15.5 23.3

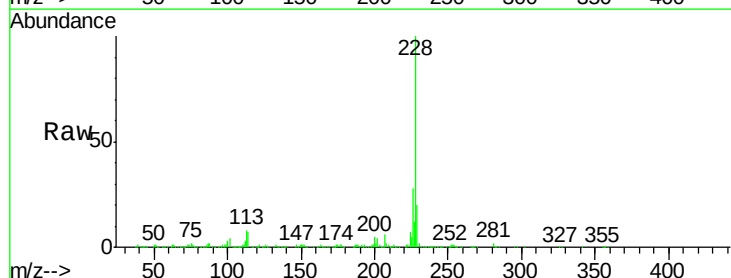

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

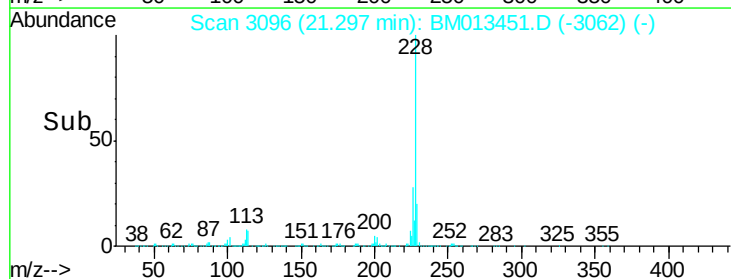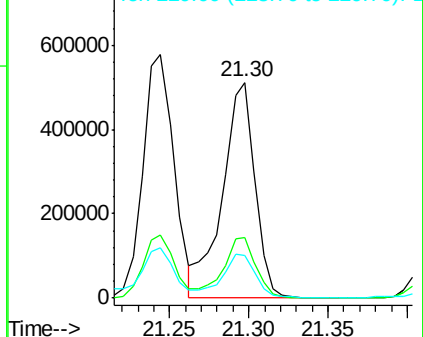

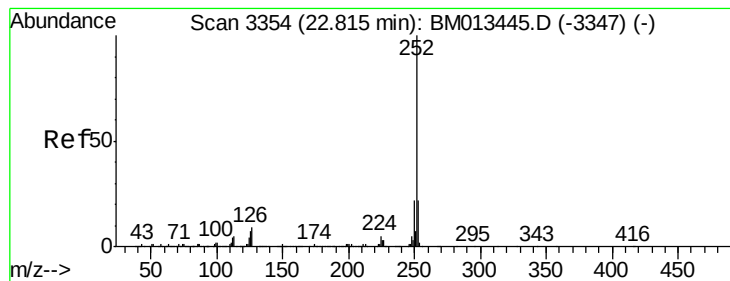

#85

Benzo(b)fluoranthene

Concen: 4.29 ng/ul

RT: 22.82 min Scan# 3355

Delta R.T. 0.01 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12


Tgt Ion:252 Resp: 307885

Ion Ratio Lower Upper

252 100

253 22.4 17.9 26.9




125 8.0 3.6 5.4#

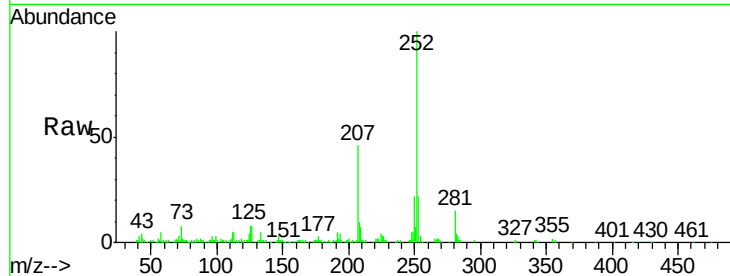

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

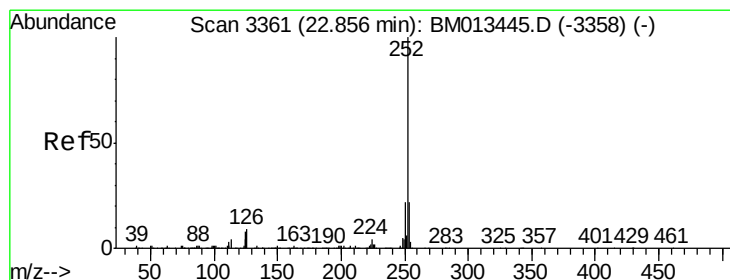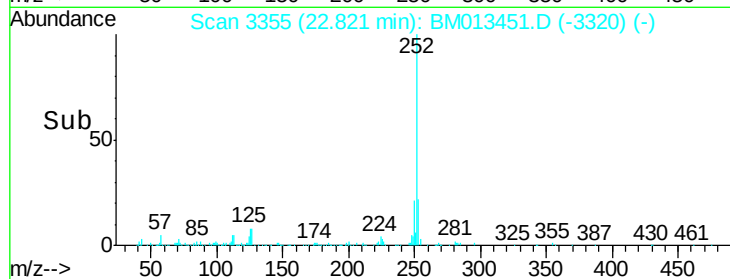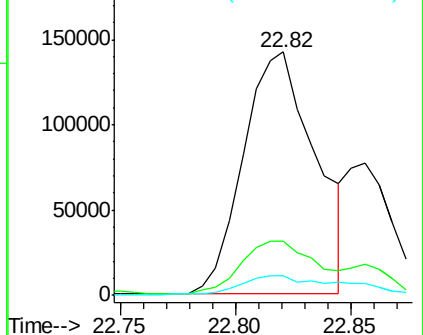

#86

Benzo(k)fluoranthene

Concen: 1.51 ng/ul

RT: 22.86 min Scan# 3361

Delta R.T. -0.00 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44


Tgt Ion:252 Resp: 102022

Ion Ratio Lower Upper

252 100

253 23.1 17.1 25.7



125 8.8 3.4 5.2#

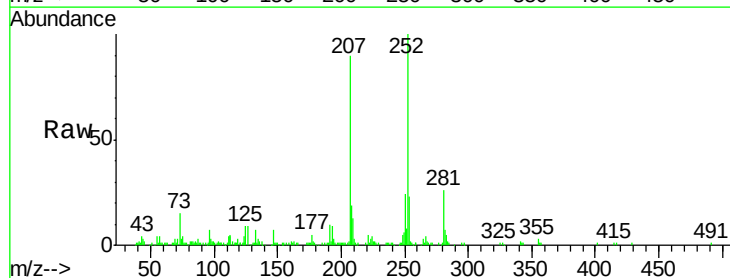


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

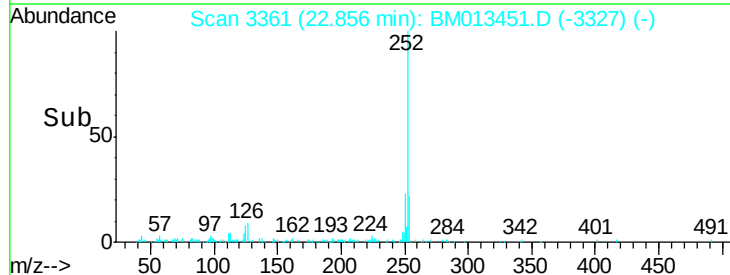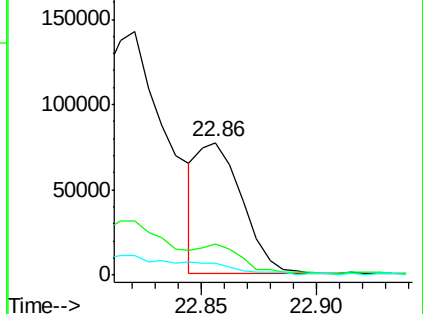

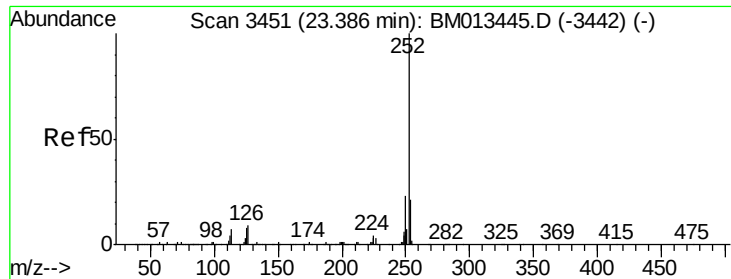

#88

Benzo(a)pyrene

Concen: 2.56 ng/ul

RT: 23.39 min Scan# 3451

Delta R.T. -0.00 min

Lab File: BM013451.D

Acq: 15 Dec 2017 22:44

Instrument :

BNA_M

ClientSampleId :

F9A12

Tgt Ion:252 Resp: 164923

Ion Ratio Lower Upper

252 100

253 20.4 18.2 27.2

125 7.9 4.0 6.0#

