


Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A09

Manual Integrations
APPROVED

Sohil
12/18/2017 2:09:50 PM

Quant Time: Dec 18 00:50:47 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

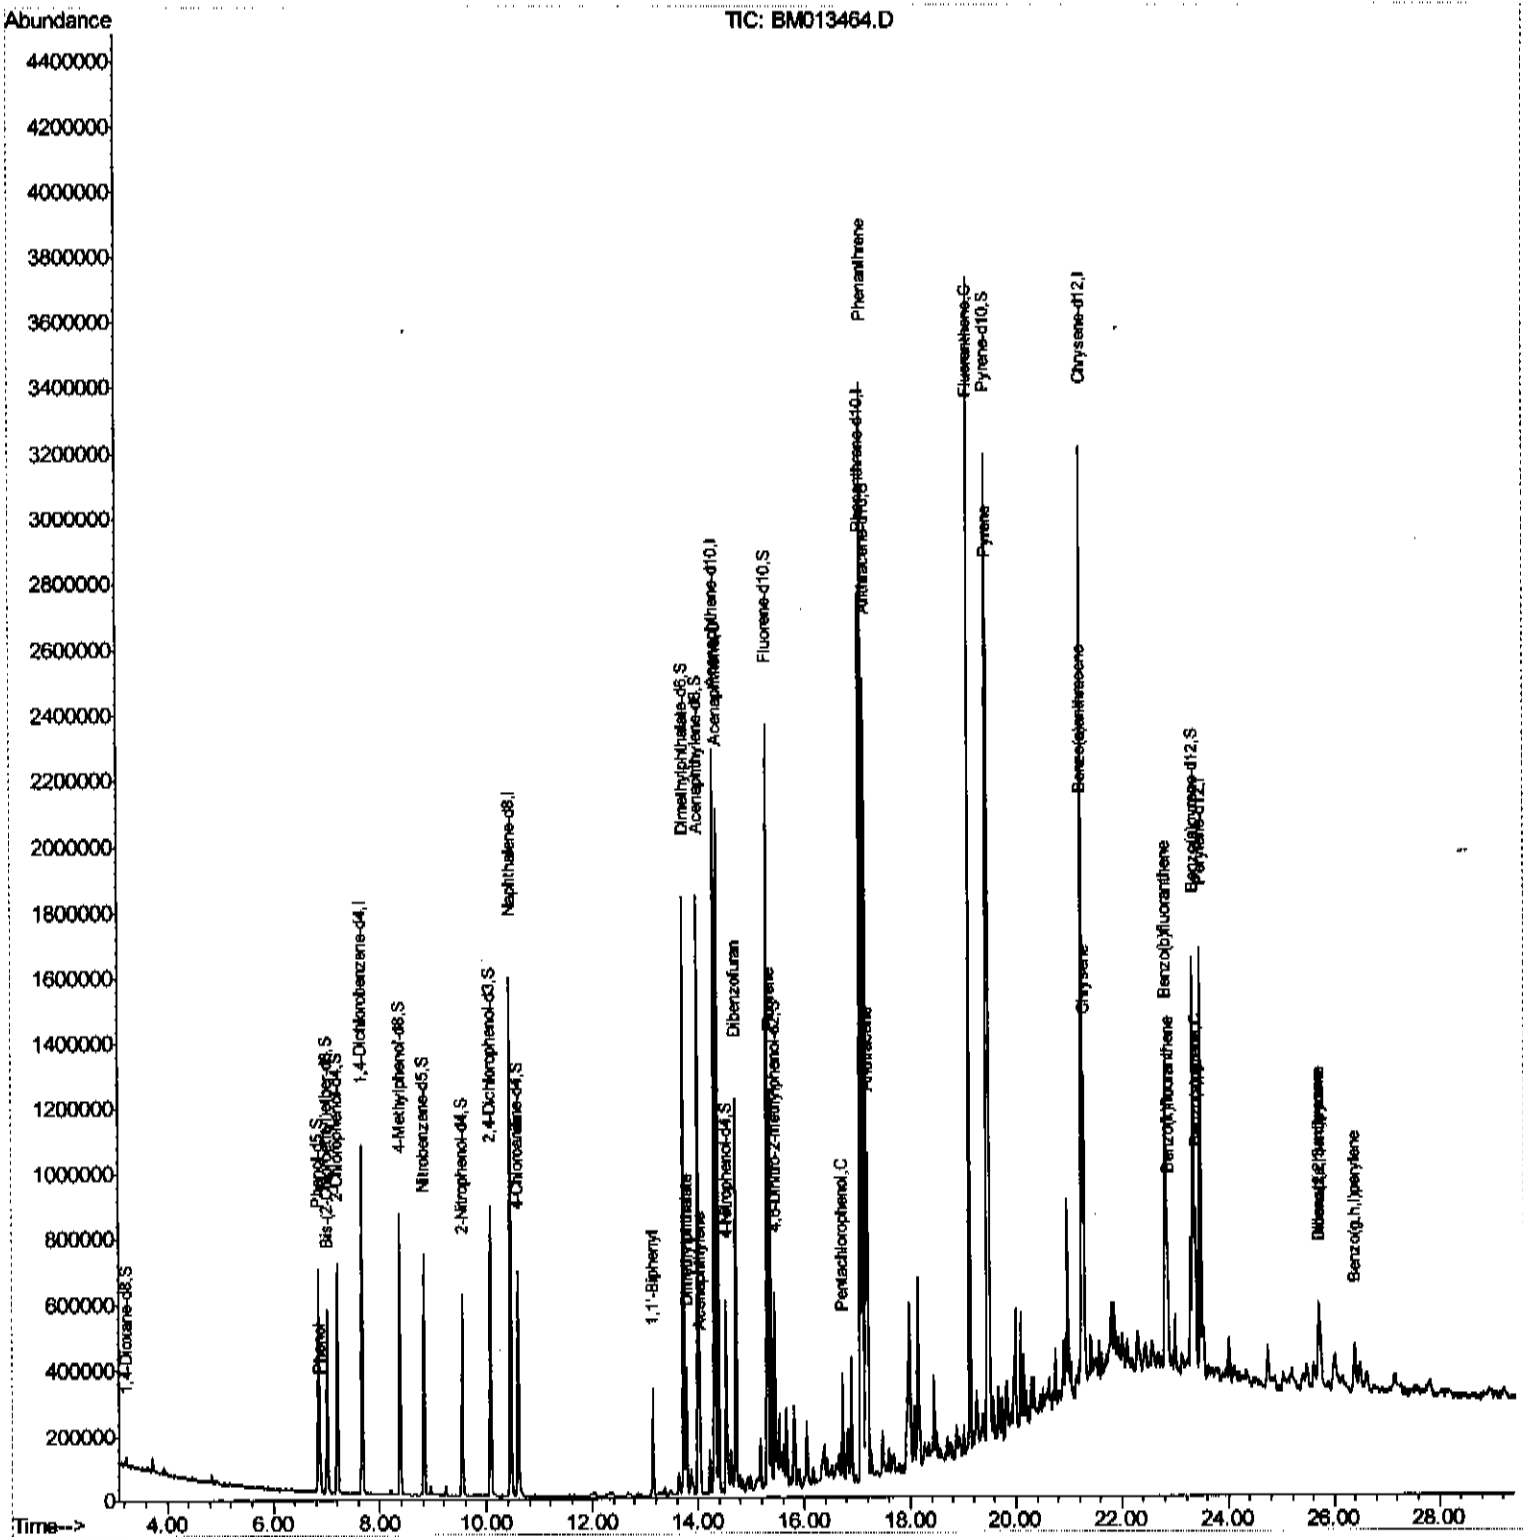


Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A09

Manual Integrations
APPROVED
Sohil
12/18/2017 2:09:50 PM

Quant Time: Dec 18 00:27:37 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

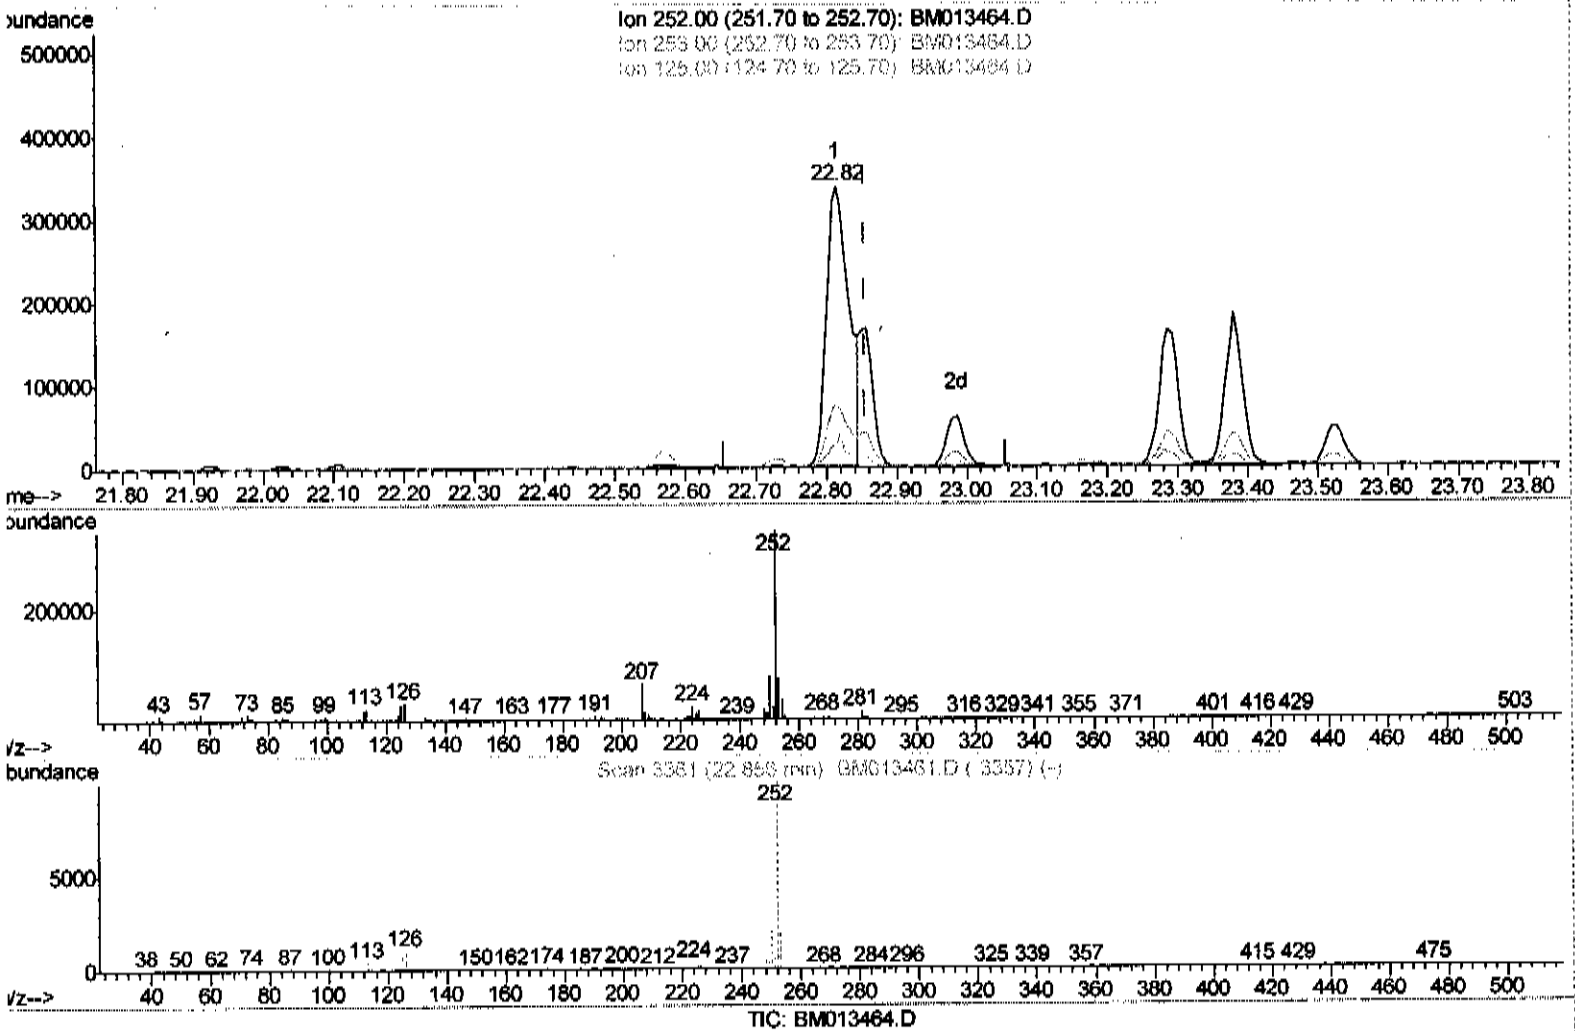

(86) Benzo(k)fluoranthene

22.815min (-0.041) 12.46ng/ul

response 759729




Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.26
125.00	4.30	8.06%
0.00	0.00	0.00

Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F9A09

Manual Integrations
APPROVED
Sohil
12/18/2017 2:09:50 PM

Quant Time: Dec 18 00:27:37 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

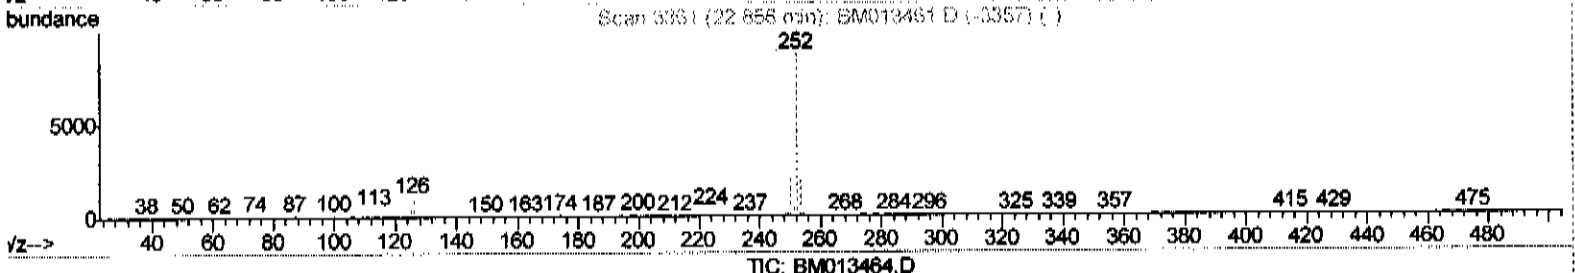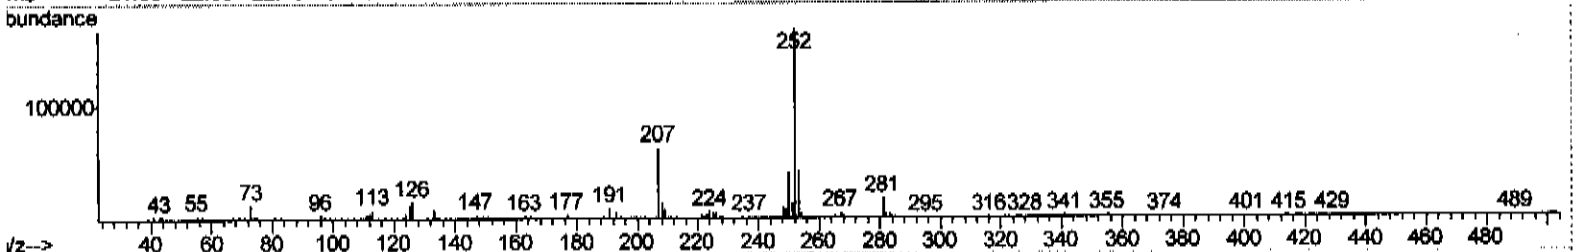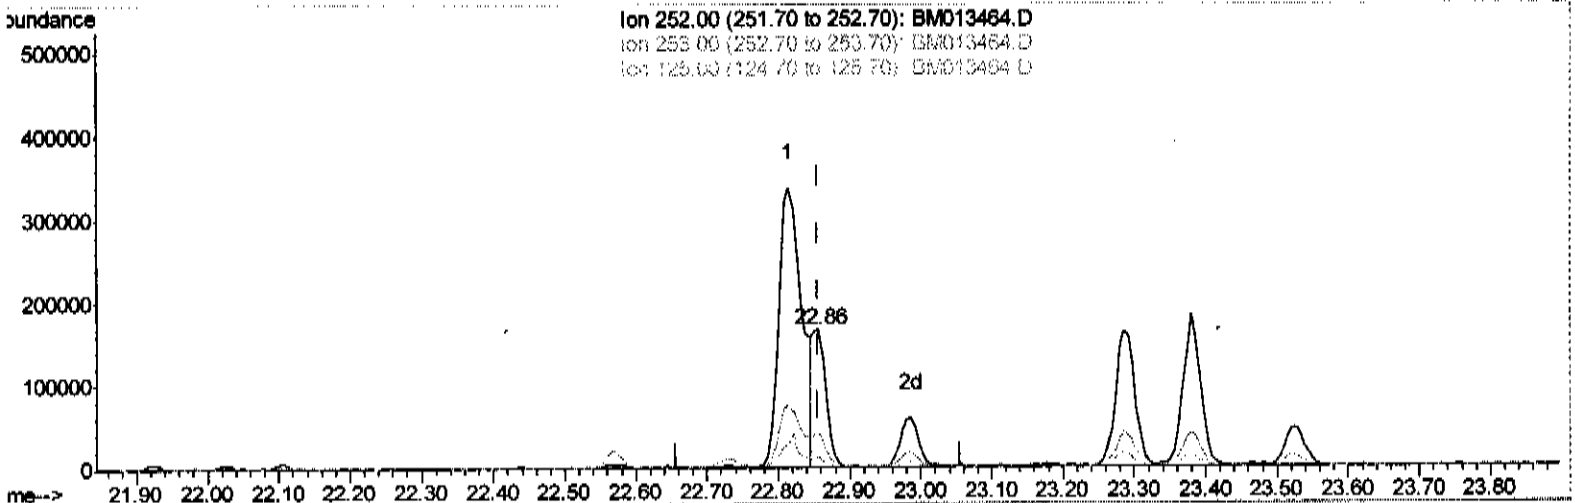

(86) Benzo(k)fluoranthene

22.856min (-0.000) 3.48ng/ul m SJ 12/18/17

response 212520


Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.86
125.00	4.30	7.47#
0.00	0.00	0.00

Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F9A09

Manual Integrations
APPROVED
Sohil
12/18/2017 2:09:50 PM

Quant Time: Dec 18 00:49:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

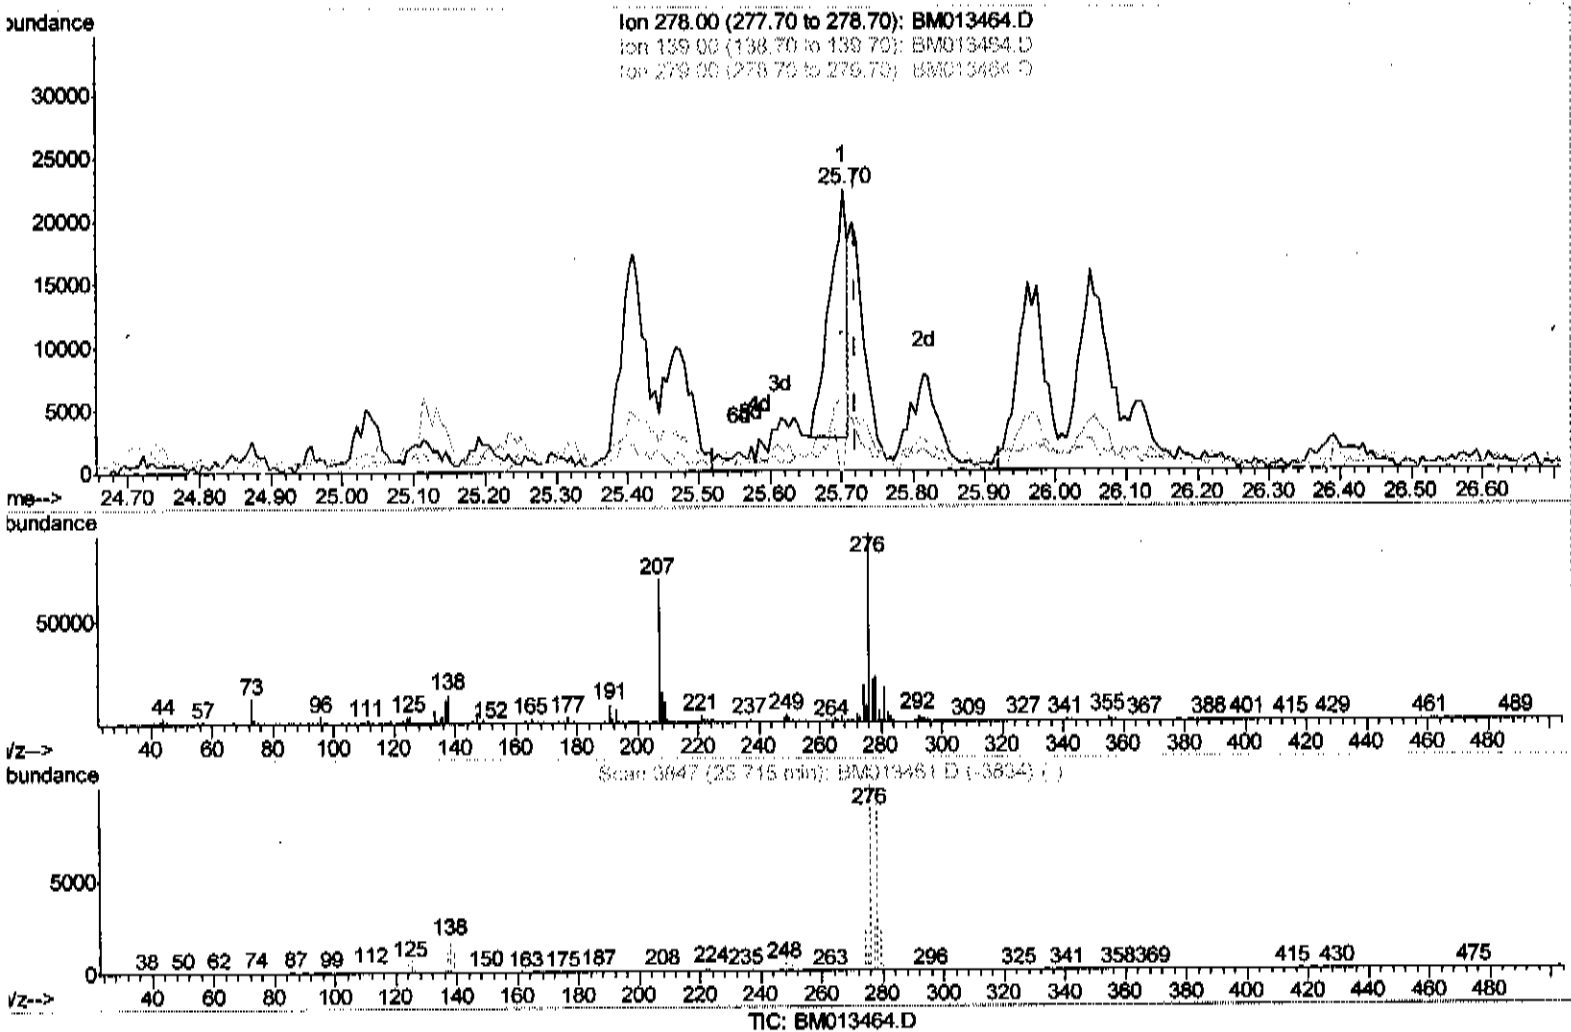

(90) Dibenzo(a,h)anthracene

25.703min (-0.018) 0.69ng/ul

response 34070


Ion	Exp%	Act%
278.00	100	100
139.00	7.30	0.00#
279.00	23.20	25.48
0.00	0.00	0.00

Data File : BM013464.D
Acq On : 16 Dec 2017 06:26
Operator : SJ/JU
Sample : I6775-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F9A09

Manual Integrations
APPROVED
Sohil
12/18/2017 2:09:50 PM

Quant Time: Dec 18 00:49:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 16 00:23:08 2017
Response via : Initial Calibration

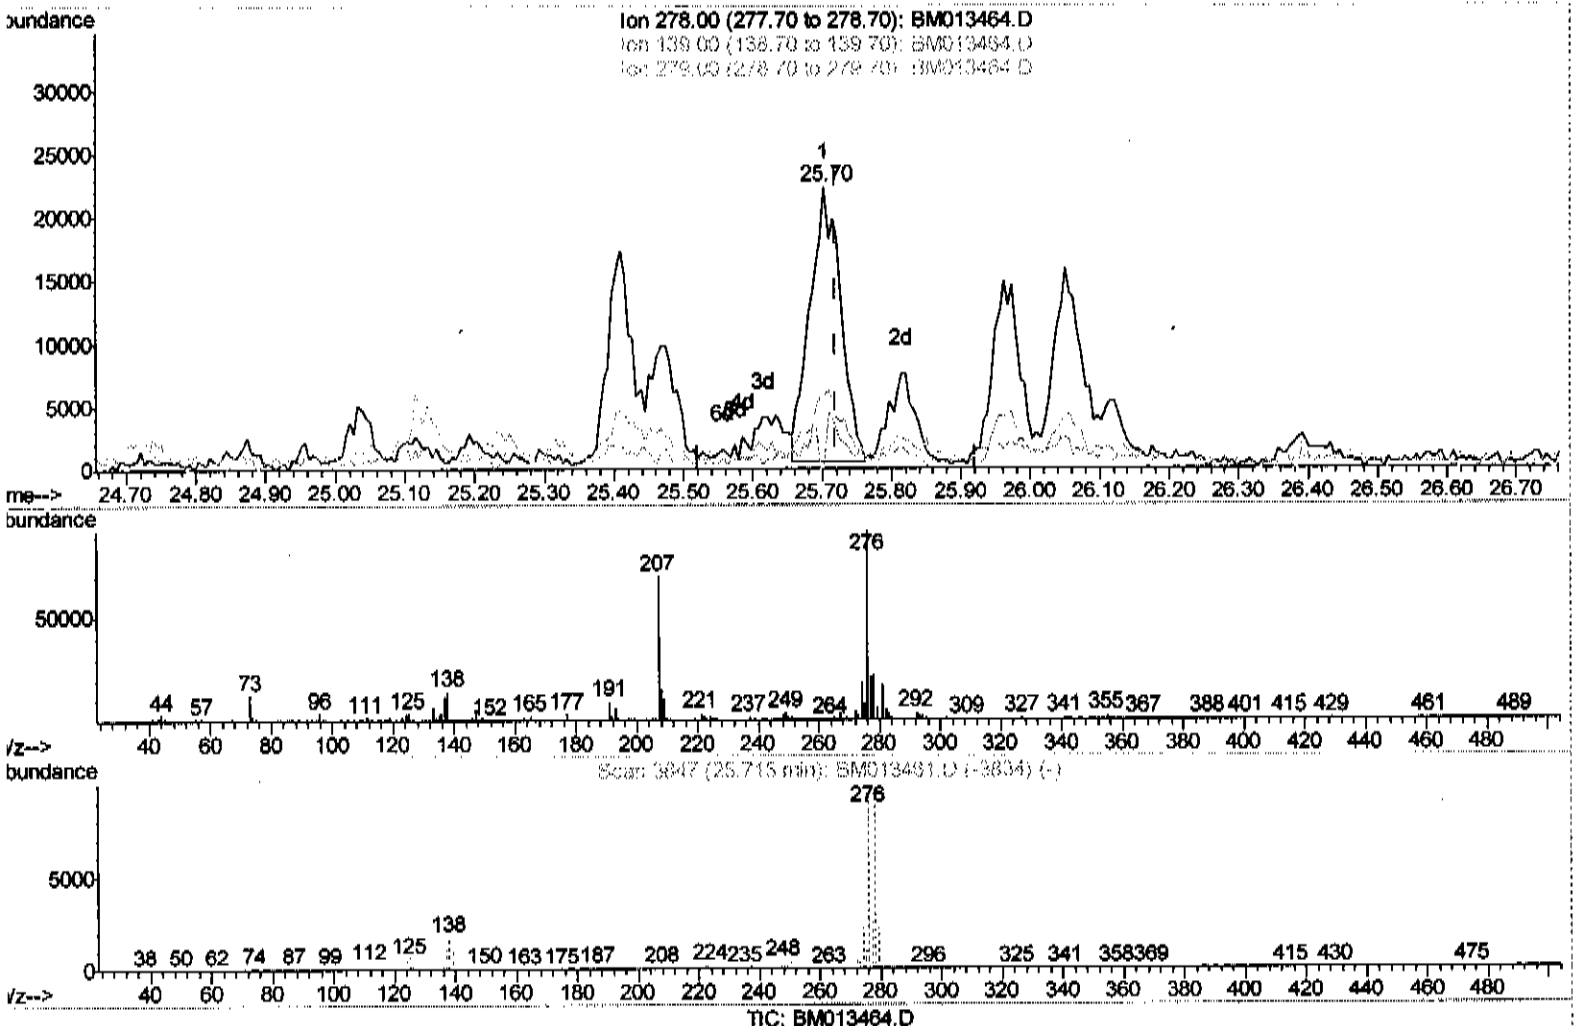

(90) Dibenzo(a,h)anthracene
25.703min (-0.018) 1.37ng/ul m SJ 12/18/17

response 67445

Ion	Exp%	Act%
278.00	100	100
139.00	7.30	0.00%
279.00	23.20	25.48
0.00	0.00	0.00

Data File : BM013464.D

Acq On : 16 Dec 2017 06:26

Operator : SJ/JU

Sample : I6775-06

Misc :

ALS Vial : 21 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

F9A09

Manual Integrations
APPROVED

Sohil

12/18/2017 2:09:50 PM

Quant Time: Dec 18 00:50:47 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M

Quant Title : SVOA CALIBRATION

Last Update : Sat Dec 16 00:23:08 2017

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	275208	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1215655	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	713964	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1517698	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1142596	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	961509	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	15619	2.81	ng/uL	0.00
5) Phenol-d5	6.85	99	361237	15.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	229390	16.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	305916	16.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	297859	14.64	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	167965	17.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	182720	17.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	322384	15.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	358585	18.35	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1118321	17.60	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1302491	16.61	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	126985	11.50	ng/ul	0.00
57) Fluorene-d10	15.32	176	900036	16.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	120580	12.63	ng/ul	0.00
70) Anthracene-d10	17.16	188	1323914	17.42	ng/ul	0.00
76) Pyrene-d10	19.46	212	1267844	22.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	828722	16.92	ng/ul	0.00

Target Compounds

					Qvalue
6) Phenol	6.88	94	54858	2.33 ng/ul#	84
40) 1,1'-Biphenyl	13.15	154	145418	2.41 ng/ul	94
44) Dimethylphthalate	13.78	163	221811	3.65 ng/ul	98
47) Acenaphthylene	14.03	152	112384	1.55 ng/ul#	91
49) Acenaphthene	14.38	153	787037	15.92 ng/ul	97
53) Dibenzofuran	14.72	168	695588	9.53 ng/ul	98
58) Fluorene	15.37	166	493526	8.18 ng/ul	96
68) Pentachlorophenol	16.72	266	37704	3.31 ng/ul	96
69) Phenanthrene	17.11	178	1917254	22.24 ng/ul	99
71) Anthracene	17.20	178	585427	6.64 ng/ul	99
74) Fluoranthene	19.13	202	2103655	19.91 ng/ul#	90
77) Pyrene	19.49	202	1491998	21.49 ng/ul#	91
80) Benzo(a)anthracene	21.24	228	478141	6.60 ng/ul	99
82) Chrysene	21.29	228	543871	8.09 ng/ul	96
85) Benzo(b)fluoranthene	22.82	252	759729	11.72 ng/ul#	98
86) Benzo(k)fluoranthene	22.86	252	212520m -	3.48 ng/ul	-
88) Benzo(a)pyrene	23.38	252	304389	5.23 ng/ul#	98
89) Indeno(1,2,3-cd)pyrene	25.70	276	242019	4.19 ng/ul#	94
90) Dibenzo(a,h)anthracene	25.70	278	67445m -	1.37 ng/ul	-
91) Benzo(g,h,i)perylene	26.39	276	181270	3.98 ng/ul#	95

(#)=qualifier out of range (m)=manual integration (+)=signals summed