

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038030.D
 Acq On : 15 Dec 2022 13:59
 Operator : CG/JU
 Sample : PB149580BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK580

Quant Time: Dec 15 23:43:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	4261	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	13125	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	7337	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.421	188	14762	0.400	ng/ul	0.00
17) Chrysene-d12	21.585	240	9594	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	9780	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	26185	4.496	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	5306	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	10319	0.297	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	2000	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.883	252	3531	0.090	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038030.D
Acq On : 15 Dec 2022 13:59
Operator : CG/JU
Sample : PB149580BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK580

Quant Time: Dec 15 23:43:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

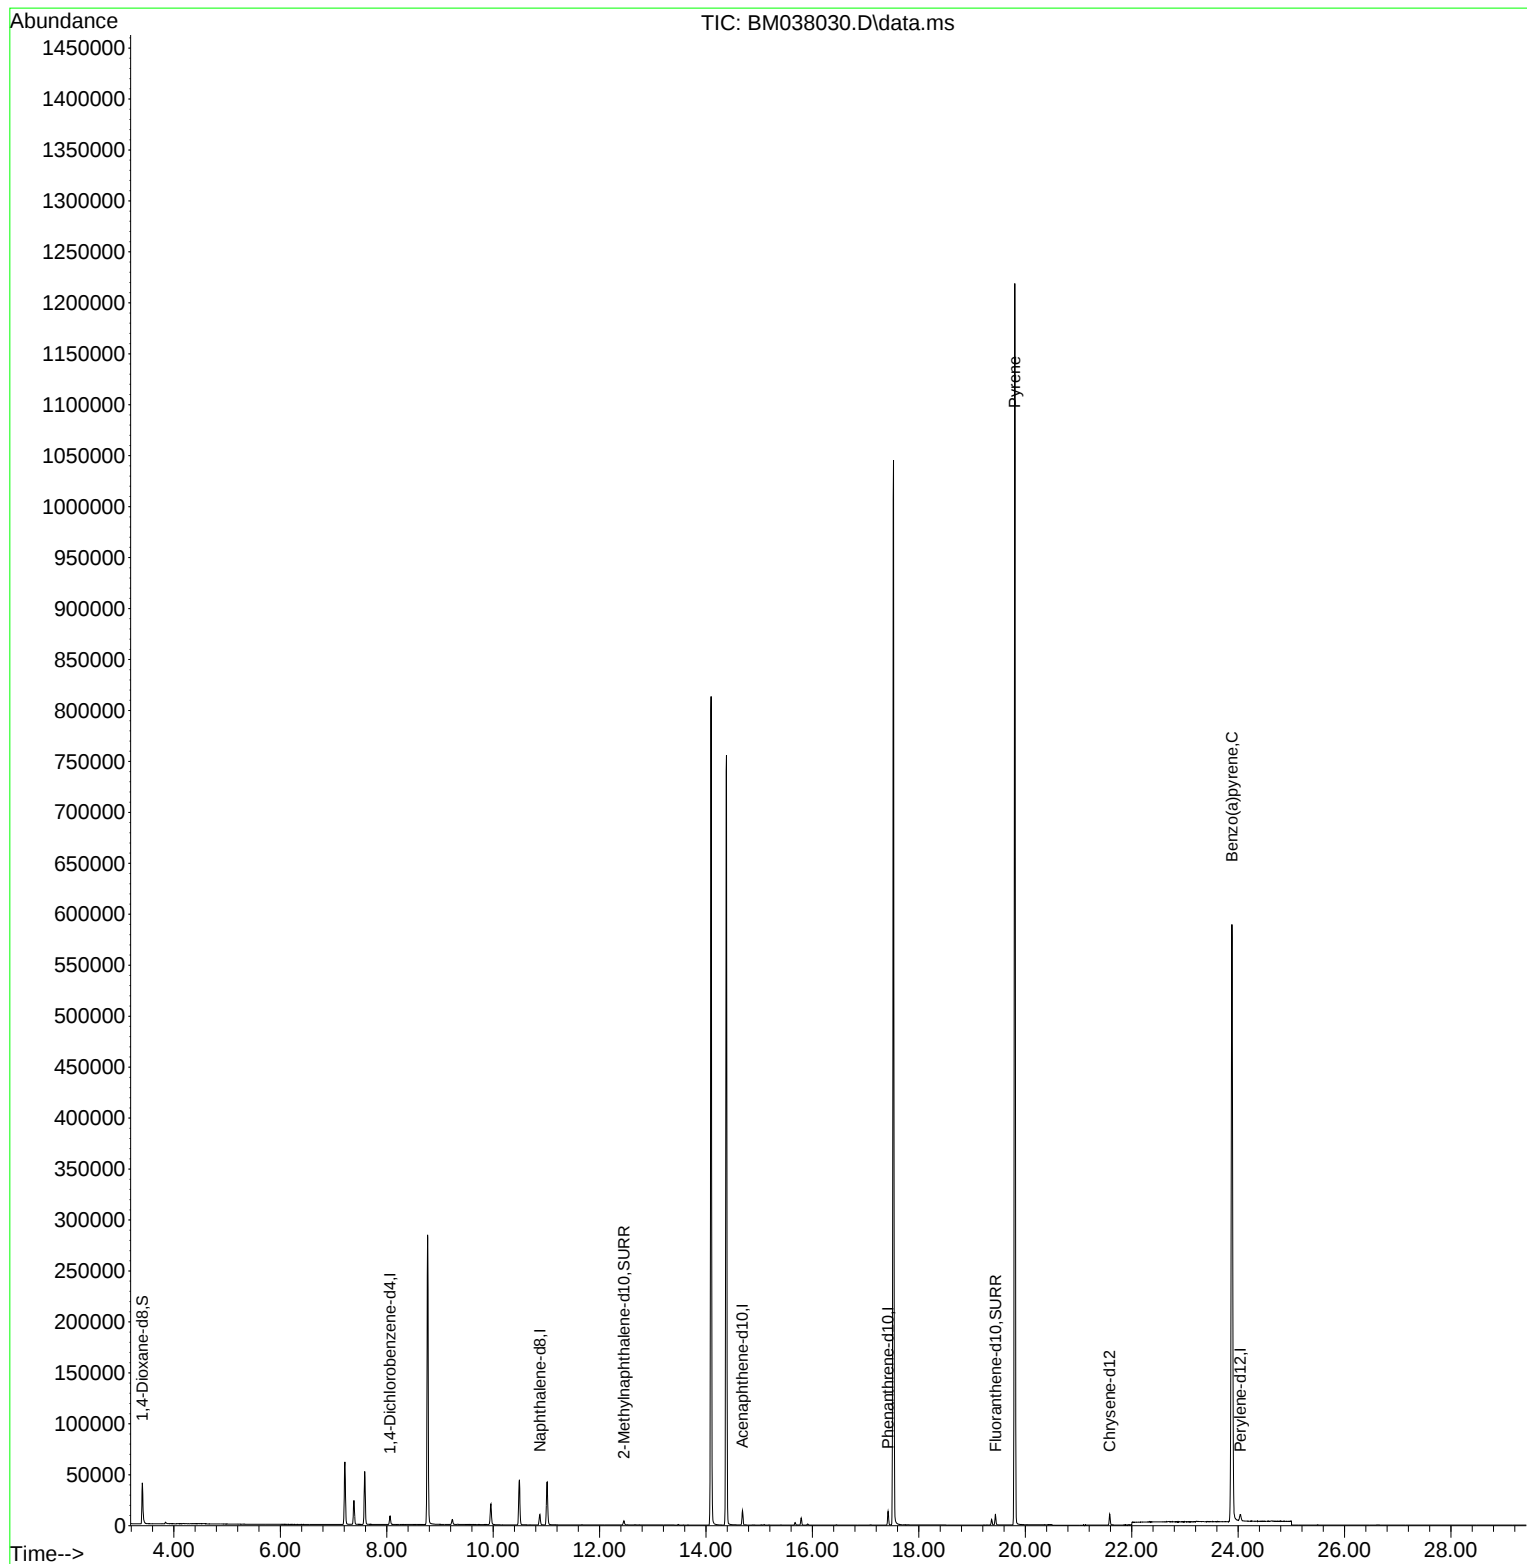

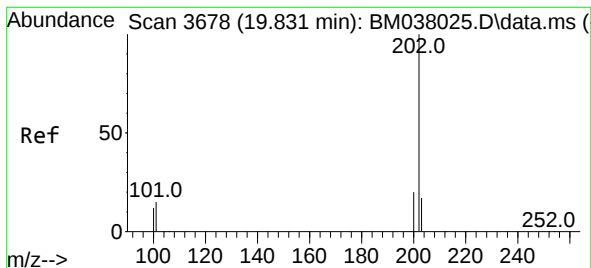

#20

Pyrene

Concen: 0.040 ng/ul

RT: 19.803 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM038030.D

Acq: 15 Dec 2022 13:59

Instrument :

BNA_M

ClientSampleId :

SBLK580





Tgt Ion:202 Resp: 2000

Ion Ratio Lower Upper

202 100

101 149.3 12.1 18.1#

100 1045.1 9.8 14.6#

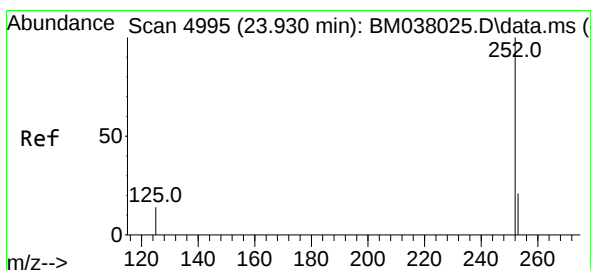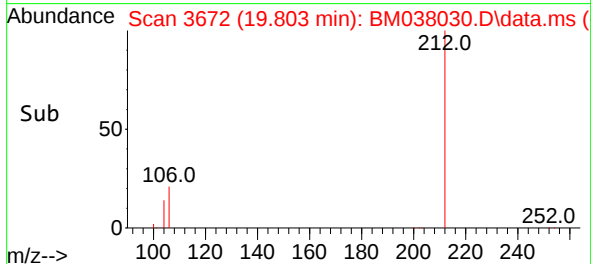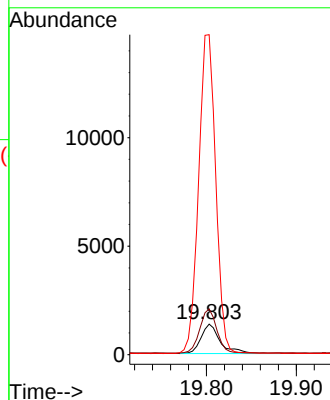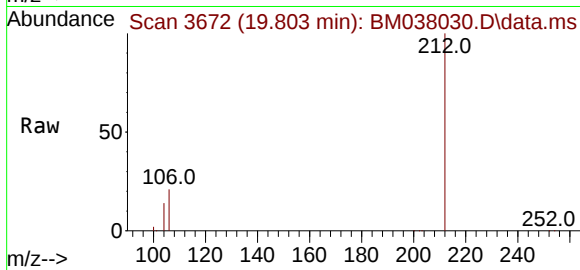

#26

Benzo(a)pyrene

Concen: 0.090 ng/ul

RT: 23.883 min Scan# 4979

Delta R.T. -0.047 min

Lab File: BM038030.D

Acq: 15 Dec 2022 13:59

Tgt Ion:252 Resp: 3531

Ion Ratio Lower Upper

252 100

253 49.4 21.9 32.9#

125 68.6 20.7 31.1#

