

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038036.D
 Acq On : 15 Dec 2022 17:41
 Operator : CG/JU
 Sample : PB149580BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK580

Quant Time: Dec 15 23:44:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	4477	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	13820	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	7887	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	15887	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	10791	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	11308	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	27411	4.480	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	5701	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	11375	0.291	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	2218	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.883	252	3877	0.086	ng/ul#	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038036.D
Acq On : 15 Dec 2022 17:41
Operator : CG/JU
Sample : PB149580BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK580

Quant Time: Dec 15 23:44:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration




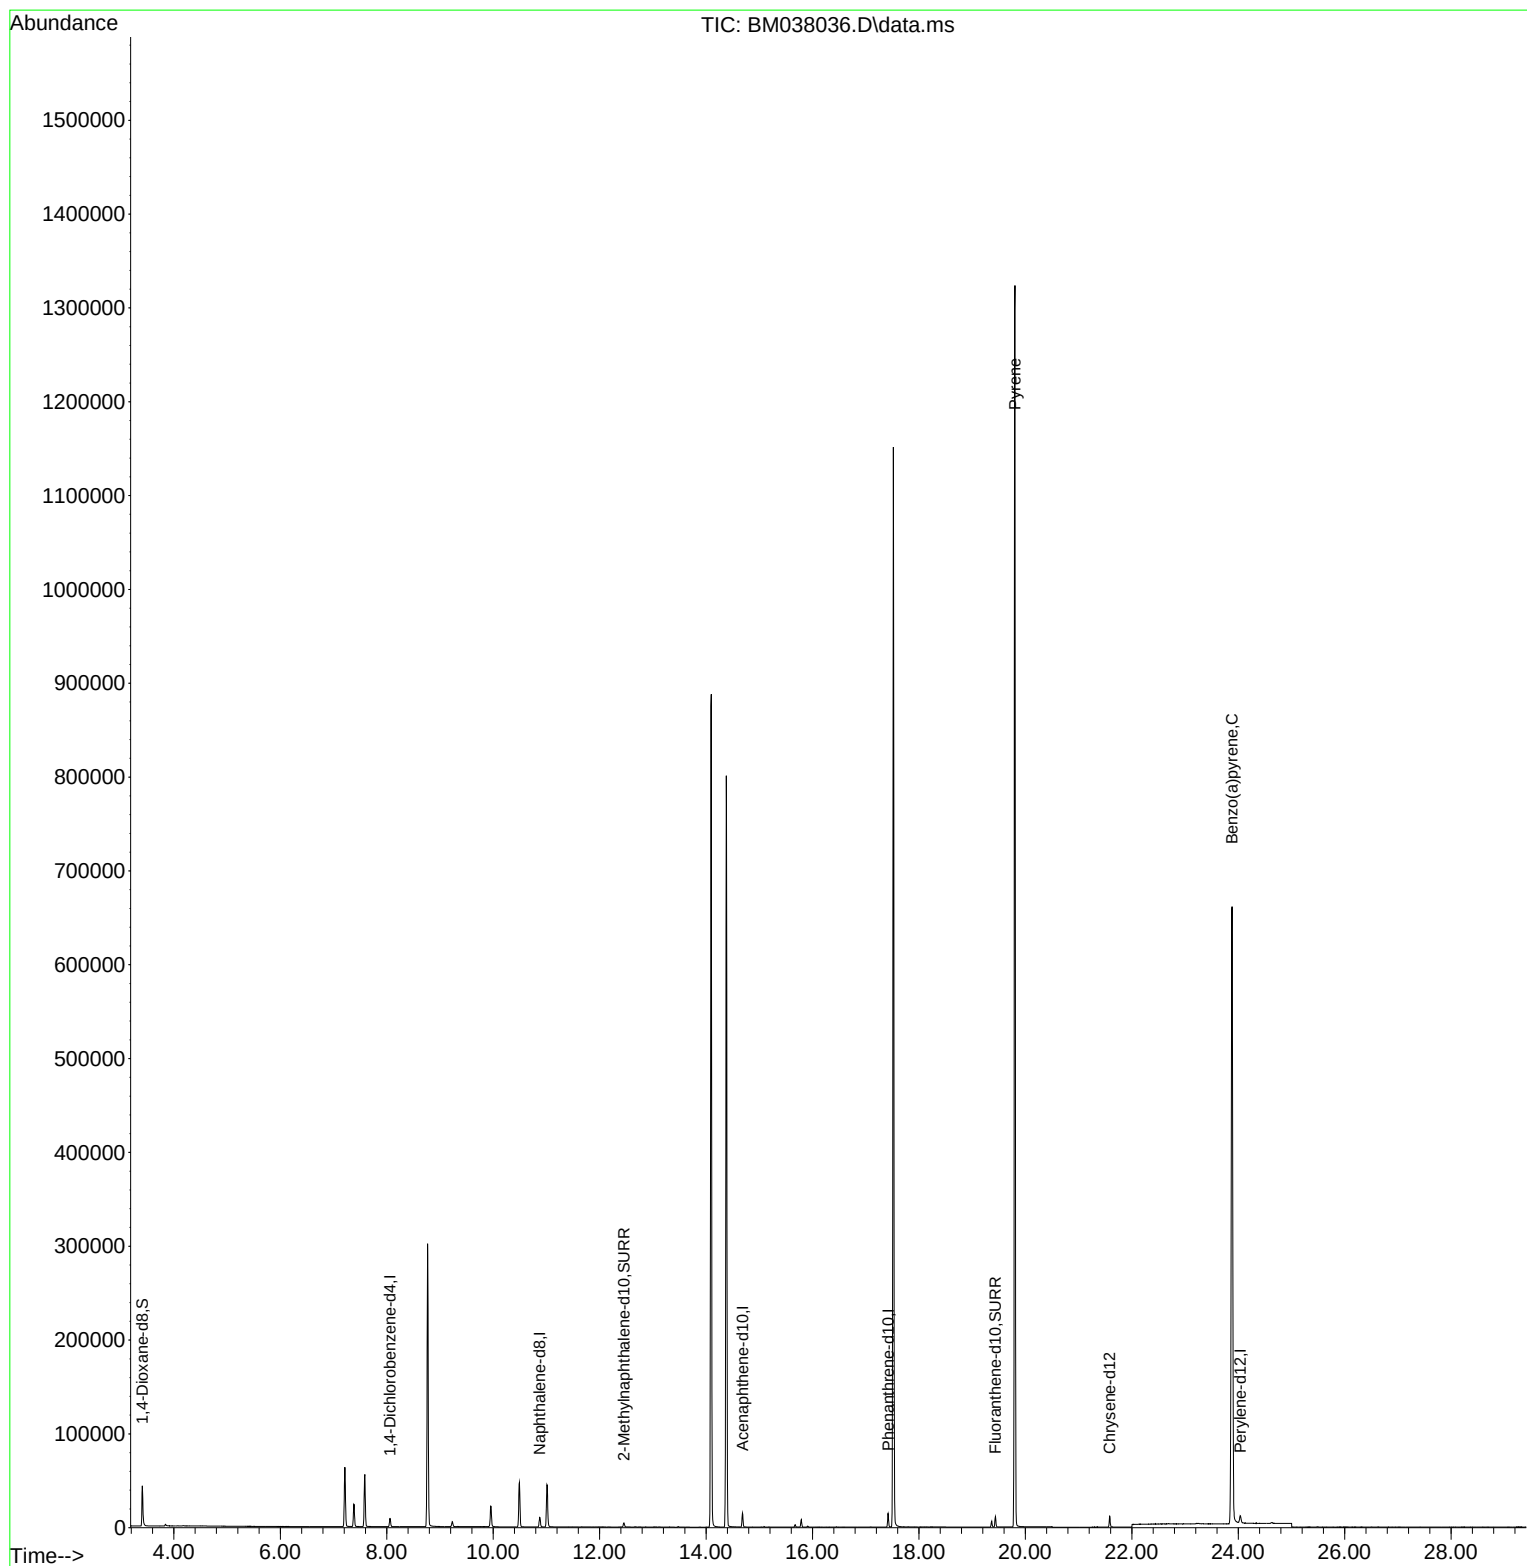


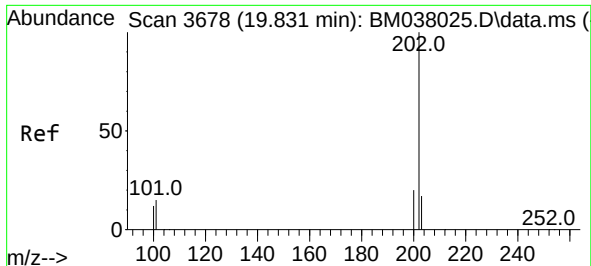

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.803 min Scan# 3
Delta R.T. -0.028 min
Lab File: BM038036.D
Acq: 15 Dec 2022 17:41

Instrument :
BNA_M
ClientSampleId :
SBLK580

Tgt Ion:202 Resp: 2218
Ion Ratio Lower Upper
202 100
101 144.7 12.1 18.1#
100 993.3 9.8 14.6#

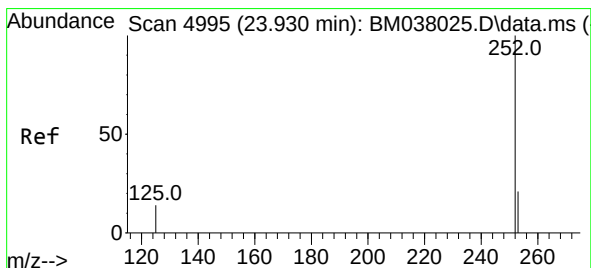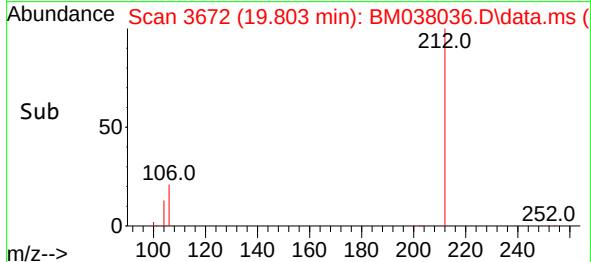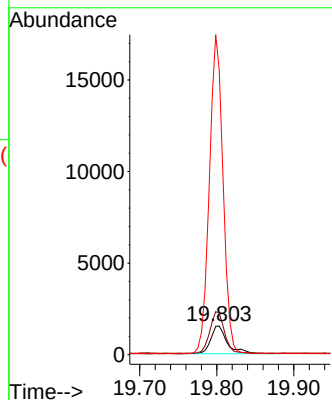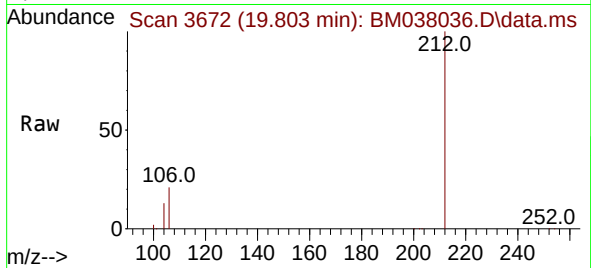

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.883 min Scan# 4979
Delta R.T. -0.047 min
Lab File: BM038036.D
Acq: 15 Dec 2022 17:41

Tgt Ion:252 Resp: 3877
Ion Ratio Lower Upper
252 100
253 49.1 21.9 32.9#
125 84.3 20.7 31.1#

