

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038037.D
 Acq On : 15 Dec 2022 18:19
 Operator : CG/JU
 Sample : N5983-03DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLB4DL

Quant Time: Dec 15 23:44:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	3552	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	10705	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	5896	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	11979	0.400	ng/ul	0.00
17) Chrysene-d12	21.586	240	7537	0.400	ng/ul	0.00
23) Perylene-d12	24.041	264	7127	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	5184	1.068	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	1015	0.065	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	1924	0.070	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.071	266	7077	1.427	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038037.D
Acq On : 15 Dec 2022 18:19
Operator : CG/JU
Sample : N5983-03DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LB4DL

Quant Time: Dec 15 23:44:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

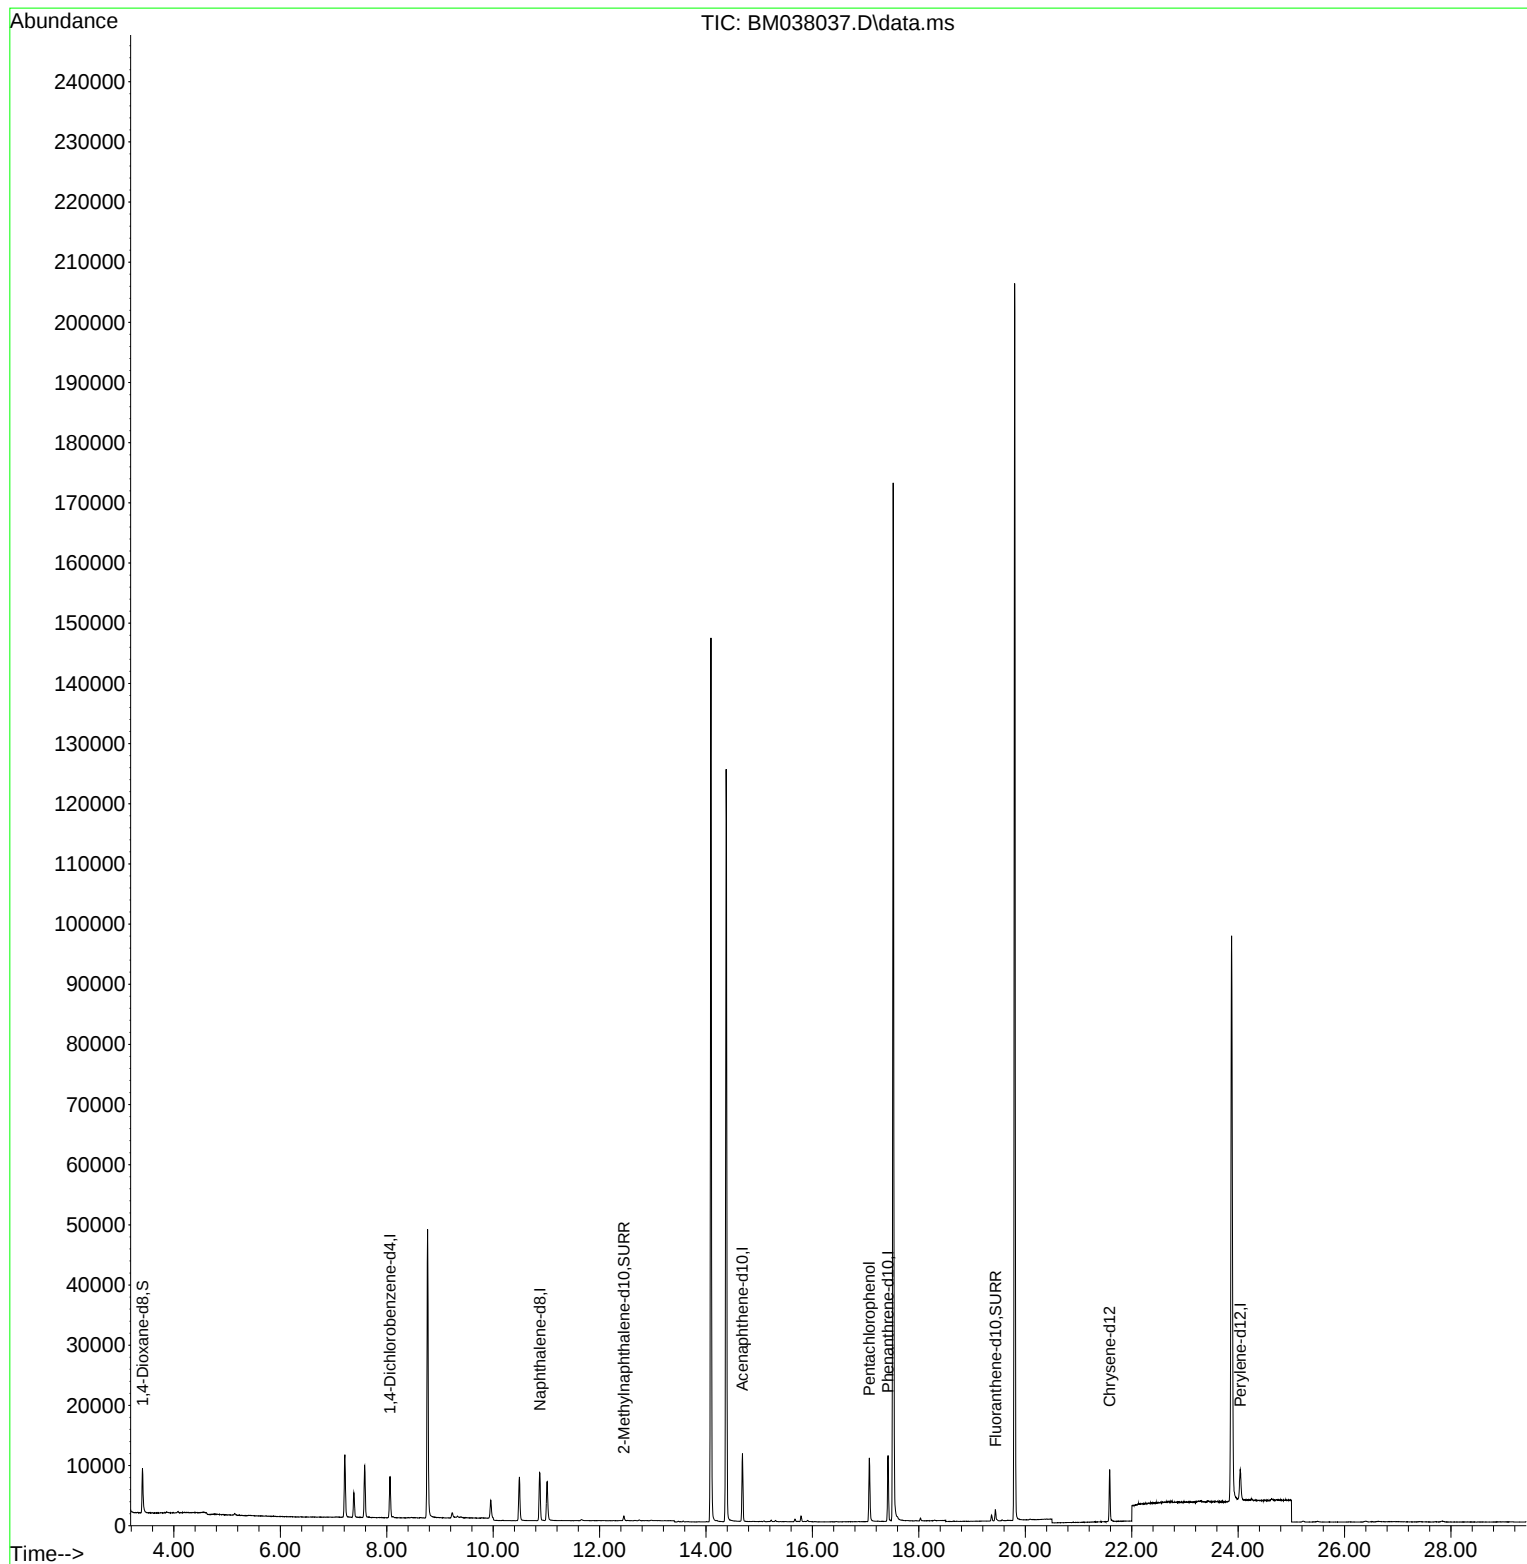

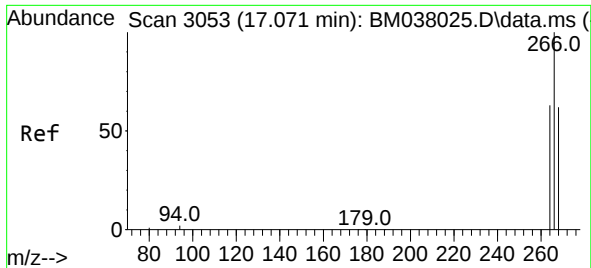

#14
 Pentachlorophenol
 Concen: 1.427 ng/ul
 RT: 17.071 min Scan# 3053
 Delta R.T. 0.000 min
 Lab File: BM038037.D
 Acq: 15 Dec 2022 18:19

Instrument :
 BNA_M
 ClientSampleId :
 C0LB4DL

Tgt Ion:	266	Resp:	7077
Ion	Ratio	Lower	Upper
266	100		
264	62.1	49.9	74.9
268	64.2	52.0	78.0

