

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038043.D
 Acq On : 15 Dec 2022 22:01
 Operator : CG/JU
 Sample : N5984-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0LC7

Quant Time: Dec 15 23:46:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	5226	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	16339	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	8949	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	19056	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	13948	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	13849	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	33175	4.644	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	7236	0.303	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	14799	0.293	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	17.067	266	39521	5.009	ng/ul	99
20) Pyrene	19.826	202	1830	0.025	ng/ul#	71
26) Benzo(a)pyrene	23.880	252	4862	0.088	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038043.D
Acq On : 15 Dec 2022 22:01
Operator : CG/JU
Sample : N5984-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LC7

Quant Time: Dec 15 23:46:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration




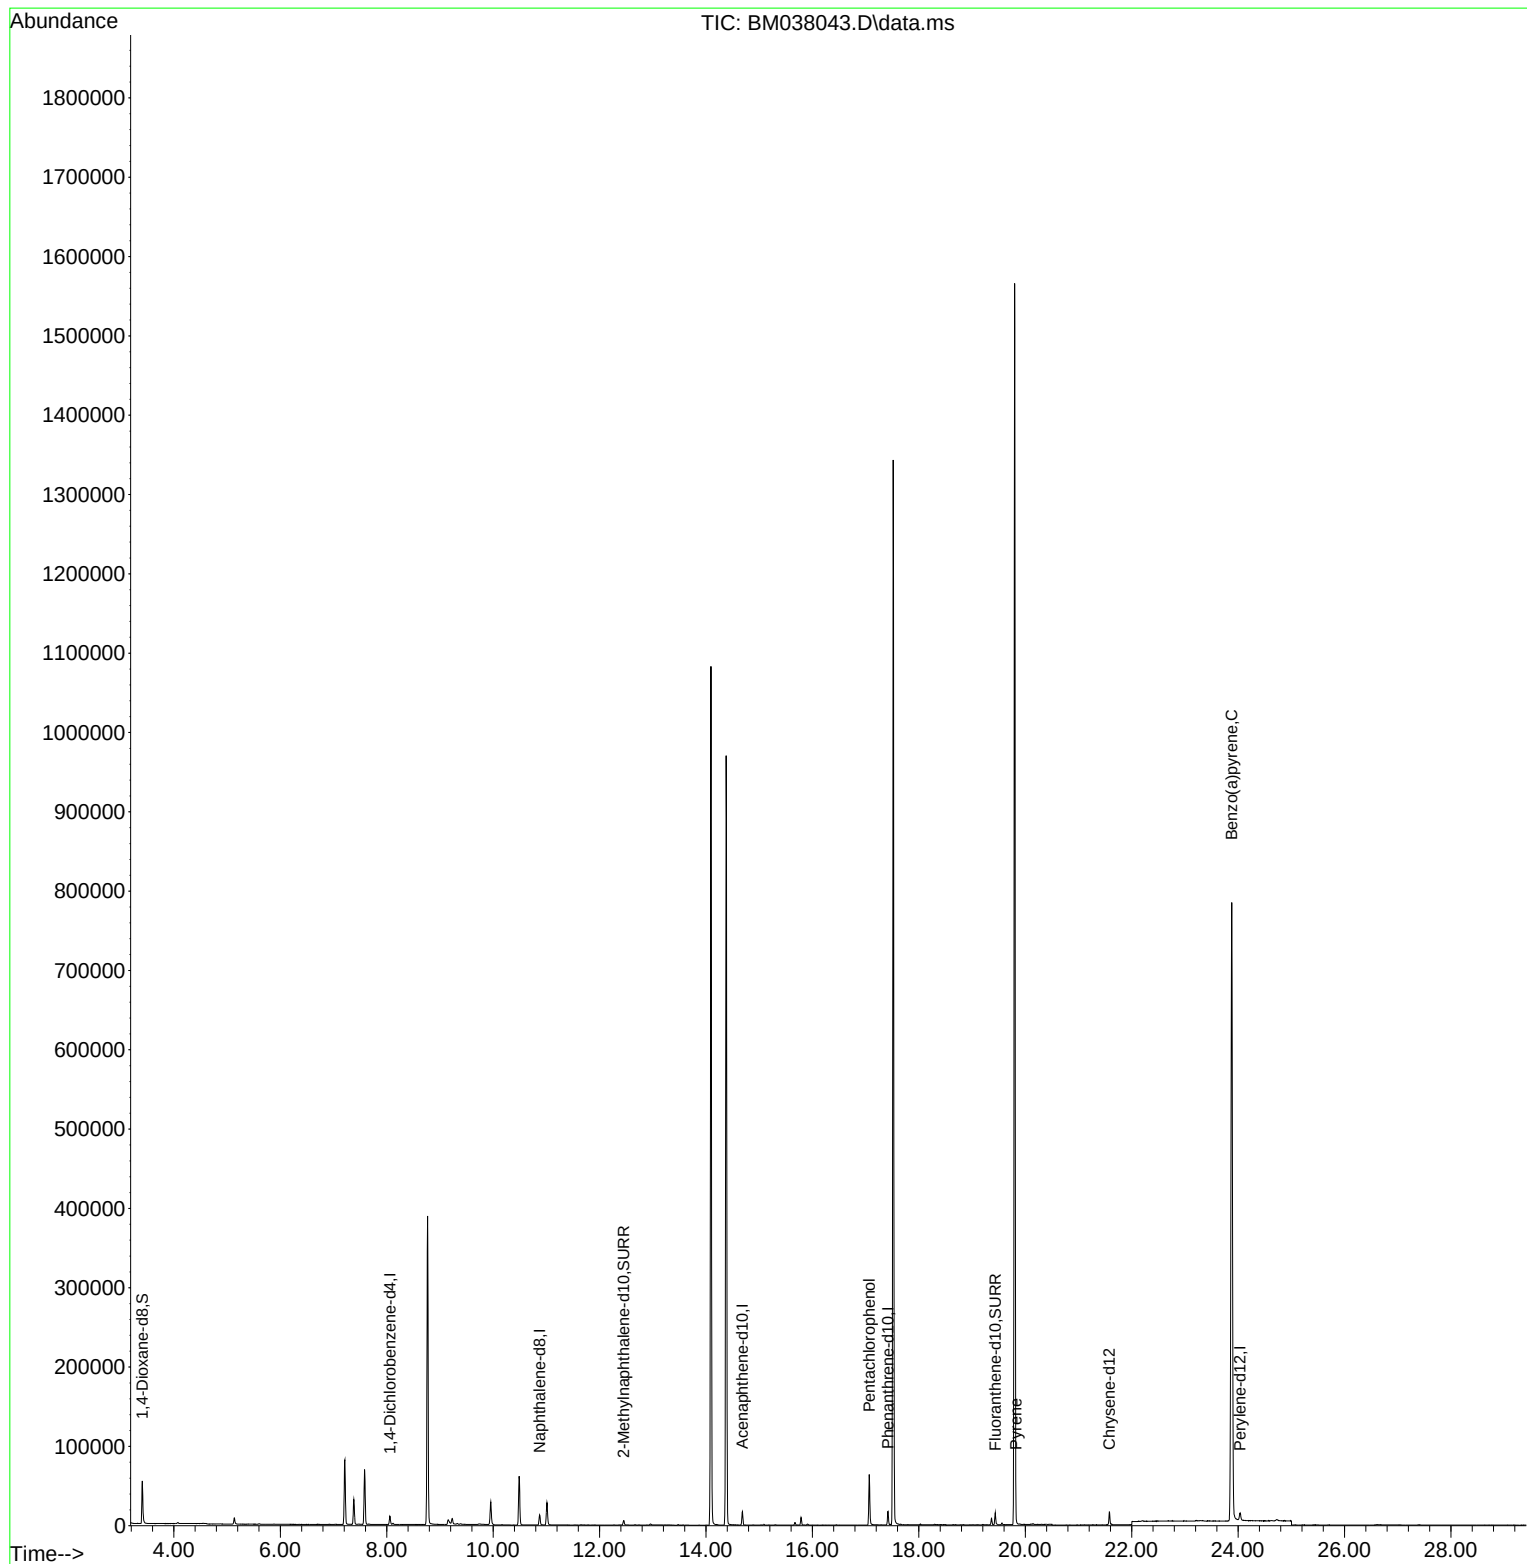


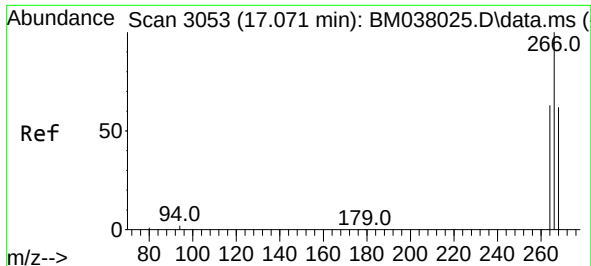

#14
 Pentachlorophenol
 Concen: 5.009 ng/ul
 RT: 17.067 min Scan# 3053
 Delta R.T. -0.004 min
 Lab File: BM038043.D
 Acq: 15 Dec 2022 22:01




Instrument :
 BNA_M
 ClientSampleId :
 C0LC7


Tgt Ion:266 Resp: 39521
 Ion Ratio Lower Upper
 266 100
 264 62.7 49.9 74.9
 268 64.3 52.0 78.0

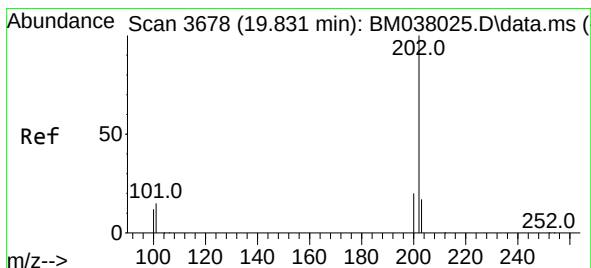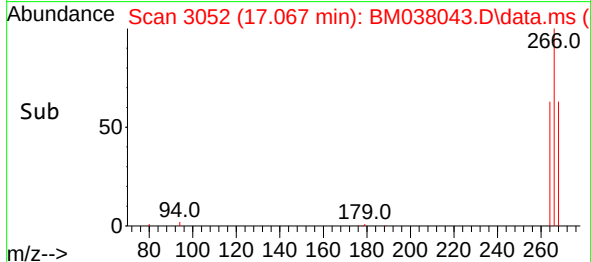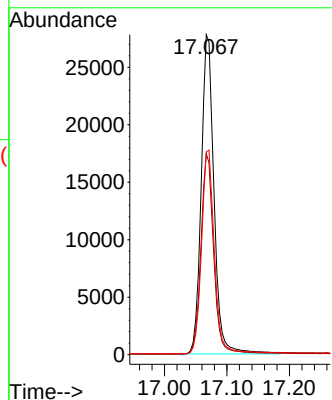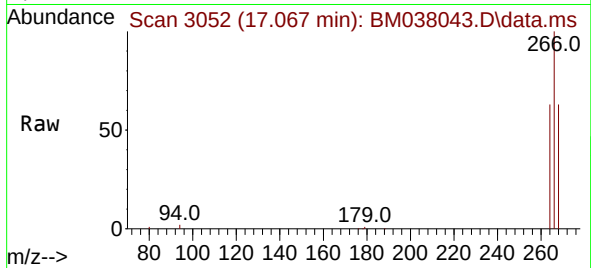

#20
 Pyrene
 Concen: 0.025 ng/ul
 RT: 19.826 min Scan# 3677
 Delta R.T. -0.005 min
 Lab File: BM038043.D
 Acq: 15 Dec 2022 22:01


Tgt Ion:202 Resp: 1830
 Ion Ratio Lower Upper
 202 100
 101 27.5 12.1 18.1#
 100 23.6 9.8 14.6#

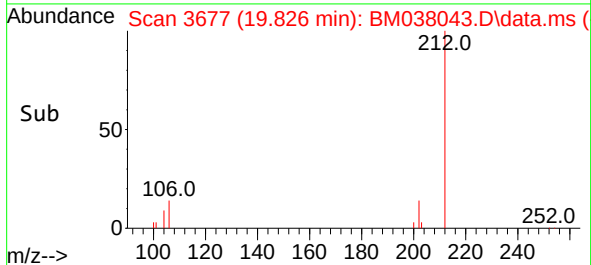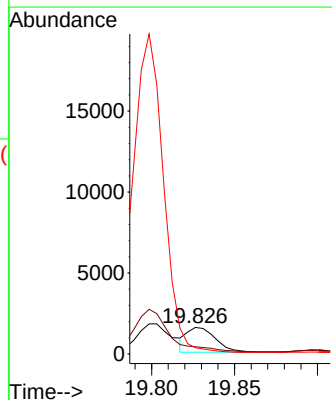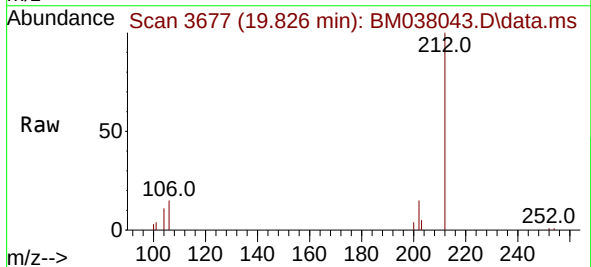

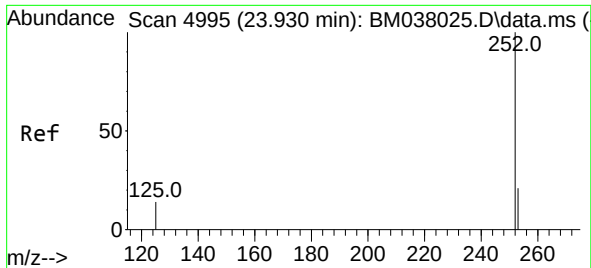

#26
 Benzo(a)pyrene
 Concen: 0.088 ng/ul
 RT: 23.880 min Scan# 4978
 Delta R.T. -0.050 min
 Lab File: BM038043.D
 Acq: 15 Dec 2022 22:01

Instrument :
 BNA_M
 ClientSampleId :
 C0LC7

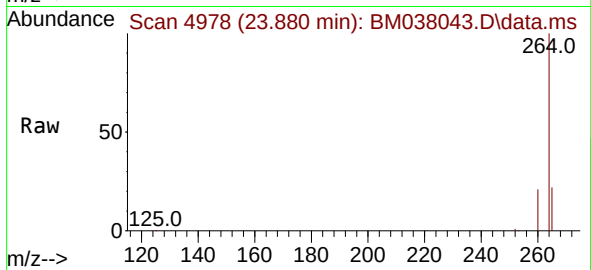

Tgt Ion:252 Resp: 4862
 Ion Ratio Lower Upper
 252 100
 253 51.1 21.9 32.9#
 125 72.6 20.7 31.1#

