

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038091.D
 Acq On : 17 Dec 2022 06:35
 Operator : CG/JU
 Sample : N5984-11DL 5X
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD6DL

Quant Time: Dec 19 03:16:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 05:21:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4324	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	12971	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.680	164	7397	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	15558	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	10950	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	10894	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	5469	0.925	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	1181	0.062	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	2473	0.062	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.067	266	5631	0.874	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038091.D
Acq On : 17 Dec 2022 06:35
Operator : CG/JU
Sample : N5984-11DL 5X
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD6DL


Quant Time: Dec 19 03:16:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 05:21:07 2022
Response via : Initial Calibration

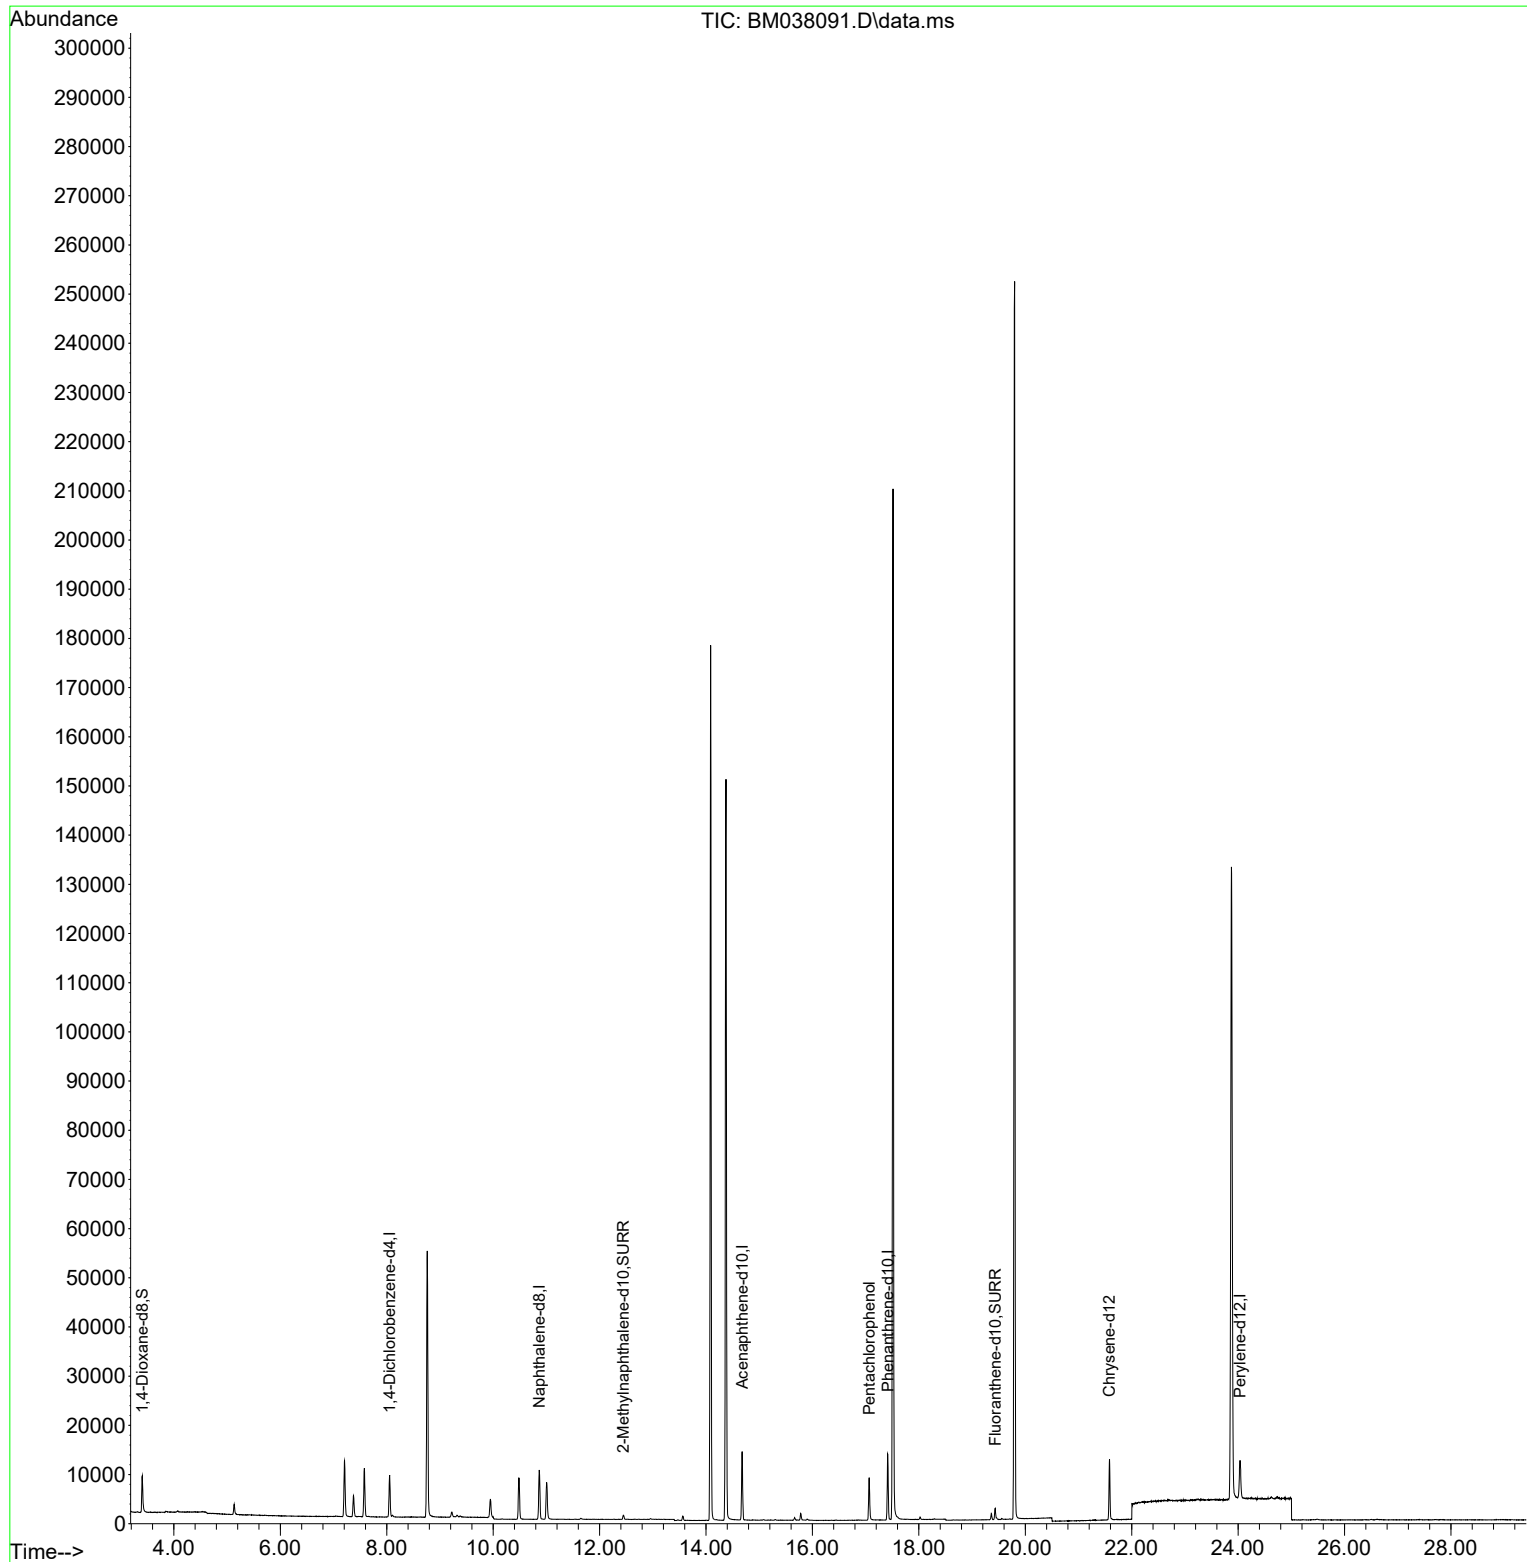

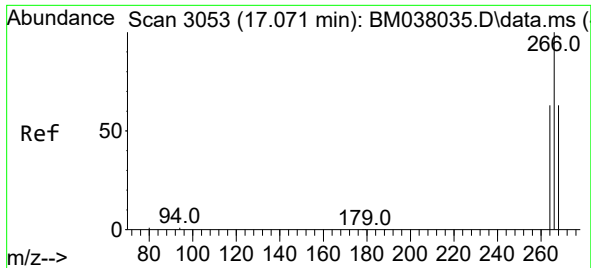

#14
 Pentachlorophenol
 Concen: 0.874 ng/ul
 RT: 17.067 min Scan# 3052
 Delta R.T. 0.000 min
 Lab File: BM038091.D
 Acq: 17 Dec 2022 06:35

Instrument :
 BNA_M
 ClientSampleId :
 COLD6DL

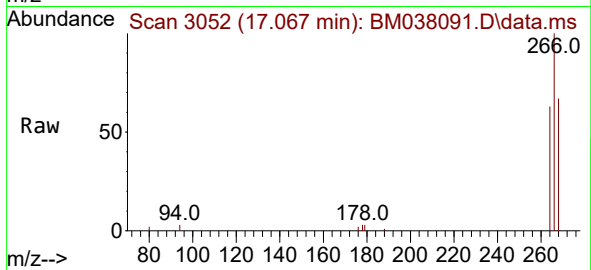

Tgt Ion:	266	Resp:	5631
Ion	Ratio	Lower	Upper
266	100		
264	62.3	49.9	74.9
268	64.9	52.0	78.0

