

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038038.D
 Acq On : 15 Dec 2022 18:56
 Operator : CG/JU
 Sample : N5983-06DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLB7DL

Quant Time: Dec 15 23:45:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	3399	0.400	ng/u1	0.00
4) Naphthalene-d8	10.873	136	10307	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.685	164	5790	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.422	188	11677	0.400	ng/u1	0.00
17) Chrysene-d12	21.586	240	7664	0.400	ng/u1	0.00
23) Perylene-d12	24.038	264	7579	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	4924	1.060	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.456	152	987	0.066	ng/u1	0.00
18) Fluoranthene-d10	19.436	212	1910	0.069	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	17.071	266	6683	1.382	ng/u1	Qvalue 99
16) Anthracene	17.552	178	1576	0.043	ng/u1#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038038.D
Acq On : 15 Dec 2022 18:56
Operator : CG/JU
Sample : N5983-06DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLB7DL

Quant Time: Dec 15 23:45:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

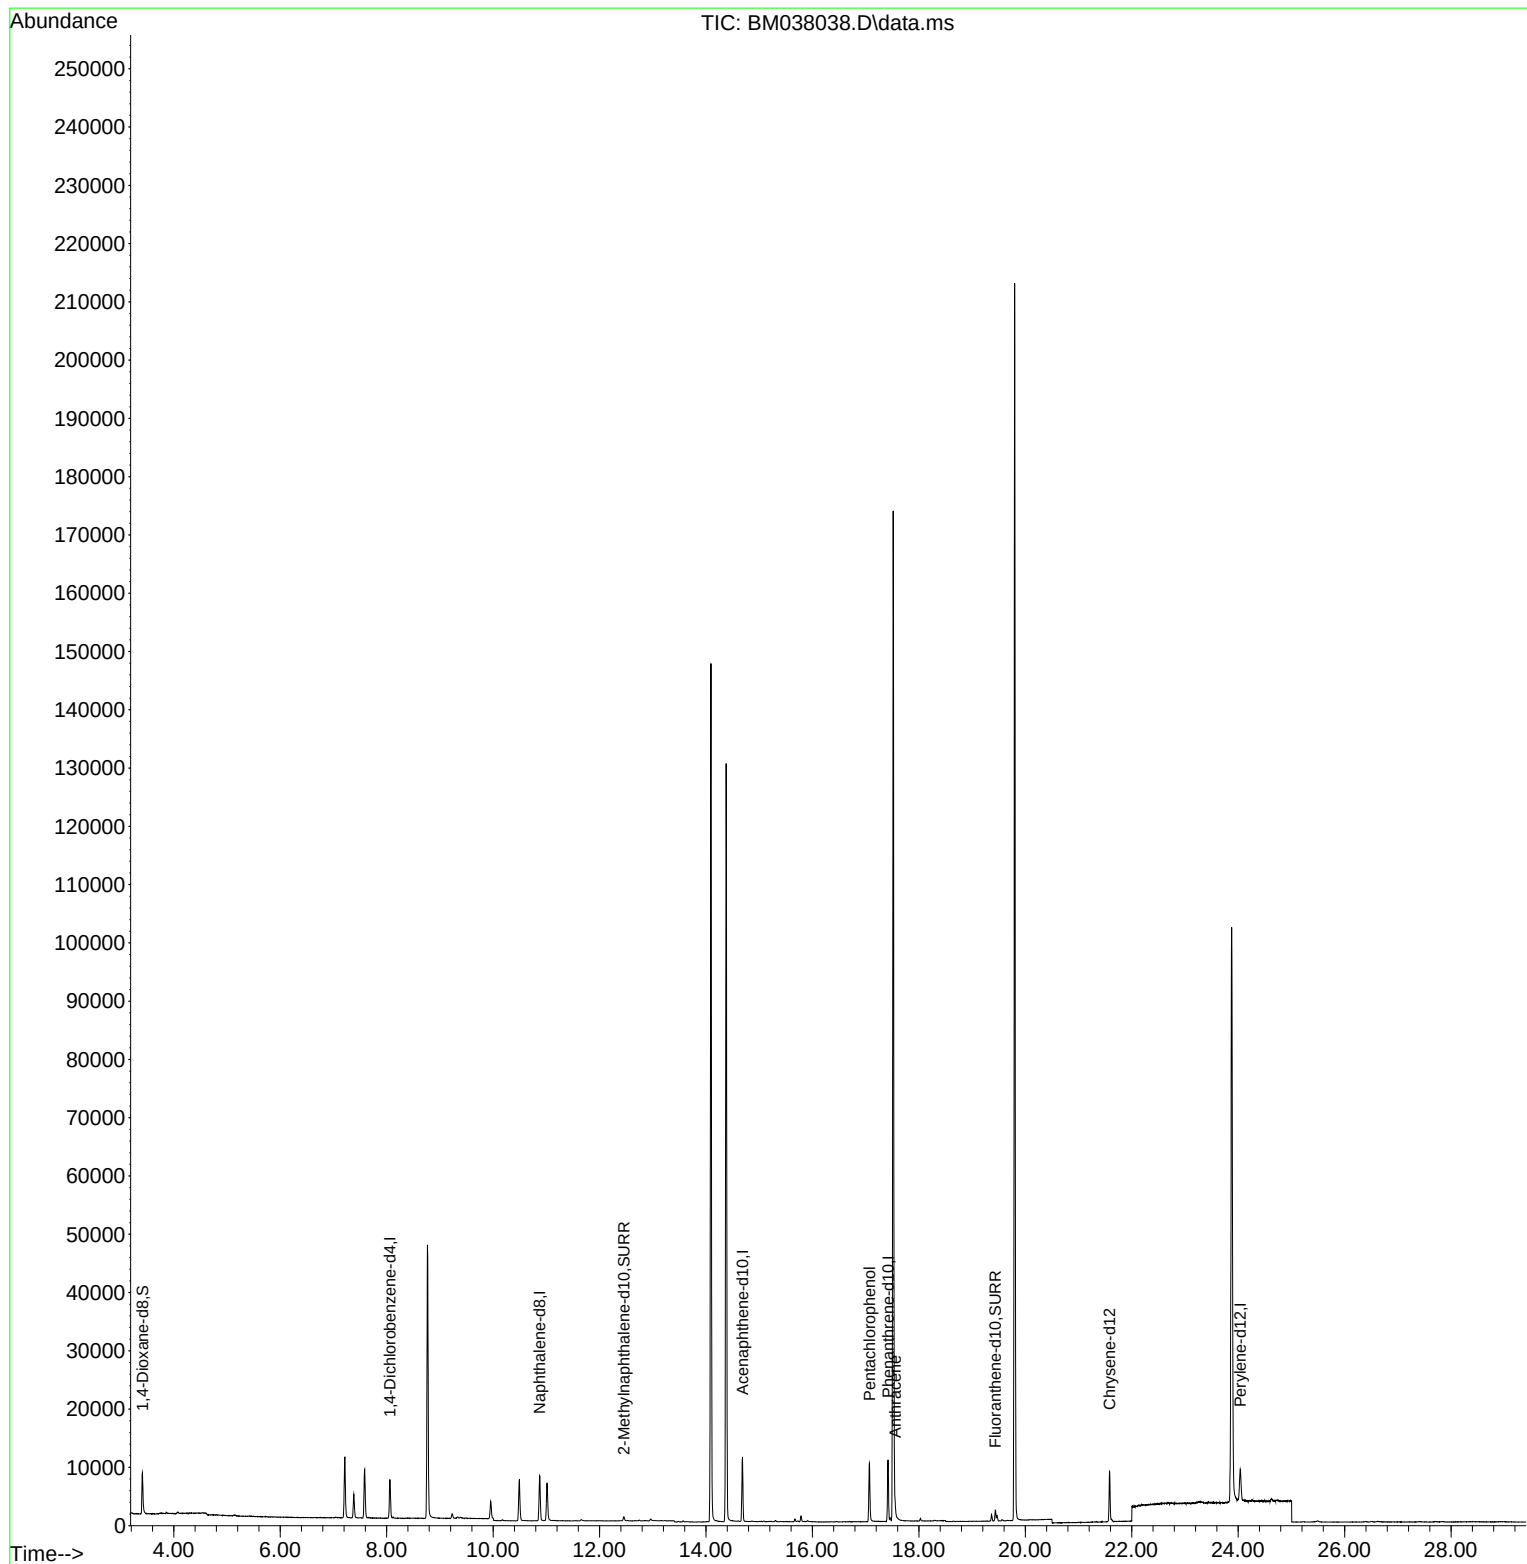

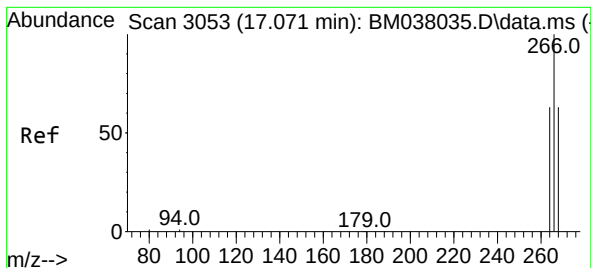

#14

Pentachlorophenol

Concen: 1.382 ng/ul

RT: 17.071 min Scan# 3053

Delta R.T. 0.000 min

Lab File: BM038038.D

Acq: 15 Dec 2022 18:56

Instrument :

BNA_M

ClientSampleId :

COLB7DL





Tgt Ion:266 Resp: 6683

Ion Ratio Lower Upper

266 100

264 61.8 49.9 74.9

268 63.8 52.0 78.0

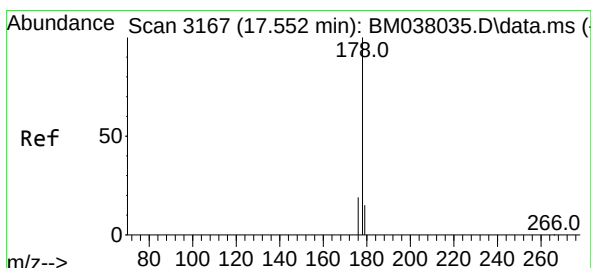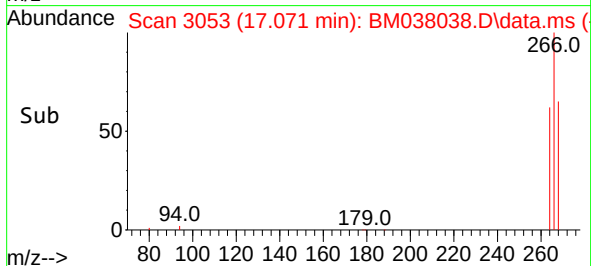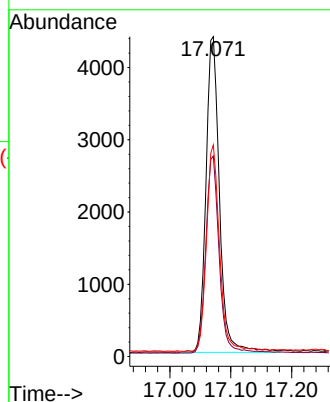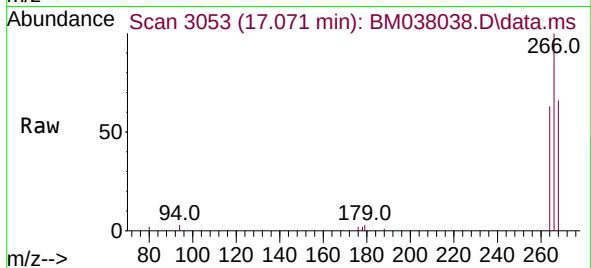

#16

Anthracene

Concen: 0.043 ng/ul

RT: 17.552 min Scan# 3167

Delta R.T. -0.004 min

Lab File: BM038038.D

Acq: 15 Dec 2022 18:56

Tgt Ion:178 Resp: 1576

Ion Ratio Lower Upper

178 100

179 25.4 13.0 19.4#

176 26.9 15.0 22.4#

