

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038045.D
 Acq On : 15 Dec 2022 23:15
 Operator : CG/JU
 Sample : N5984-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD7

Quant Time: Dec 16 00:17:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4983	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	15380	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	8513	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.421	188	17502	0.400	ng/ul	0.00
17) Chrysene-d12	21.582	240	12172	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	12066	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	30768	4.518	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	7116	0.317	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	13966	0.317	ng/ul	0.00
Target Compounds						
						Qvalue
7) 2-Methylnaphthalene	12.528	142	665	0.023	ng/ul	95
14) Pentachlorophenol	17.071	266	29812	4.114	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038045.D
Acq On : 15 Dec 2022 23:15
Operator : CG/JU
Sample : N5984-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD7

Quant Time: Dec 16 00:17:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration




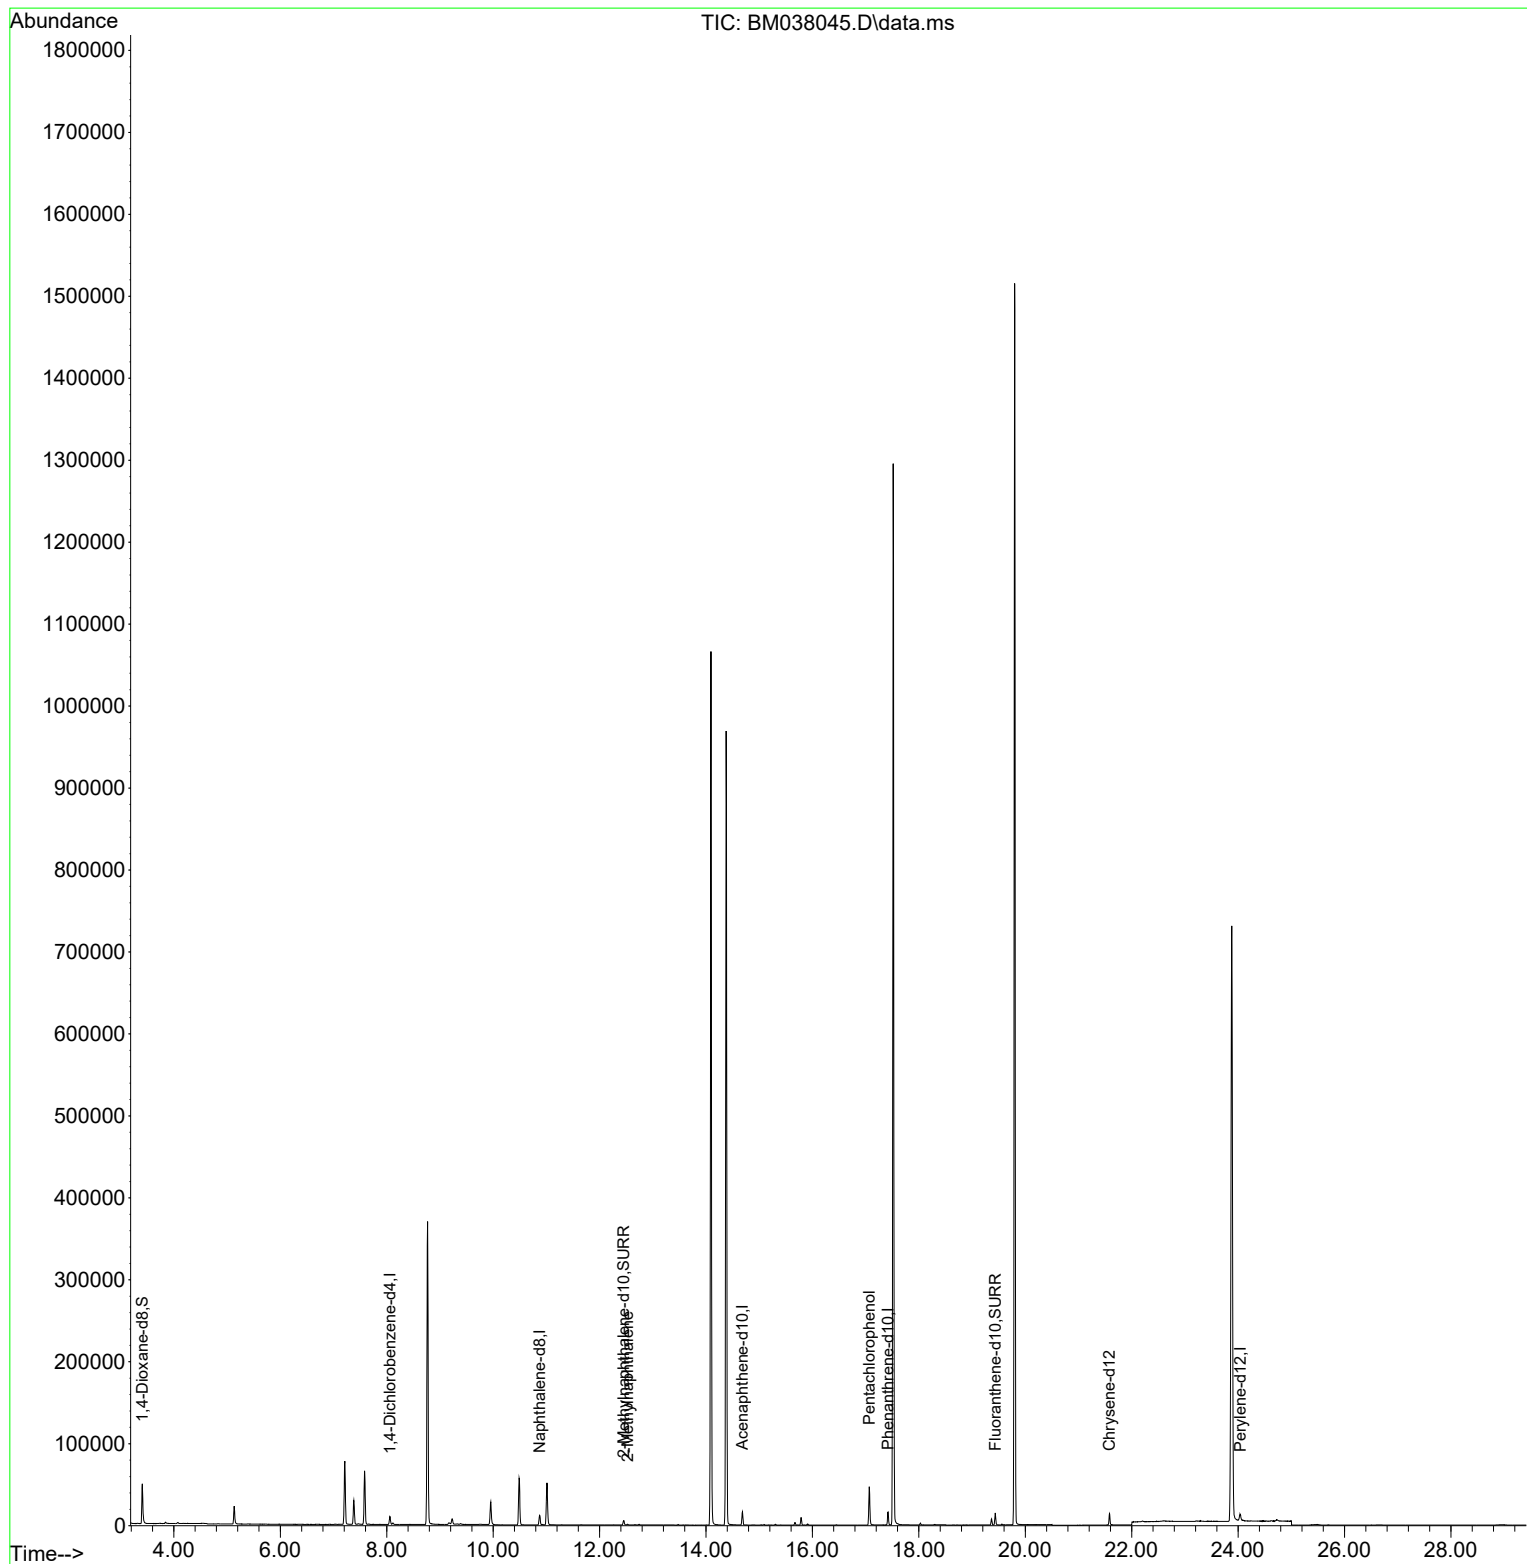


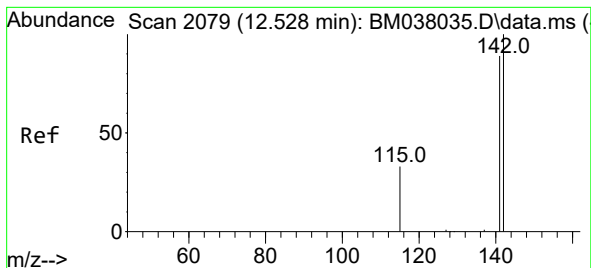

#7
2-Methylnaphthalene
Concen: 0.023 ng/ul
RT: 12.528 min Scan# 2079
Delta R.T. -0.000 min
Lab File: BM038045.D
Acq: 15 Dec 2022 23:15

Instrument :
BNA_M
ClientSampleId :
COLD7

Tgt Ion:142 Resp: 665
Ion Ratio Lower Upper
142 100
141 92.5 70.4 105.6

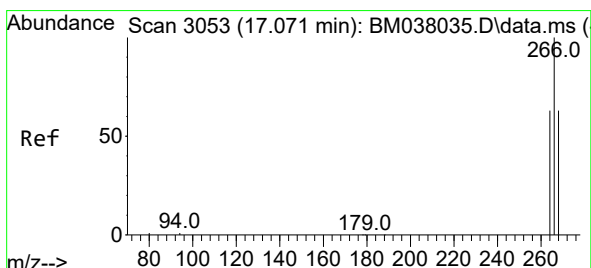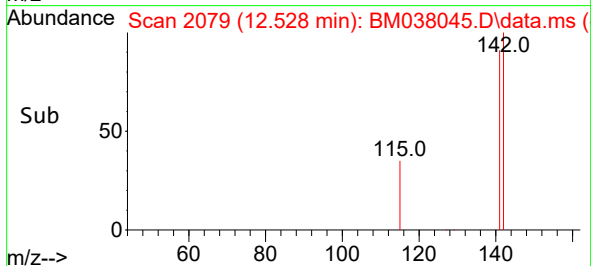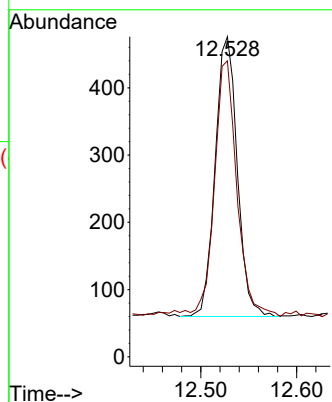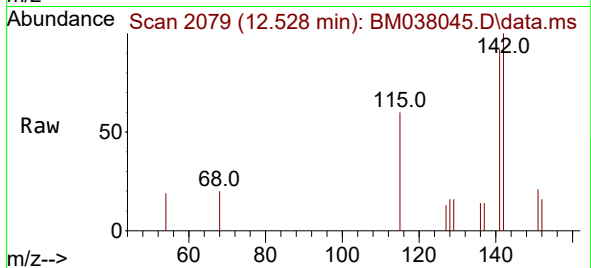

#14
Pentachlorophenol
Concen: 4.114 ng/ul
RT: 17.071 min Scan# 3053
Delta R.T. -0.000 min
Lab File: BM038045.D
Acq: 15 Dec 2022 23:15

Tgt Ion:266 Resp: 29812
Ion Ratio Lower Upper
266 100
264 62.6 49.9 74.9
268 63.8 52.0 78.0

