

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038046.D
 Acq On : 15 Dec 2022 23:52
 Operator : CG/JU
 Sample : N5984-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD0

Quant Time: Dec 16 01:34:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	5182	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	16242	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	8933	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	18989	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	14508	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	14899	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	31997	4.518	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	7262	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	15327	0.291	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.071	266	571	0.073	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038046.D
Acq On : 15 Dec 2022 23:52
Operator : CG/JU
Sample : N5984-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD0

Quant Time: Dec 16 01:34:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

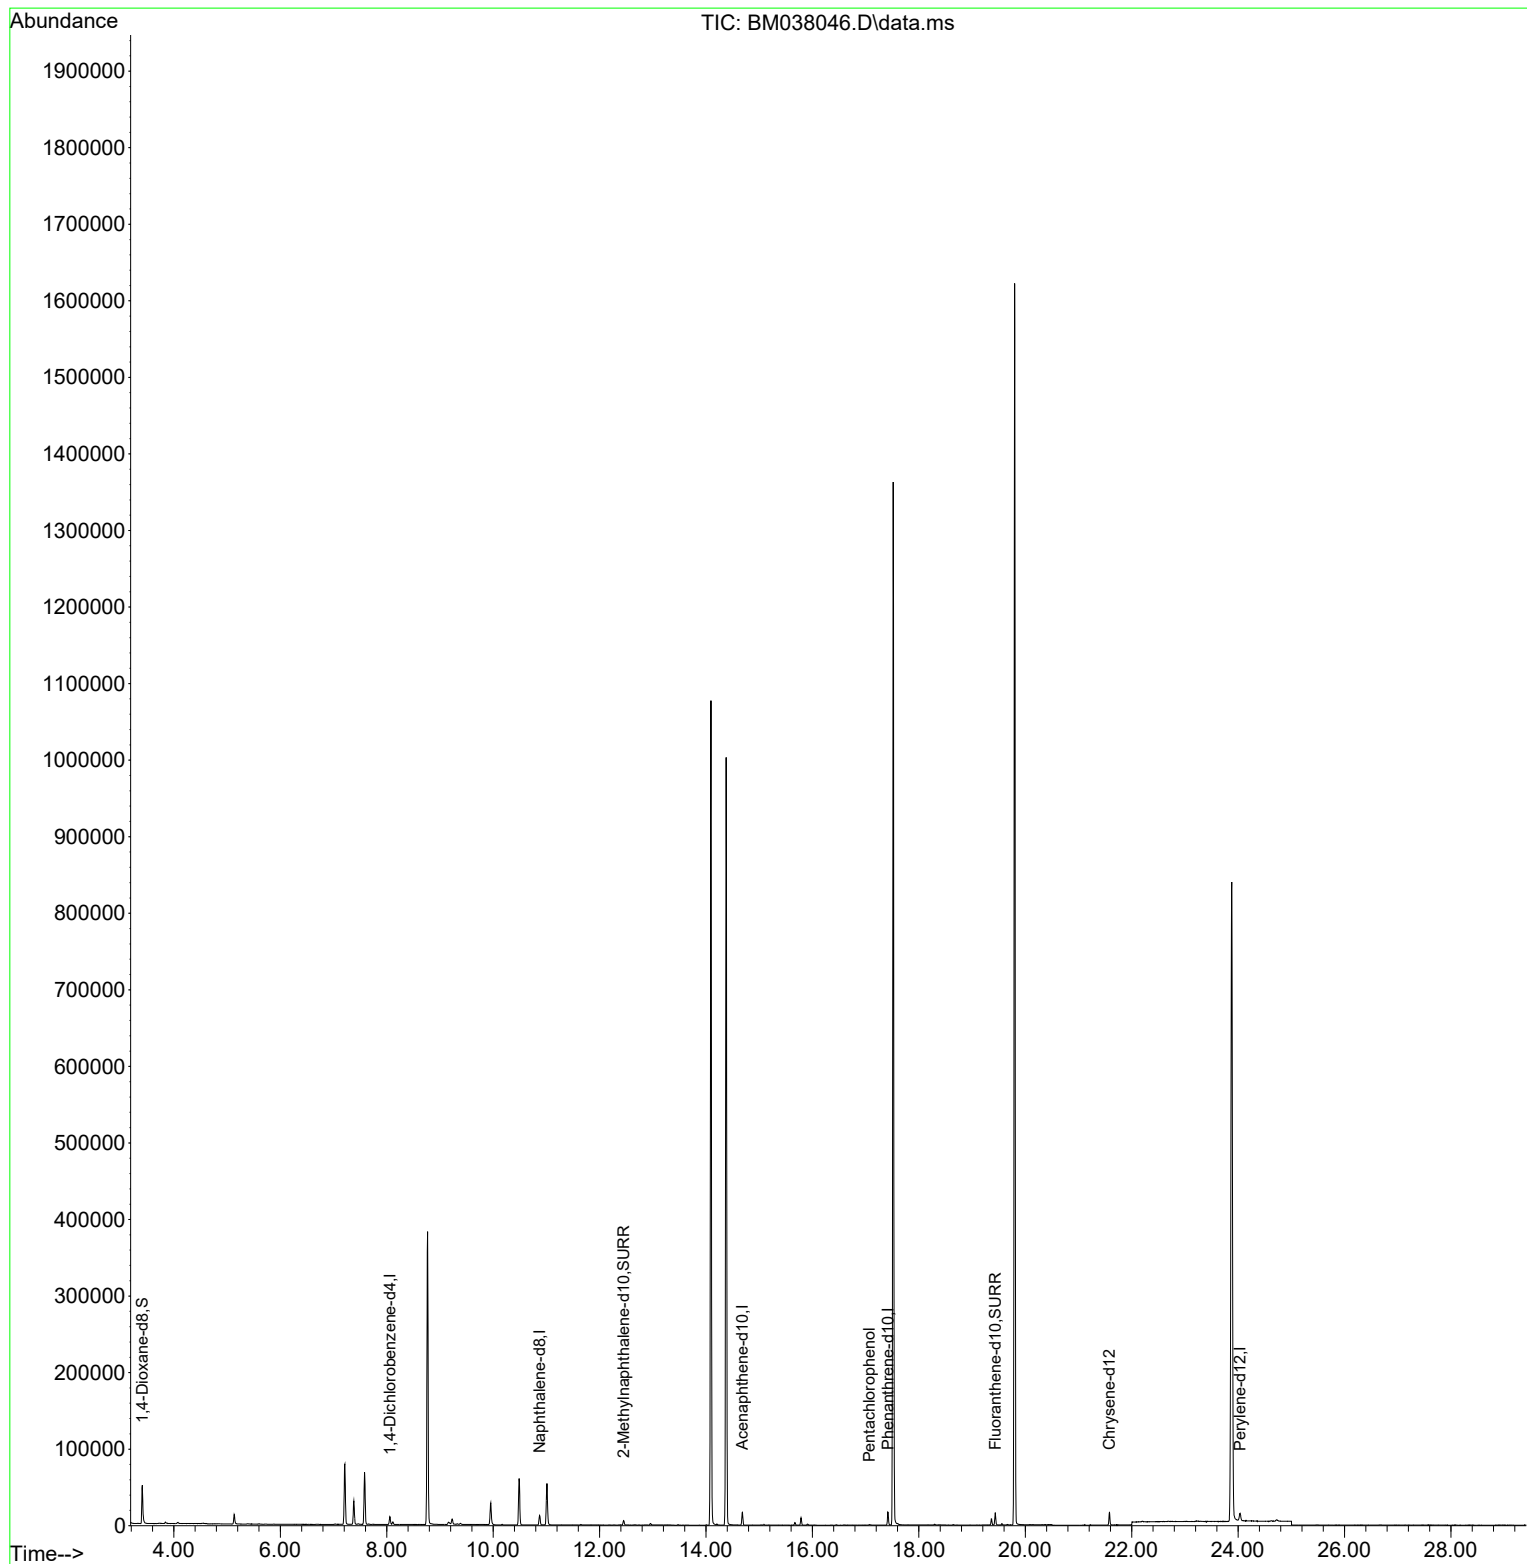

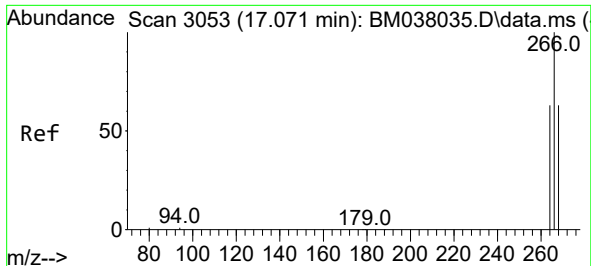

#14

Pentachlorophenol

Concen: 0.073 ng/ul

RT: 17.071 min Scan# 3053

Delta R.T. 0.000 min

Lab File: BM038046.D


Acq: 15 Dec 2022 23:52

Instrument :

BNA_M

ClientSampleId :

COLD0

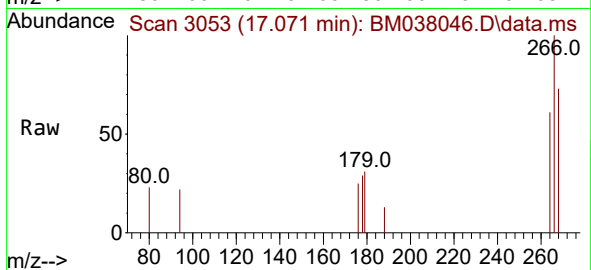

Tgt Ion:266 Resp: 571

Ion Ratio Lower Upper

266 100

264 63.4 49.9 74.9

268 71.6 52.0 78.0

