

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038047.D
 Acq On : 16 Dec 2022 00:30
 Operator : CG/JU
 Sample : N5984-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD1

Quant Time: Dec 16 01:34:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	5145	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	16020	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	8836	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	18341	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	13644	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	14184	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	23967	3.408	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	5553	0.237	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	11585	0.234	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.071	266	337	0.044	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038047.D
Acq On : 16 Dec 2022 00:30
Operator : CG/JU
Sample : N5984-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD1

Quant Time: Dec 16 01:34:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

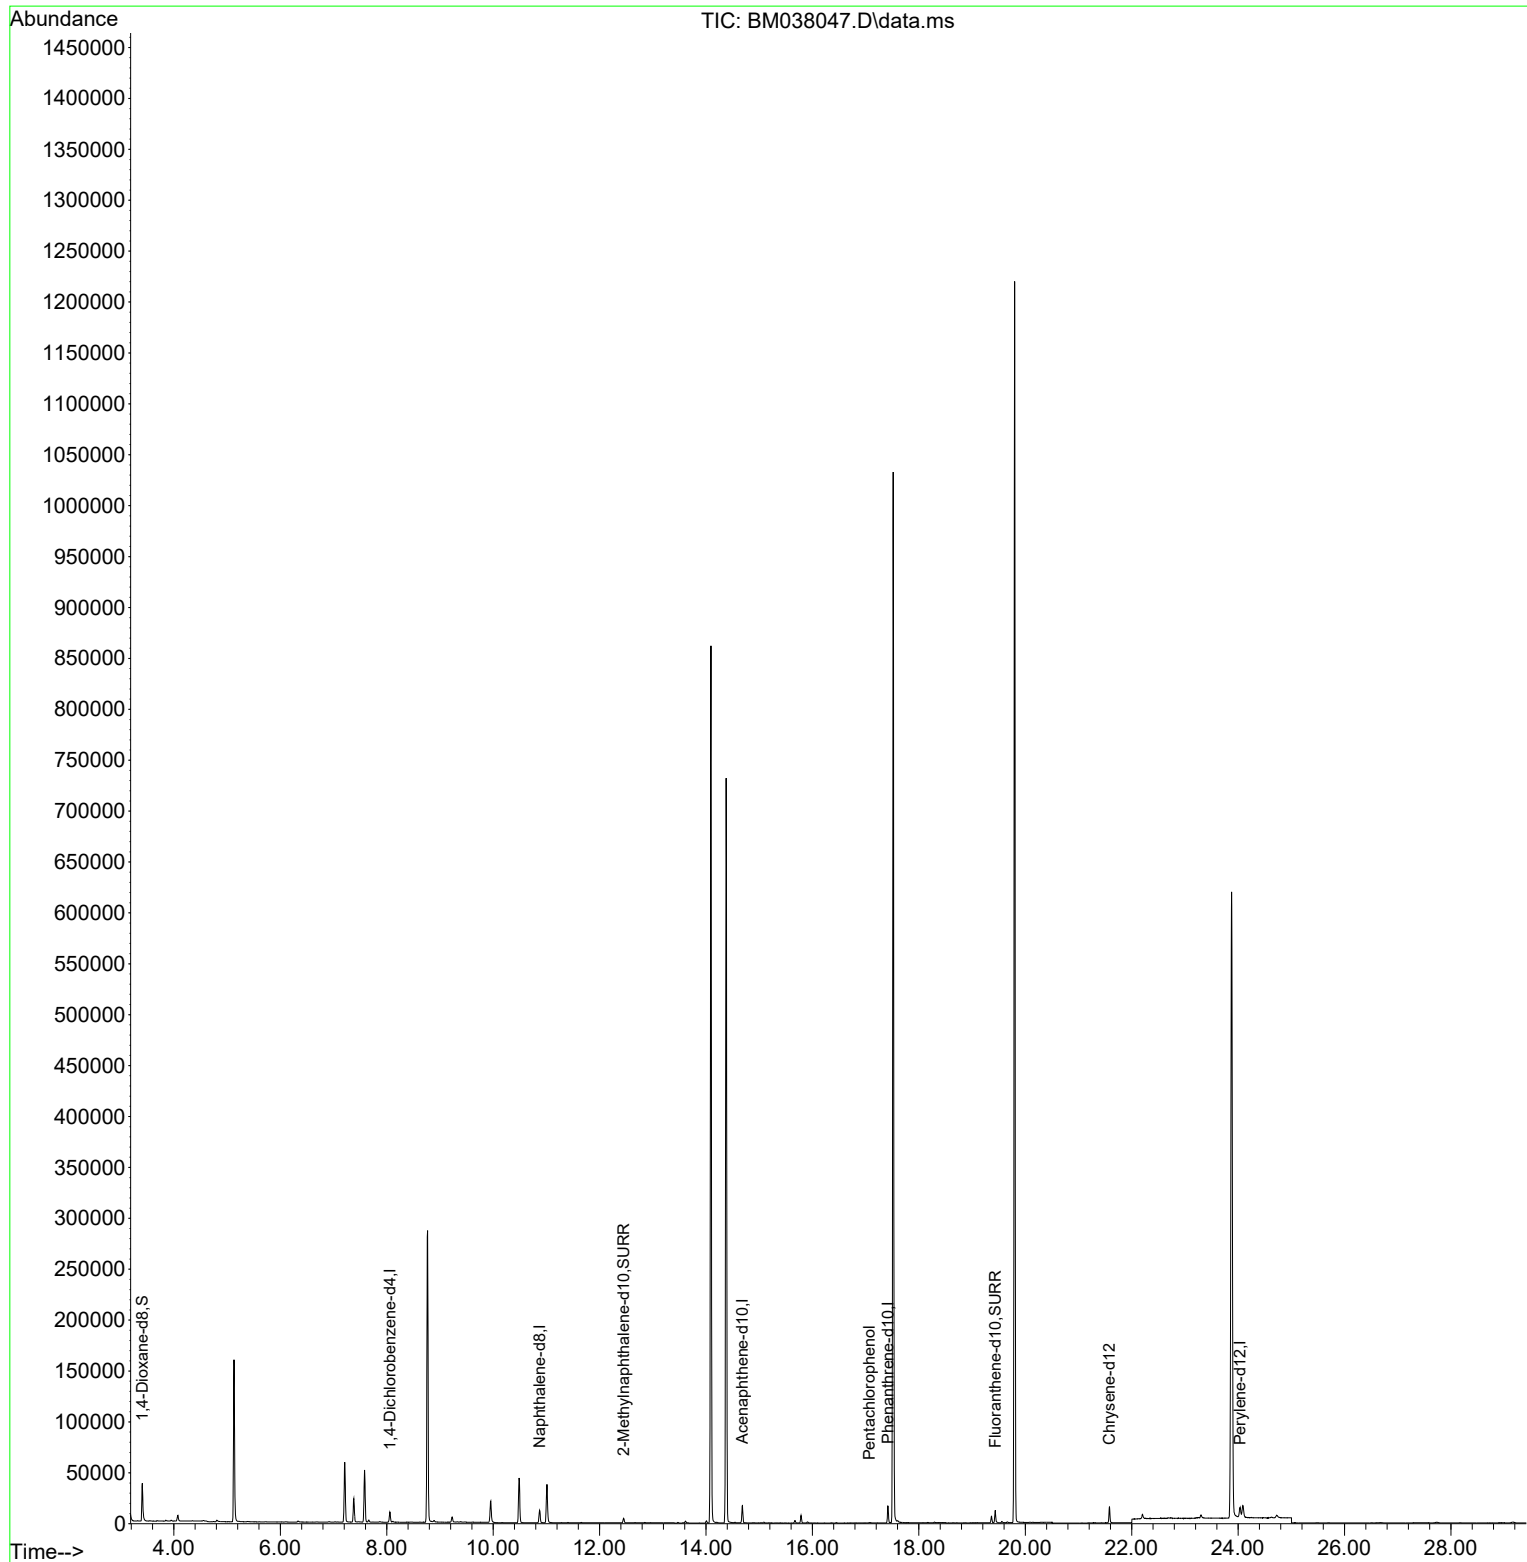

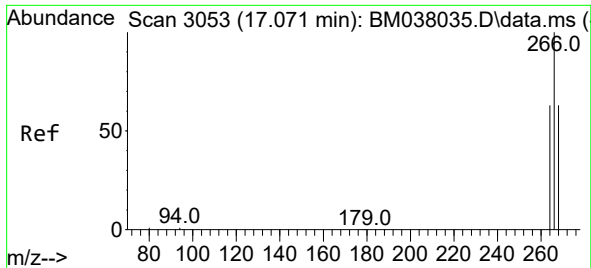

#14

Pentachlorophenol

Concen: 0.044 ng/ul

RT: 17.071 min Scan# 30

Delta R.T. 0.000 min

Lab File: BM038047.D


Acq: 16 Dec 2022 00:30

Instrument :

BNA_M

ClientSampleId :

COLD1

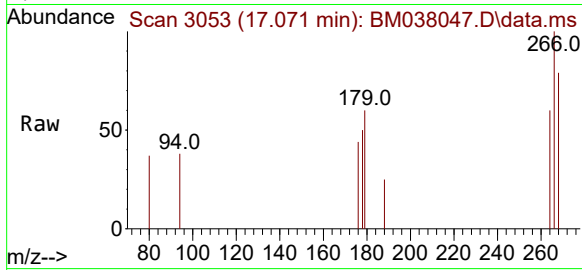

Tgt Ion:266 Resp: 337

Ion Ratio Lower Upper

266 100

264 52.8 49.9 74.9

268 61.7 52.0 78.0

