

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038051.D
 Acq On : 16 Dec 2022 02:57
 Operator : CG/JU
 Sample : N5984-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD6

Quant Time: Dec 16 03:37:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4769	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	14881	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	8512	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	18236	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	13621	0.400	ng/ul	0.00
23) Perylene-d12	24.041	264	14130	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	26198	4.019	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	6283	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	13821	0.280	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.067	266	34016	4.505	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038051.D
Acq On : 16 Dec 2022 02:57
Operator : CG/JU
Sample : N5984-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD6


Quant Time: Dec 16 03:37:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

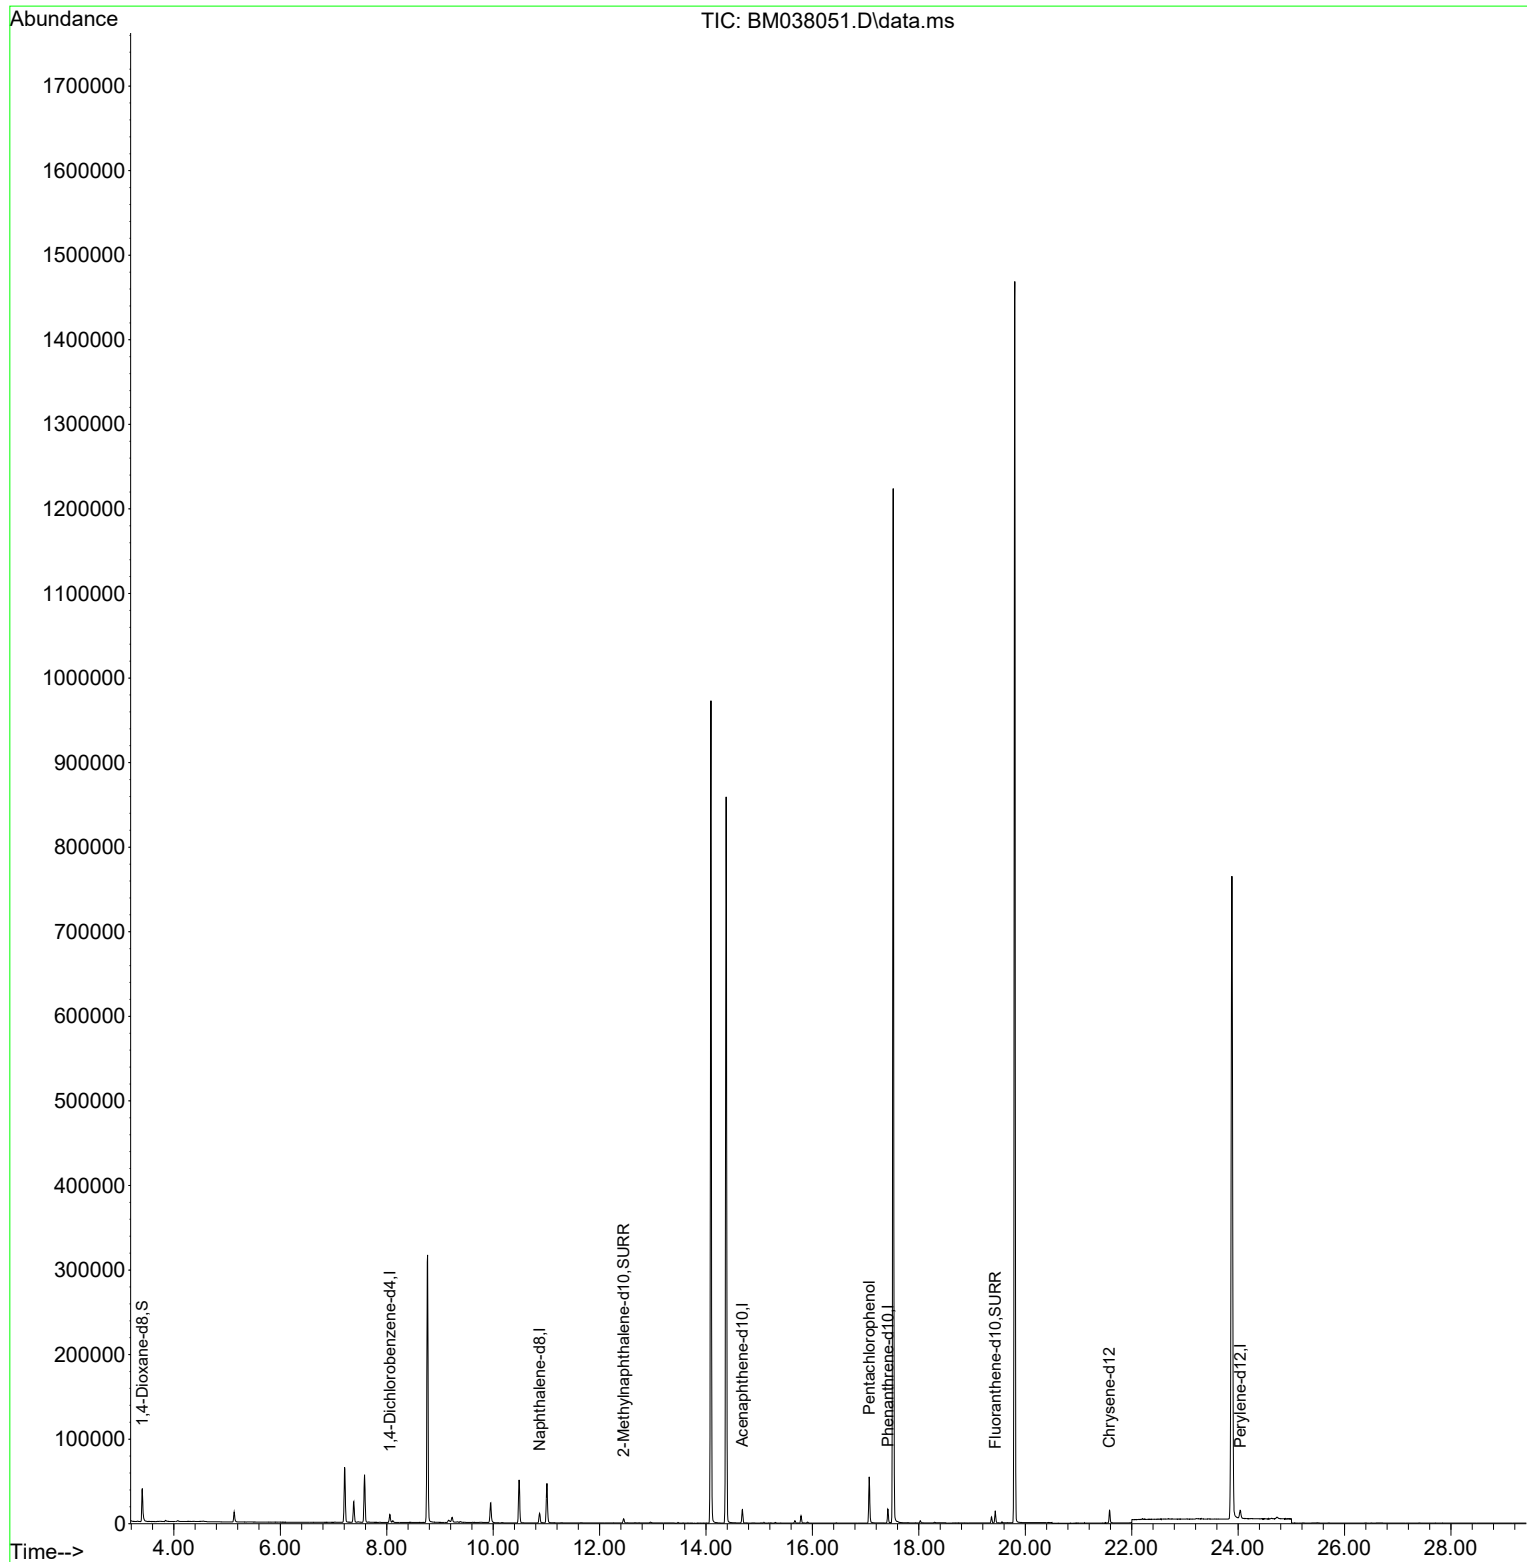

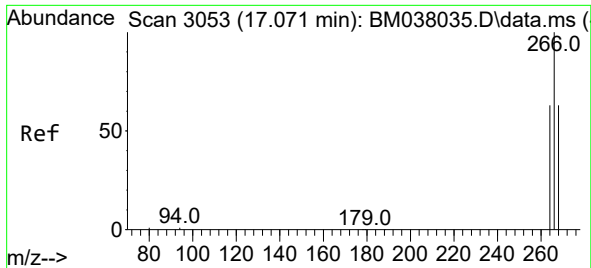

#14
 Pentachlorophenol
 Concen: 4.505 ng/ul
 RT: 17.067 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM038051.D
 Acq: 16 Dec 2022 02:57

Instrument :
 BNA_M
 ClientSampleId :
 C0LD6

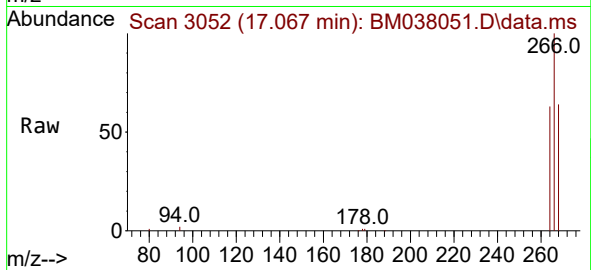

Tgt Ion:266 Resp: 34016
 Ion Ratio Lower Upper
 266 100
 264 62.6 49.9 74.9
 268 64.0 52.0 78.0

