

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038055.D
 Acq On : 16 Dec 2022 06:01
 Operator : CG/JU
 Sample : N5984-15
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLF1

Quant Time: Dec 16 06:34:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4540	0.400	ng/ul	0.00
4) Naphthalene-d8	10.873	136	13703	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.680	164	7450	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	16269	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	13946	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	15289	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	19464	3.137	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	4323	0.216	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	10139	0.201	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	17.071	266	2035	0.302	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038055.D
Acq On : 16 Dec 2022 06:01
Operator : CG/JU
Sample : N5984-15
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLF1

Quant Time: Dec 16 06:34:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

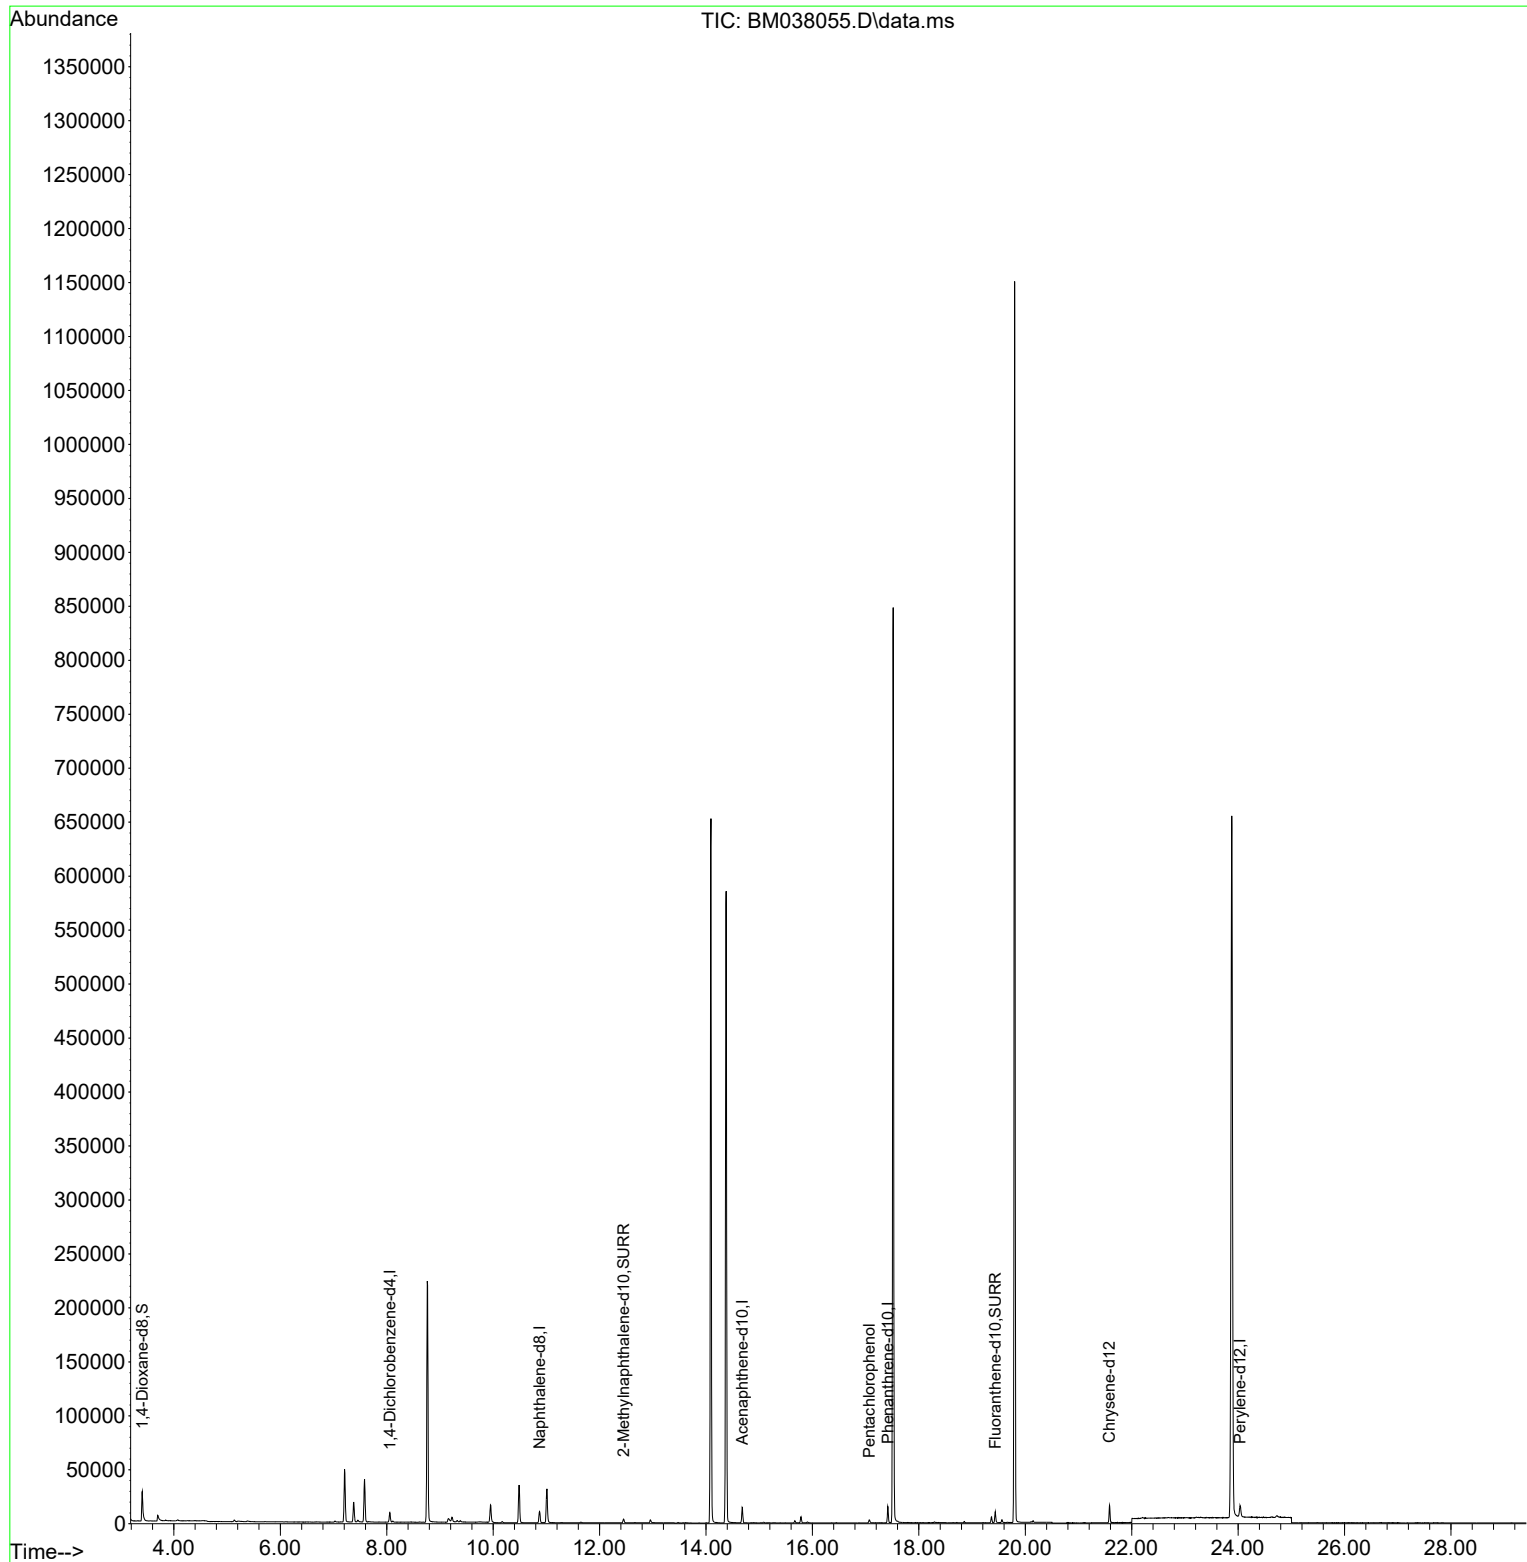

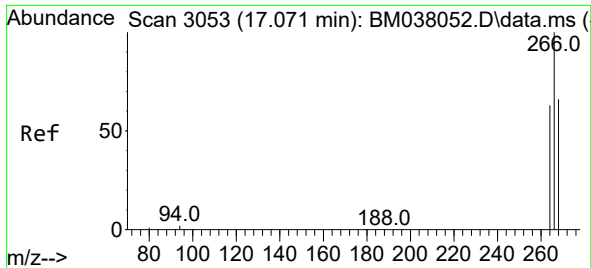

#14

Pentachlorophenol

Concen: 0.302 ng/ul

RT: 17.071 min Scan# 30

Delta R.T. 0.000 min

Lab File: BM038055.D


Acq: 16 Dec 2022 06:01

Instrument :

BNA_M

ClientSampleId :

COLF1

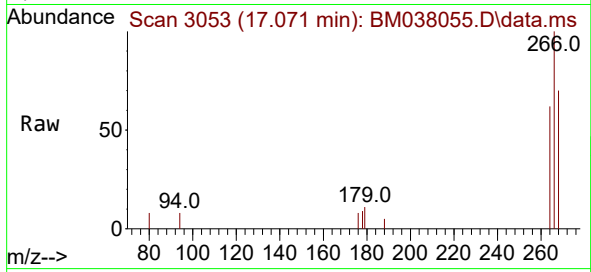

Tgt Ion:266 Resp: 2035

Ion Ratio Lower Upper

266 100

264 62.5 49.9 74.9

268 65.4 52.0 78.0

