

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038078.D
 Acq On : 16 Dec 2022 21:58
 Operator : CG/JU
 Sample : N5925-17
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBYC6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/19/2022
 Supervised By :mohammad ahmed 12/19/2022

Quant Time: Dec 16 23:22:22 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4924	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	15867	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	9604	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	20804	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	16784	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	15454	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	22567	3.353	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.451	152	6113	0.264	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	13931	0.229	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.917	128	28583	0.595	ng/ul	100
7) 2-Methylnaphthalene	12.522	142	5271	0.178	ng/ul	100
8) 1-Methylnaphthalene	12.737	142	2445	0.081	ng/ul	98
10) Acenaphthylene	14.402	152	35401	0.703	ng/ul	99
11) Acenaphthene	14.745	153	4498	0.118	ng/ul	97
12) Fluorene	15.725	166	5804	0.137	ng/ul	99
14) Pentachlorophenol	17.071	266	554	0.064	ng/ul	99
15) Phenanthrene	17.459	178	153777	2.195	ng/ul	99
16) Anthracene	17.552	178	32757	0.506	ng/ul	100
19) Fluoranthene	19.464	202	466629	5.383	ng/ul	96
20) Pyrene	19.826	202	331372m	3.745	ng/ul	
21) Benzo(a)anthracene	21.565	228	212310	2.928	ng/ul	99
22) Chrysene	21.621	228	206943	2.829	ng/ul	98
24) Benzo(b)fluoranthene	23.290	252	296361	4.044	ng/ul	92
25) Benzo(k)fluoranthene	23.333	252	96861m	1.369	ng/ul	
26) Benzo(a)pyrene	23.930	252	158917	2.575	ng/ul#	85
27) Indeno(1,2,3-cd)pyrene	26.605	276	118056	1.524	ng/ul#	86
28) Dibenzo(a,h)anthracene	26.612	278	29268	0.485	ng/ul	97
29) Benzo(g,h,i)perylene	27.400	276	80316	1.220	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038078.D
Acq On : 16 Dec 2022 21:58
Operator : CG/JU
Sample : N5925-17
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBYC6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022


Quant Time: Dec 16 23:22:22 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

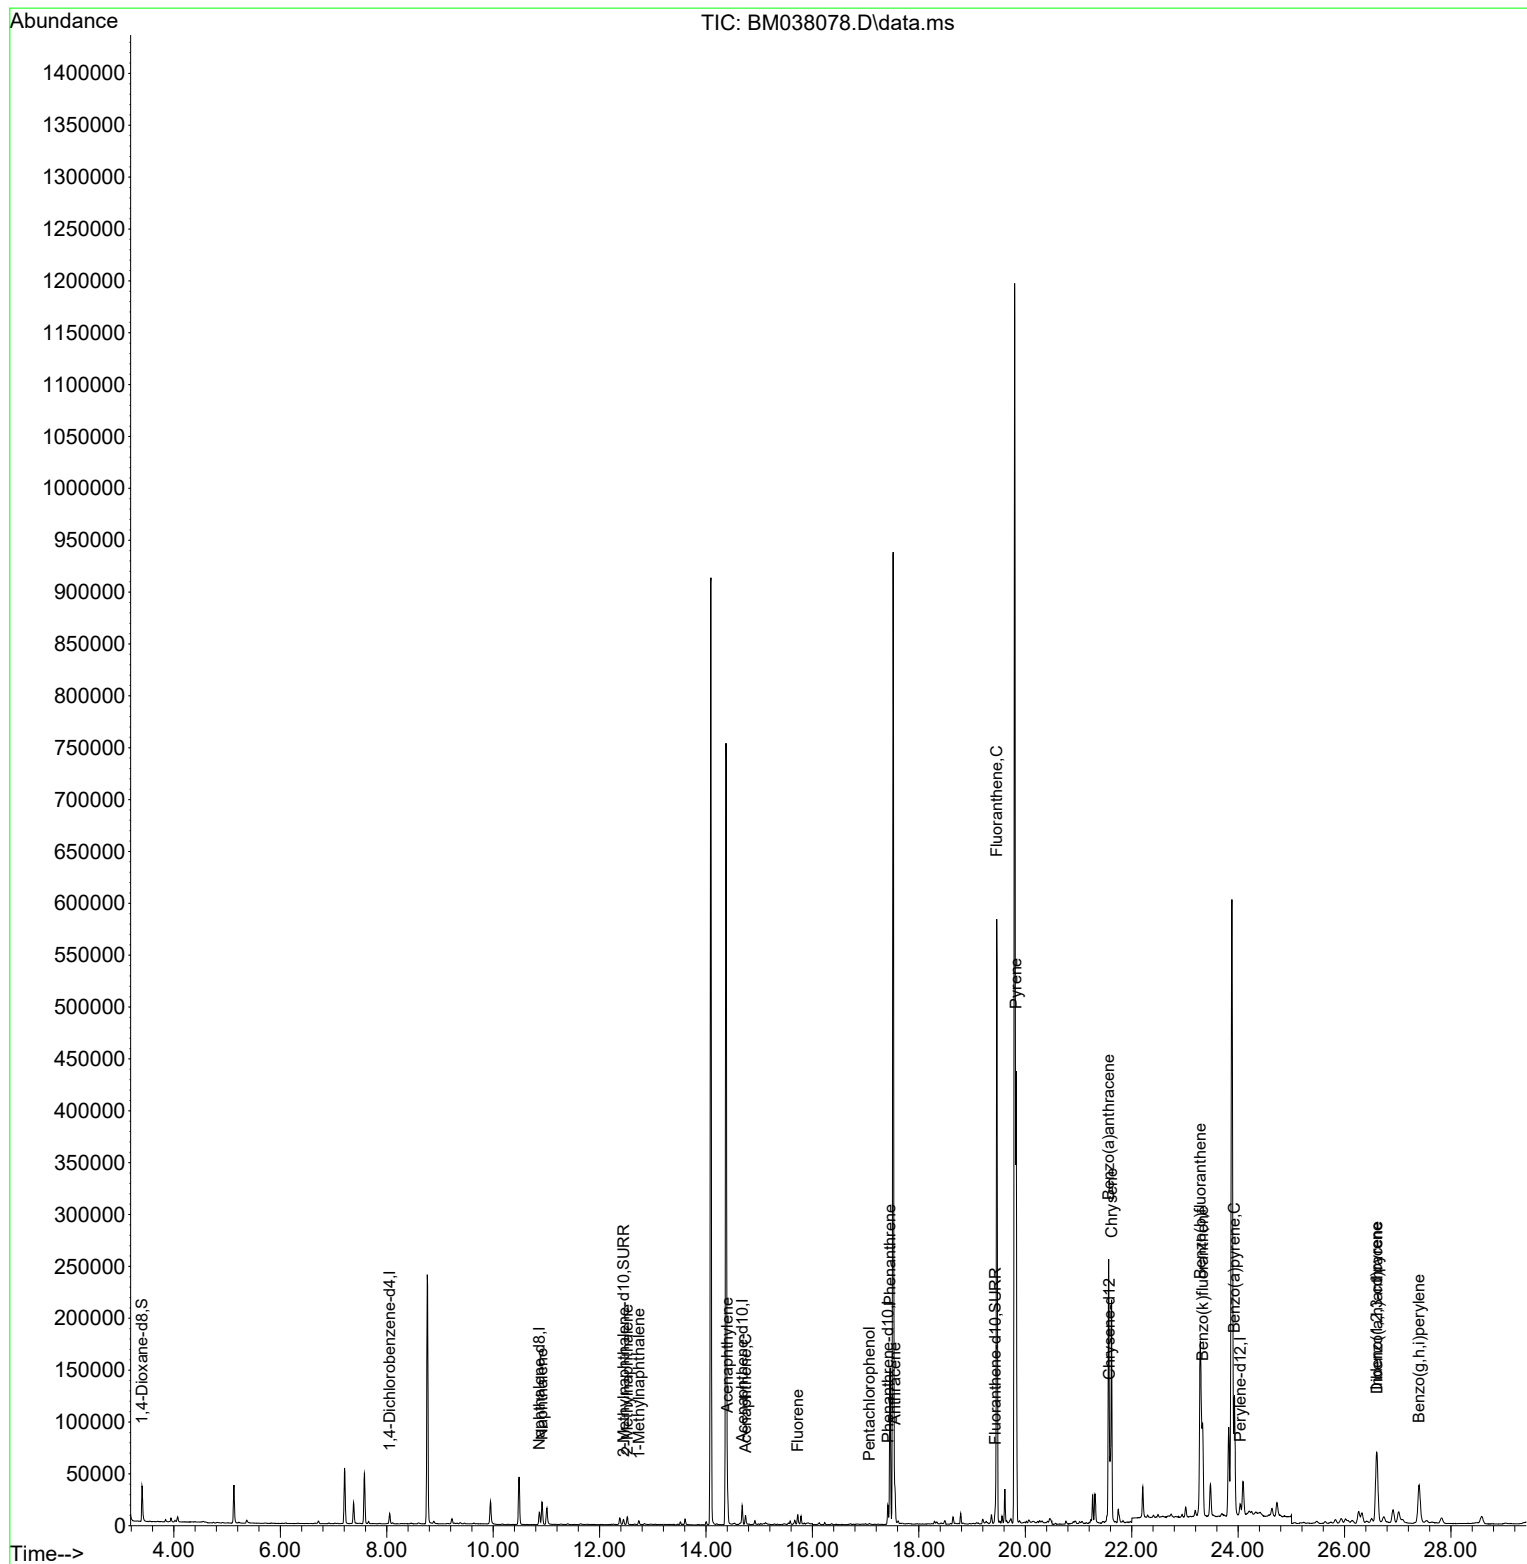



#5
Naphthalene
Concen: 0.595 ng/ul
RT: 10.917 min Scan# 1786
Delta R.T. -0.011 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6



Tgt Ion:128 Resp: 2858
Ion Ratio Lower Upper
128 100
129 11.6 9.1 13.7
127 13.0 10.4 15.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022

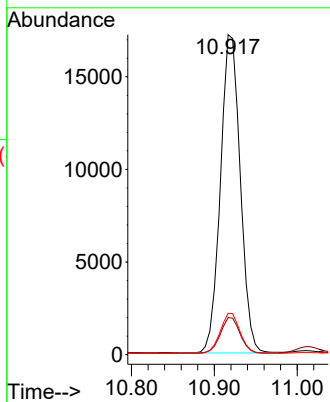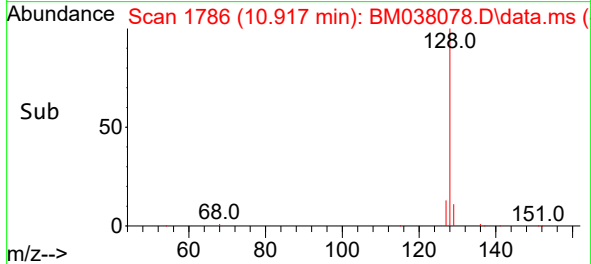

#7
2-Methylnaphthalene
Concen: 0.178 ng/ul
RT: 12.522 min Scan# 2078
Delta R.T. -0.005 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58


Tgt Ion:142 Resp: 5271
Ion Ratio Lower Upper
142 100
141 87.8 70.4 105.6

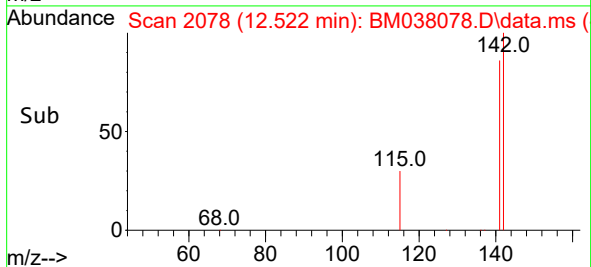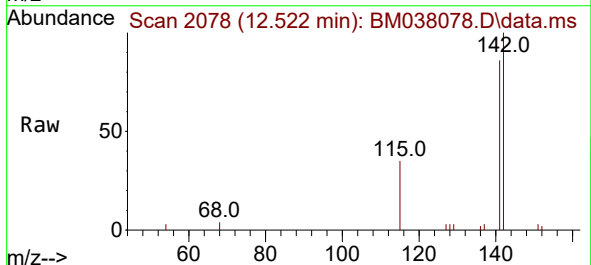



#8
1-Methylnaphthalene
Concen: 0.081 ng/ul
RT: 12.737 min Scan# 2117
Delta R.T. -0.011 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6



Tgt Ion:142 Resp: 2449
Ion Ratio Lower Upper
142 100
141 90.4 73.6 110.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022

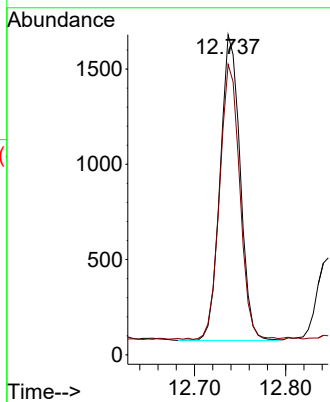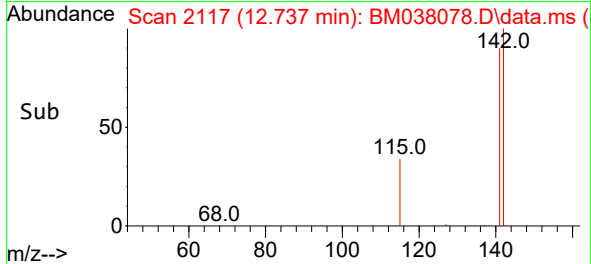

#10
Acenaphthylene
Concen: 0.703 ng/ul
RT: 14.402 min Scan# 2454
Delta R.T. -0.005 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58


Tgt Ion:152 Resp: 35401
Ion Ratio Lower Upper
152 100
151 19.7 15.5 23.3
153 13.6 11.0 16.4

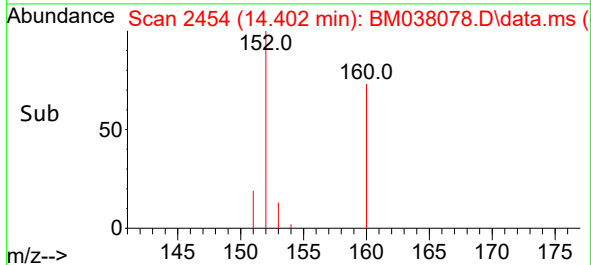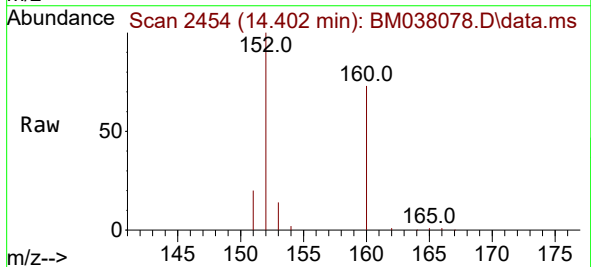



#11
Acenaphthene
Concen: 0.118 ng/ul
RT: 14.745 min Scan# 21
Delta R.T. -0.005 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6



Tgt Ion:153 Resp: 4498
Ion Ratio Lower Upper
153 100
152 51.7 39.5 59.3
154 88.4 69.2 103.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022

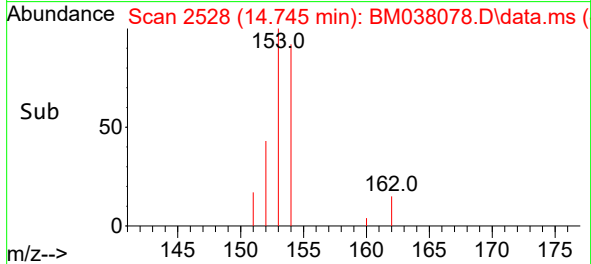

#12
Fluorene
Concen: 0.137 ng/ul
RT: 15.725 min Scan# 2740
Delta R.T. -0.005 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58


Tgt Ion:166 Resp: 5804
Ion Ratio Lower Upper
166 100
165 99.3 79.0 118.4
167 15.9 11.1 16.7

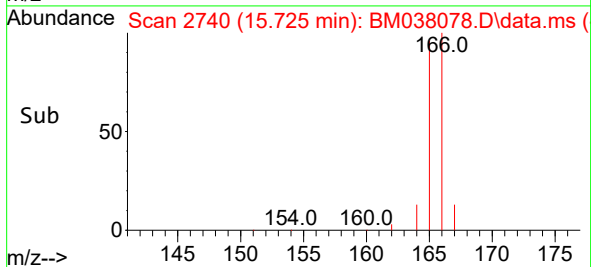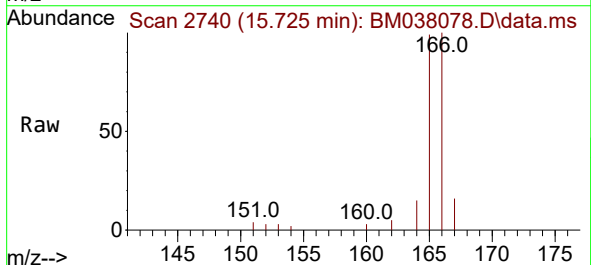



#14
Pentachlorophenol
Concen: 0.064 ng/ul
RT: 17.071 min Scan# 3053
Delta R.T. 0.000 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6




Tgt Ion:266 Resp: 554
Ion Ratio Lower Upper
266 100
264 61.9 49.9 74.9
268 64.4 52.0 78.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022

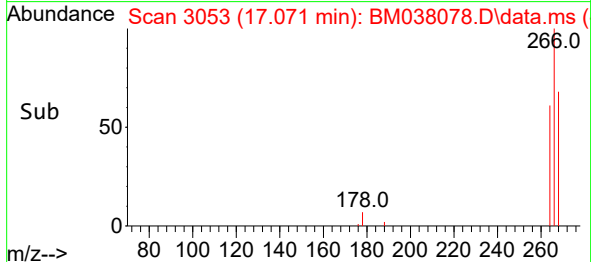


#15
Phenanthrene
Concen: 2.195 ng/ul
RT: 17.459 min Scan# 3145
Delta R.T. -0.004 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58

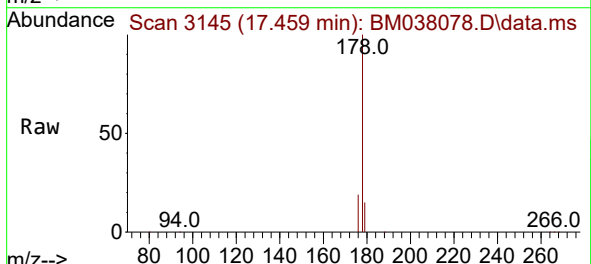


Tgt Ion:178 Resp: 153777
Ion Ratio Lower Upper
178 100
179 15.4 12.6 19.0
176 19.4 15.8 23.6

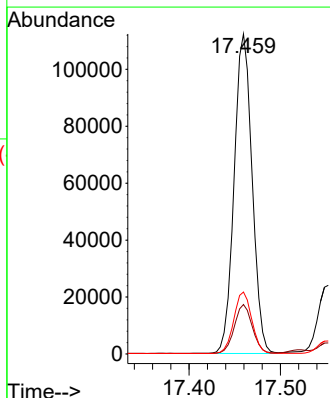



#16
 Anthracene
 Concen: 0.506 ng/ul
 RT: 17.552 min Scan# 3167
 Delta R.T. -0.004 min
 Lab File: BM038078.D
 Acq: 16 Dec 2022 21:58




Instrument :
 BNA_M
 ClientSampleId :
 DBYC6




Tgt Ion:178 Resp: 3275
 Ion Ratio Lower Upper
 178 100
 179 16.2 13.0 19.4
 176 19.0 15.0 22.4

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 12/19/2022
 Supervised By :mohammad ahmed 12/19/2022




#19
 Fluoranthene
 Concen: 5.383 ng/ul
 RT: 19.464 min Scan# 3599
 Delta R.T. -0.005 min
 Lab File: BM038078.D
 Acq: 16 Dec 2022 21:58

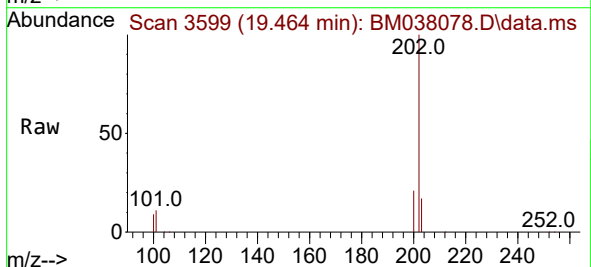


Tgt Ion:202 Resp: 466629
 Ion Ratio Lower Upper
 202 100
 101 11.4 10.6 15.8
 100 8.7 7.9 11.9

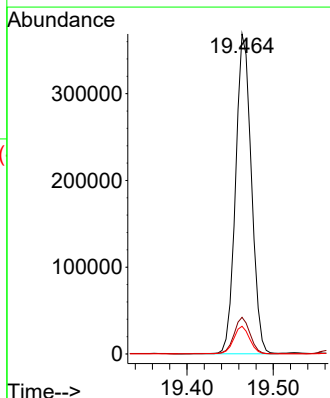



#20
Pyrene
Concen: 3.745 ng/ul m
RT: 19.826 min Scan# 3
Delta R.T. -0.005 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6




Tgt Ion:202 Resp: 331372
Ion Ratio Lower Upper
202 100
101 13.8 12.1 18.1
100 11.3 9.8 14.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022

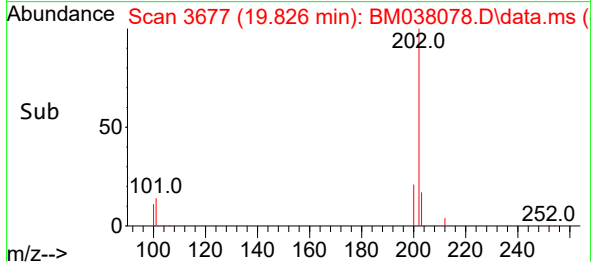


#21
Benzo(a)anthracene
Concen: 2.928 ng/ul
RT: 21.565 min Scan# 4186
Delta R.T. -0.003 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58

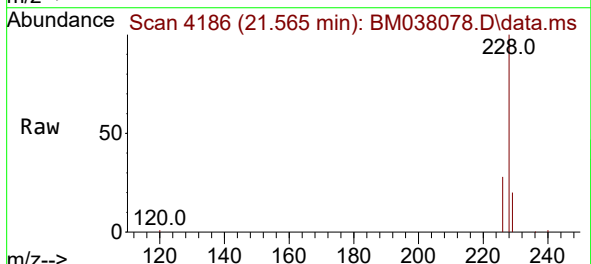

Tgt Ion:228 Resp: 212310
Ion Ratio Lower Upper
228 100
229 19.7 15.9 23.9
226 28.4 22.1 33.1

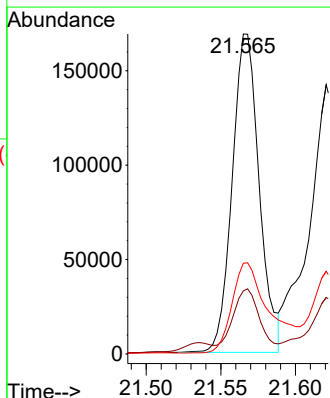



#22

Chrysene

Concen: 2.829 ng/ul

RT: 21.621 min Scan# 41

Delta R.T. -0.003 min

Lab File: BM038078.D


Acq: 16 Dec 2022 21:58

Instrument :

BNA_M

ClientSampleId :

DBYC6

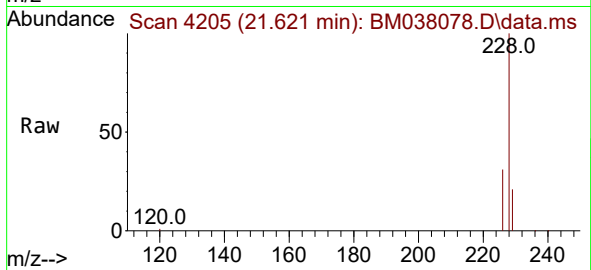

Tgt Ion:228 Resp: 20694

Ion Ratio Lower Upper

228 100

226 30.7 24.1 36.1




229 21.0 15.7 23.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/19/2022

Supervised By :mohammad ahmed 12/19/2022

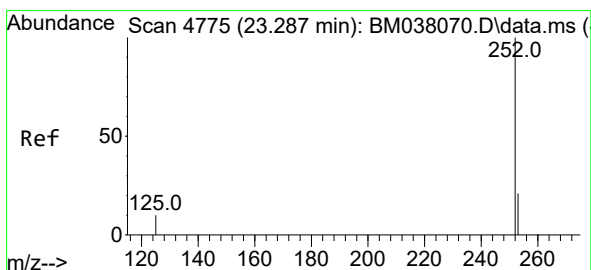

#24

Benzo(b)fluoranthene

Concen: 4.044 ng/ul

RT: 23.290 min Scan# 4776

Delta R.T. 0.003 min

Lab File: BM038078.D

Acq: 16 Dec 2022 21:58




Tgt Ion:252 Resp: 296361


Ion Ratio Lower Upper

252 100

253 22.9 0.0 51.8


125 15.6 0.0 42.2

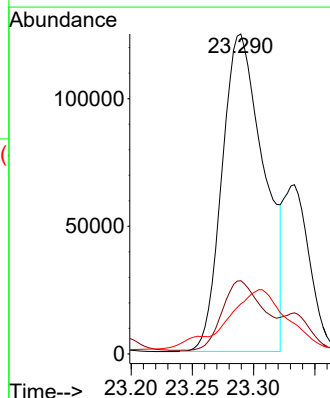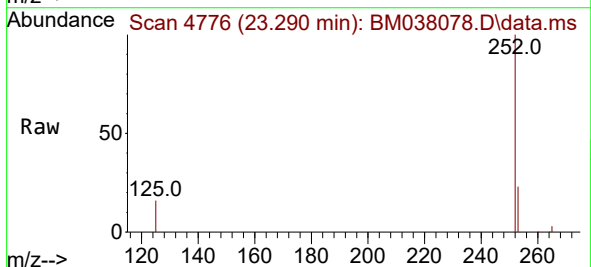



#25
Benzo(k)fluoranthene
Concen: 1.369 ng/ul m
RT: 23.333 min Scan# 4791
Delta R.T. -0.003 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6




Tgt Ion:252 Resp: 9686
Ion Ratio Lower Upper
252 100
253 24.3 20.8 31.2
125 18.0 17.1 25.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/19/2022
Supervised By :mohammad ahmed 12/19/2022

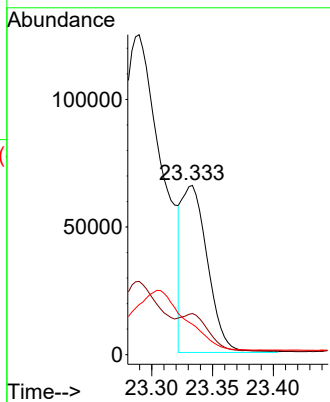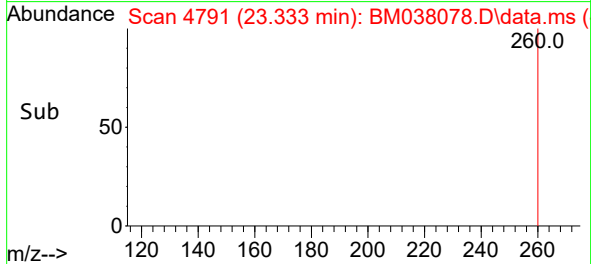


#26
Benzo(a)pyrene
Concen: 2.575 ng/ul
RT: 23.930 min Scan# 4995
Delta R.T. 0.000 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58

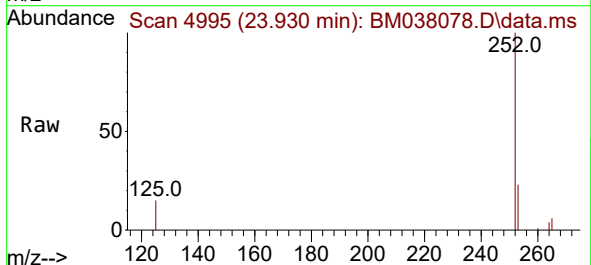


Tgt Ion:252 Resp: 158917
Ion Ratio Lower Upper
252 100
253 23.1 21.9 32.9
125 14.7 20.7 31.1#

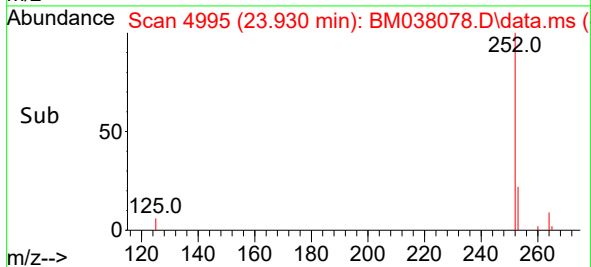



#27
Indeno(1,2,3-cd)pyrene
Concen: 1.524 ng/ul
RT: 26.605 min Scan# 5840
Delta R.T. -0.003 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58




Instrument :
BNA_M
ClientSampleId :
DBYC6




Tgt Ion: 276 Resp: 11805
Ion Ratio Lower Upper
276 100
138 25.3 26.6 40.0
227 0.0 0.1 0.1

Manual Integrations
APPROVED



Reviewed By : Jagrut Upadhyay 12/19/2022
Supervised By : mohammad ahmed 12/19/2022

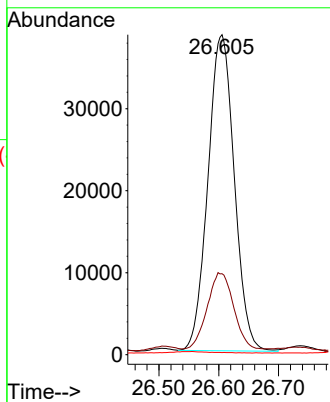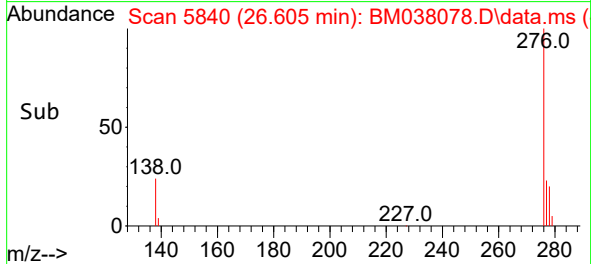


#28
Dibenzo(a,h)anthracene
Concen: 0.485 ng/ul
RT: 26.612 min Scan# 5842
Delta R.T. -0.010 min
Lab File: BM038078.D
Acq: 16 Dec 2022 21:58

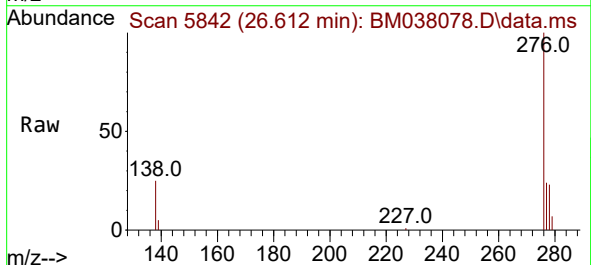


Tgt Ion: 278 Resp: 29268
Ion Ratio Lower Upper
278 100
139 23.5 19.0 28.6
279 30.3 22.4 33.6

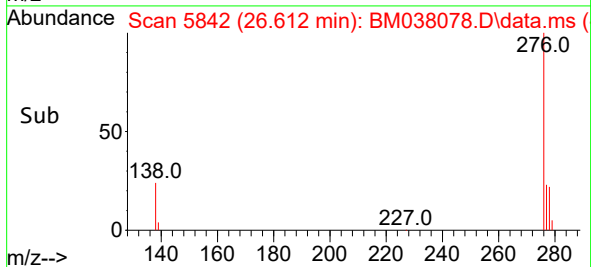



#29
 Benzo(g,h,i)perylene
 Concen: 1.220 ng/ul
 RT: 27.400 min Scan# 6077
 Delta R.T. 0.000 min
 Lab File: BM038078.D
 Acq: 16 Dec 2022 21:58

Instrument :
 BNA_M
 ClientSampleId :
 DBYC6

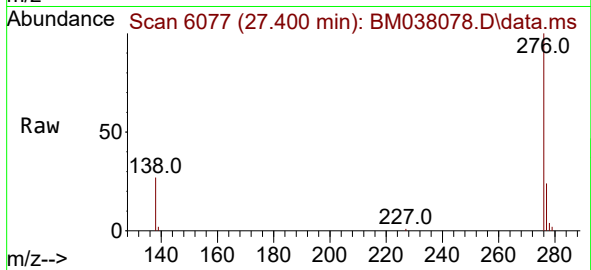

Tgt Ion:276 Resp: 80310
 Ion Ratio Lower Upper
 276 100
 138 26.6 24.1 36.1
 277 24.3 19.0 28.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/19/2022
 Supervised By :mohammad ahmed 12/19/2022

