

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038086.D
 Acq On : 17 Dec 2022 02:54
 Operator : CG/JU
 Sample : N5984-12DL 2X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD7DL

Quant Time: Dec 17 05:00:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 21:53:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	5670	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	17626	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	10334	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	21883	0.400	ng/ul	0.00
17) Chrysene-d12	21.582	240	15876	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	15188	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	16476	2.126	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	4352	0.169	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	9159	0.159	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.067	266	19382	2.139	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038086.D
Acq On : 17 Dec 2022 02:54
Operator : CG/JU
Sample : N5984-12DL 2X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LD7DL


Quant Time: Dec 17 05:00:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 15 21:53:17 2022
Response via : Initial Calibration

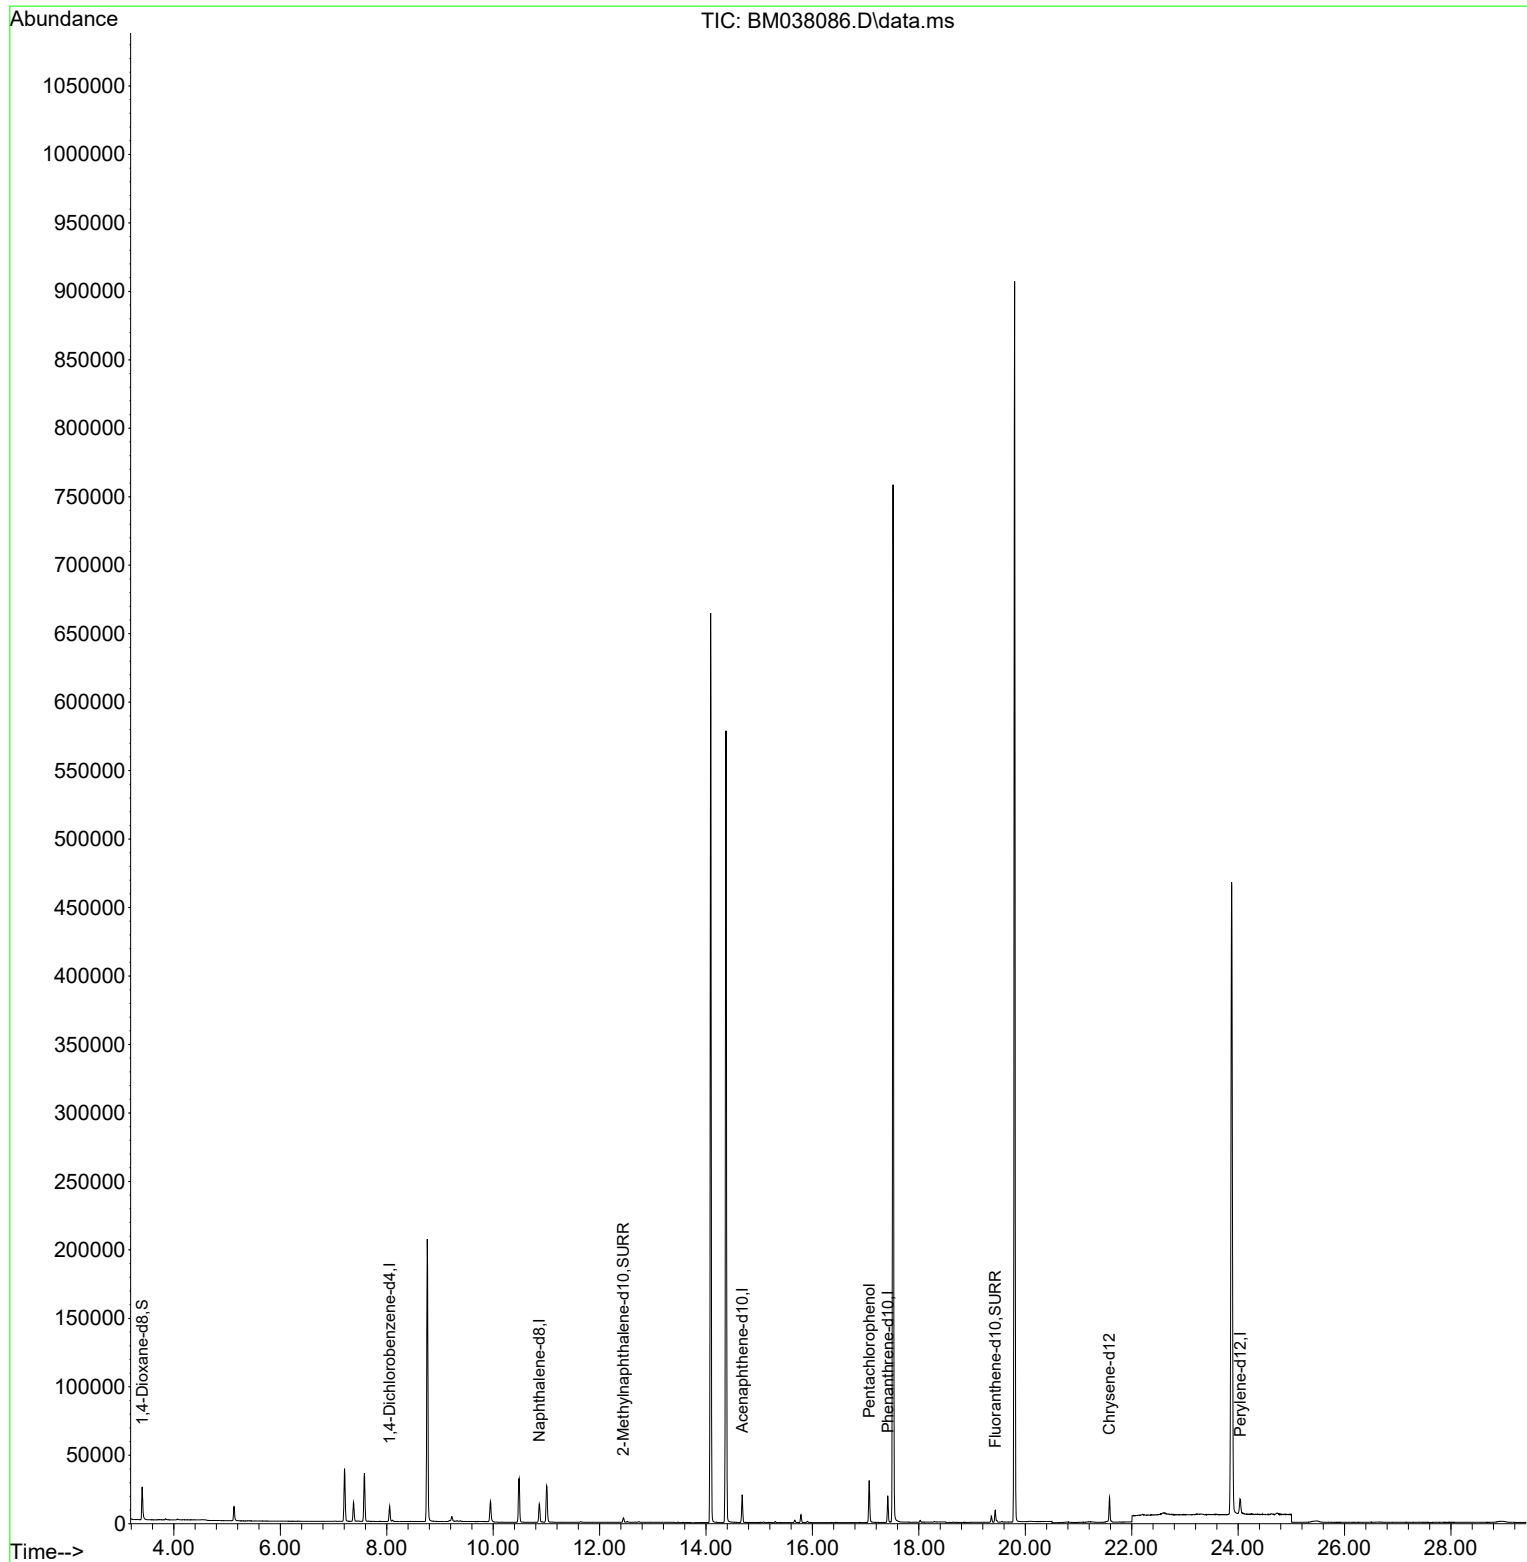

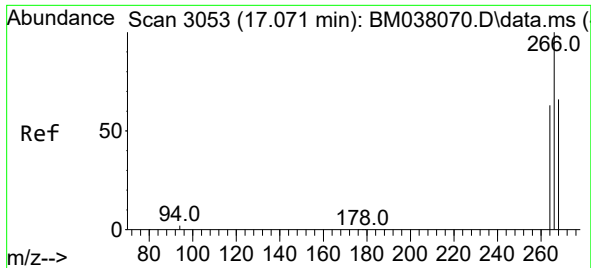

#14
 Pentachlorophenol
 Concen: 2.139 ng/ul
 RT: 17.067 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM038086.D
 Acq: 17 Dec 2022 02:54

Instrument :
 BNA_M
 ClientSampleId :
 C0LD7DL

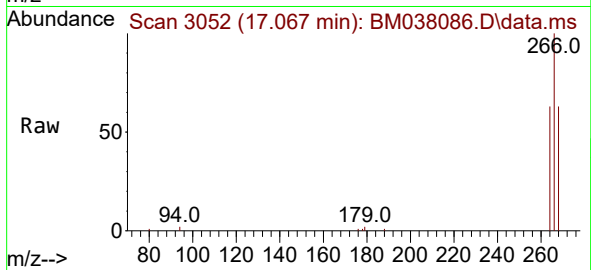

Tgt Ion:266 Resp: 19382
 Ion Ratio Lower Upper
 266 100
 264 62.7 49.9 74.9
 268 63.9 52.0 78.0

