

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038089.D
 Acq On : 17 Dec 2022 05:21
 Operator : CG/JU
 Sample : N6127-01
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFZ50

Quant Time: Dec 19 03:16:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 05:21:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4594	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	14172	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.680	164	8086	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	16502	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	11375	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	11297	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	23821	3.794	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	6468	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	14965	0.363	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	3617	0.639	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038089.D
Acq On : 17 Dec 2022 05:21
Operator : CG/JU
Sample : N6127-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFZ50


Quant Time: Dec 19 03:16:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 05:21:07 2022
Response via : Initial Calibration

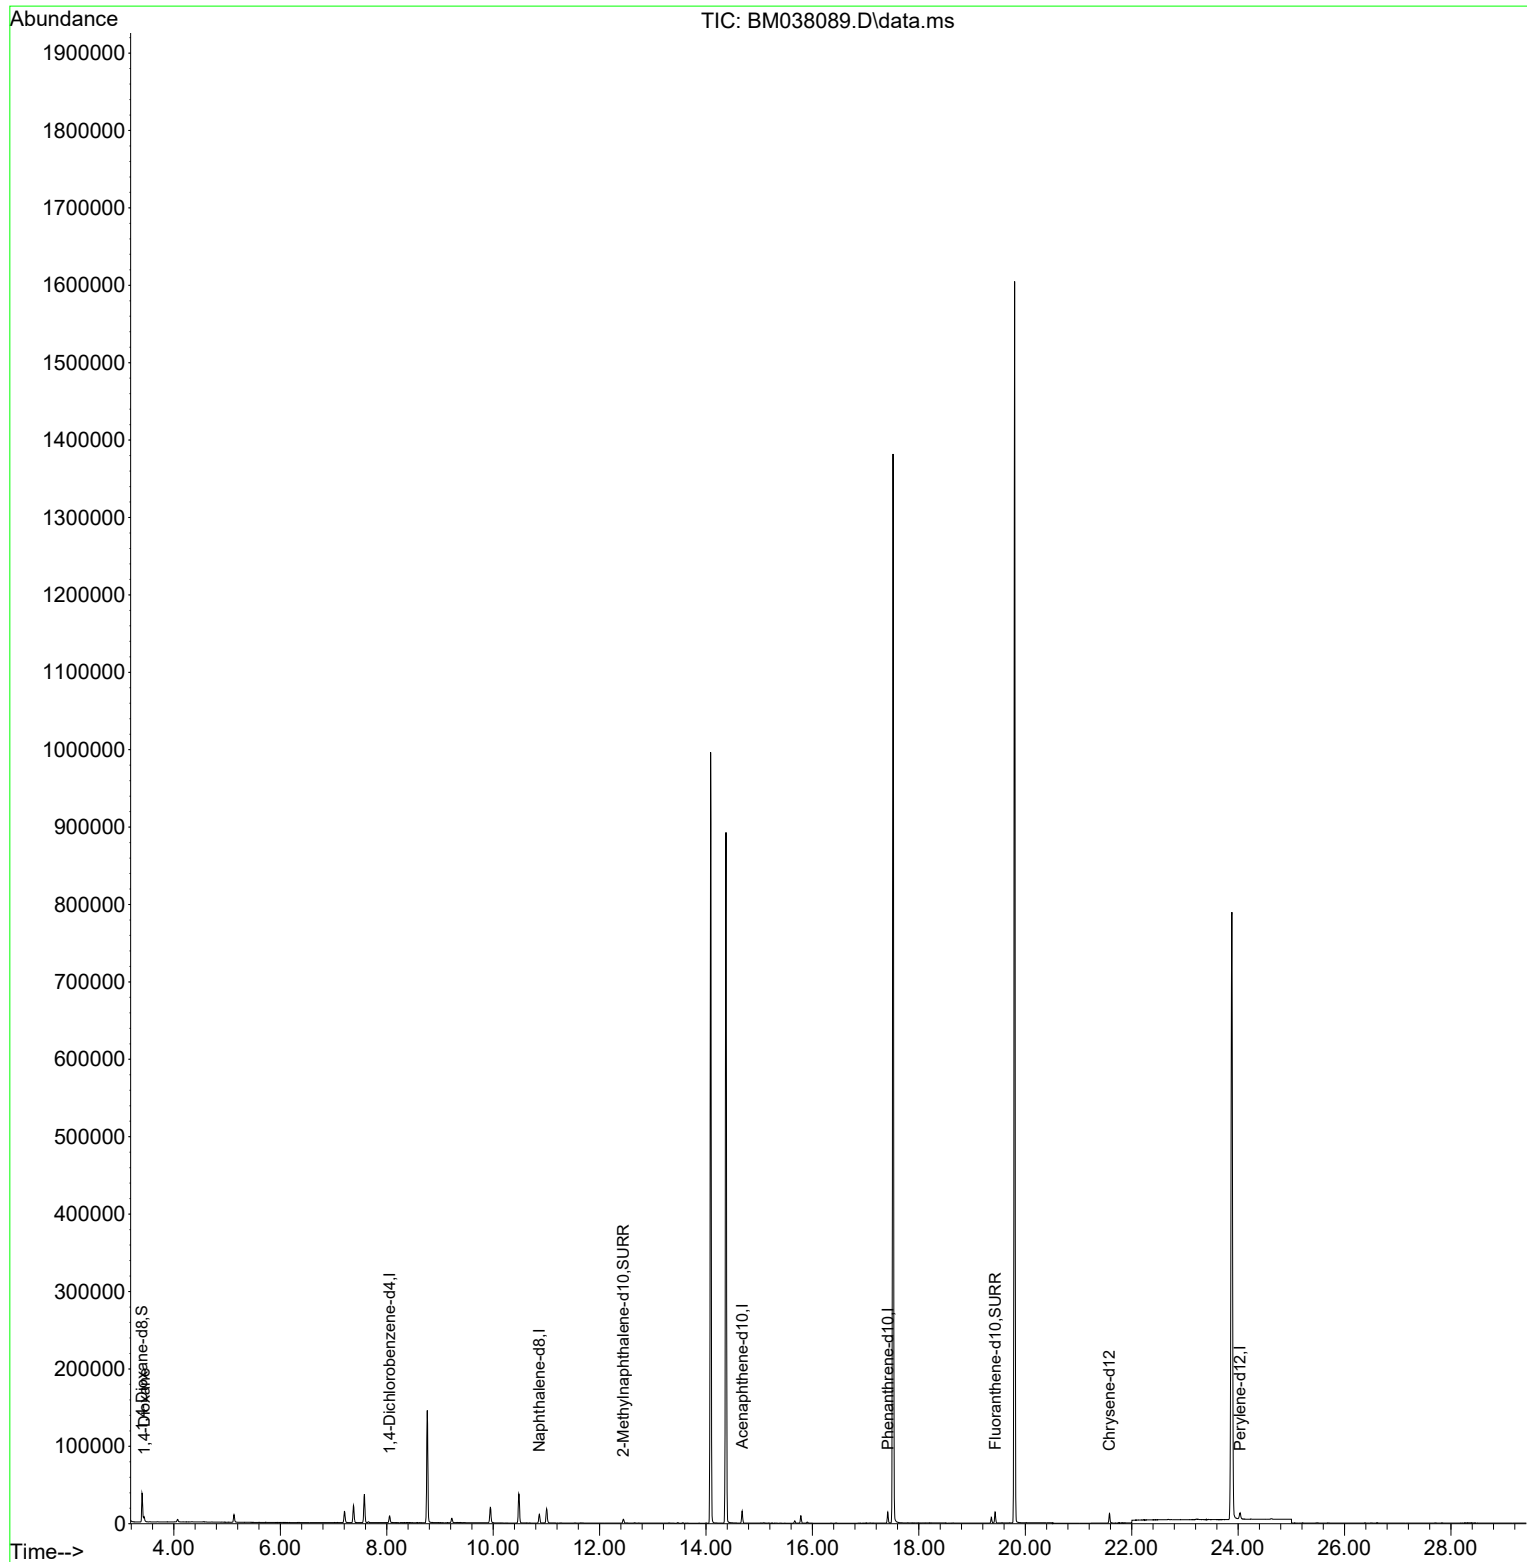


Abundance Scan 62 (3.444 min): BM038087.D\data.ms (-55)

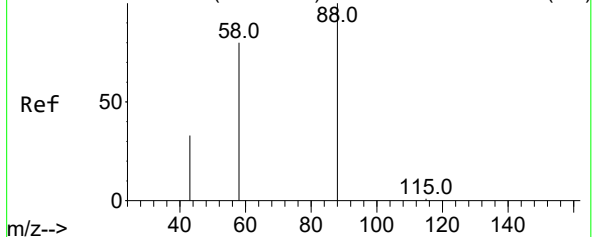

Abundance Scan 62 (3.444 min): BM038089.D\data.ms

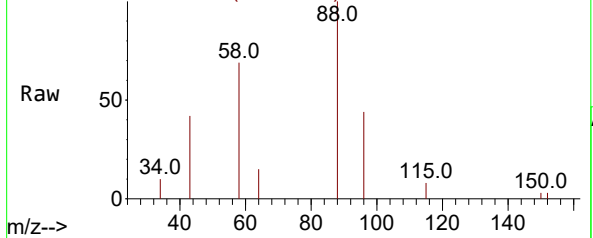

Abundance Scan 62 (3.444 min): BM038089.D\data.ms (-48)

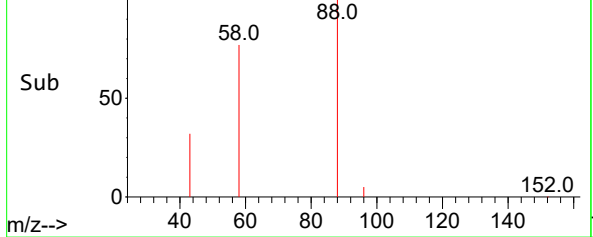

#2
1,4-Dioxane
Concen: 0.639 ng/ul
RT: 3.444 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM038089.D
Acq: 17 Dec 2022 05:21

Instrument :
BNA_M
ClientSampleId :
BFZ50

Tgt Ion:	88	Resp:	3617
Ion	Ratio	Lower	Upper
88	100		
43	41.7	31.4	47.0
58	68.9	50.2	75.2

