

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
 Data File : BM038090.D
 Acq On : 17 Dec 2022 05:58
 Operator : CG/JU
 Sample : N5984-03DL 5X
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0LC7DL

Quant Time: Dec 19 03:16:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 17 05:21:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4673	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	14110	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.680	164	8002	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	16652	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	11808	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	11847	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	6160	0.964	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	1391	0.068	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	2686	0.063	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.067	266	7197	1.044	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121522\
Data File : BM038090.D
Acq On : 17 Dec 2022 05:58
Operator : CG/JU
Sample : N5984-03DL 5X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LC7DL


Quant Time: Dec 19 03:16:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 05:21:07 2022
Response via : Initial Calibration

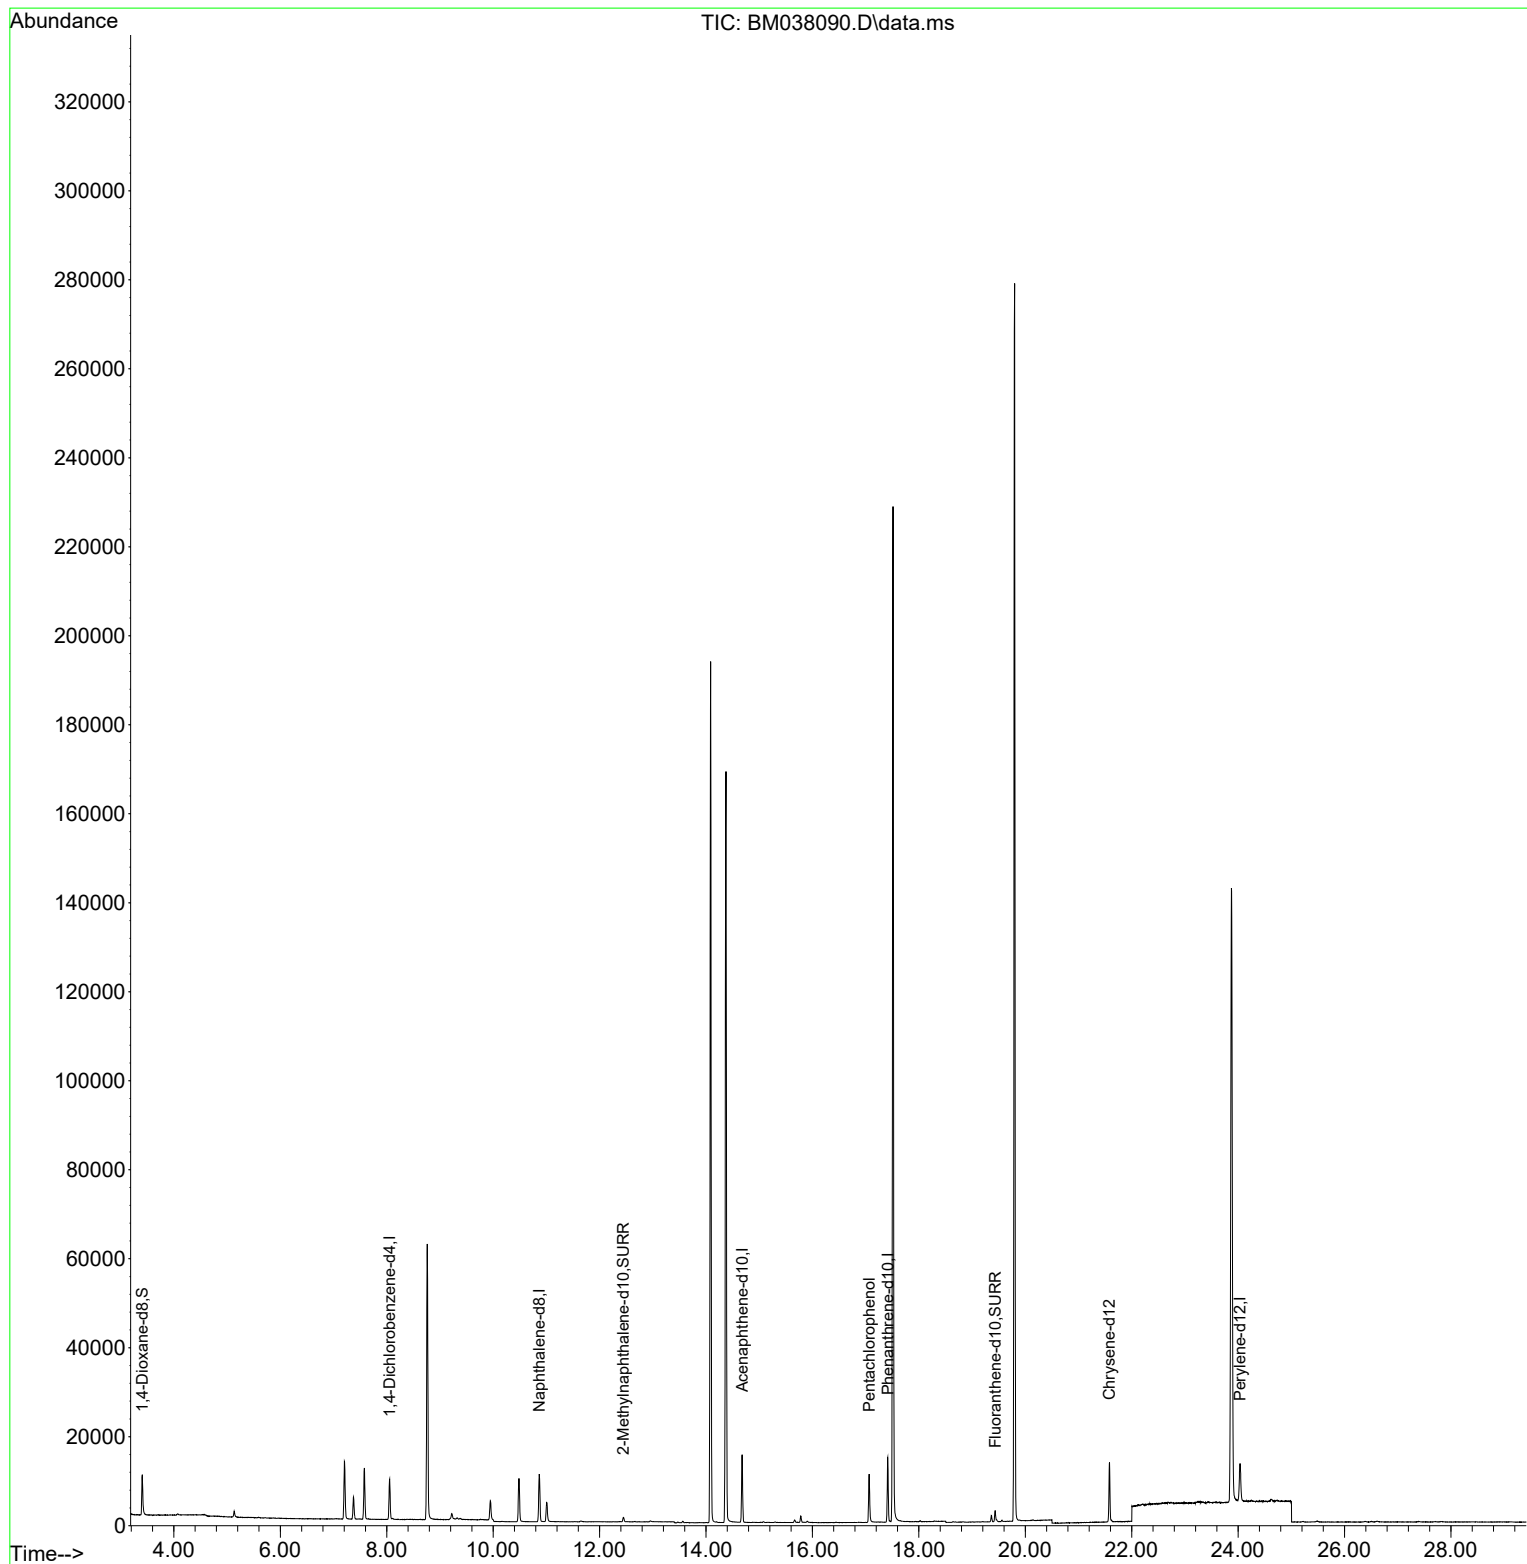

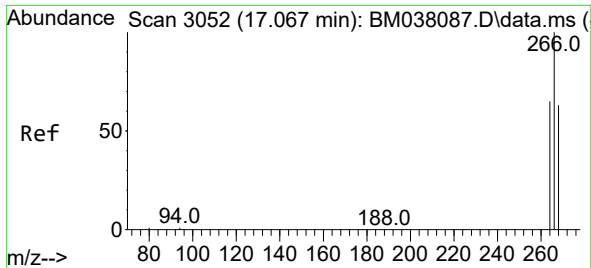

#14
Pentachlorophenol
Concen: 1.044 ng/ul
RT: 17.067 min Scan# 30
Delta R.T. 0.000 min
Lab File: BM038090.D
Acq: 17 Dec 2022 05:58

Instrument :
BNA_M
ClientSampleId :
C0LC7DL

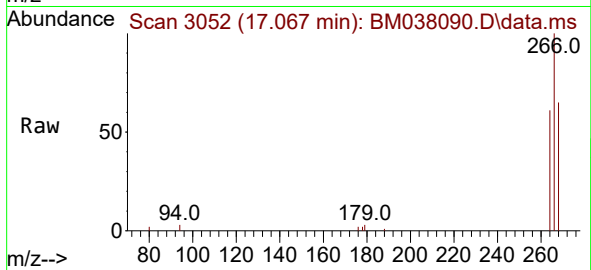

Tgt Ion:	266	Resp:	7197
Ion	Ratio	Lower	Upper
266	100		
264	62.8	49.9	74.9
268	64.4	52.0	78.0

