

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043360.D
 Acq On : 15 Dec 2023 16:34
 Operator : MA/JU
 Sample : PB157639BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	29	34	42	rVB	113728	162793	2.24%	0.181%
2	3.805	101	105	128	rBV	1460029	2292737	31.50%	2.544%
3	4.134	157	161	166	rBV	24812	33817	0.46%	0.038%
4	4.369	196	201	205	rBV8	4815	10381	0.14%	0.012%
5	5.863	451	455	459	rBV7	3511	7789	0.11%	0.009%
6	6.975	639	644	650	rBV8	4496	10385	0.14%	0.012%
7	7.151	666	674	690	rVB	1721614	2762208	37.94%	3.065%
8	7.328	697	704	715	rBV	1393323	2187674	30.05%	2.427%
9	7.516	729	736	745	rBV	1726298	2702417	37.12%	2.999%
10	7.993	809	817	829	rVB	1332839	2108769	28.97%	2.340%
11	8.698	930	937	958	rBV	2079409	3370133	46.30%	3.740%
12	9.163	1008	1016	1025	rBV	1664039	2744776	37.71%	3.046%
13	9.334	1039	1045	1048	rBV7	4705	7965	0.11%	0.009%
14	9.881	1130	1138	1152	rBV	1306966	2227843	30.60%	2.472%
15	10.416	1220	1229	1240	rBV	1923480	3177398	43.65%	3.526%
16	10.669	1263	1272	1276	rVB	7819	19242	0.26%	0.021%
17	10.798	1286	1294	1304	rBV	1832717	3152410	43.31%	3.498%
18	10.945	1309	1319	1327	rBV	2152878	3763205	51.70%	4.176%
19	12.386	1557	1564	1571	rBV2	36356	67468	0.93%	0.075%
20	12.963	1656	1662	1663	rBV6	5619	8312	0.11%	0.009%
21	13.522	1750	1757	1765	rBV	37044	64459	0.89%	0.072%
22	13.598	1765	1770	1776	rVB8	5800	11494	0.16%	0.013%
23	14.039	1838	1845	1860	rBV	3527401	4936841	67.82%	5.478%
24	14.322	1885	1893	1902	rBV	3872520	5846478	80.31%	6.487%
25	14.622	1937	1944	1952	rBV	2696943	4051792	55.66%	4.496%
26	14.722	1956	1961	1964	rBV7	7415	9636	0.13%	0.011%
27	14.816	1968	1977	1993	rBV	1858784	2798773	38.45%	3.106%
28	14.986	2001	2006	2009	rVV6	4136	8149	0.11%	0.009%
29	15.039	2009	2015	2024	rVB6	6276	15519	0.21%	0.017%
30	15.404	2071	2077	2084	rBV10	6976	16528	0.23%	0.018%
31	15.616	2106	2113	2120	rBV	4855623	6923816	95.11%	7.683%
32	15.733	2126	2133	2145	rBV	1603037	2198555	30.20%	2.440%
33	15.851	2149	2153	2158	rVB2	22688	33932	0.47%	0.038%
34	16.016	2175	2181	2186	rVB7	6810	12986	0.18%	0.014%
35	16.404	2241	2247	2250	rVB7	7094	9922	0.14%	0.011%
36	16.663	2285	2291	2293	rBV5	5179	7779	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043360.D
 Acq On : 15 Dec 2023 16:34
 Operator : MA/JU
 Sample : PB157639BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	17.039	2352	2355	2359	rVB6	6372	7737	0.11%	0.009%
38	17.145	2371	2373	2379	rVB5	6666	9661	0.13%	0.011%
39	17.363	2402	2410	2420	rBV	3114570	4437338	60.96%	4.924%
40	17.463	2420	2427	2439	rBV2	5154776	7267473	99.83%	8.064%
41	17.751	2471	2476	2483	rBV6	8186	16497	0.23%	0.018%
42	18.262	2558	2563	2571	rBV6	11640	22662	0.31%	0.025%
43	19.315	2737	2742	2749	rBV3	52111	79454	1.09%	0.088%
44	19.386	2749	2754	2759	rBV	52755	74724	1.03%	0.083%
45	19.539	2777	2780	2784	rBV6	8321	11826	0.16%	0.013%
46	19.692	2804	2806	2809	rBV4	11470	11270	0.15%	0.013%
47	19.751	2810	2816	2825	rVV	5601488	7279529	100.00%	8.077%
48	20.756	2983	2987	2992	rVB	96154	109921	1.51%	0.122%
49	21.539	3115	3120	3133	rVB2	2752509	3621914	49.75%	4.019%
50	23.803	3498	3505	3516	rVB2	2986797	5824261	80.01%	6.463%
51	23.903	3519	3522	3525	rVV2	126181	207824	2.85%	0.231%
52	23.962	3525	3532	3541	rVB	1648560	3374891	46.36%	3.745%




Sum of corrected areas: 90121363

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043360.D
Acq On : 15 Dec 2023 16:34
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

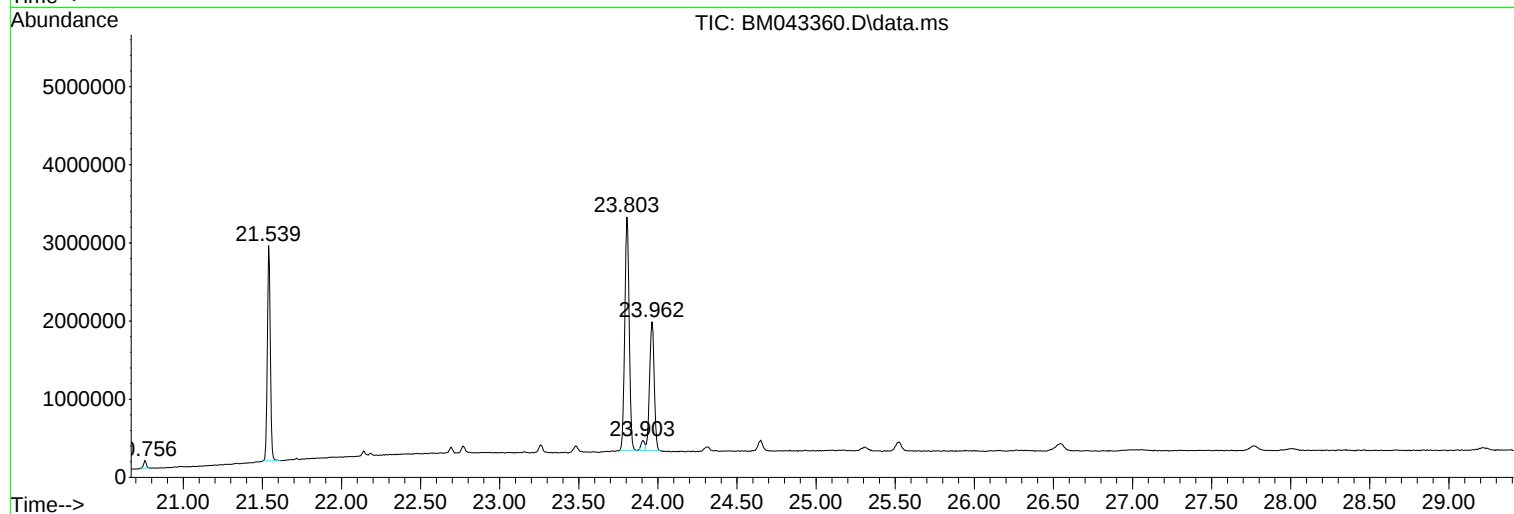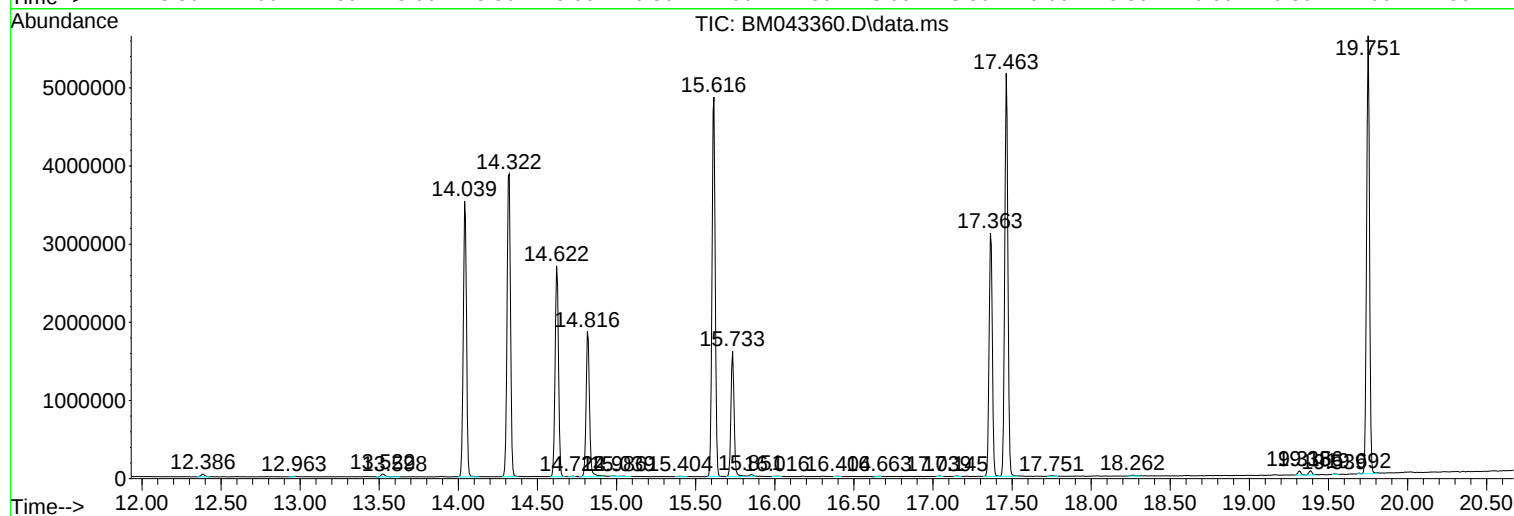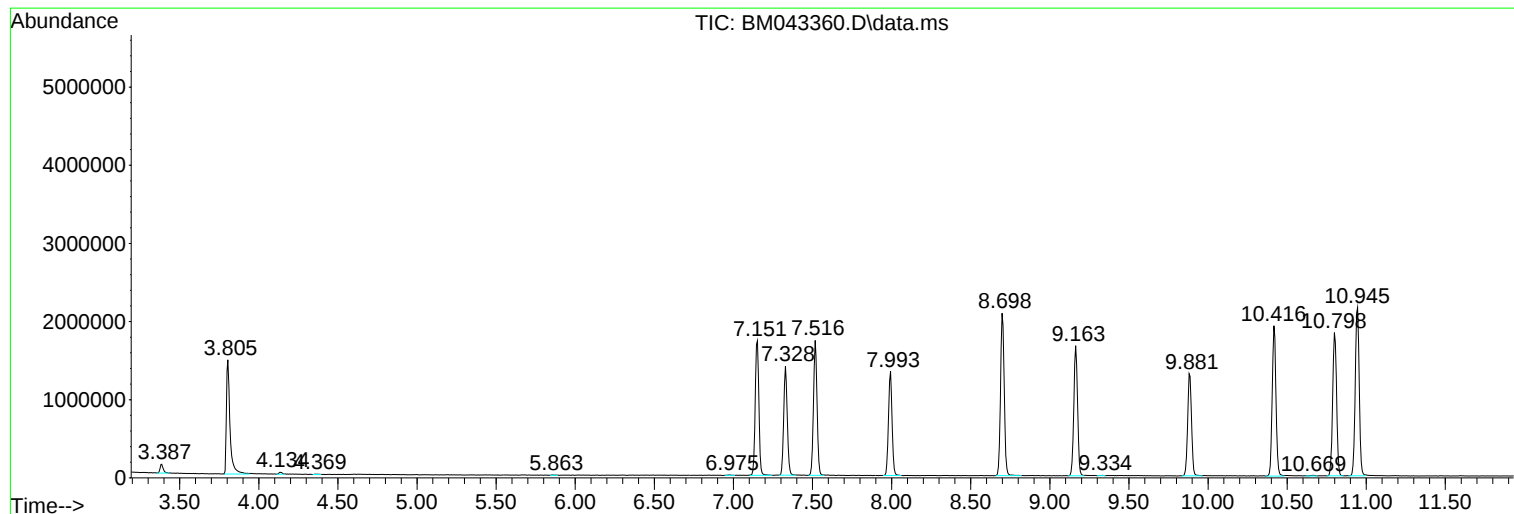

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043360.D
Acq On : 15 Dec 2023 16:34
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043360.D
Acq On : 15 Dec 2023 16:34
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------