

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043363.D
 Acq On : 15 Dec 2023 18:23
 Operator : MA/JU
 Sample : PB157812BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	43	rVB	116651	157511	2.00%	0.162%
2	3.805	101	105	130	rBV	1548179	2350663	29.91%	2.412%
3	4.140	157	162	172	rVB	93701	129150	1.64%	0.133%
4	7.152	663	674	688	rBV	1802139	2829491	36.01%	2.903%
5	7.328	694	704	718	rBV	1456473	2299666	29.26%	2.359%
6	7.516	729	736	747	rBV	1711576	2718908	34.60%	2.789%
7	7.993	810	817	827	rBV	1527052	2388663	30.40%	2.451%
8	8.699	929	937	948	rBV	2104941	3443219	43.82%	3.533%
9	9.163	1008	1016	1027	rBV	1728389	2850063	36.27%	2.924%
10	9.887	1129	1139	1148	rBV	1347700	2331519	29.67%	2.392%
11	10.416	1221	1229	1240	rBV	1985198	3345958	42.58%	3.433%
12	10.798	1286	1294	1304	rVB	2183716	3645843	46.39%	3.740%
13	10.945	1310	1319	1334	rBV	2244992	3886271	49.45%	3.987%
14	12.387	1559	1564	1570	rBV2	35897	60211	0.77%	0.062%
15	12.604	1596	1601	1606	rVB9	6012	11298	0.14%	0.012%
16	13.522	1751	1757	1766	rVB	39052	65372	0.83%	0.067%
17	13.592	1766	1769	1775	rBV6	6642	11676	0.15%	0.012%
18	14.039	1838	1845	1853	rBV	3838974	5279392	67.18%	5.416%
19	14.316	1884	1892	1904	rBV2	4320307	6379523	81.18%	6.545%
20	14.622	1937	1944	1954	rBV	3319612	4844466	61.65%	4.970%
21	14.722	1957	1961	1966	rVB8	5975	10154	0.13%	0.010%
22	14.816	1970	1977	1993	rBV	2045870	2974567	37.85%	3.052%
23	15.039	2010	2015	2021	rBV8	11763	20583	0.26%	0.021%
24	15.610	2103	2112	2121	rBV	5259524	7579860	96.45%	7.777%
25	15.733	2127	2133	2147	rBV	1700031	2361147	30.05%	2.422%
26	15.851	2149	2153	2159	rVB3	25617	43120	0.55%	0.044%
27	16.392	2240	2245	2251	rVB5	18311	30671	0.39%	0.031%
28	17.039	2352	2355	2361	rVB6	7434	12019	0.15%	0.012%
29	17.151	2369	2374	2377	rBV2	8787	12584	0.16%	0.013%
30	17.363	2403	2410	2417	rBV	3900087	5338911	67.94%	5.477%
31	17.463	2420	2427	2441	rBV2	5606170	7858497	100.00%	8.062%
32	17.751	2473	2476	2482	rBV8	5759	8797	0.11%	0.009%
33	18.257	2557	2562	2568	rBV6	29681	48860	0.62%	0.050%
34	19.316	2737	2742	2749	rBV2	57922	87343	1.11%	0.090%
35	19.386	2749	2754	2759	rBV	51478	75295	0.96%	0.077%
36	19.539	2776	2780	2784	rBV5	19403	27277	0.35%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043363.D
Acq On : 15 Dec 2023 18:23
Operator : MA/JU
Sample : PB157812BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.692	2803	2806	2808	rBV3	7314	8088	0.10%	0.008%
38	19.745	2809	2815	2823	rVV	5593434	7735542	98.44%	7.936%
39	20.757	2983	2987	2991	rBV	80588	100985	1.29%	0.104%
40	21.539	3114	3120	3129	rBV	3242644	4226257	53.78%	4.336%
41	23.803	3497	3505	3513	rBV2	3062523	5975829	76.04%	6.131%
42	23.956	3524	3531	3542	rVB	1928423	3905694	49.70%	4.007%


Sum of corrected areas: 97470943

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043363.D
Acq On : 15 Dec 2023 18:23
Operator : MA/JU
Sample : PB157812BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

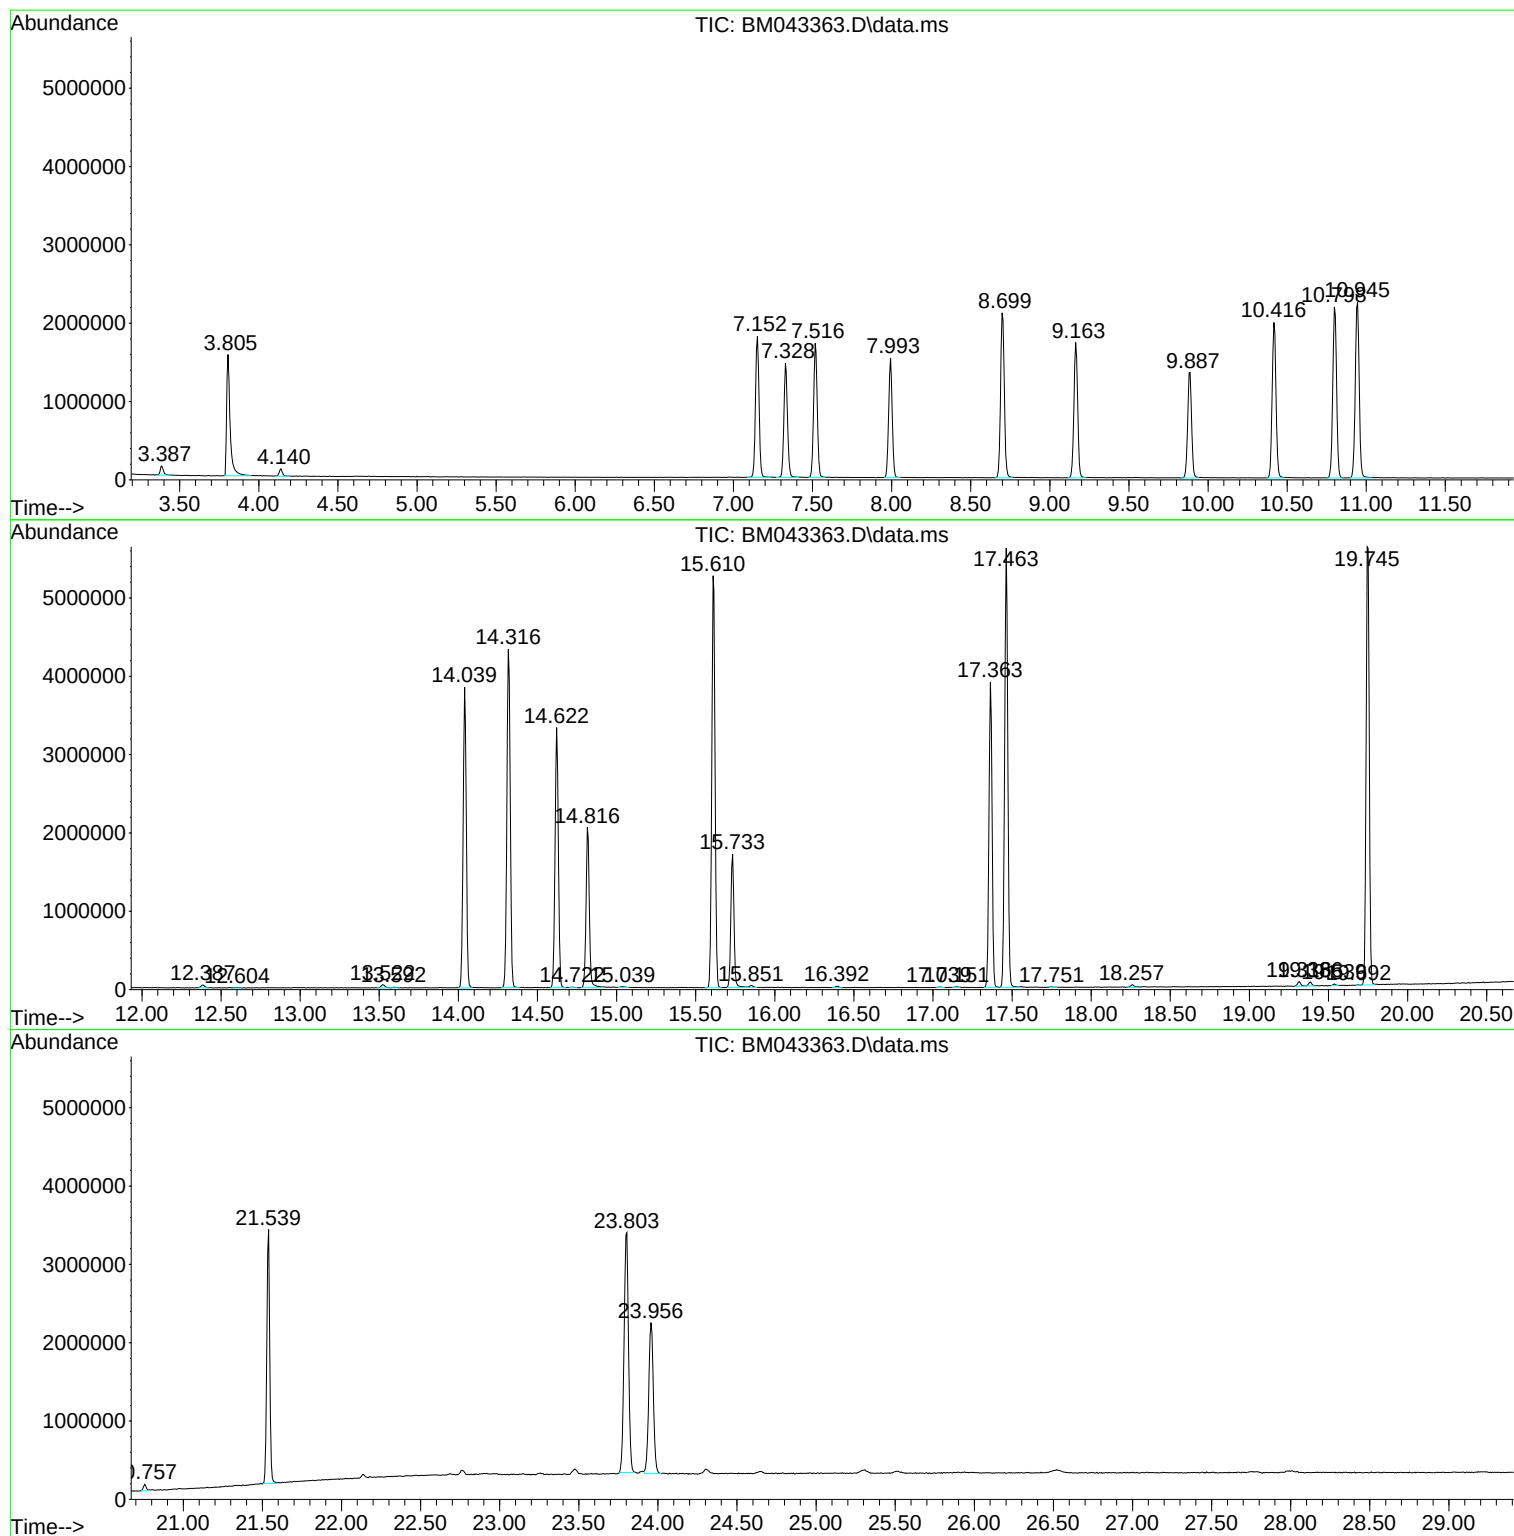

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043363.D
Acq On : 15 Dec 2023 18:23
Operator : MA/JU
Sample : PB157812BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043363.D
Acq On : 15 Dec 2023 18:23
Operator : MA/JU
Sample : PB157812BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------