

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043365.D
 Acq On : 15 Dec 2023 19:35
 Operator : MA/JU
 Sample : 05830-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	23	28	36	rBV	5482681	7670282	11.67%	4.388%
2	3.416	36	39	55	rVB	2222630	3035356	4.62%	1.736%
3	3.810	103	106	120	rBV	397509	636717	0.97%	0.364%
4	4.675	245	253	272	rBV	40414865	65717084	100.00%	37.594%
5	7.151	668	674	687	rVB	354551	588597	0.90%	0.337%
6	7.328	698	704	714	rBV	1580728	2483021	3.78%	1.420%
7	7.516	729	736	747	rBV	1355627	2161977	3.29%	1.237%
8	7.993	808	817	825	rBV	1643621	2584151	3.93%	1.478%
9	8.698	930	937	949	rBV	1074462	1744149	2.65%	0.998%
10	9.163	1008	1016	1027	rBV	1916275	3132219	4.77%	1.792%
11	9.887	1131	1139	1152	rBV	1398717	2390611	3.64%	1.368%
12	10.416	1222	1229	1241	rBV	2074636	3478805	5.29%	1.990%
13	10.798	1285	1294	1302	rBV	2338493	4001588	6.09%	2.289%
14	10.945	1310	1319	1335	rBV	2164575	3737456	5.69%	2.138%
15	12.386	1558	1564	1571	rVB	39382	68895	0.10%	0.039%
16	13.522	1752	1757	1762	rBV	49066	81393	0.12%	0.047%
17	14.039	1838	1845	1856	rBV	4510656	6152191	9.36%	3.519%
18	14.316	1885	1892	1904	rVB	5058666	7393784	11.25%	4.230%
19	14.622	1937	1944	1951	rBV	3498064	5133966	7.81%	2.937%
20	14.816	1971	1977	1990	rBV	327074	534755	0.81%	0.306%
21	15.610	2105	2112	2122	rBV	6323052	8973112	13.65%	5.133%
22	15.733	2125	2133	2148	rVV	1917006	2690835	4.09%	1.539%
23	17.363	2403	2410	2417	rBV	3892332	5357107	8.15%	3.065%
24	17.463	2420	2427	2437	rBV2	6348643	9060707	13.79%	5.183%
25	18.262	2558	2563	2570	rBV	236097	349399	0.53%	0.200%
26	18.351	2573	2578	2583	rVB2	183609	264122	0.40%	0.151%
27	19.315	2738	2742	2747	rVB	66748	90773	0.14%	0.052%
28	19.380	2750	2753	2757	rVV	63526	84154	0.13%	0.048%
29	19.533	2776	2779	2784	rBV2	97771	133247	0.20%	0.076%
30	19.751	2809	2816	2822	rBV	6536028	8717824	13.27%	4.987%
31	20.751	2983	2986	2992	rVB	141443	162655	0.25%	0.093%
32	21.256	3068	3072	3080	rBV	255493	387211	0.59%	0.222%
33	21.533	3114	3119	3129	rVB	3171728	4130769	6.29%	2.363%
34	22.133	3218	3221	3225	rBV2	97392	124897	0.19%	0.071%
35	22.762	3324	3328	3333	rVB	153380	237919	0.36%	0.136%
36	23.474	3445	3449	3459	rVB	188153	338544	0.52%	0.194%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043365.D
Acq On : 15 Dec 2023 19:35
Operator : MA/JU
Sample : 05830-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	23.797	3497	3504	3515	rVB	3533331	6987466	10.63%	3.997%
38	23.956	3524	3531	3543	rVB	1956296	3990980	6.07%	2.283%




Sum of corrected areas: 174808718

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043365.D
Acq On : 15 Dec 2023 19:35
Operator : MA/JU
Sample : 05830-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

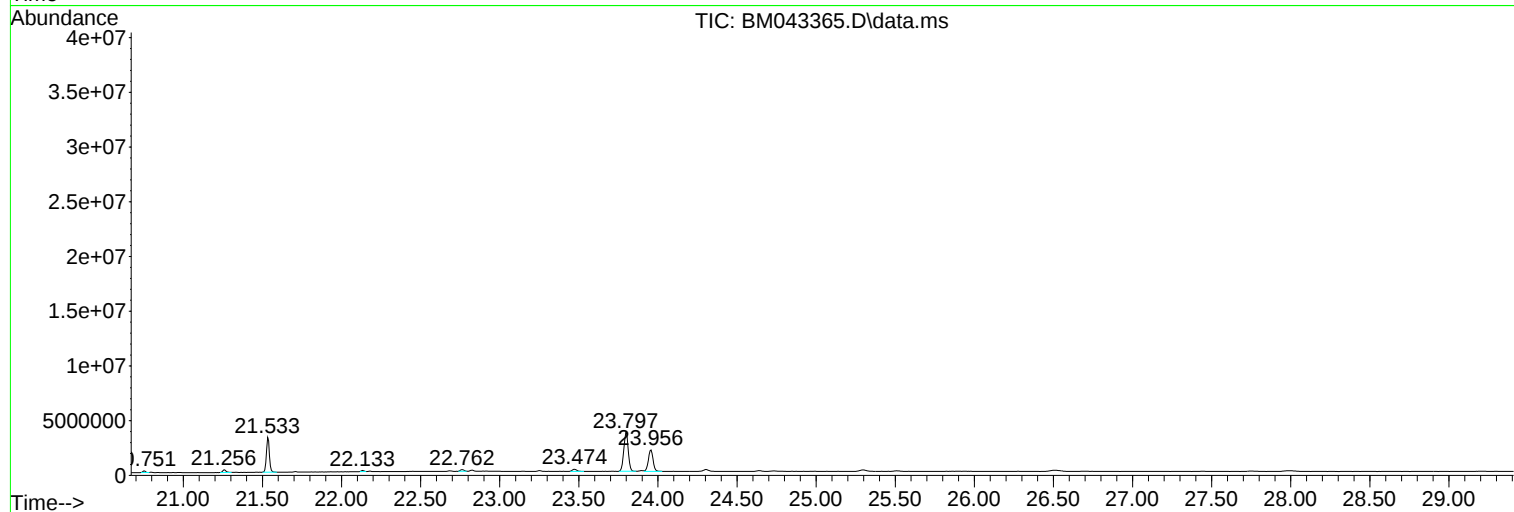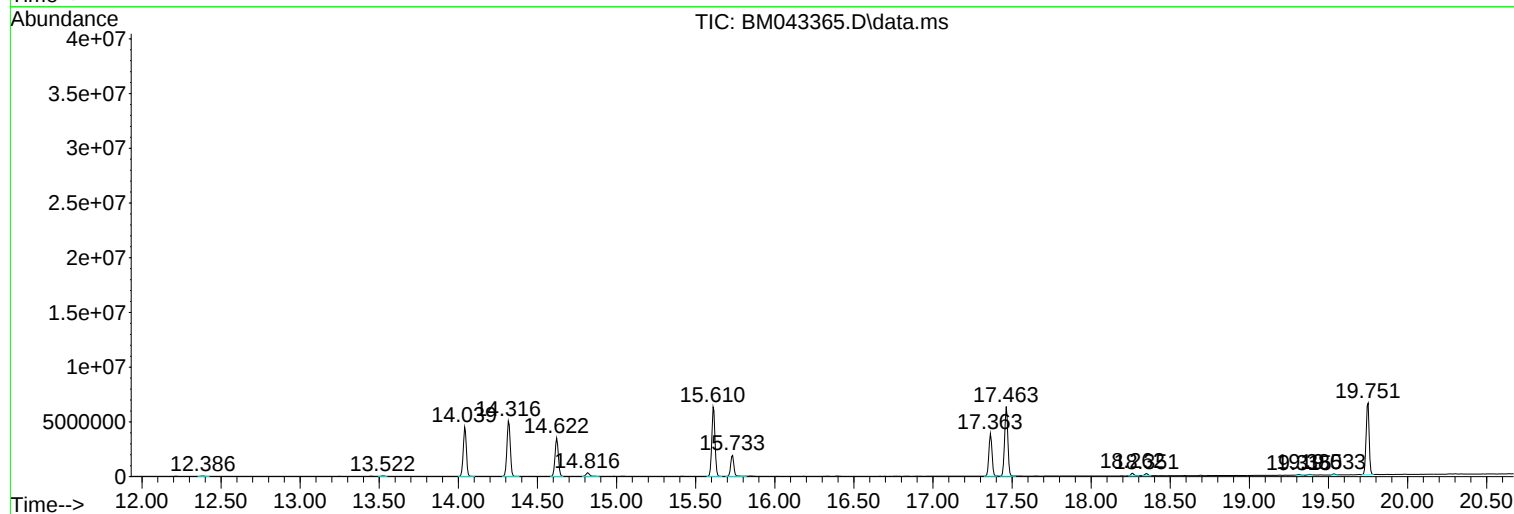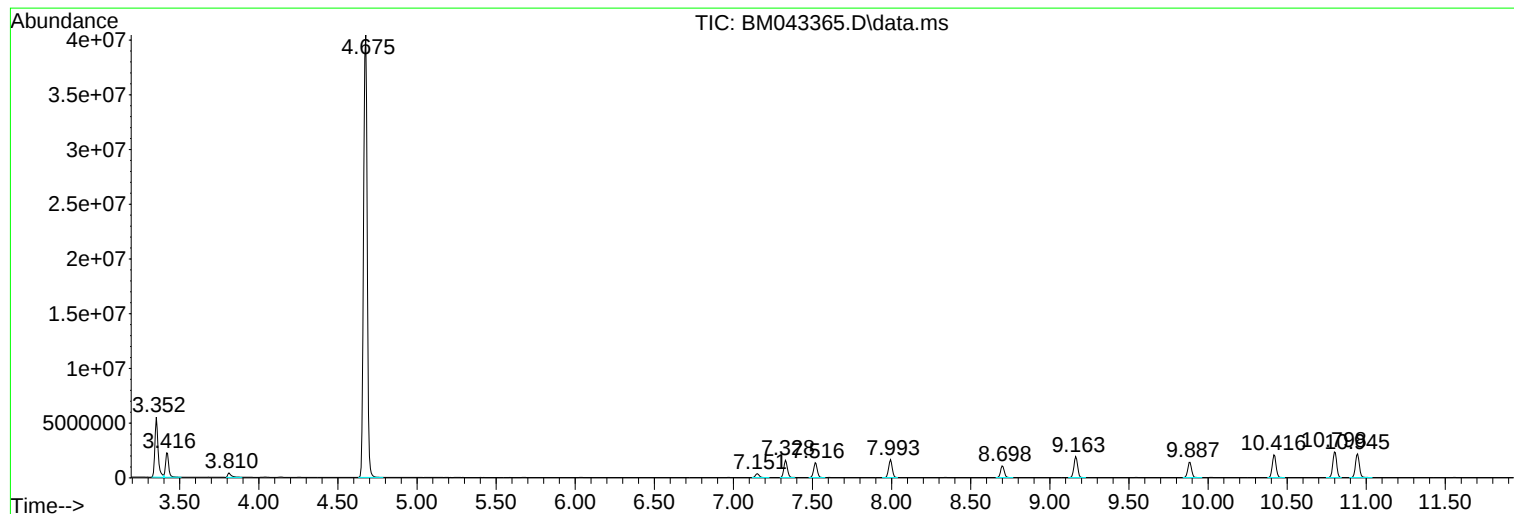

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043365.D
Acq On : 15 Dec 2023 19:35
Operator : MA/JU
Sample : 05830-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043365.D
Acq On : 15 Dec 2023 19:35
Operator : MA/JU
Sample : 05830-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc