

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043367.D
 Acq On : 15 Dec 2023 20:48
 Operator : MA/JU
 Sample : 05830-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	45	rVB	104856	146710	1.51%	0.138%
2	3.681	81	84	92	rBV	20672	36568	0.38%	0.034%
3	3.810	102	106	122	rBV	590044	978513	10.05%	0.920%
4	4.040	141	145	150	rVB	24438	40191	0.41%	0.038%
5	4.140	157	162	167	rVB	29904	40207	0.41%	0.038%
6	5.093	317	324	329	rVB3	21226	39298	0.40%	0.037%
7	5.681	419	424	428	rVB6	8132	13967	0.14%	0.013%
8	6.040	481	485	489	rVB6	8187	10419	0.11%	0.010%
9	6.963	638	642	649	rBV8	6918	14468	0.15%	0.014%
10	7.151	668	674	682	rBV	411712	650548	6.68%	0.612%
11	7.328	695	704	716	rBV	1763937	2809170	28.85%	2.642%
12	7.516	728	736	747	rBV	1545417	2482410	25.49%	2.335%
13	7.993	810	817	824	rBV	1710984	2694382	27.67%	2.534%
14	8.698	929	937	948	rBV	1207286	1967546	20.20%	1.851%
15	9.163	1008	1016	1029	rBV	2186757	3543294	36.38%	3.333%
16	9.410	1056	1058	1063	rVB5	8033	12024	0.12%	0.011%
17	9.540	1074	1080	1085	rBV4	10937	21373	0.22%	0.020%
18	9.739	1109	1114	1121	rBV5	14576	24687	0.25%	0.023%
19	9.881	1130	1138	1151	rBV	1596096	2744689	28.18%	2.582%
20	10.416	1221	1229	1238	rBV	2257733	3772989	38.74%	3.549%
21	10.798	1286	1294	1306	rBV	2414512	4108477	42.19%	3.864%
22	10.945	1309	1319	1333	rBV	2401400	4193648	43.06%	3.945%
23	11.363	1380	1390	1395	rBV	9519	25111	0.26%	0.024%
24	11.551	1415	1422	1428	rBV2	26718	62597	0.64%	0.059%
25	12.210	1529	1534	1539	rVB5	21523	38195	0.39%	0.036%
26	12.381	1557	1563	1569	rVB	44607	74684	0.77%	0.070%
27	12.592	1596	1599	1605	rVB7	7606	12307	0.13%	0.012%
28	12.986	1662	1666	1670	rVB5	7254	10997	0.11%	0.010%
29	13.245	1706	1710	1717	rVB3	14213	26692	0.27%	0.025%
30	13.451	1738	1745	1752	rVB4	21323	40799	0.42%	0.038%
31	13.522	1752	1757	1765	rBV2	56896	97460	1.00%	0.092%
32	13.592	1765	1769	1772	rBV3	9907	11151	0.11%	0.010%
33	14.039	1836	1845	1852	rBV	4472898	6208596	63.75%	5.840%
34	14.269	1880	1884	1885	rBV4	16667	18906	0.19%	0.018%
35	14.316	1885	1892	1901	rVB2	5160726	7737836	79.46%	7.278%
36	14.622	1936	1944	1952	rBV	3567986	5283581	54.25%	4.970%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043367.D
 Acq On : 15 Dec 2023 20:48
 Operator : MA/JU
 Sample : 05830-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	14.716	1957	1960	1965	rVB7	8494	13178	0.14%	0.012%
38	14.822	1971	1978	1990	rBV3	733034	1700948	17.47%	1.600%
39	15.033	2010	2014	2024	rVB3	19230	36537	0.38%	0.034%
40	15.421	2070	2080	2082	rBV4	13680	27329	0.28%	0.026%
41	15.610	2104	2112	2126	rBV	6549338	9210277	94.58%	8.663%
42	15.733	2126	2133	2147	rVV	2082406	2935285	30.14%	2.761%
43	15.851	2148	2153	2160	rVB4	29448	55219	0.57%	0.052%
44	16.016	2178	2181	2189	rVB10	6101	11215	0.12%	0.011%
45	16.169	2203	2207	2214	rBV9	6486	13419	0.14%	0.013%
46	16.327	2229	2234	2239	rVB8	7756	15439	0.16%	0.015%
47	16.392	2240	2245	2249	rVB5	28798	42054	0.43%	0.040%
48	16.763	2305	2308	2312	rBV4	12580	17092	0.18%	0.016%
49	16.968	2338	2343	2345	rBV6	5857	9762	0.10%	0.009%
50	17.033	2348	2354	2361	rVB6	13077	28007	0.29%	0.026%
51	17.127	2366	2370	2372	rBV5	8738	13367	0.14%	0.013%
52	17.363	2403	2410	2420	rBV	4087370	5568829	57.18%	5.238%
53	17.463	2420	2427	2437	rBV2	7004527	9738442	100.00%	9.160%
54	17.663	2455	2461	2467	rBV3	11905	23930	0.25%	0.023%
55	18.039	2520	2525	2529	rVB6	16403	27756	0.29%	0.026%
56	18.262	2557	2563	2571	rBV	279519	436003	4.48%	0.410%
57	18.345	2574	2577	2583	rVB4	23145	38656	0.40%	0.036%
58	18.592	2616	2619	2622	rBV5	7733	11852	0.12%	0.011%
59	18.692	2632	2636	2641	rVB2	42038	50649	0.52%	0.048%
60	19.315	2737	2742	2746	rBV2	74270	106530	1.09%	0.100%
61	19.386	2749	2754	2757	rBV	72099	104215	1.07%	0.098%
62	19.533	2775	2779	2785	rBV	123240	176226	1.81%	0.166%
63	19.692	2803	2806	2809	rBV5	18419	23839	0.24%	0.022%
64	19.751	2809	2816	2823	rVV	7373982	9583431	98.41%	9.014%
65	19.980	2852	2855	2860	rVB2	23359	28440	0.29%	0.027%
66	20.756	2983	2987	2991	rBV	104765	114134	1.17%	0.107%
67	21.256	3068	3072	3081	rBV	213738	352248	3.62%	0.331%
68	21.539	3114	3120	3131	rBV	3372386	4321739	44.38%	4.065%
69	23.803	3497	3505	3515	rVB2	3778520	7375559	75.74%	6.937%
70	23.956	3524	3531	3543	rVB	2068047	4109910	42.20%	3.866%


Sum of corrected areas: 106316006

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043367.D
Acq On : 15 Dec 2023 20:48
Operator : MA/JU
Sample : 05830-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

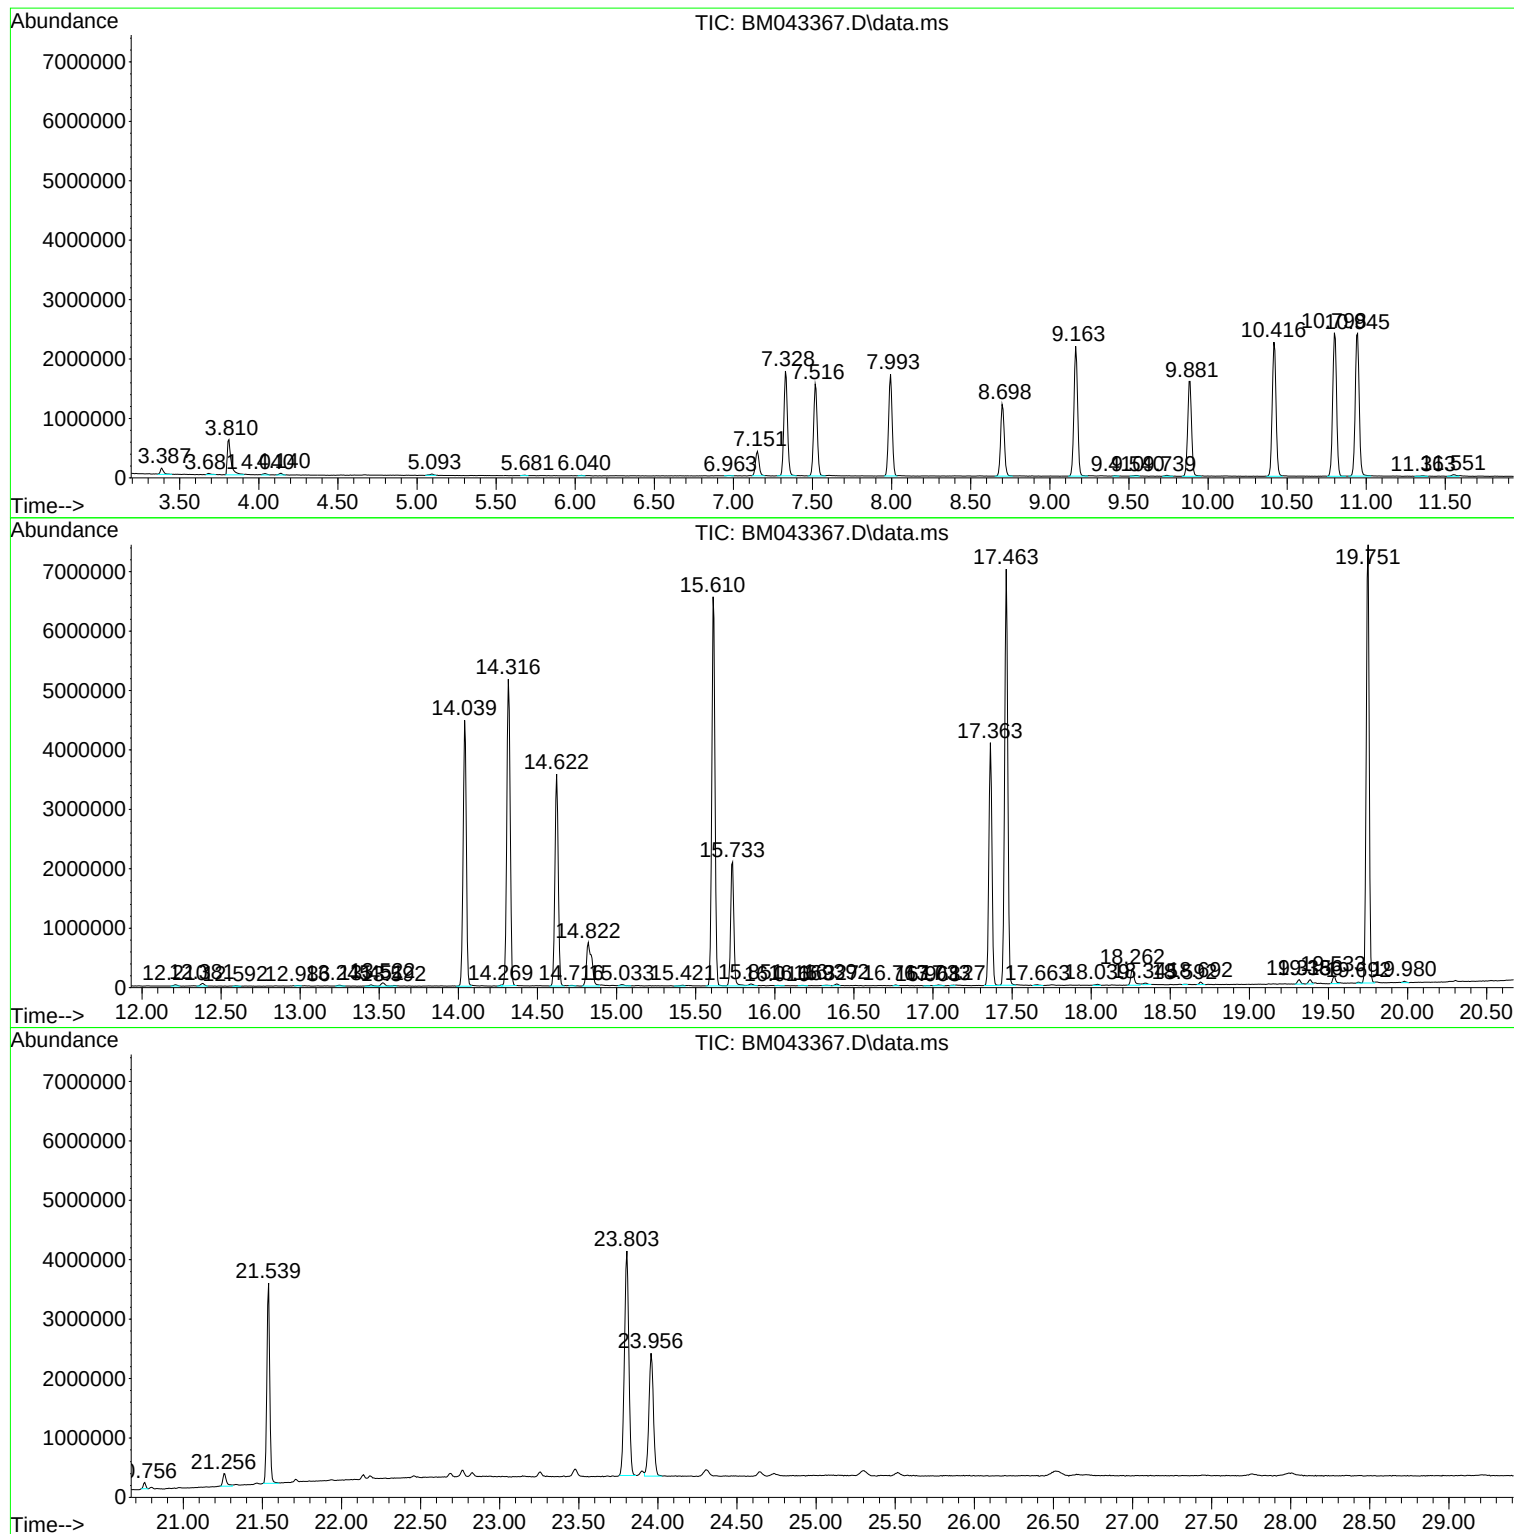

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043367.D
Acq On : 15 Dec 2023 20:48
Operator : MA/JU
Sample : 05830-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043367.D
Acq On : 15 Dec 2023 20:48
Operator : MA/JU
Sample : 05830-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc