

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043378.D
 Acq On : 16 Dec 2023 03:27
 Operator : MA/JU
 Sample : 05794-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	45	rVB	115920	165685	1.68%	0.144%
2	3.687	81	85	91	rBV	18848	31271	0.32%	0.027%
3	3.810	102	106	125	rBV	625251	976613	9.91%	0.852%
4	4.040	141	145	151	rVB	36850	54650	0.55%	0.048%
5	4.140	158	162	168	rVB	38321	53754	0.55%	0.047%
6	5.075	317	321	323	rBV2	17129	22975	0.23%	0.020%
7	6.981	638	645	651	rBV2	34791	70610	0.72%	0.062%
8	7.151	668	674	690	rVB	520259	852093	8.65%	0.743%
9	7.334	696	705	716	rBV	2066709	3289809	33.38%	2.869%
10	7.522	730	737	747	rBV	1943295	3079760	31.25%	2.686%
11	7.604	747	751	755	rVB3	12430	15014	0.15%	0.013%
12	7.992	808	817	825	rBV	2022691	3315707	33.65%	2.891%
13	8.051	825	827	834	rVB8	9386	13987	0.14%	0.012%
14	8.563	909	914	920	rBV4	19197	33849	0.34%	0.030%
15	8.704	931	938	950	rBV	1541335	2459814	24.96%	2.145%
16	9.169	1009	1017	1026	rBV	2508487	4186997	42.49%	3.651%
17	9.263	1029	1033	1039	rVB7	15325	26683	0.27%	0.023%
18	9.492	1065	1072	1079	rBV	114660	205017	2.08%	0.179%
19	9.886	1126	1139	1151	rBV	2001513	3360122	34.10%	2.930%
20	10.027	1157	1163	1172	rVB8	14438	35094	0.36%	0.031%
21	10.110	1172	1177	1185	rBV	40573	72885	0.74%	0.064%
22	10.422	1222	1230	1239	rBV	2791282	4629944	46.98%	4.038%
23	10.592	1252	1259	1262	rBV9	8013	16595	0.17%	0.014%
24	10.804	1286	1295	1303	rBV	3017292	5012500	50.86%	4.371%
25	10.945	1311	1319	1333	rBV	2756381	4735683	48.05%	4.130%
26	11.345	1382	1387	1390	rBV7	6328	12020	0.12%	0.010%
27	11.592	1424	1429	1439	rBV2	57661	111783	1.13%	0.097%
28	12.292	1543	1548	1554	rBV10	9578	19975	0.20%	0.017%
29	12.386	1558	1564	1570	rVV	55256	93820	0.95%	0.082%
30	12.592	1594	1599	1604	rVV7	10692	16622	0.17%	0.014%
31	12.633	1604	1606	1612	rVB	8596	10559	0.11%	0.009%
32	12.910	1648	1653	1659	rVV6	16381	29629	0.30%	0.026%
33	12.986	1661	1666	1675	rVV	164990	266665	2.71%	0.233%
34	13.239	1704	1709	1715	rBV	148742	219527	2.23%	0.191%
35	13.527	1752	1758	1763	rBV	48605	86117	0.87%	0.075%
36	13.598	1766	1770	1777	rVV8	15317	26857	0.27%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
 Data File : BM043378.D
 Acq On : 16 Dec 2023 03:27
 Operator : MA/JU
 Sample : 05794-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	14.045	1839	1846	1854	rBV	4858216	6662259	67.60%	5.810%
38	14.104	1854	1856	1860	rVV5	18539	25093	0.25%	0.022%
39	14.151	1860	1864	1870	rVB6	32112	49056	0.50%	0.043%
40	14.274	1879	1885	1886	rBV2	28918	41041	0.42%	0.036%
41	14.321	1886	1893	1903	rVB2	5874869	8656472	87.84%	7.549%
42	14.445	1911	1914	1920	rVB7	9980	14249	0.14%	0.012%
43	14.510	1921	1925	1930	rVB7	16190	22739	0.23%	0.020%
44	14.586	1932	1938	1939	rBV	51229	74077	0.75%	0.065%
45	14.627	1939	1945	1955	rVV	4178046	6205275	62.97%	5.411%
46	14.721	1959	1961	1966	rVB5	11334	13106	0.13%	0.011%
47	14.821	1972	1978	1990	rBV	416487	661458	6.71%	0.577%
48	15.051	2010	2017	2023	rVB5	45478	99775	1.01%	0.087%
49	15.145	2027	2033	2035	rVB7	10764	16676	0.17%	0.015%
50	15.192	2039	2041	2045	rVB4	9094	10493	0.11%	0.009%
51	15.368	2067	2071	2075	rBV	49781	64490	0.65%	0.056%
52	15.421	2075	2080	2082	rVV	37389	54698	0.56%	0.048%
53	15.445	2082	2084	2088	rVB	22475	27310	0.28%	0.024%
54	15.615	2105	2113	2121	rBV	7101454	9854717	100.00%	8.594%
55	15.733	2127	2133	2146	rBV	1858219	2664530	27.04%	2.324%
56	15.857	2149	2154	2163	rVB5	35416	71683	0.73%	0.063%
57	16.180	2205	2209	2214	rVB8	21607	28694	0.29%	0.025%
58	16.398	2241	2246	2251	rVB3	41343	76981	0.78%	0.067%
59	16.509	2263	2265	2268	rVB3	14630	14874	0.15%	0.013%
60	17.133	2367	2371	2372	rBV4	17359	19973	0.20%	0.017%
61	17.368	2404	2411	2421	rBV	4186396	6021030	61.10%	5.251%
62	17.468	2421	2428	2437	rVV	6941218	9570116	97.11%	8.346%
63	17.598	2447	2450	2455	rBV4	14429	30351	0.31%	0.026%
64	17.656	2457	2460	2466	rVB	57905	79997	0.81%	0.070%
65	18.262	2558	2563	2571	rBV2	121842	201450	2.04%	0.176%
66	18.339	2573	2576	2581	rVB	51046	72143	0.73%	0.063%
67	18.456	2594	2596	2602	rVB3	17790	25244	0.26%	0.022%
68	19.121	2705	2709	2713	rBV	96159	136951	1.39%	0.119%
69	19.315	2738	2742	2749	rBV	76486	113872	1.16%	0.099%
70	19.386	2750	2754	2758	rBV	62281	84882	0.86%	0.074%
71	19.539	2776	2780	2783	rBV3	58059	78831	0.80%	0.069%
72	19.750	2810	2816	2822	rBV	6461425	8622720	87.50%	7.519%
73	21.538	3115	3120	3129	rVB	3350737	4458659	45.24%	3.888%
74	23.803	3498	3505	3514	rVB2	3824911	7559356	76.71%	6.592%
75	23.956	3525	3531	3542	rVB	2249697	4576463	46.44%	3.991%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043378.D
Acq On : 16 Dec 2023 03:27
Operator : MA/JU
Sample : 05794-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 114672469

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043378.D
Acq On : 16 Dec 2023 03:27
Operator : MA/JU
Sample : 05794-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

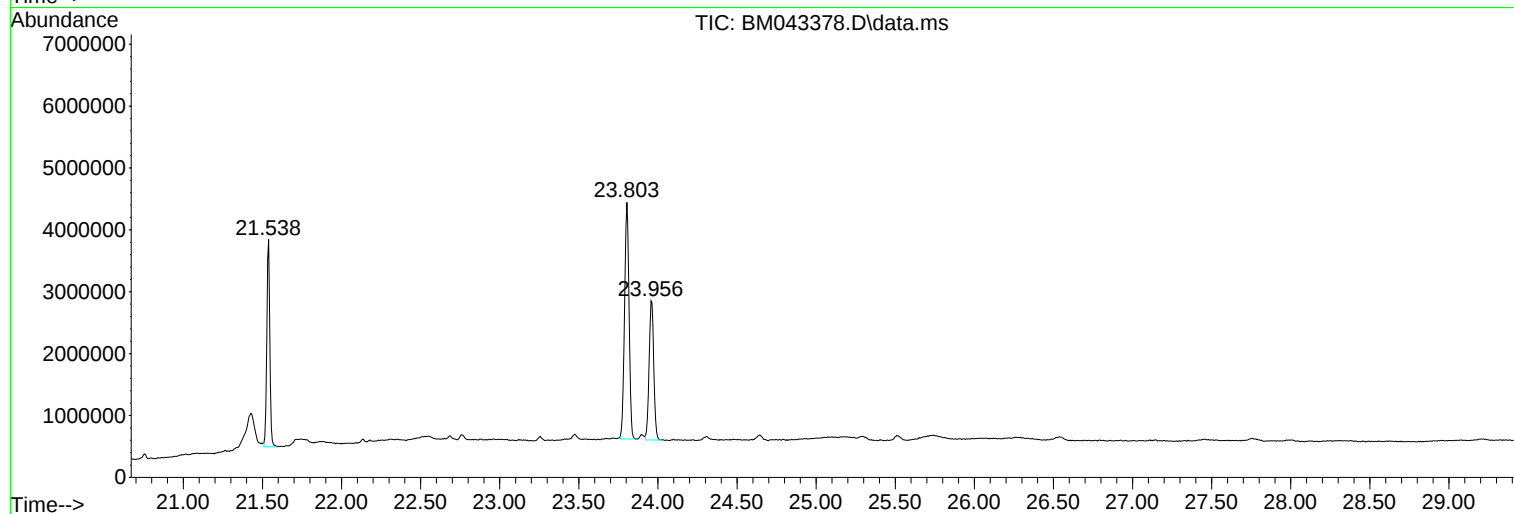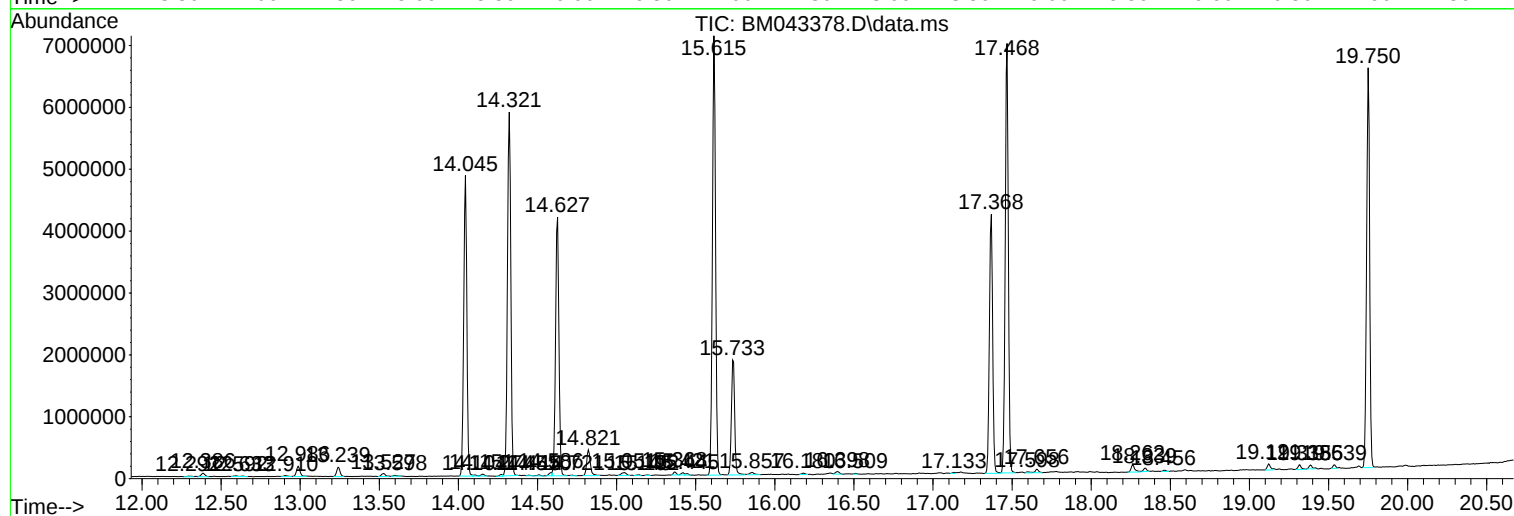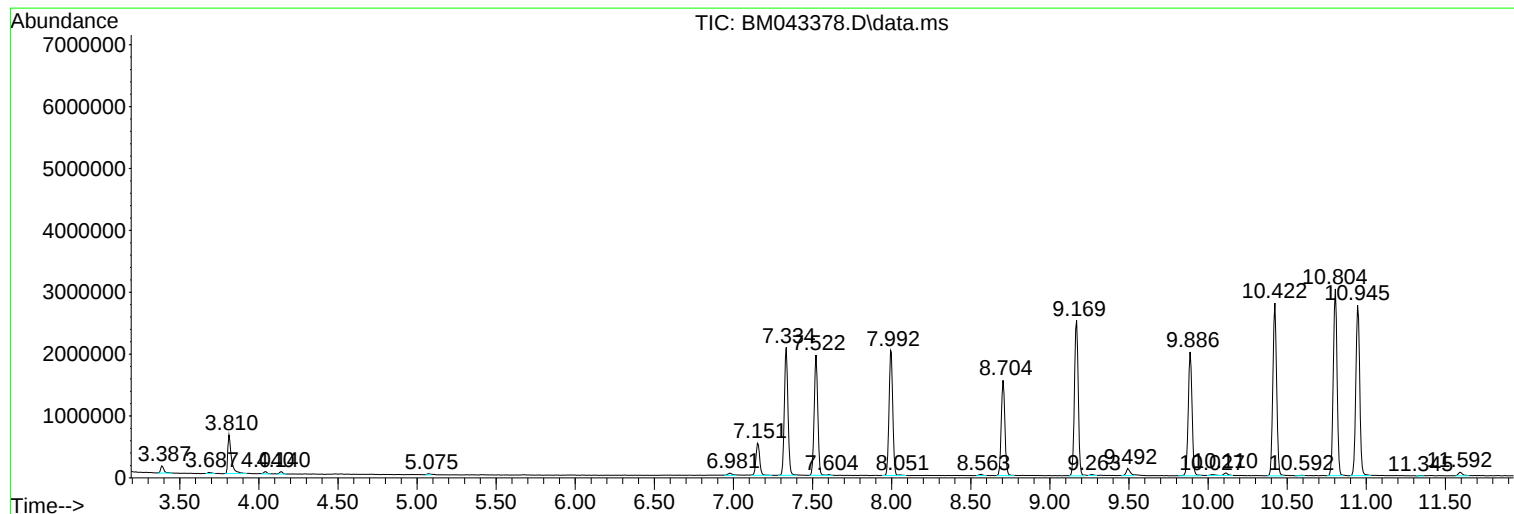

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043378.D
Acq On : 16 Dec 2023 03:27
Operator : MA/JU
Sample : 05794-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121523\
Data File : BM043378.D
Acq On : 16 Dec 2023 03:27
Operator : MA/JU
Sample : 05794-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc