

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:07:32 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

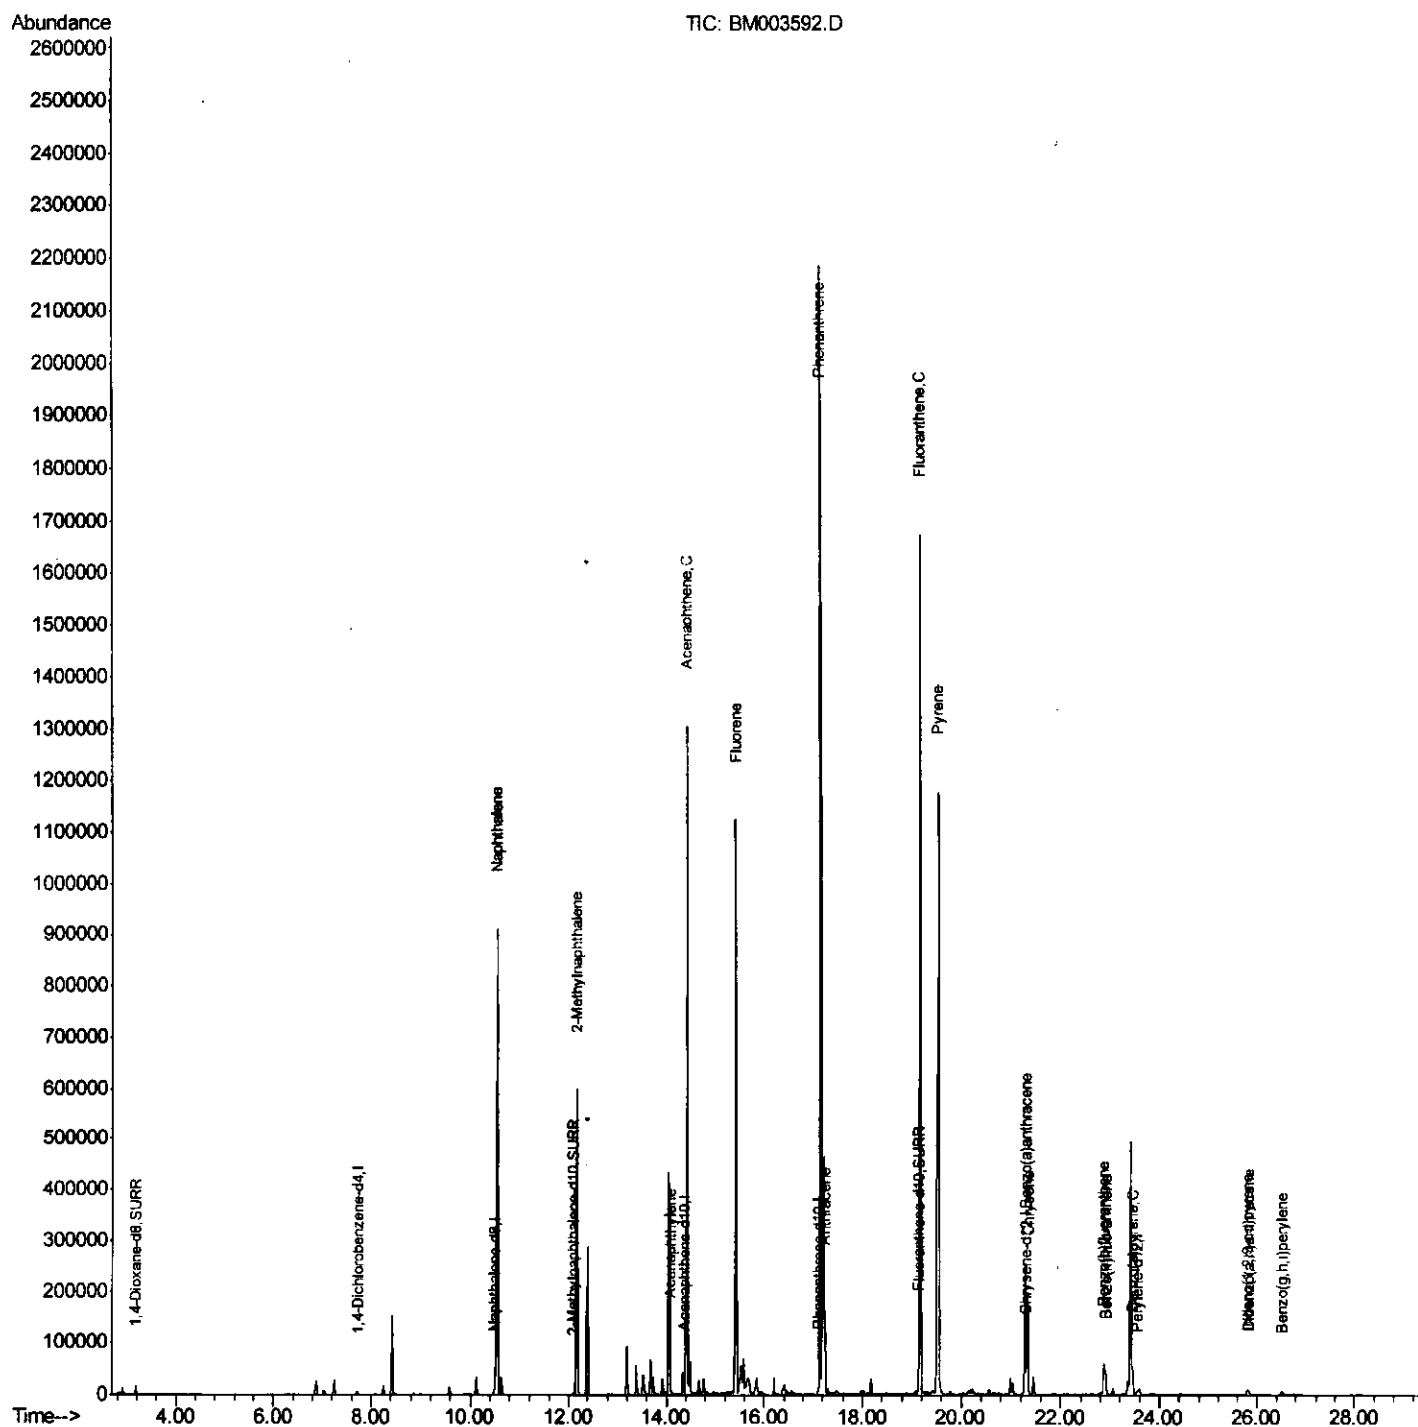

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121515\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/I2
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 03:03:24 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

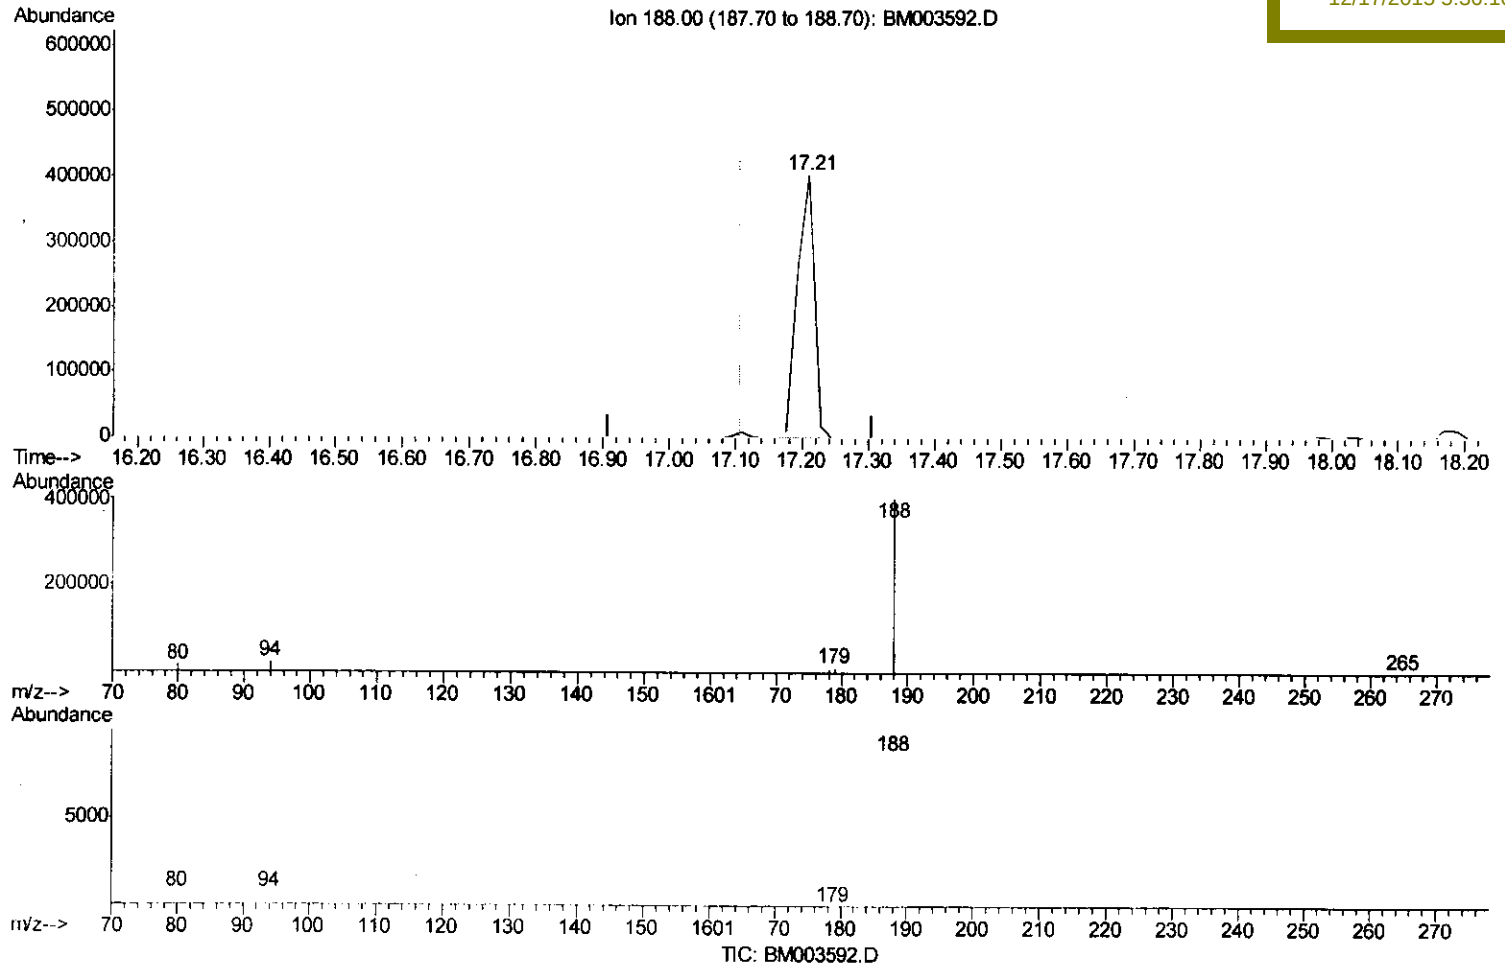

(12) Phenanthrene-d10 (I)

17.210min (+0.103) 0.40ng/ul

response 709852

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	5.75#
80.00	11.90	3.96#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 03:03:24 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

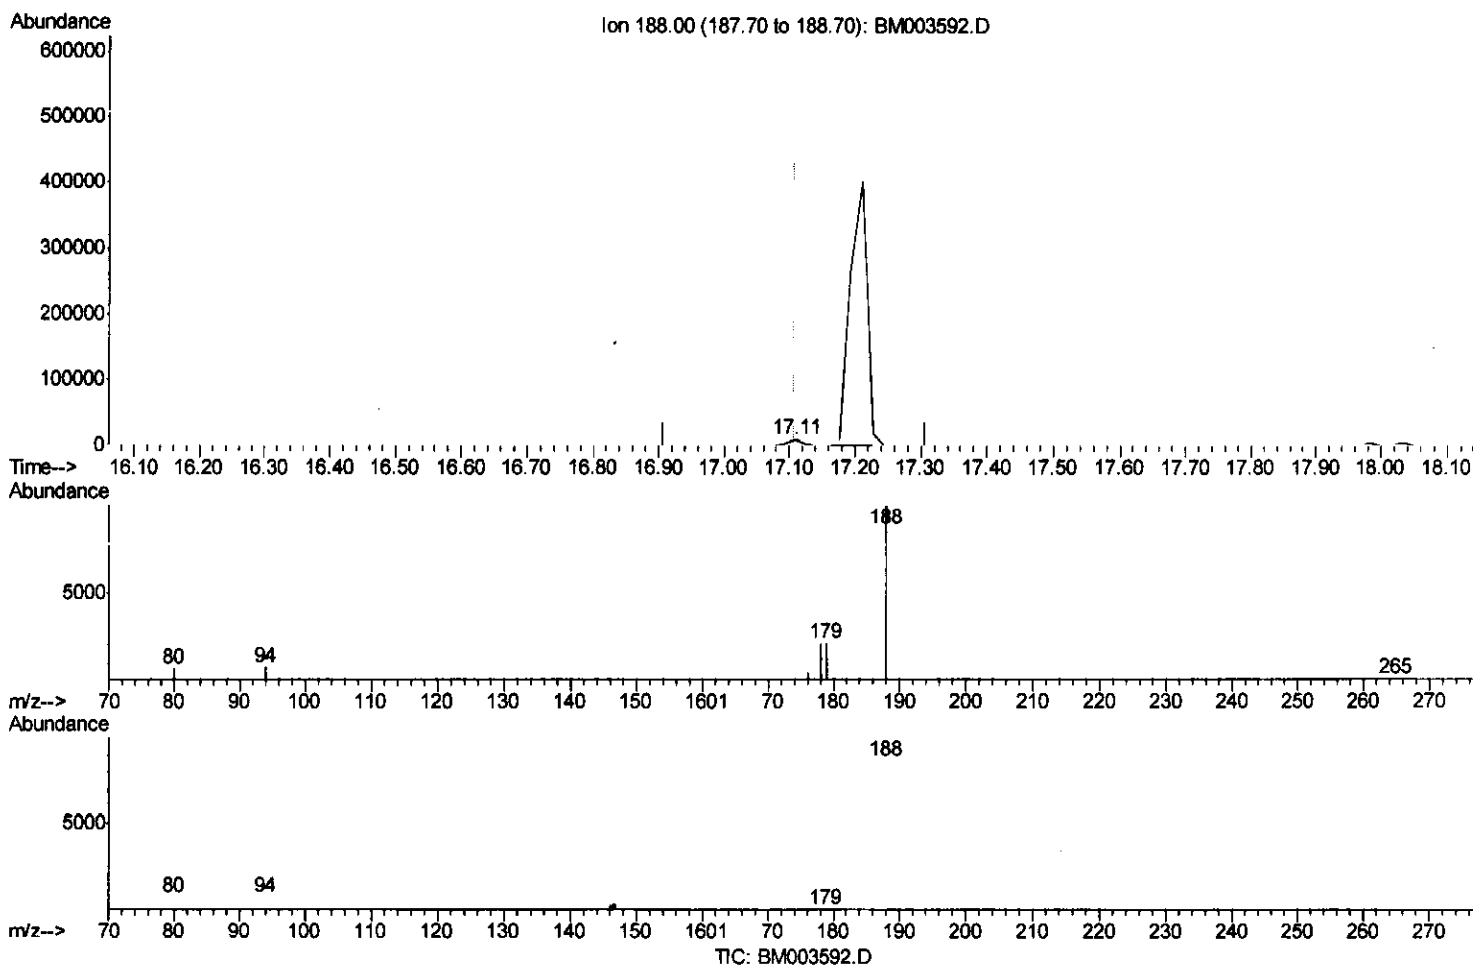

(12) Phenanthrene-d10 (I)

17.108min (0.000) 0.40ng/ul m

response 14777

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.81#
80.00	11.90	7.22#
0.00	0.00	0.00

U.M
 12/18/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 03:03:24 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

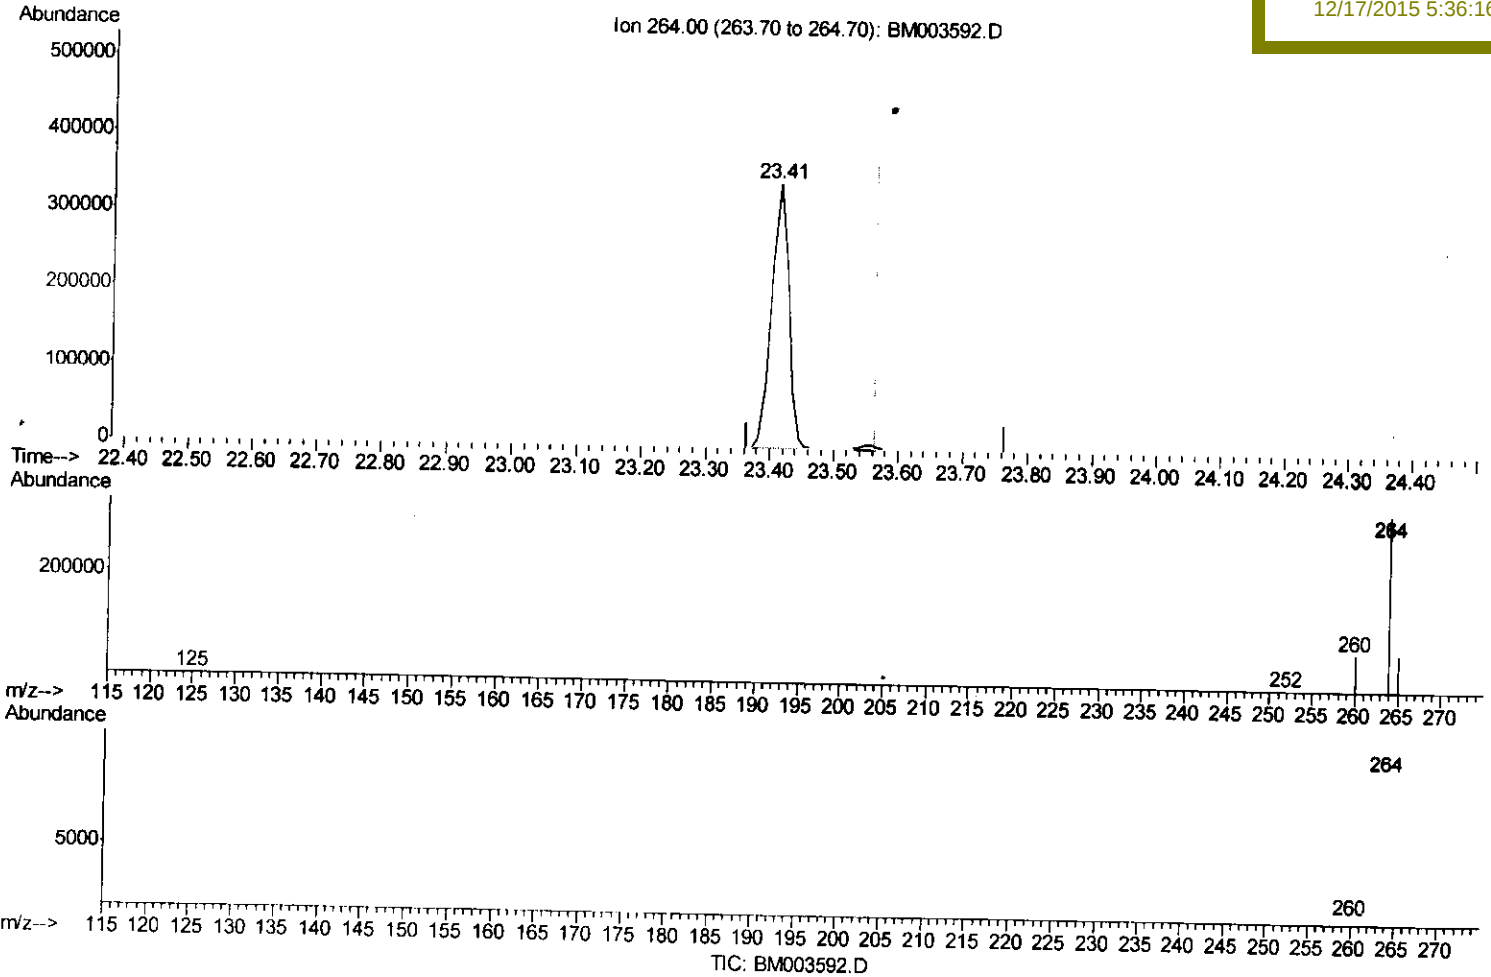

(22) Perylene-d12 (I)

23.413min (-0.153) 0.40ng/ui

response 619243

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	21.29
265.00	38.20	21.54#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 03:03:24 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

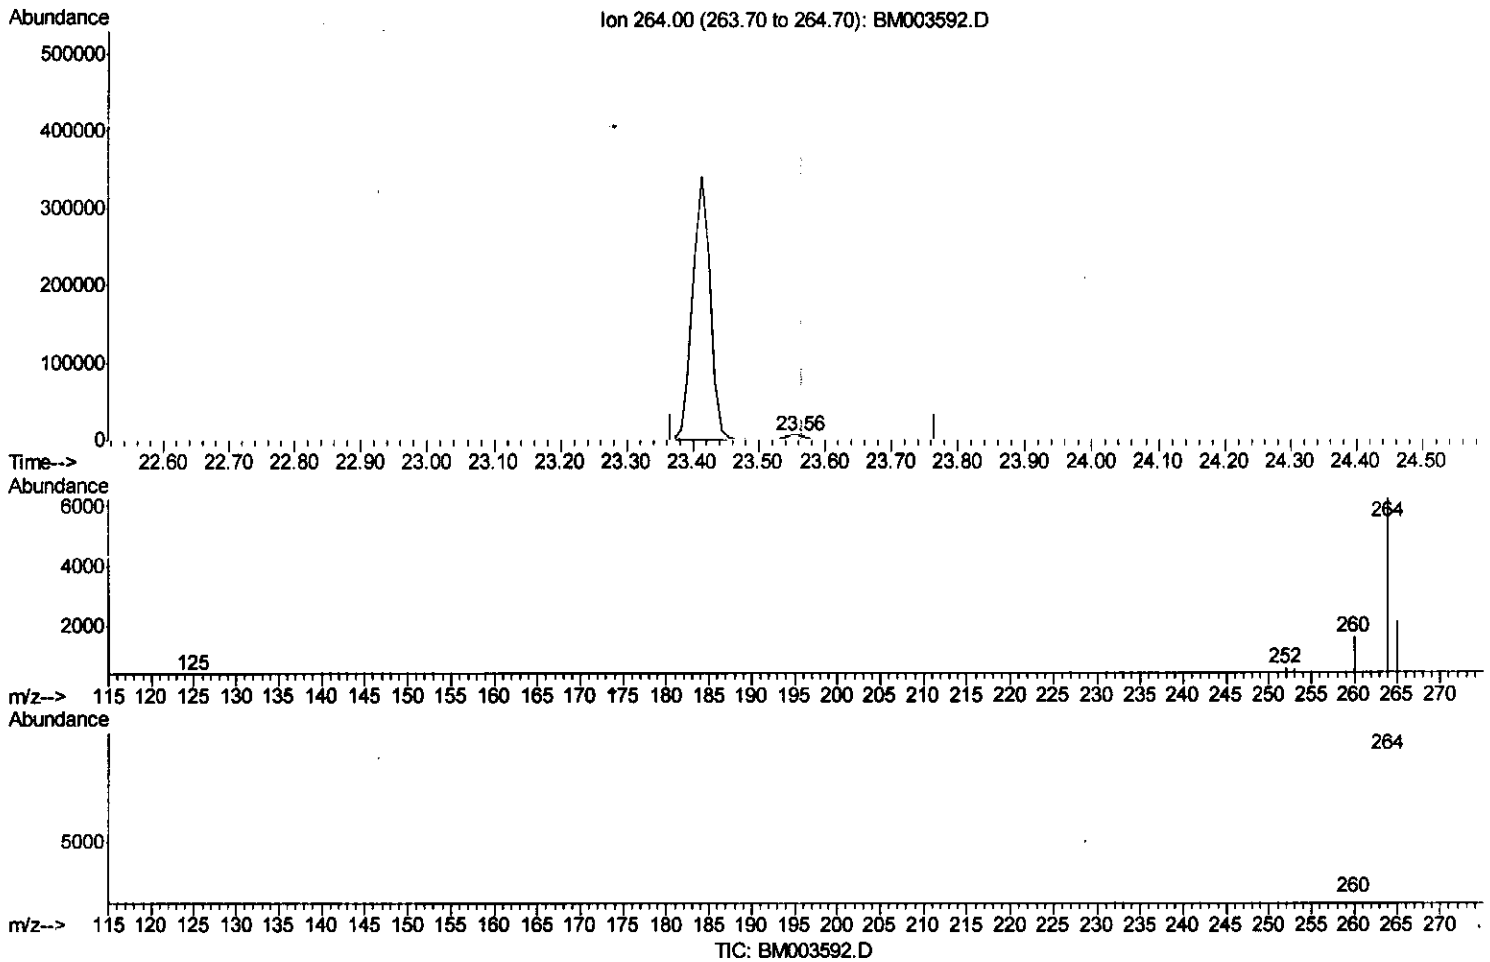

(22) Perylene-d12 (I)

23.559min (-0.007) 0.40ng/ul m

response 13753

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	25.78
265.00	38.20	34.36
0.00	0.00	0.00

U, M
 12/18/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

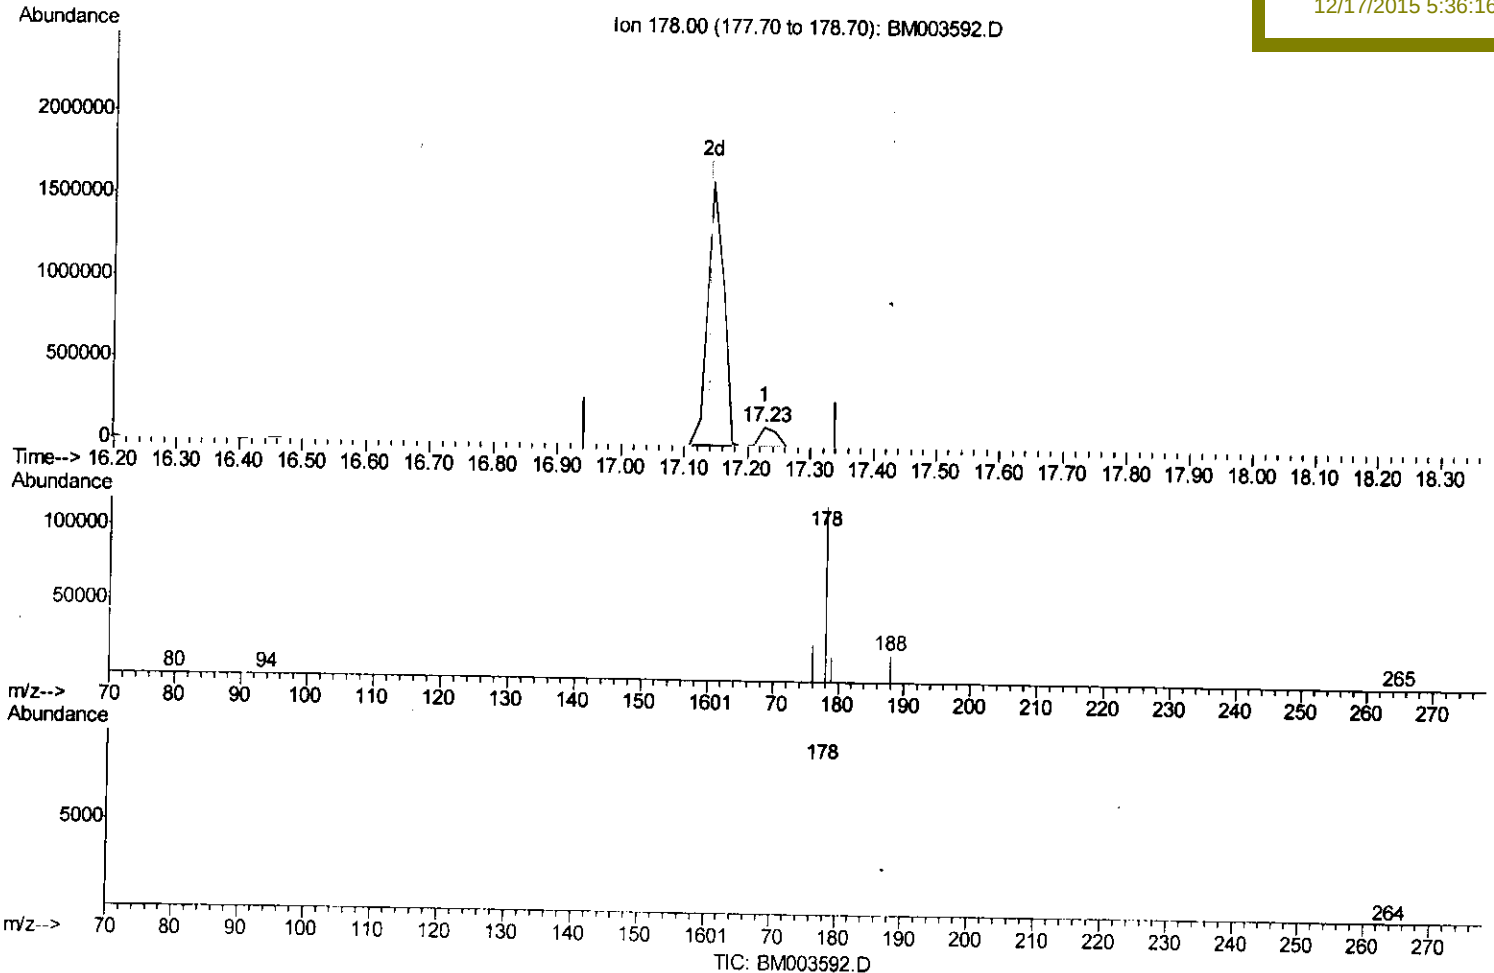

(14) Phenanthrene

17.228min (+0.086) 6.00ng/ul

response 228706

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	21.25#
179.00	17.70	14.75
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-STM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

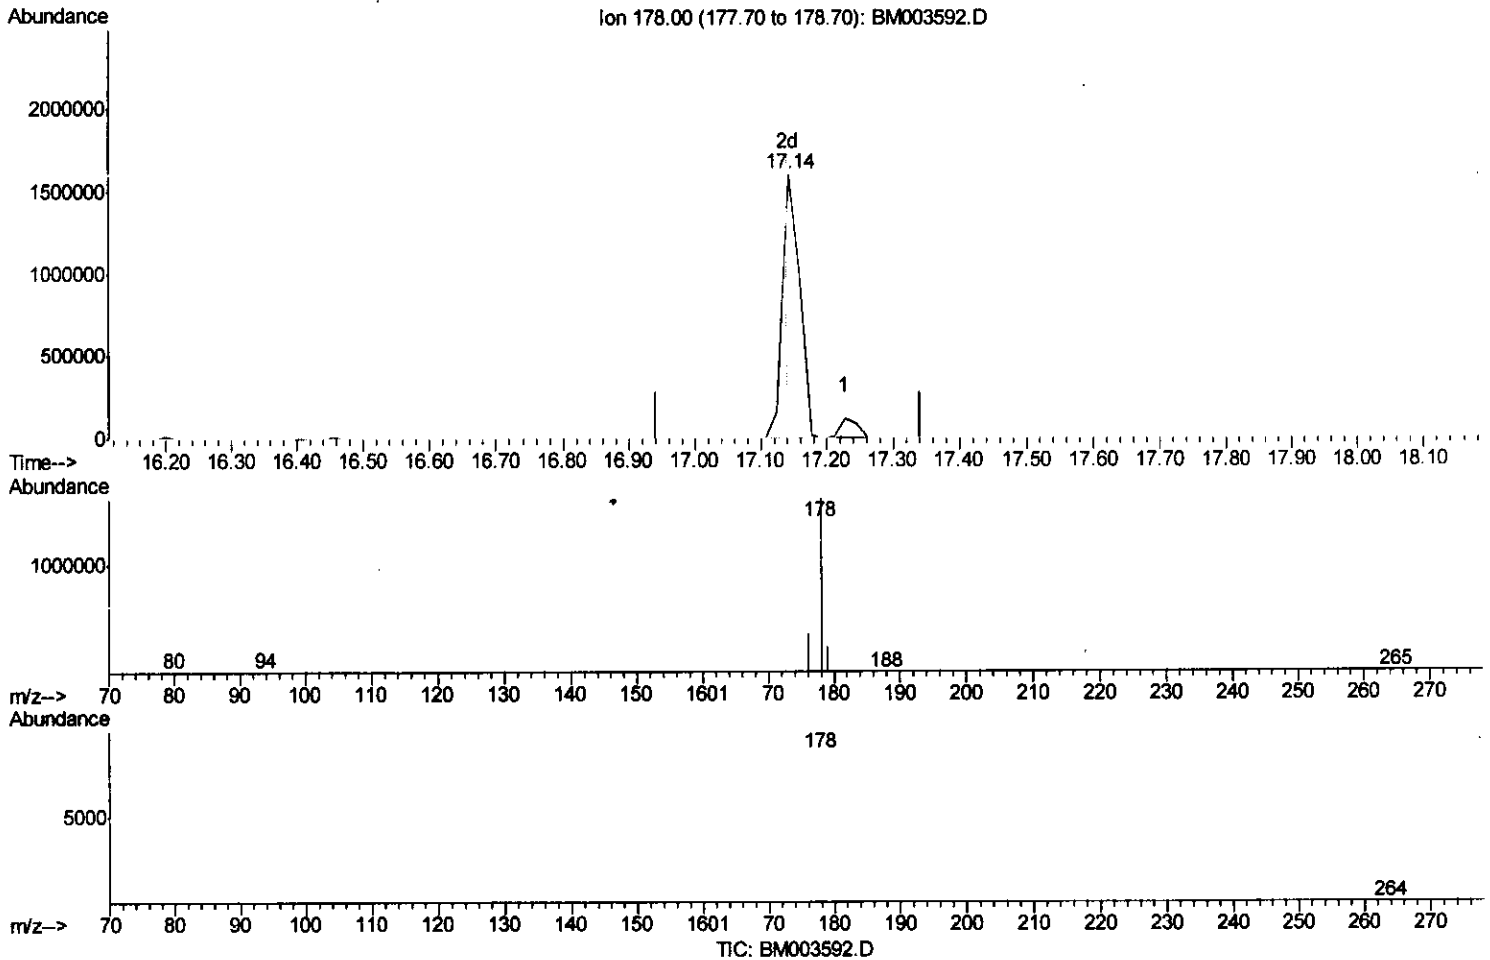

(14) Phenanthrene

17.142min (0.000) 74.69ng/ul m U.M

response 2846750

12/18/15

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	21.75#
179.00	17.70	14.61
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

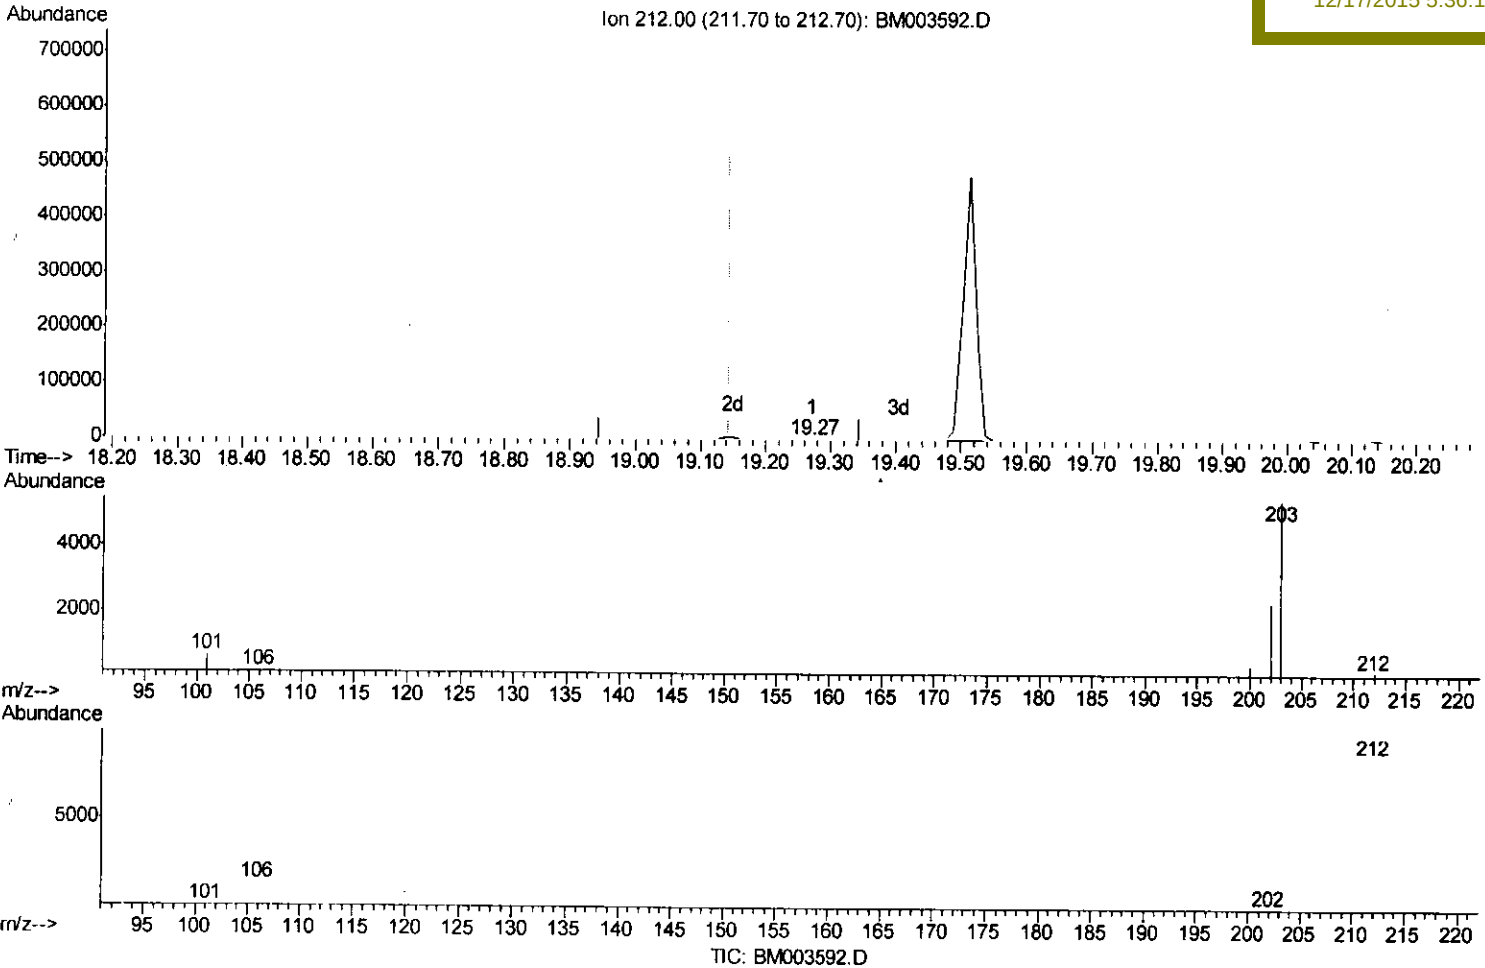

(16) Fluoranthene-d10 (SURR)

19.271min (+0.126) 0.01ng/ul

response 240

Ion	Exp%	Act%
212.00	100	100
106.00	0.00	0.00
104.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

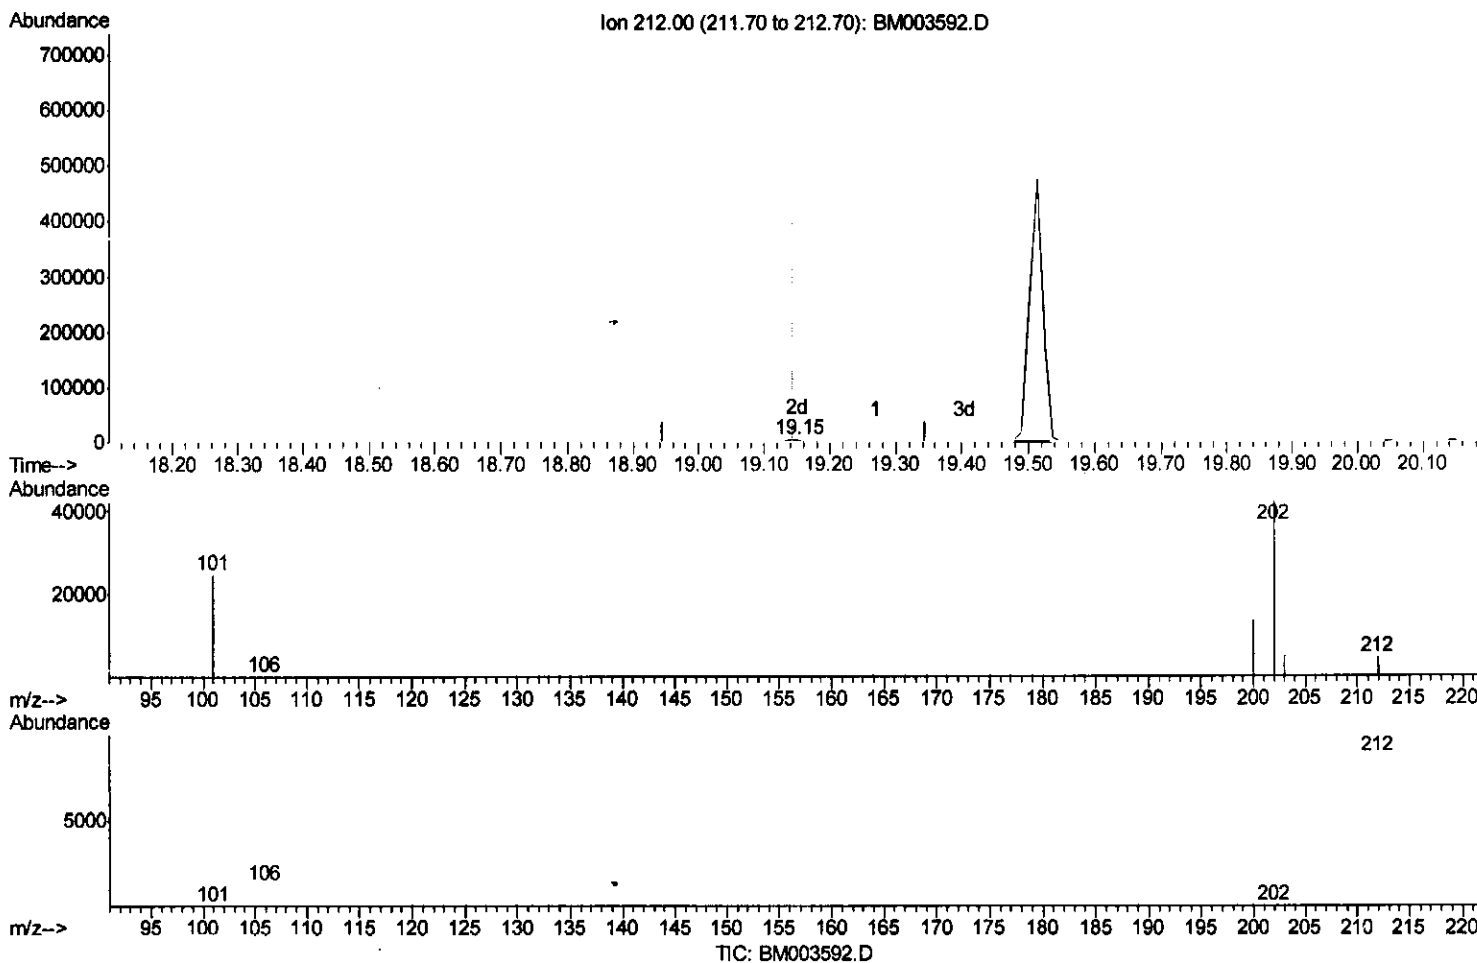

(16) Fluoranthene-d10 (SURR)

19.150min (+0.005) 0.27ng/ul m

response 8612

Ion	Exp%	Act%
212.00	100	100
106.00	0.00	0.00
104.00	0.00	0.00
0.00	0.00	0.00

U.M
 12/18/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

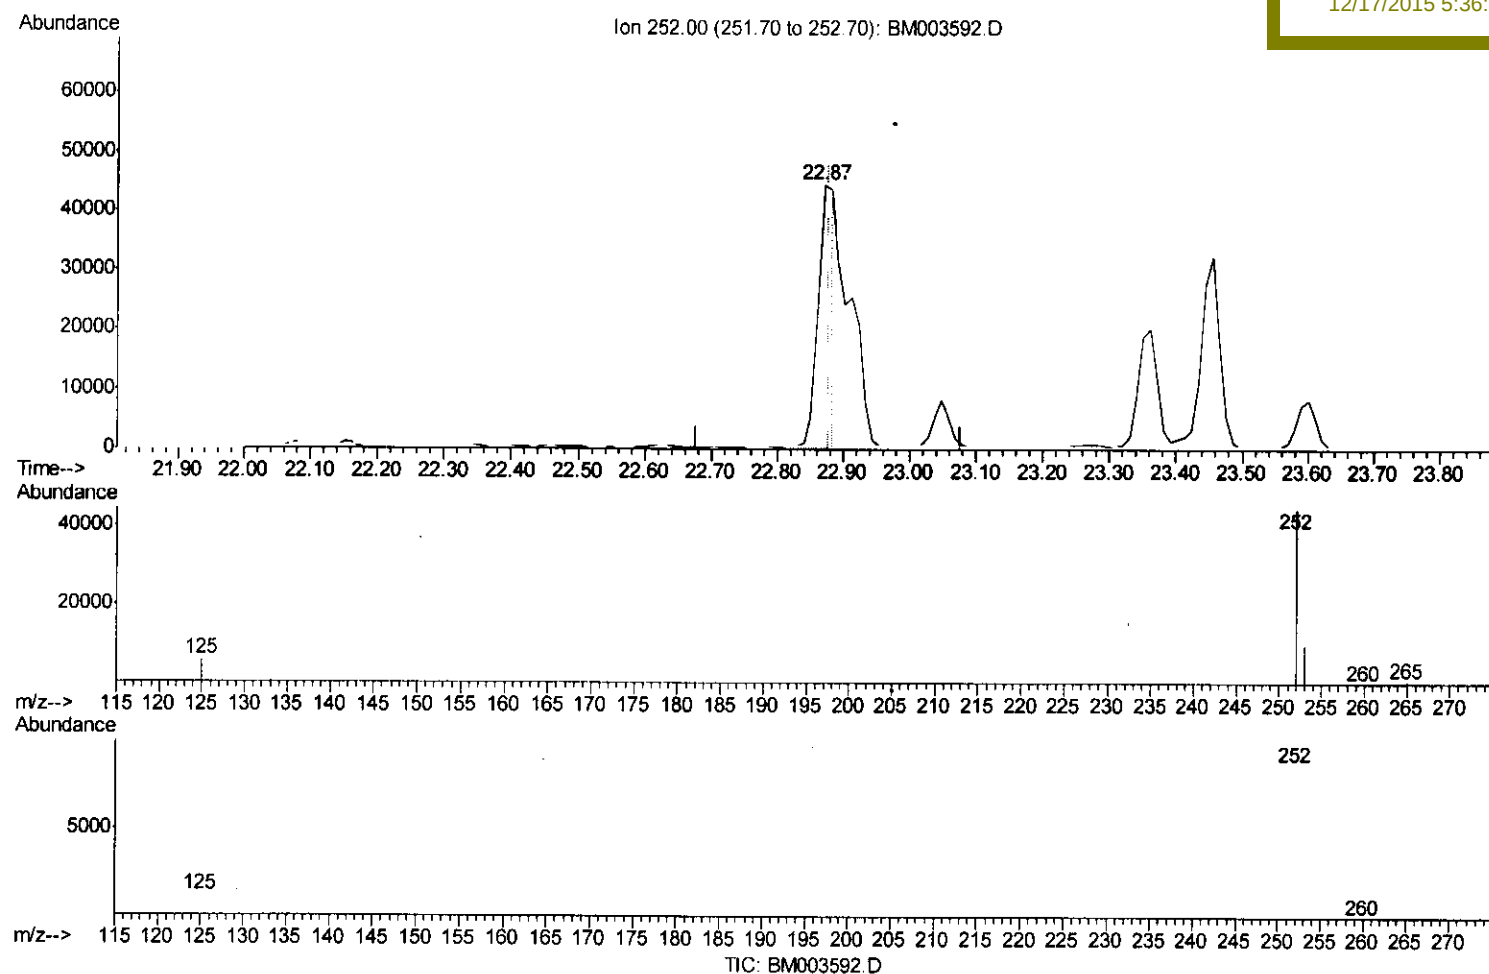

(23) Benzo(b)fluoranthene

22.871min (-0.007) 1.54ng/ul

response 72222

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	22.05
125.00	14.40	12.77
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

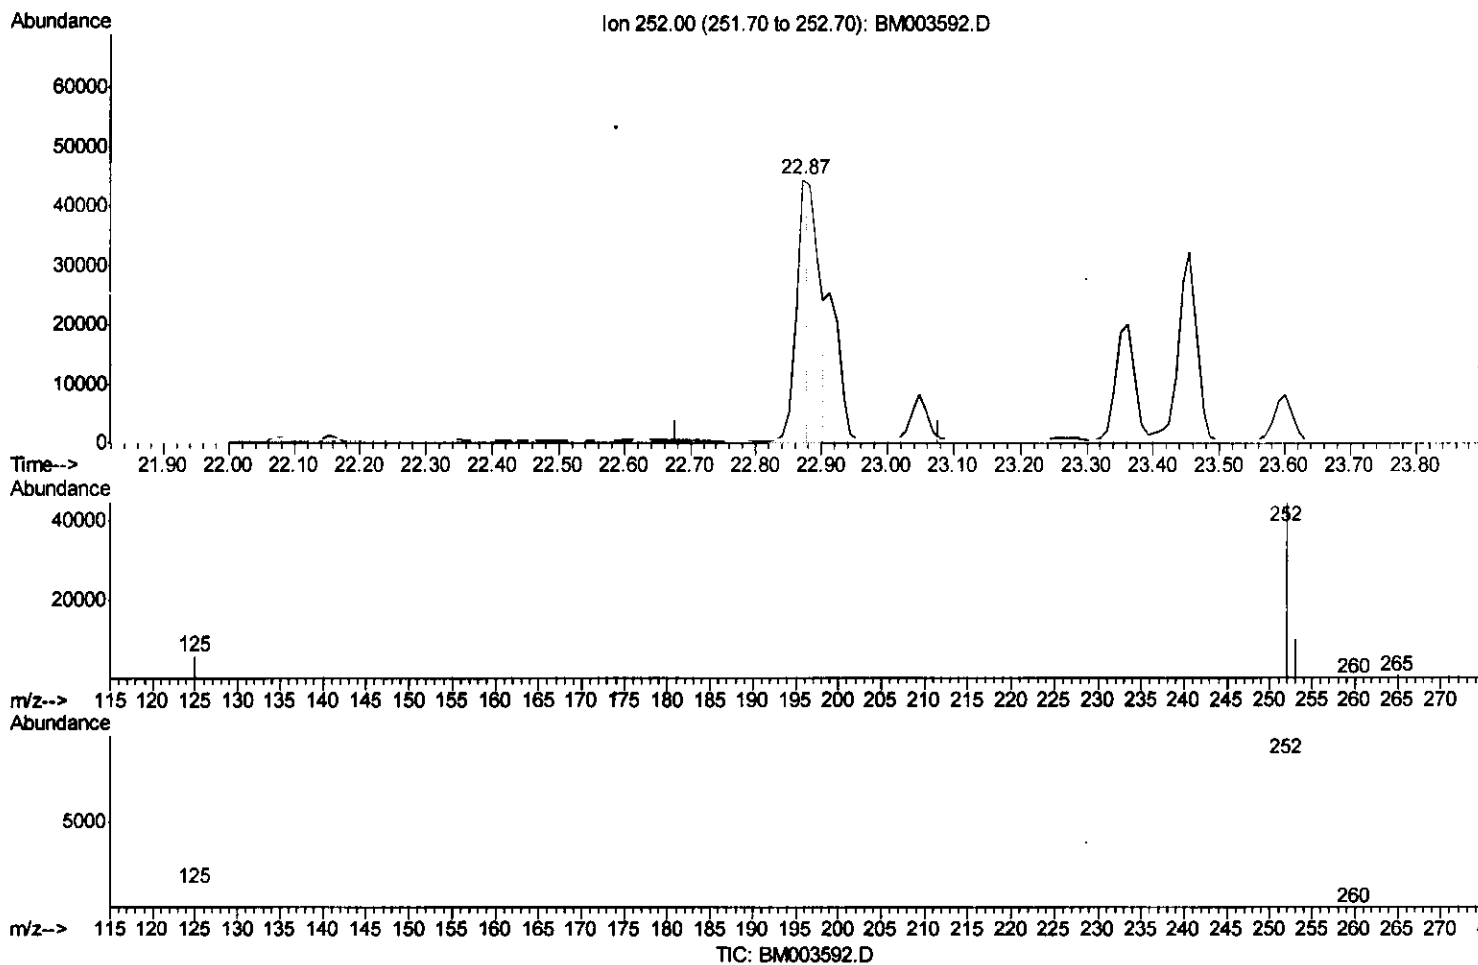

(23) Benzo(b)fluoranthene

22.871min (-0.007) 2.32ng/ul m

response 108740

UM
 12/18/15

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	22.05
125.00	14.40	12.77
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

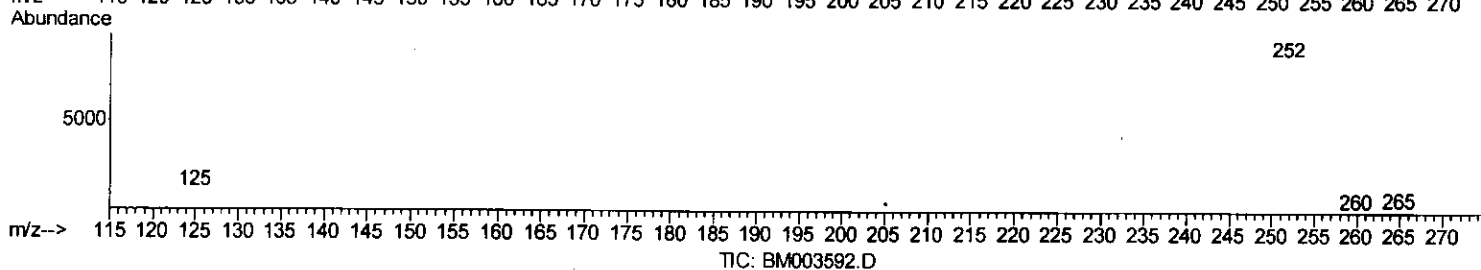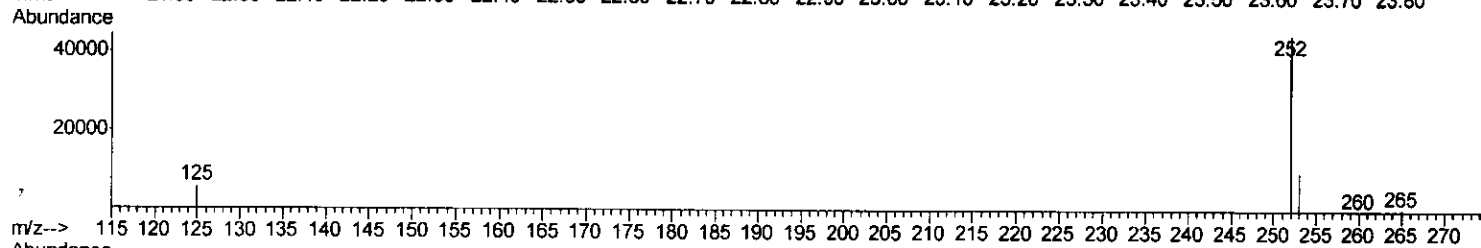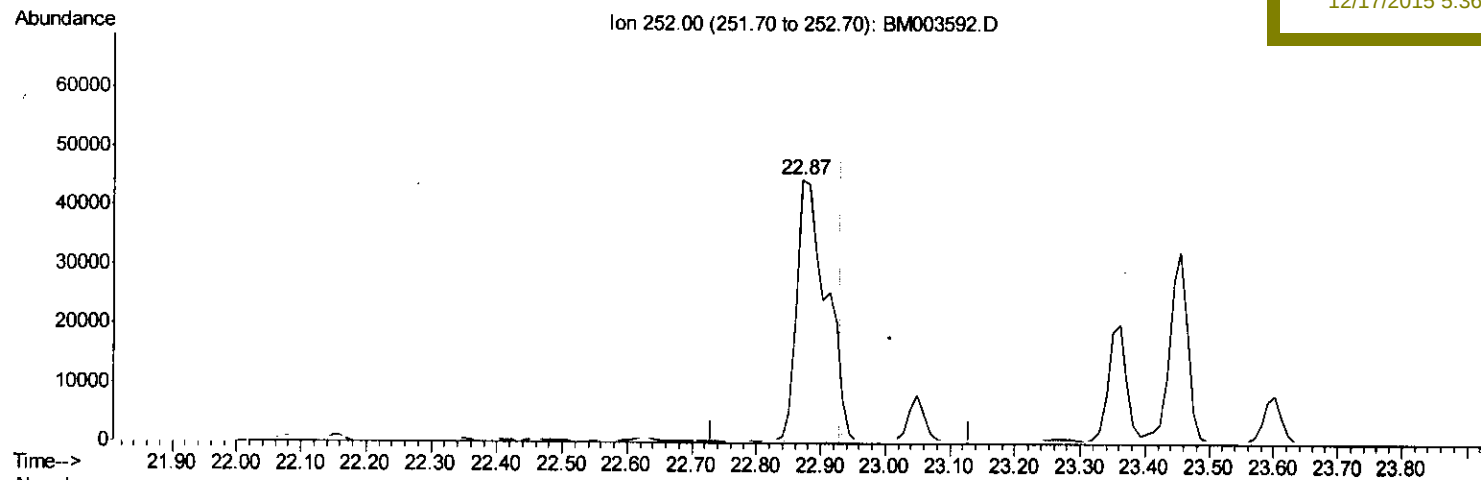

(24) Benzo(k)fluoranthene

22.871min (-0.059) 3.28ng/ul

response 139443

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	22.05
125.00	13.00	12.77
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR +5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

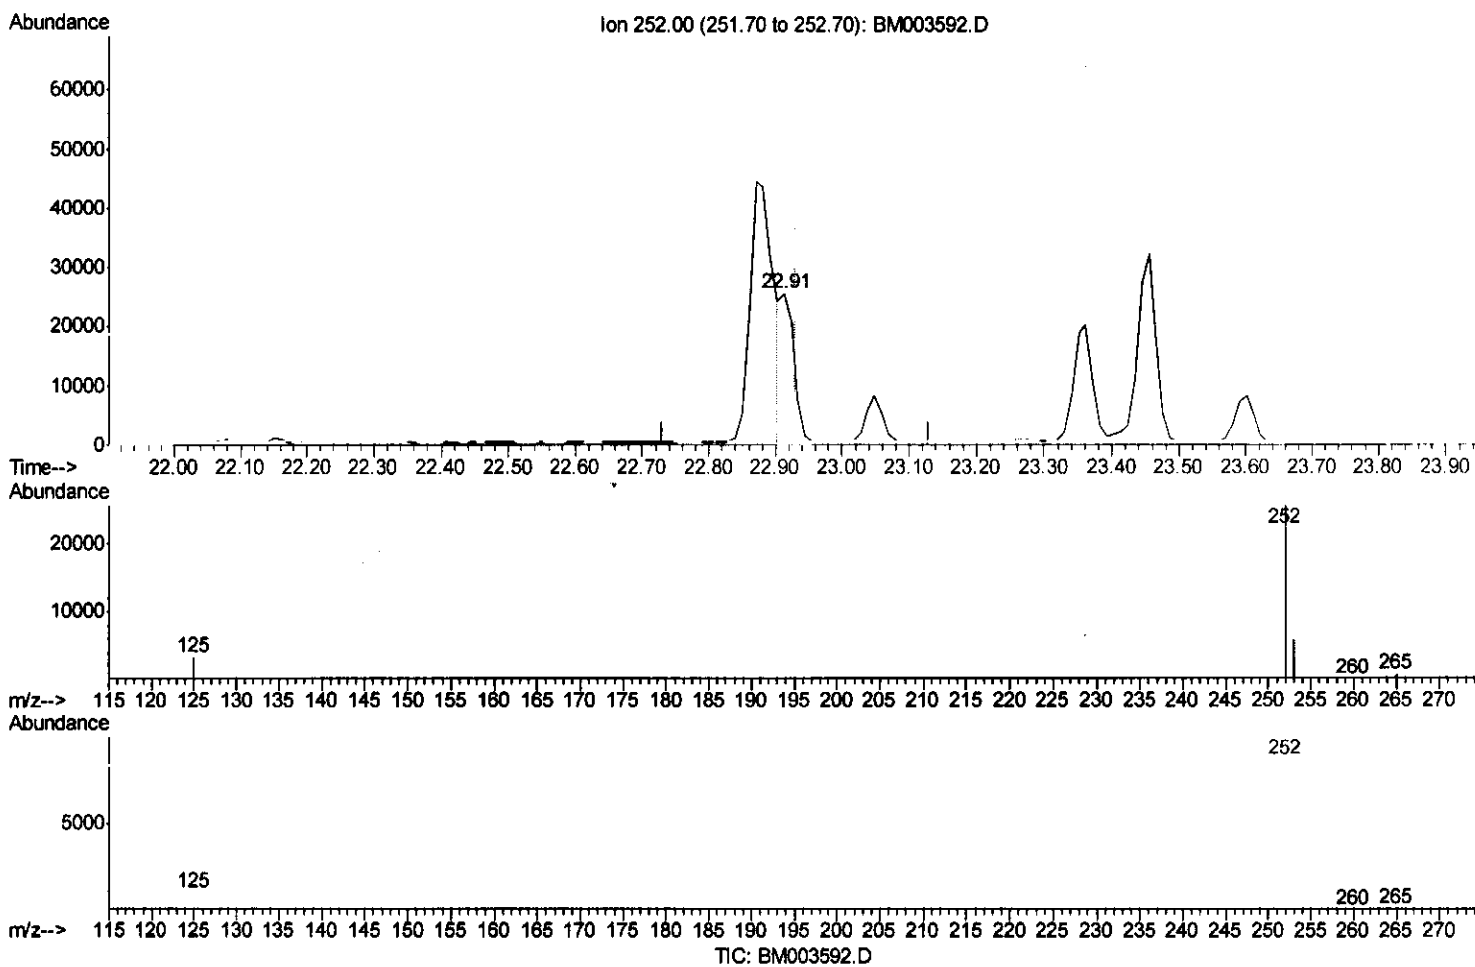

(24) Benzo(k)fluoranthene

22.913min (-0.017) 0.83ng/ul m

response 35116

Ion Exp% Act%

252.00	100	100
253.00	24.80	23.32
125.00	13.00	13.01
0.00	0.00	0.00

U.M
 12/18/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

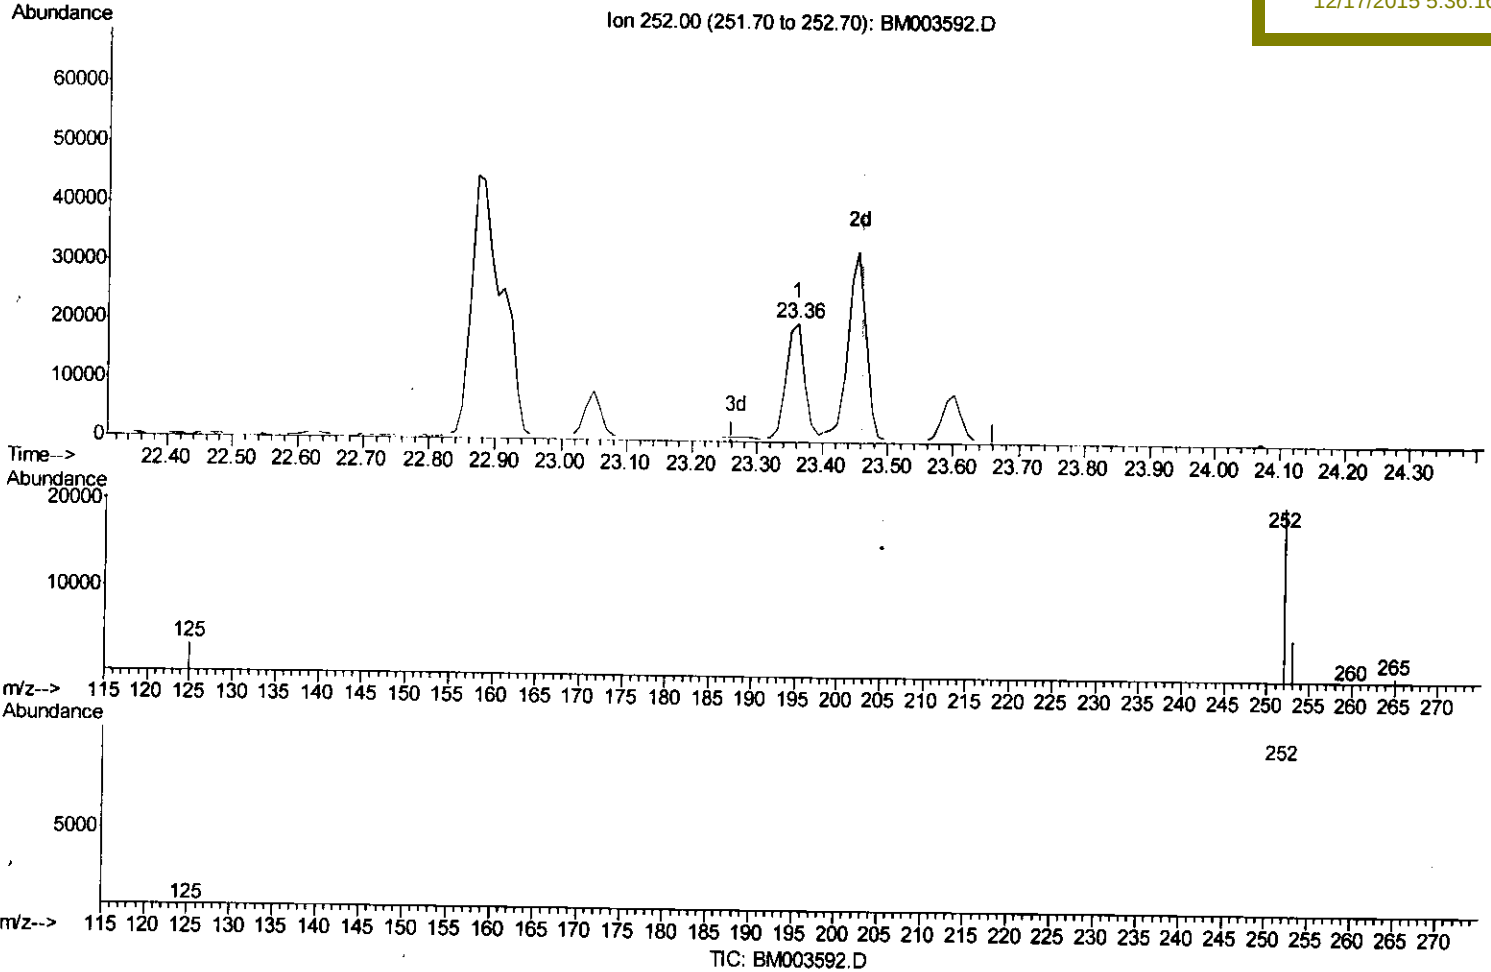

(25) Benzo(a)pyrene (C)

23.361min (-0.101) 1.00ng/ul

response 39534

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	24.45
125.00	15.90	16.66
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

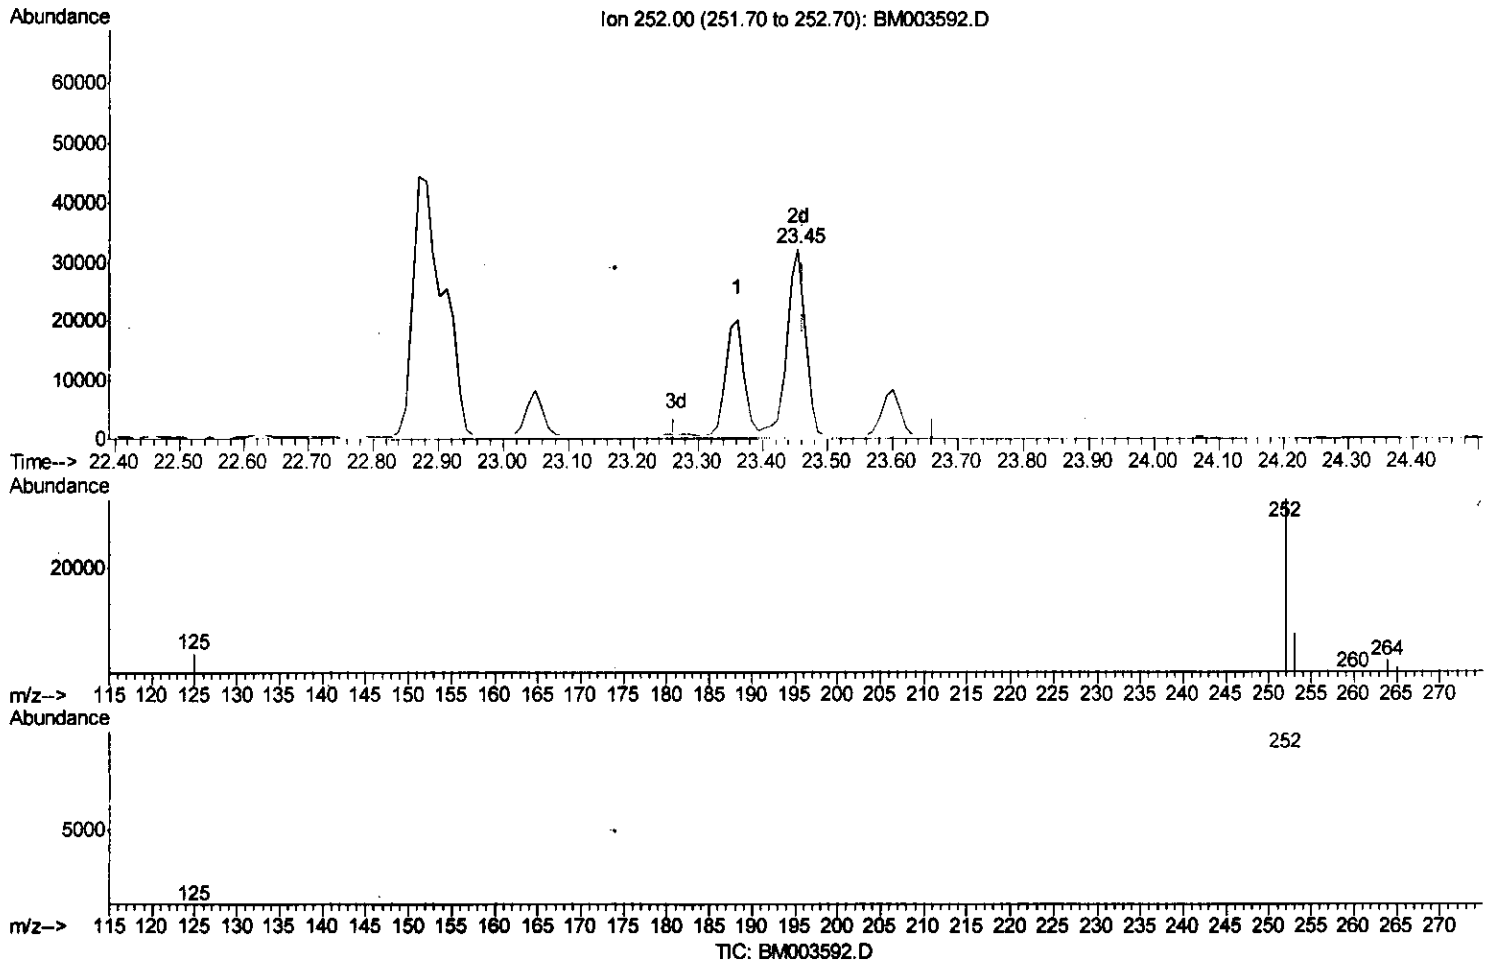

(25) Benzo(a)pyrene (C)

23.455min (-0.007) 1.65ng/ul m

response 65424

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.91
125.00	15.90	12.84
0.00	0.00	0.00

U.M
 12/18/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
Data File : BM003592.D
Acq On : 16 Dec 2015 23:55
Operator : UM/IZ
Sample : G4767-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample ID :
D9N38

Quant Time: Dec 17 08:05:22 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 02:56:38 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMdadoda
12/17/2015 5:36:16 PM

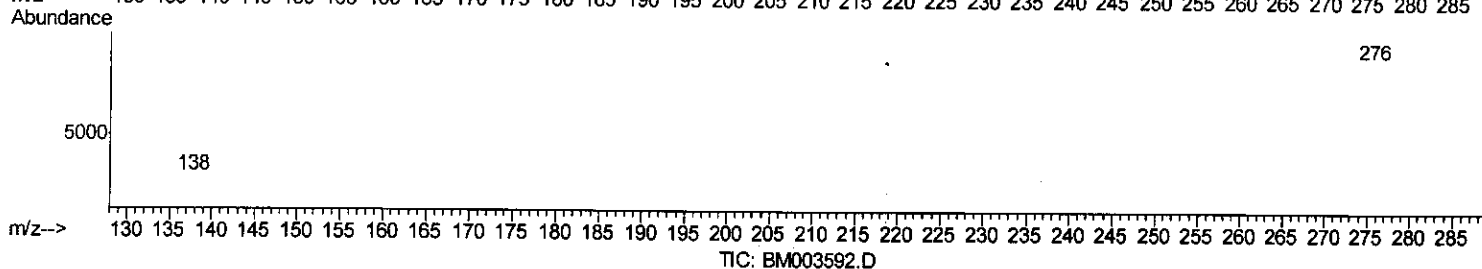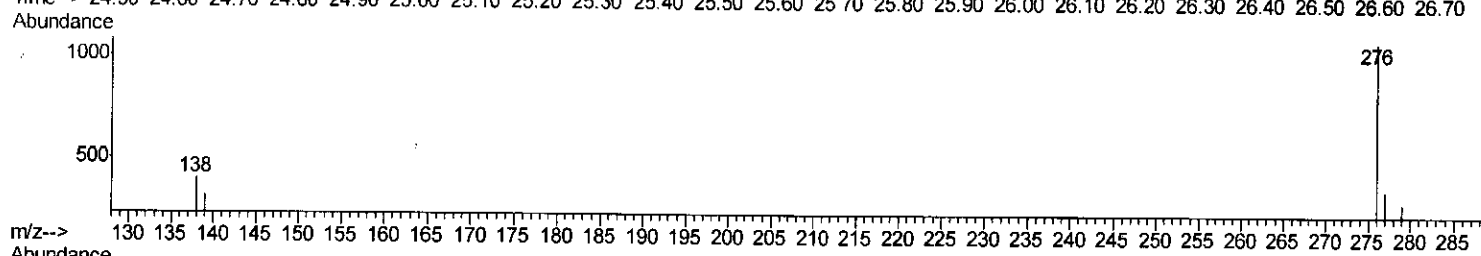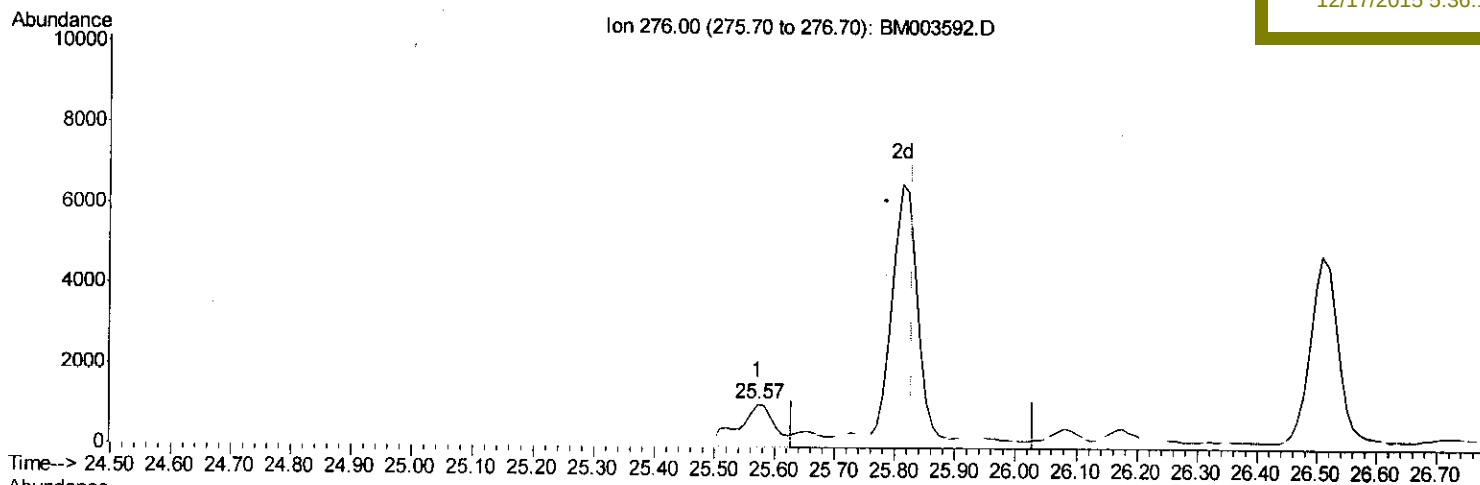

(26) Indeno(1,2,3-cd)pyrene

25.571min (-0.257) 0.10ng/ul

response 4529

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	0.00#
277.00	24.80	21.31
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

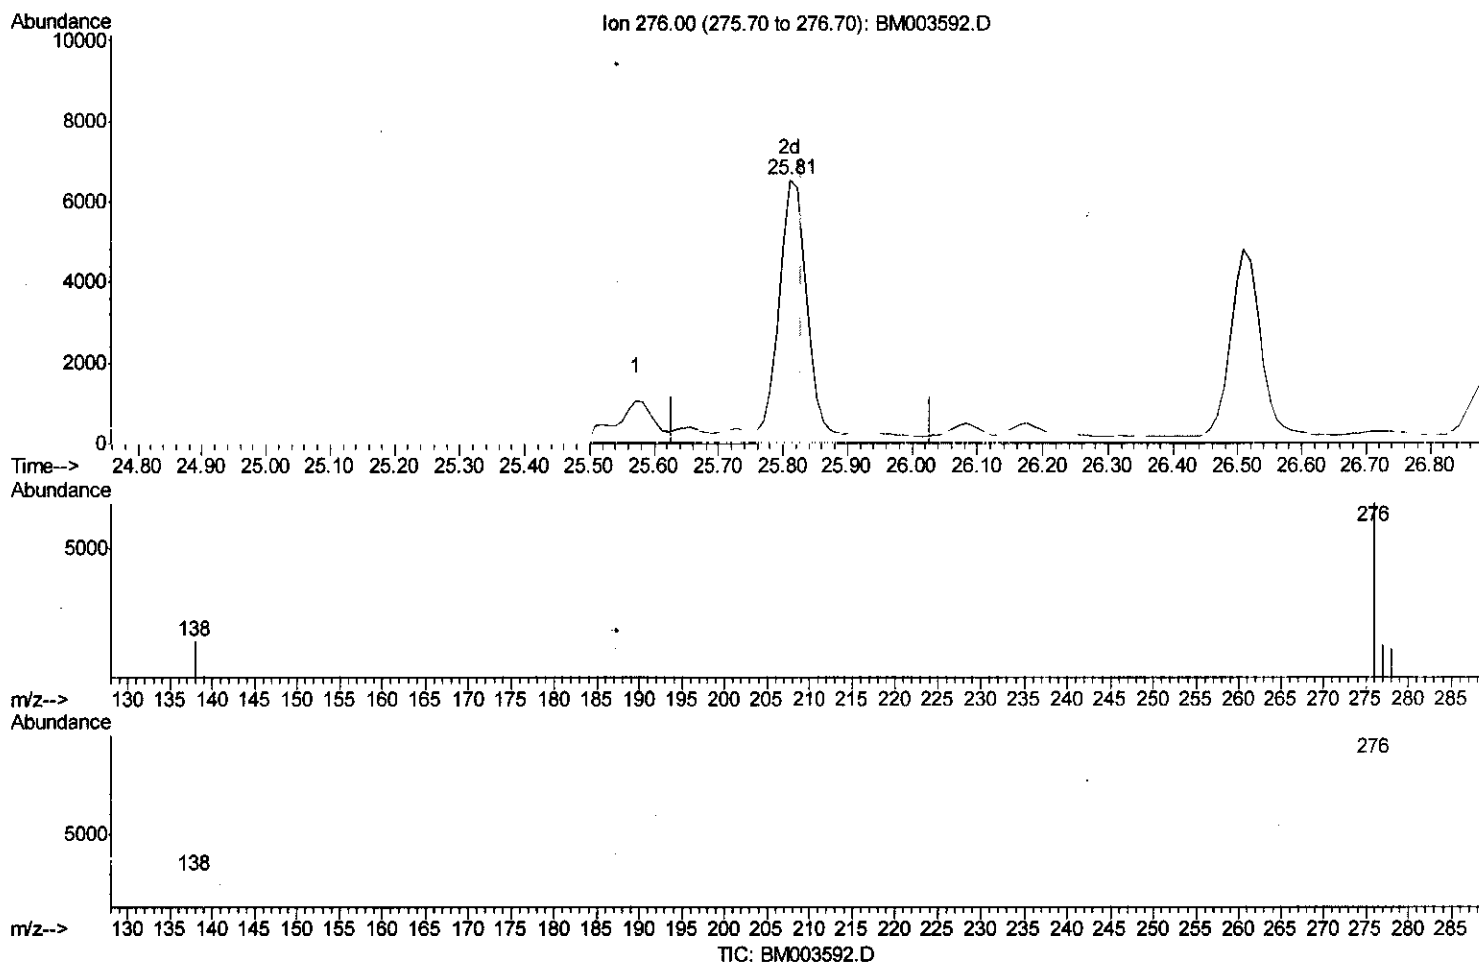

(26) Indeno(1,2,3-cd)pyrene

25.811min (-0.017) 0.43ng/ul m

response 19827

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	0.00#
277.00	24.80	4.87#
0.00	0.00	0.00

U.M
 12/18/15




Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

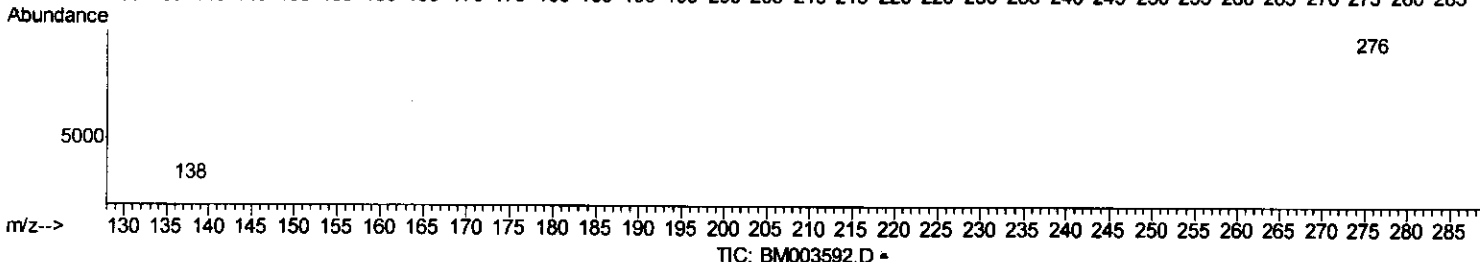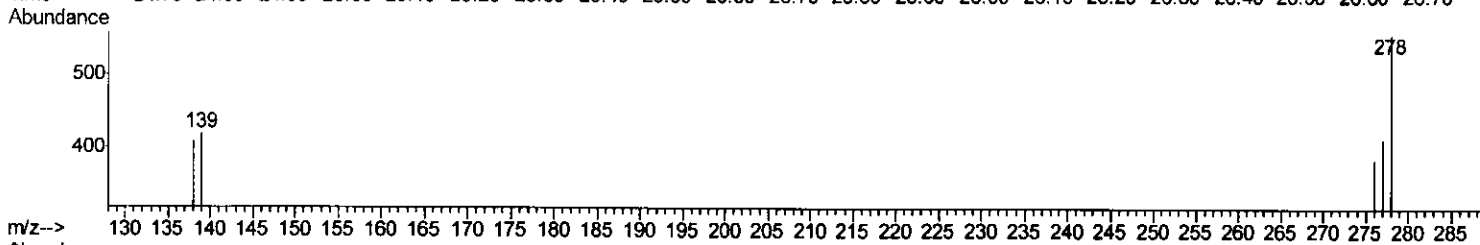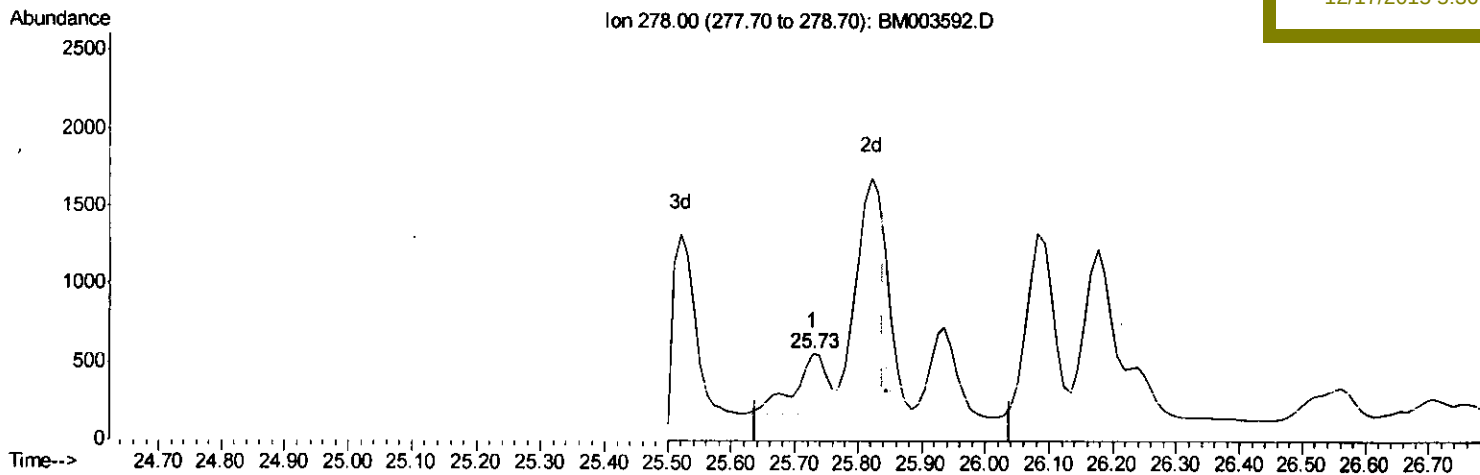

(27) Dibenzo(a,h)anthracene

25.727min (-0.111) 0.04ng/ul

response 1485

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	74.96#
279.00	25.20	56.53#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

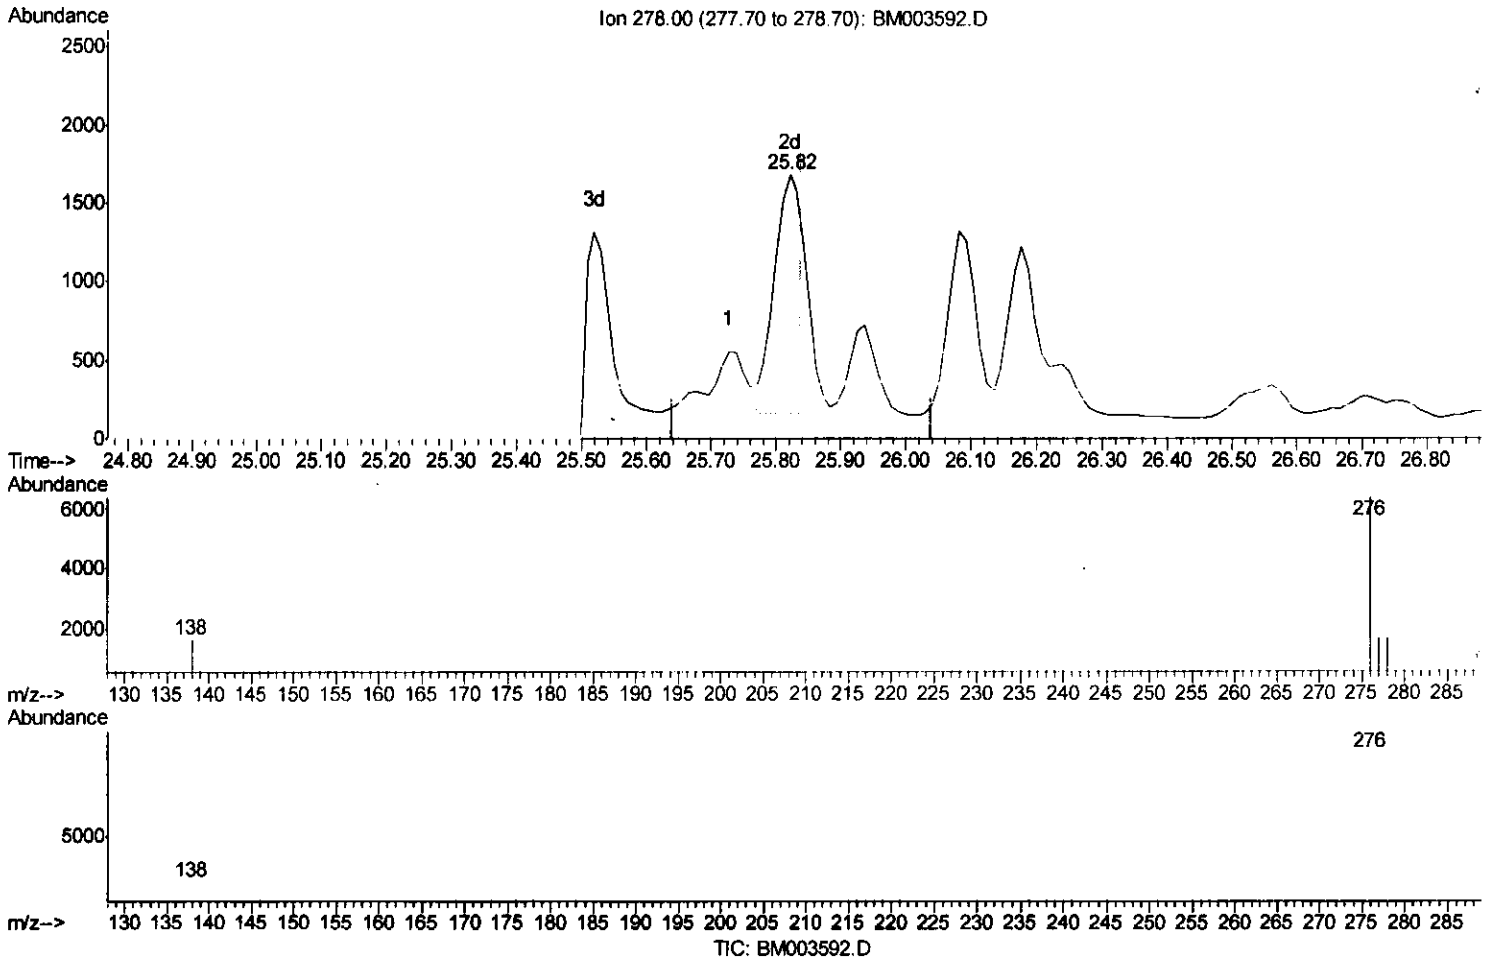

(27) Dibenzo(a,h)anthracene

25.821min (-0.017) 0.14ng/ul m

response 5150

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	36.76#
279.00	25.20	33.97#
0.00	0.00	0.00

U.M
 12/18/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
Data File : BM003592.D
Acq On : 16 Dec 2015 23:55
Operator : UM/IZ
Sample : G4767-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9N38

Quant Time: Dec 17 08:05:22 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 02:56:38 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMdadoda
12/17/2015 5:36:16 PM

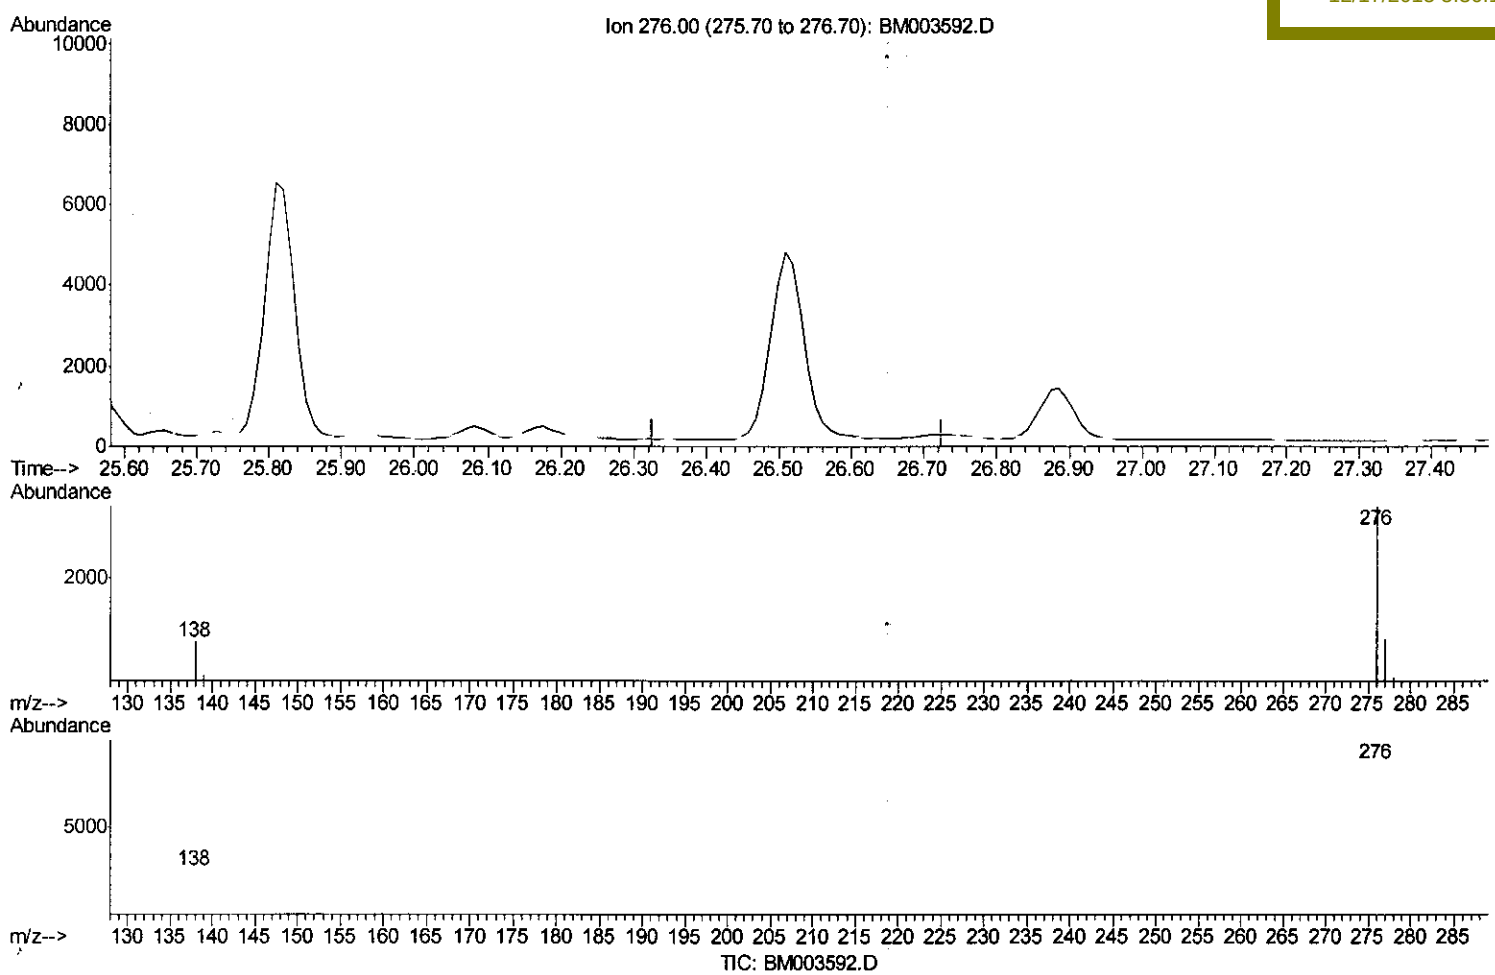

(28) Benzo(g,h,i)perylene

26.526min (-26.526) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	23.60	0.00#
138.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Quant Time: Dec 17 08:05:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

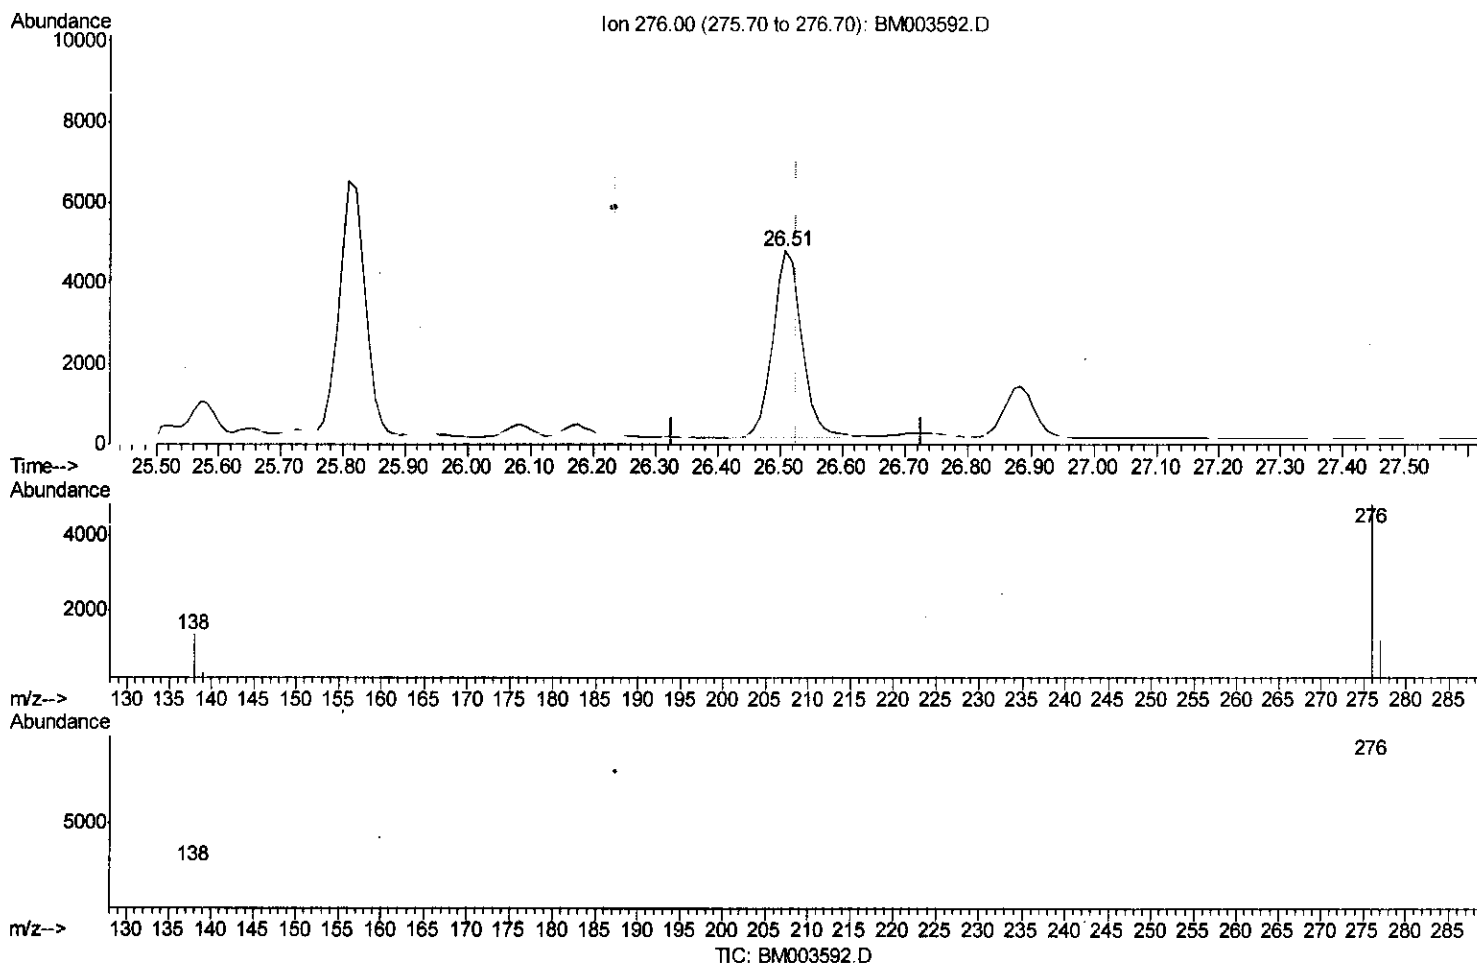

(28) Benzo(g,h,i)perylene

26.509min (-0.017) 0.38ng/ul m

response 15142

Ion Exp% Act%

276.00 100 100

277.00 23.60 25.47

138.00 28.10 28.45

0.00 0.00 0.00

U.M
 12/18/15

Data Path : Z:\HPCHEM1\BNA_M\Data\BM121615\
 Data File : BM003592.D
 Acq On : 16 Dec 2015 23:55
 Operator : UM/IZ
 Sample : G4767-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9N38

Quant Time: Dec 17 08:07:32 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Quant Update : Thu Dec 17 02:56:38 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 12/17/2015 5:36:16 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	3396	0.40	ng/ul	0.00
4) Naphthalene-d8	10.50	136	14536	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.37	164	9131	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.11	188	14777m	0.40	ng/ul	0.00
18) Chrysene-d12	21.31	240	12709	0.40	ng/ul	0.00
22) Perylene-d12	23.56	264	13753m	0.40	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	13026	8.97	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.09	152	4331	0.25	ng/ul	-0.01
16) Fluoranthene-d10	19.15	212	8612m	0.27	ng/ul	0.00

Target Compounds

						Qvalue
5) Naphthalene	10.55	128	1241862	37.92	ng/ul	99
7) 2-Methylnaphthalene	12.16	142	420606	19.13	ng/ul	100
9) Acenaphthylene	14.07	152	74099	2.12	ng/ul#	92
10) Acenaphthene	14.42	153	780268	27.75	ng/ul	88
11) Fluorene	15.41	166	734909	23.58	ng/ul	85
14) Phenanthrene	17.14	178	2846750m	74.69	ng/ul	
15) Anthracene	17.23	178	231925	7.03	ng/ul#	94
17) Fluoranthene	19.17	202	1553921	37.54	ng/ul	97
19) Pyrene	19.54	202	1071022	31.22	ng/ul	98
20) Benzo(a)anthracene	21.29	228	222085	7.16	ng/ul	95
21) Chrysene	21.34	228	177029	4.98	ng/ul	96
23) Benzo(b)fluoranthene	22.87	252	108740m	2.32	ng/ul	
24) Benzo(k)fluoranthene	22.91	252	35116m	0.83	ng/ul	
25) Benzo(a)pyrene	23.45	252	65424m	1.65	ng/ul	
26) Indeno(1,2,3-cd)pyrene	25.81	276	19827m	0.43	ng/ul	
27) Dibenzo(a,h)anthracene	25.82	278	5150m	0.14	ng/ul	
28) Benzo(g,h,i)perylene	26.51	276	15142m	0.38	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed