

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121616\
 Data File : BM008345.D
 Acq On : 15 Dec 2016 16:24
 Operator : UM/SJ
 Sample : H6039-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8S2

Manual Integrations
 APPROVED

sohil
 12/16/2016 6:20:30 PM

Quant Time: Dec 16 02:54:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 16 02:33:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	127155	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	523674	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	353148	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	674705	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	693225	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	681626	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	4471	1.65	ng/uL	0.00
5) Phenol-d5	6.87	99	65036	6.59	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.02	67	199319	35.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	202778	27.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	125528	16.43	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	131755	34.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	144049	34.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	236660	30.79	ng/ul	0.01
29) 4-Chloroaniline-d4	10.67	131	15063m	1.71	ng/ul	0.07
43) Dimethylphthalate-d6	13.73	166	876536	37.34	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1056609	38.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	11094m	3.21	ng/ul	0.08
57) Fluorene-d10	15.31	176	743833	36.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	99256	24.71	ng/ul	0.00
70) Anthracene-d10	17.16	188	1073568	36.52	ng/ul	0.00
76) Pyrene-d10	19.46	212	1146919	42.84	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	1031965	36.05	ng/ul	0.00

Target Compounds					Qvalue
56) Diethylphthalate	15.14	149	53735	2.35 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121616\
Data File : BM008345.D
Acq On : 15 Dec 2016 16:24
Operator : UM/SJ
Sample : H6039-06
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DA8S2

Manual Integrations
APPROVED

sohil
12/16/2016 6:20:30 PM

Quant Time: Dec 16 02:54:30 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 16 02:33:30 2016
Response via : Initial Calibration

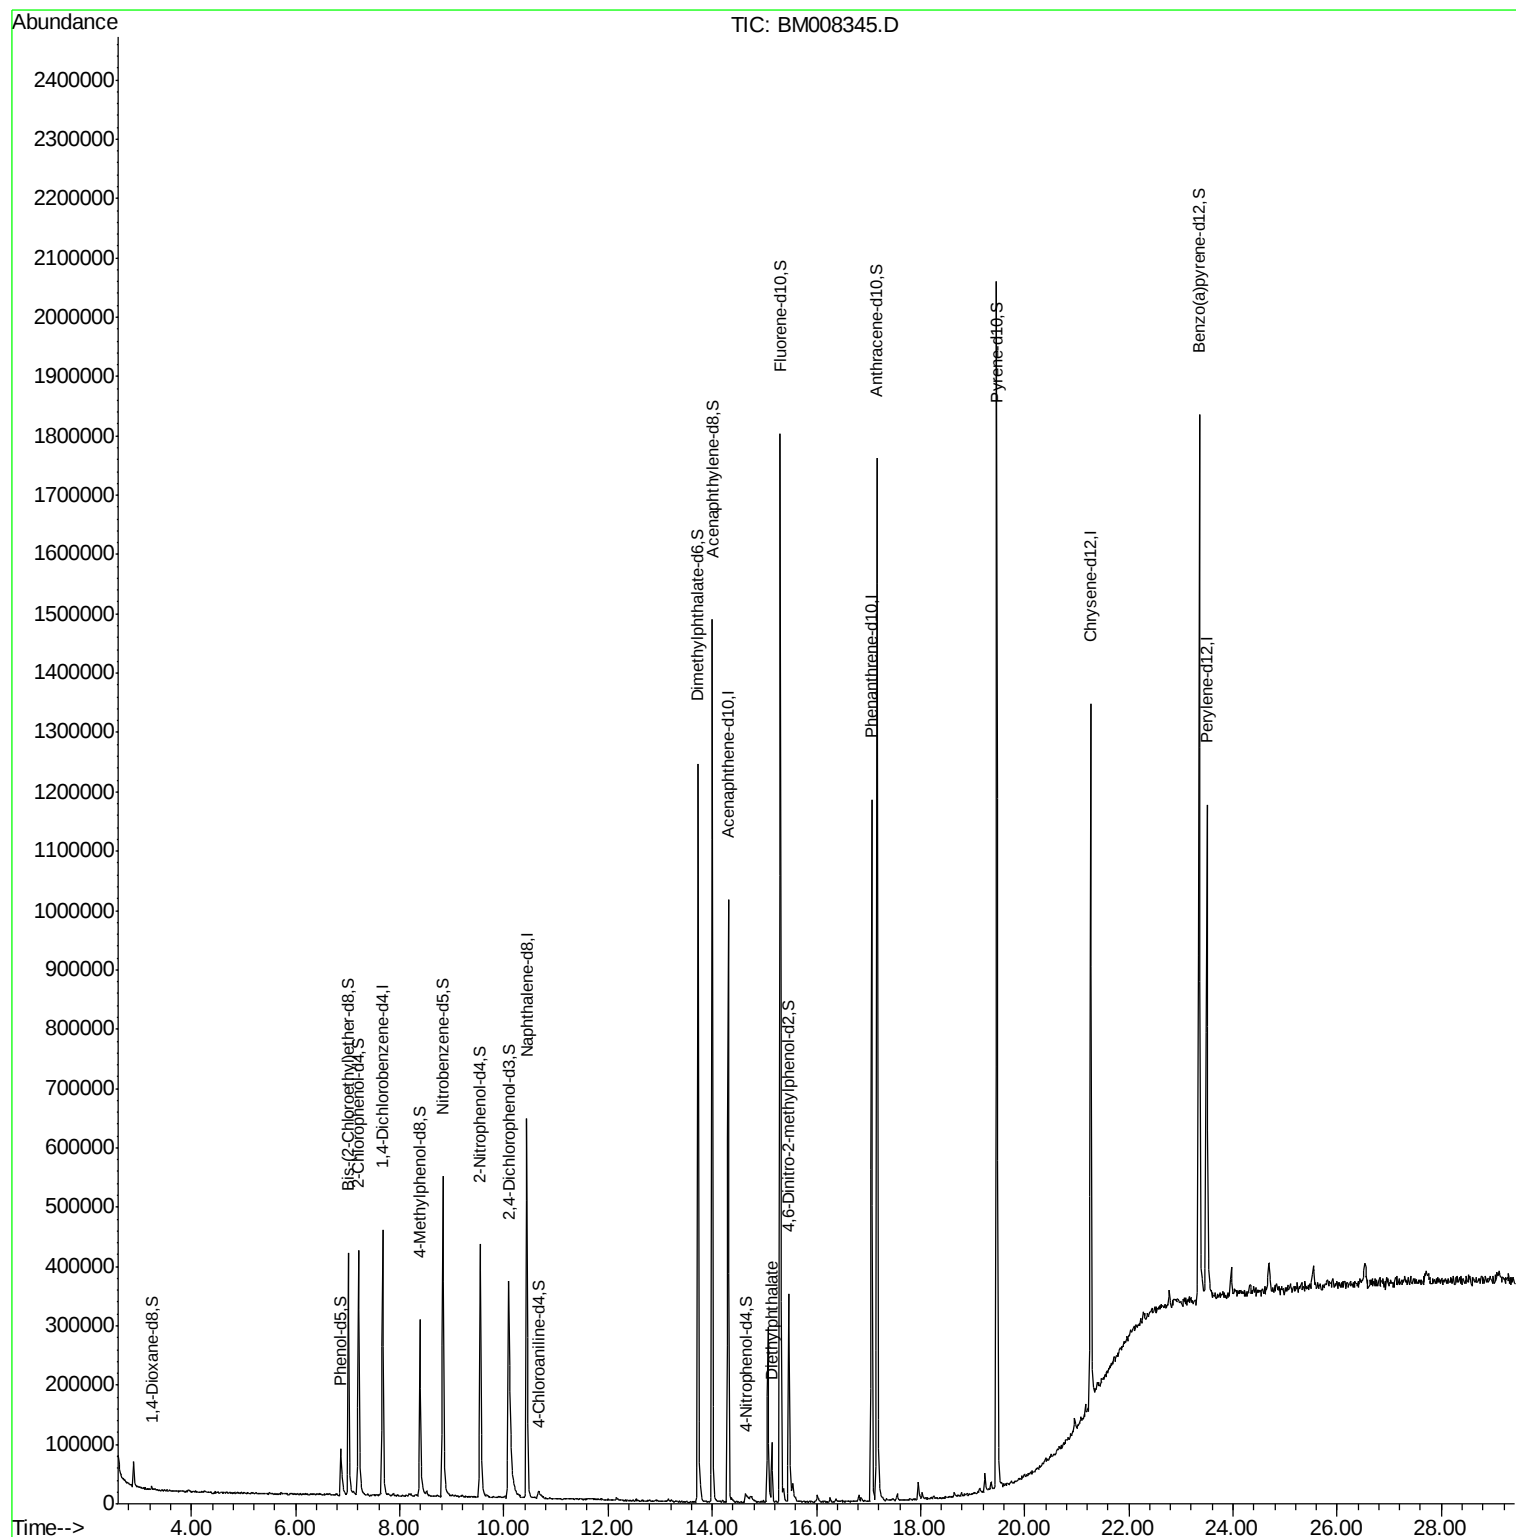

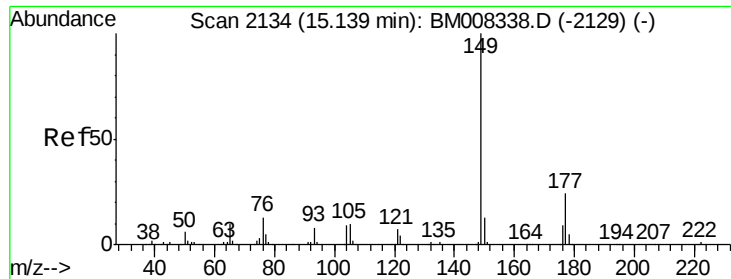

#56
 Diethylphthalate
 Concen: 2.35 ng/ul
 RT: 15.14 min Scan# 2135
 Delta R.T. 0.01 min
 Lab File: BM008345.D
 Acq: 15 Dec 2016 16:24

Instrument :
 BNA_M
 ClientSampleId :
 DA8S2

Tgt Ion:	149	Resp:	53735
Ion Ratio	Lower	Upper	
149	100		
177	21.8	18.5	27.7
150	13.7	10.6	15.8

Manual Integrations
 APPROVED

sohil
 12/16/2016 6:20:30 PM

