



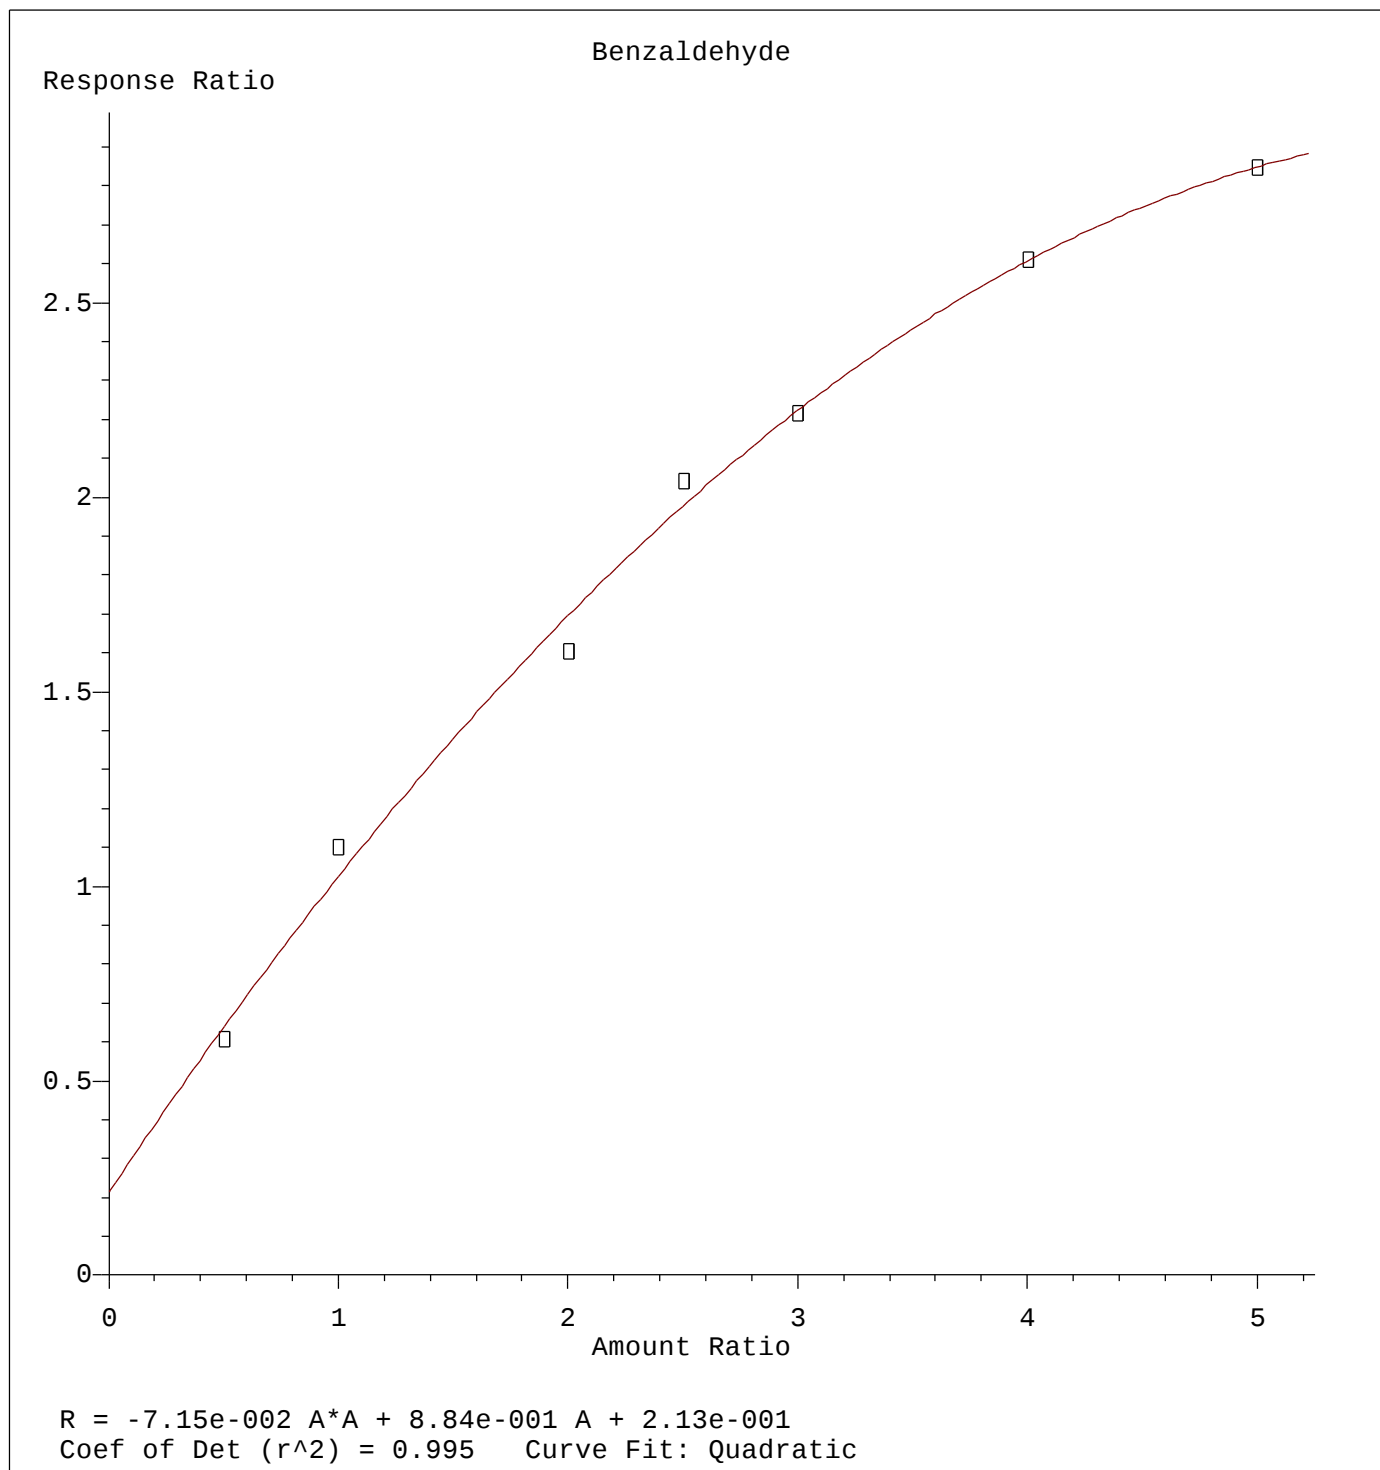

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121619.M
Calibration Table Last Updated: Mon Dec 16 19:58:15 2019

Hexachlorocyclopentadiene

Response Ratio

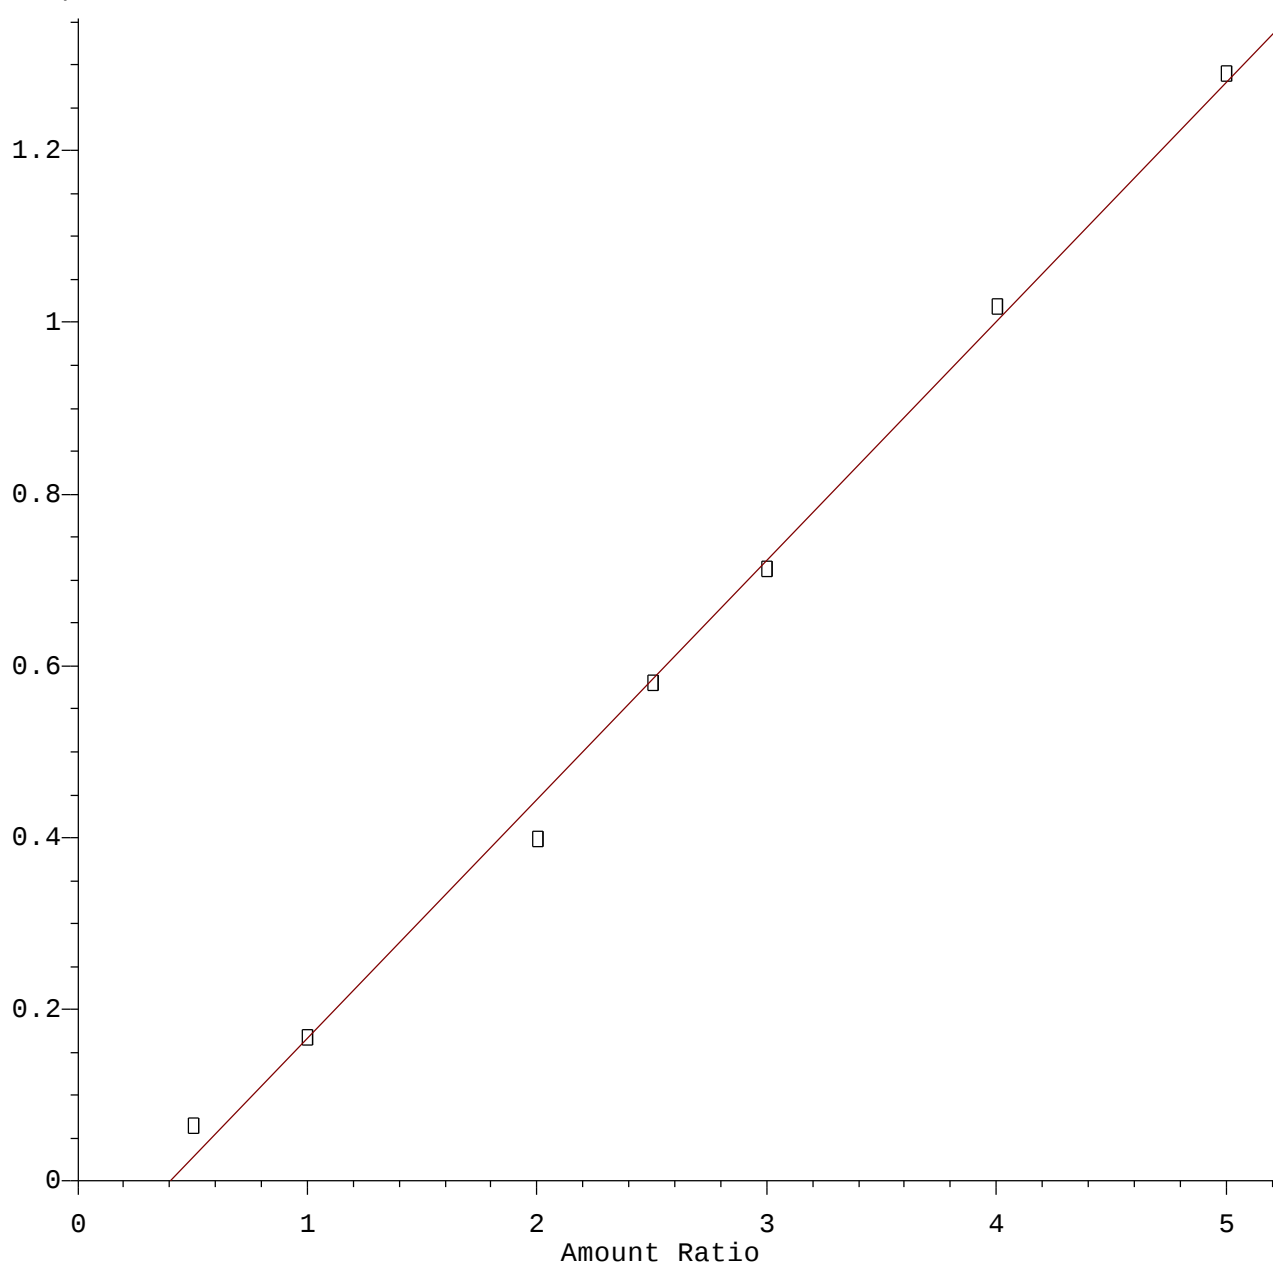


Resp Ratio = $2.78 \times 10^{-1} \times \text{Amt} - 1.11 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121619.M
Calibration Table Last Updated: Mon Dec 16 19:58:15 2019


2,4-Dinitrophenol

Response Ratio

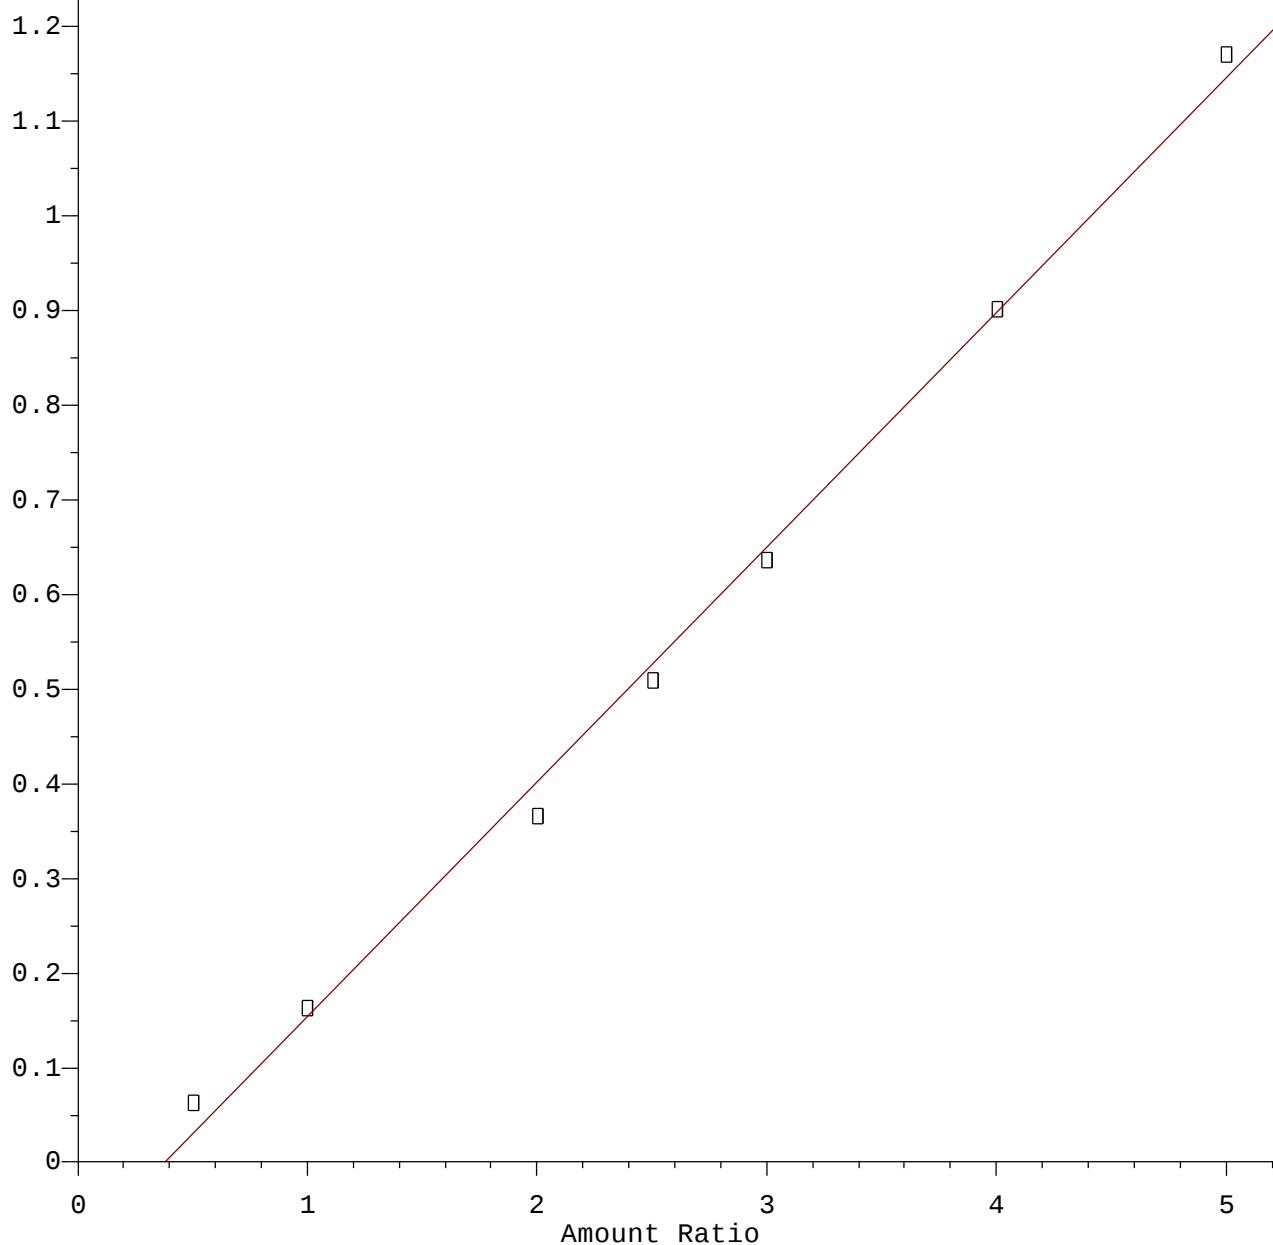

Resp Ratio = $2.48 \times 10^{-1} \times \text{Amt} - 9.43 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121619.M
Calibration Table Last Updated: Mon Dec 16 19:58:15 2019

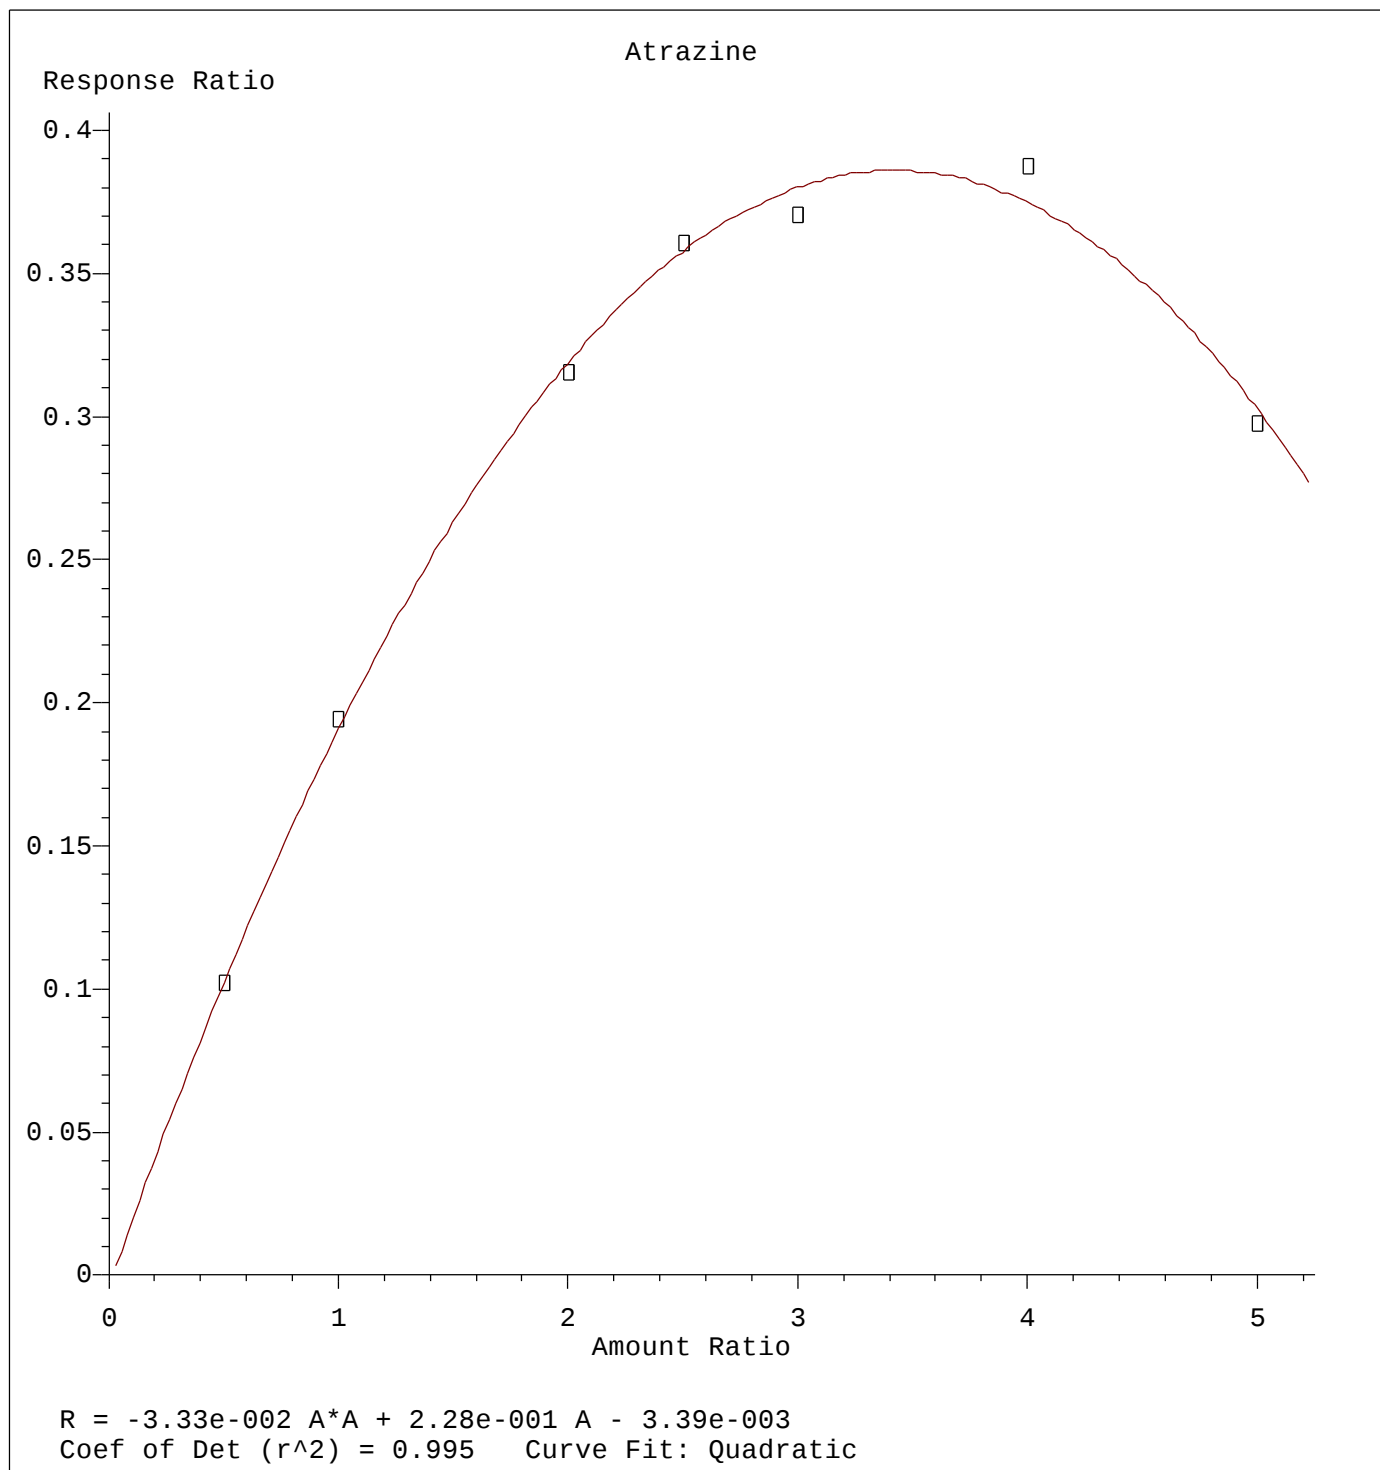

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121619.M
Calibration Table Last Updated: Mon Dec 16 19:58:15 2019