
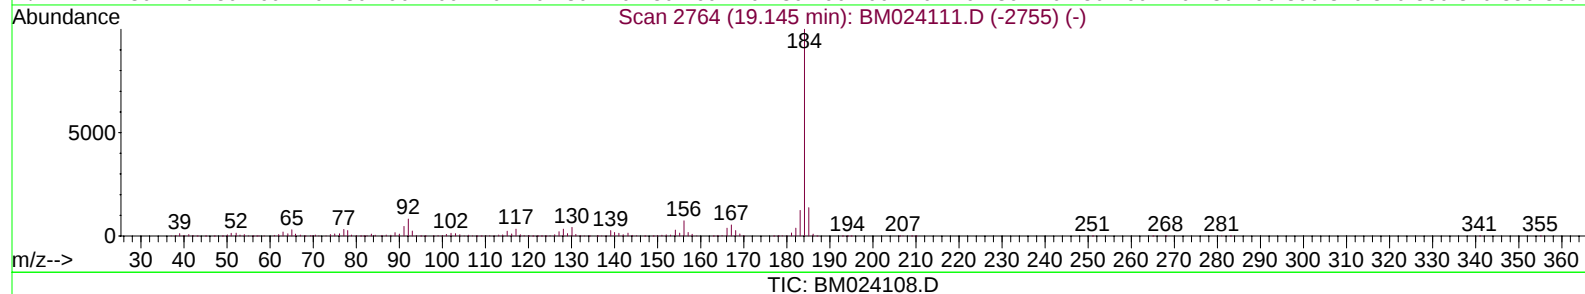
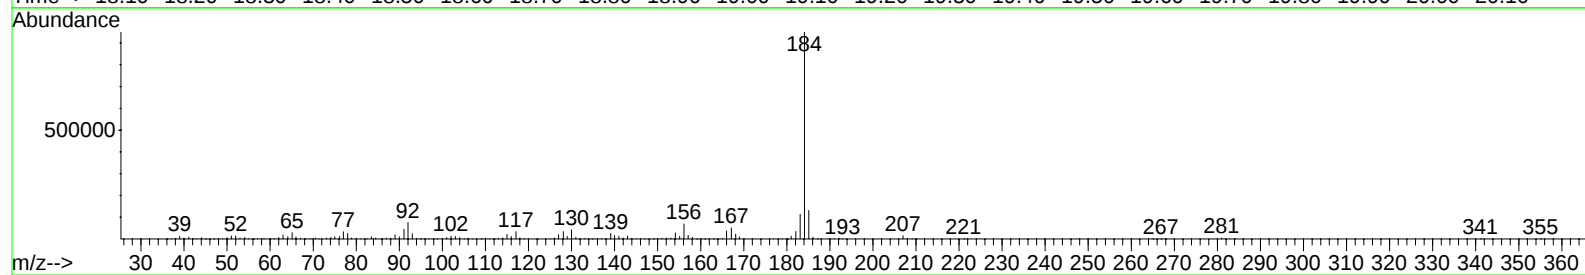


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM121619\
Data File : BM024108.D
Acq On : 16 Dec 2019 14:56
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 18:14:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 17:25:31 2019
Response via : Initial Calibration

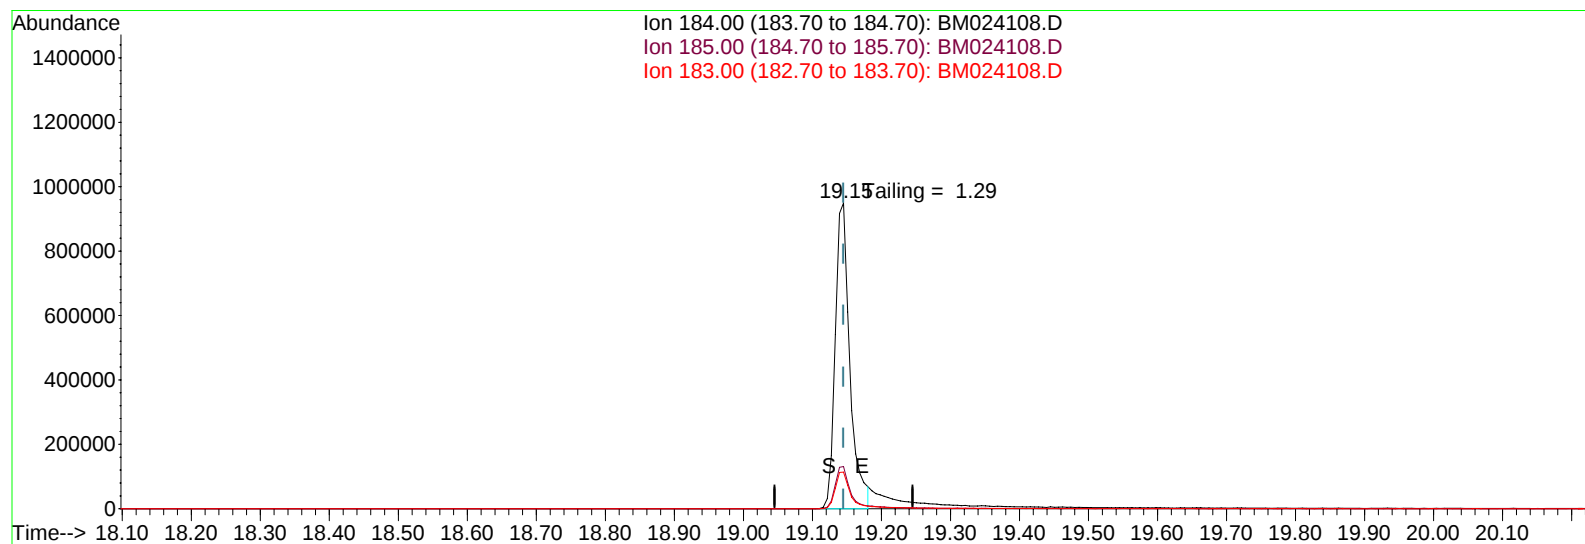

(77) Benzidine




19.145min (0.000) 0.00ng

response 1494479

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	13.81
183.00	12.40	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM121619\
Data File : BM024108.D
Acq On : 16 Dec 2019 14:56
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 18:14:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 17:25:31 2019
Response via : Initial Calibration

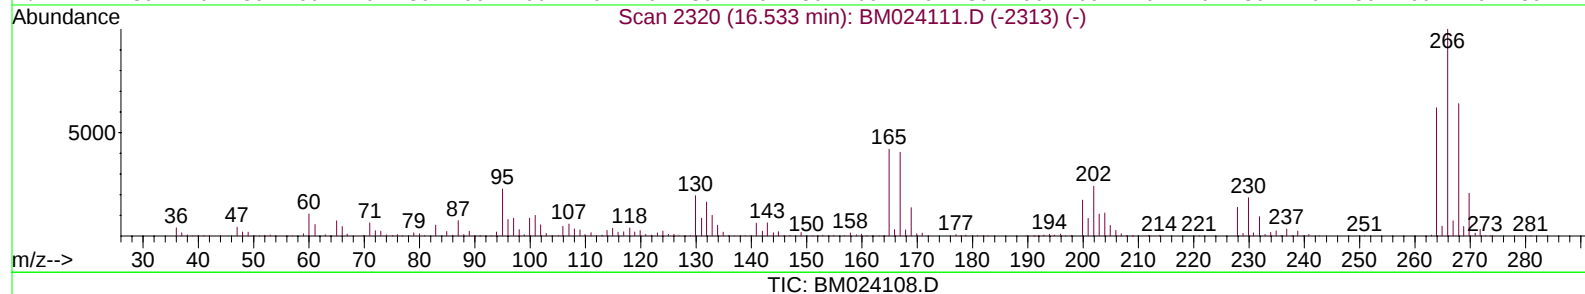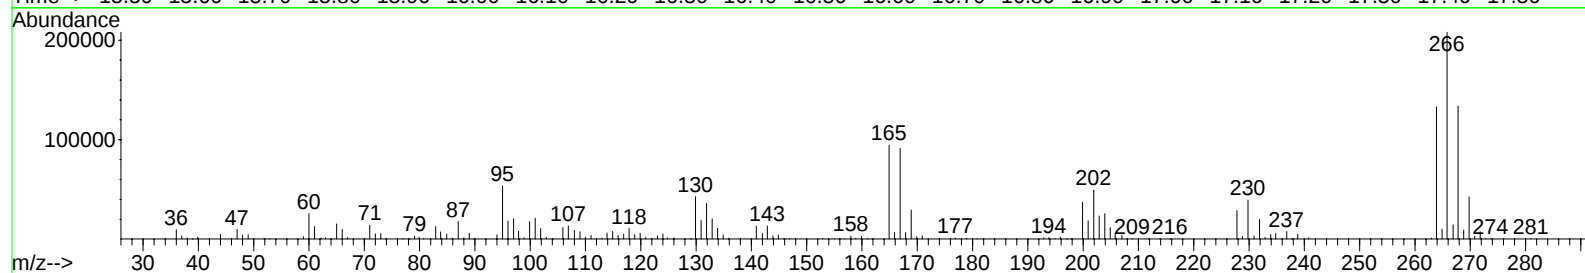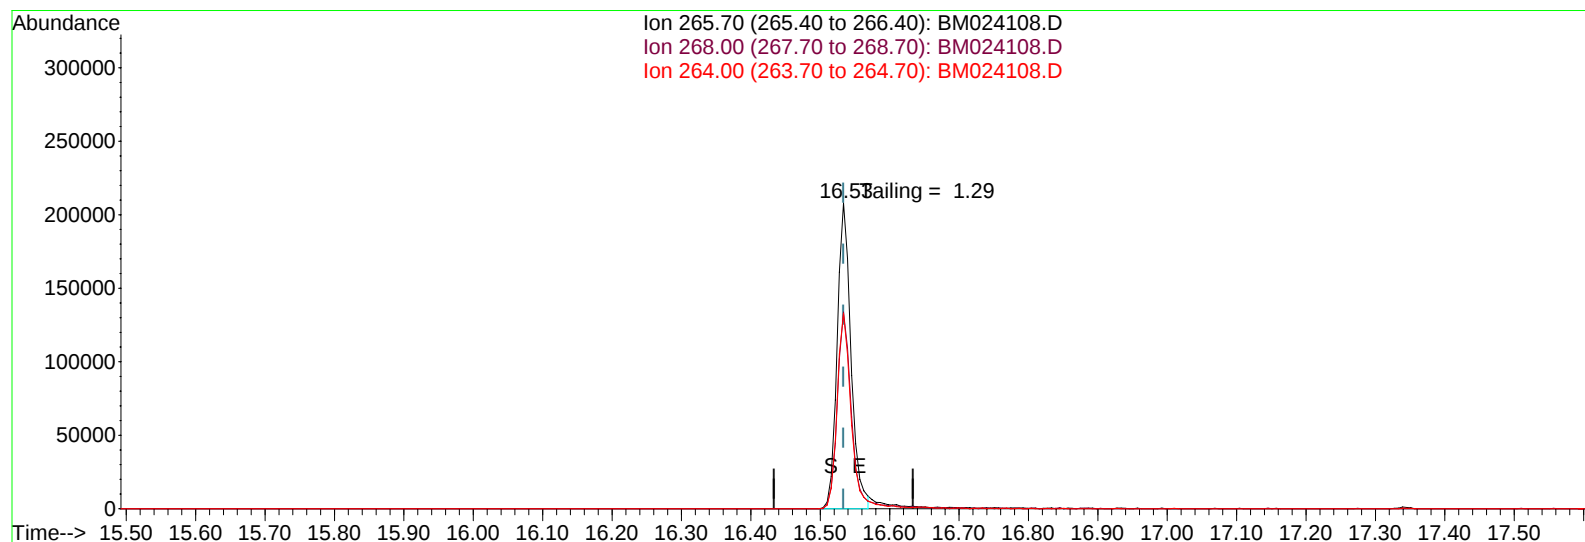

(70) Pentachlorophenol (C)

16.533min (+0.000) 0.00ng

response 296310

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.31
264.00	62.00	63.94
0.00	0.00	0.00