
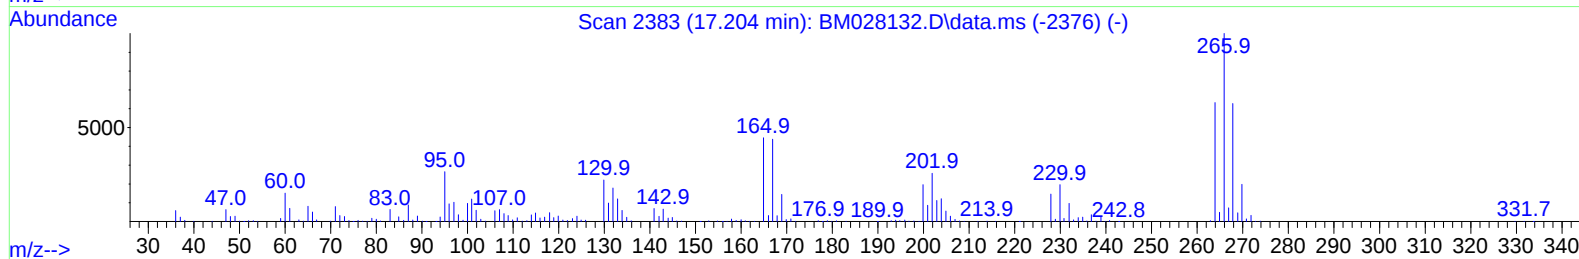
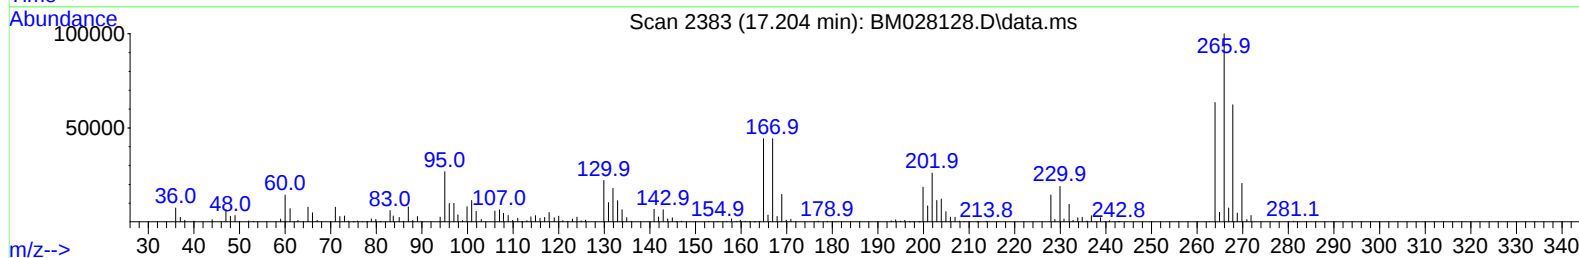


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121620\  
Data File : BM028128.D  
Acq On : 15 Dec 2020 15:43  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 04:20:31 2020  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM121620.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 16 01:58:38 2020  
Response via : Initial Calibration

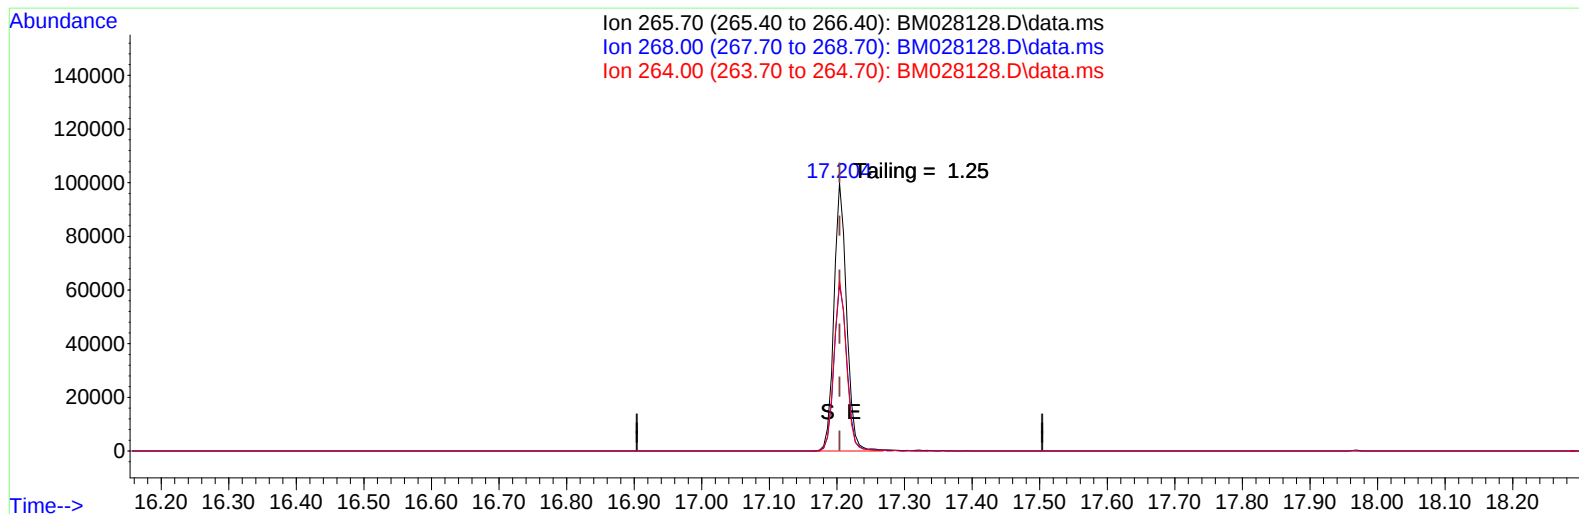

TIC: BM028128.D\data.ms

**(70) Pentachlorophenol (C)**




17.204min (-0.000) 0.00 ng

response 129848

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.40  | 62.32  |
| 264.00 | 63.30  | 63.47  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121620\  
 Data File : BM028128.D  
 Acq On : 15 Dec 2020 15:43  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 04:20:31 2020  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM121620.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 16 01:58:38 2020  
 Response via : Initial Calibration

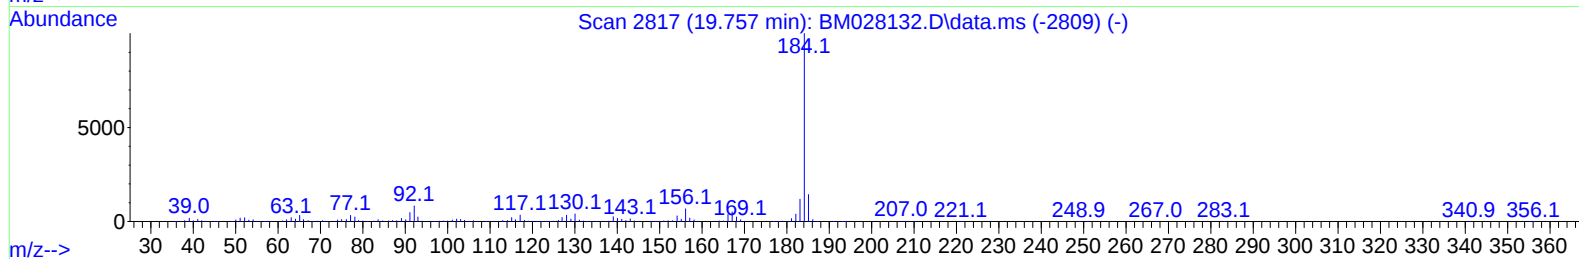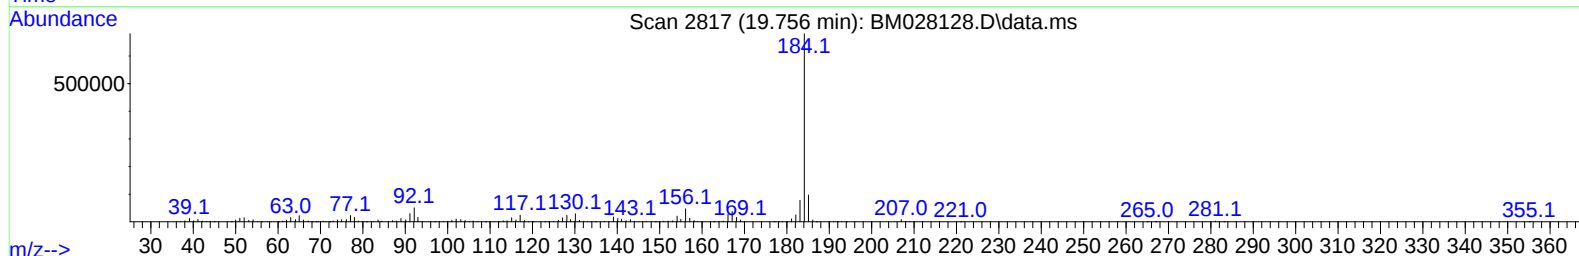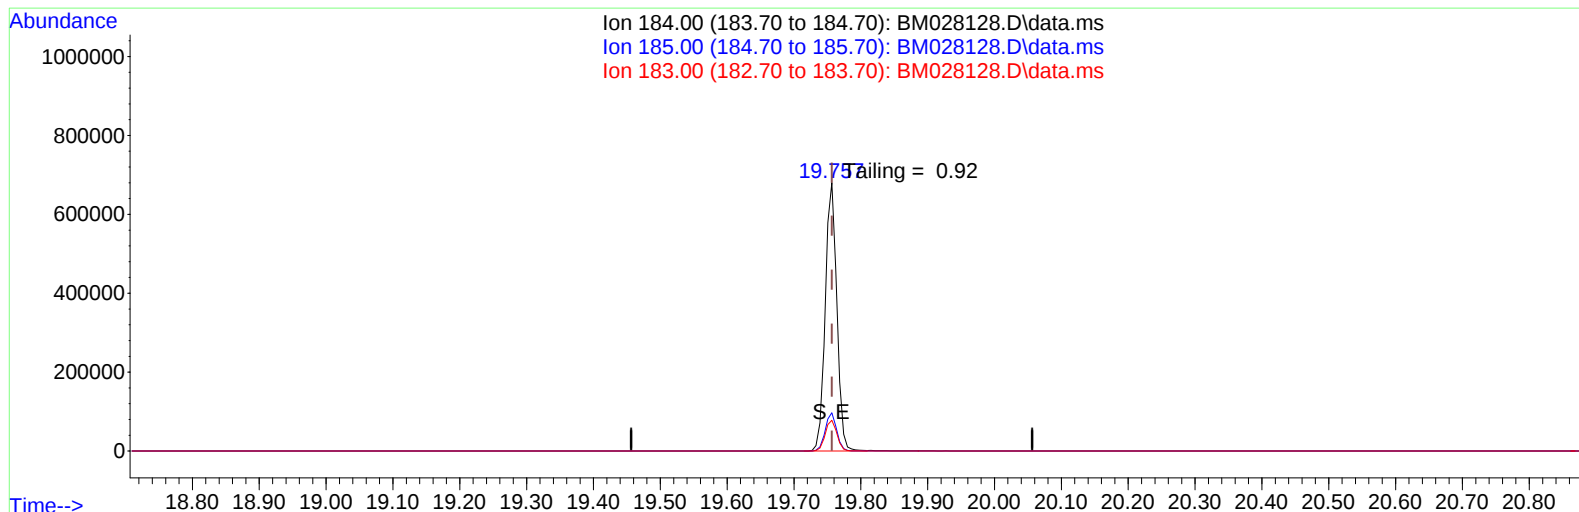

TIC: BM028128.D\data.ms

**(77) Benzidine**

19.756min (-0.000) 0.00 ng

response 821746

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.25  |
| 183.00 | 12.10  | 11.46  |
| 0.00   | 0.00   | 0.00   |