
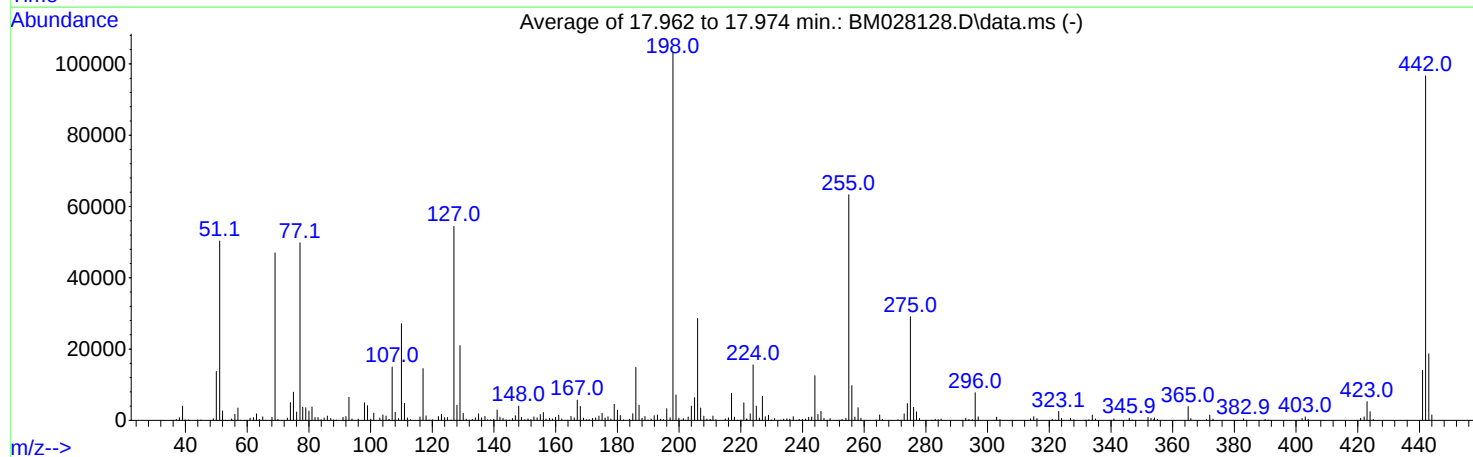


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121620\
 Data File : BM028128.D
 Acq On : 15 Dec 2020 15:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 16 01:58:38 2020

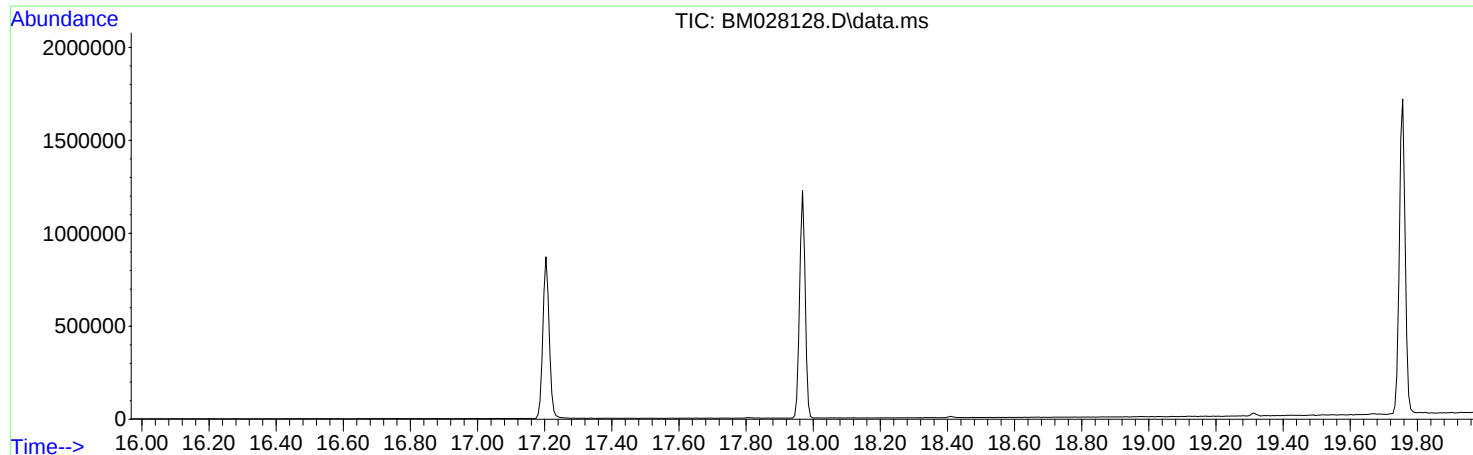

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	50315	PASS
68	69	0.00	2	1.8	860	PASS
69	198	0.00	100	45.5	47005	PASS
70	69	0.00	2	0.6	272	PASS
127	198	10	80	52.7	54419	PASS
197	198	0.00	2	0.7	713	PASS
198	198	100	100	100.0	103208	PASS
199	198	5	9	6.9	7132	PASS
275	198	10	60	28.2	29072	PASS
365	198	1	100	3.8	3873	PASS
441	198	0.01	100	13.6	14034	PASS
442	198	50	100	93.6	96632	PASS
443	442	15	24	19.3	18669	PASS