


Data Path : Z:\HPCHEM1\BNA M\Data\bm121715\
 Data File : BM003595.D
 Acq On : 17 Dec 2015 10:44
 Operator : UM/IZ
 Sample : DFTPP60
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP60

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM121515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 18 00:41:46 2015

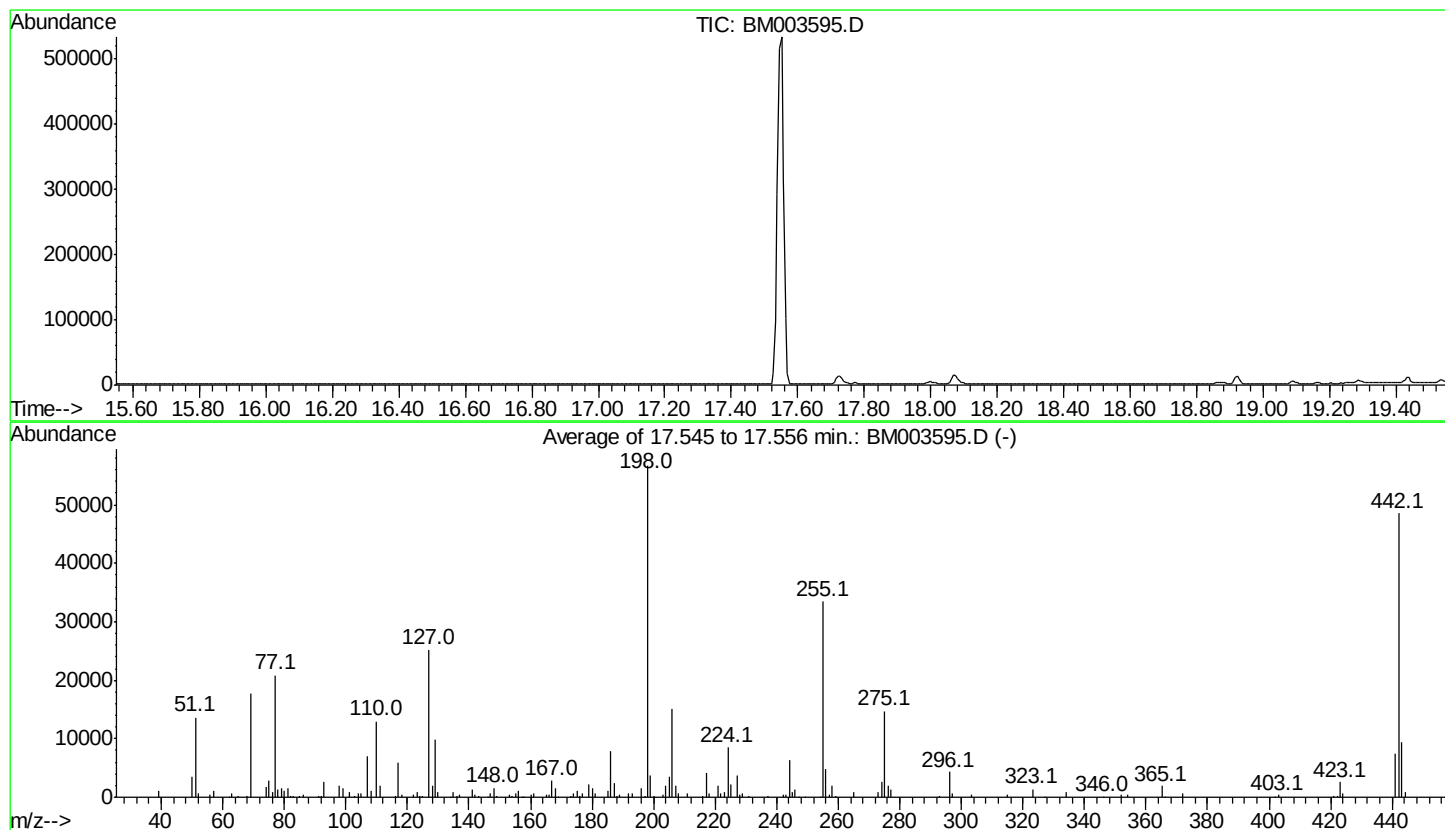

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	13592	PASS
68	69	0.00	2	1.6	284	PASS
69	198	0.00	100	31.1	17643	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.6	25259	PASS
197	198	0.00	1	0.5	261	PASS
198	198	100	100	100.0	56693	PASS
199	198	5	9	6.7	3793	PASS
275	198	10	60	25.9	14665	PASS
365	198	1	100	3.3	1885	PASS
441	443	0.01	100	80.0	7473	PASS
442	198	50	100	85.7	48576	PASS
443	442	15	24	19.2	9343	PASS

Scan 2451 (17.503 min): BM003595.D
DFTPP60

m/z	Abundance
43.00	721.0
45.00	481.0
60.00	424.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	1332.0
43.00	644.0
45.00	443.0
50.10	4410.0
51.10	17192.0
52.10	879.0
56.00	581.0
57.00	1278.0
60.00	364.0
62.00	321.0
63.00	775.0
65.00	426.0
68.00	460.0
69.00	22392.0
74.00	2362.0
75.00	3737.0
76.10	1142.0
77.10	26176.0
78.10	1838.0
79.00	1765.0
80.00	1379.0
81.00	1763.0
82.00	476.0
83.00	536.0
85.00	454.0
86.00	556.0
91.00	406.0
92.00	533.0
93.00	3320.0
98.00	2544.0
99.00	2001.0
101.00	1148.0
103.00	394.0
104.00	708.0
105.00	732.0
107.00	8935.0
108.00	1327.0
110.00	15989.0
111.00	2630.0
116.00	491.0
117.00	7123.0
118.00	586.0
122.00	653.0
123.00	965.0
124.00	439.0
125.00	382.0
127.00	30752.0
128.00	2456.0
129.00	12122.0
130.00	982.0
134.00	346.0
135.00	1084.0
136.10	376.0
137.10	569.0
141.00	1553.0
142.00	566.0
143.00	409.0
146.00	321.0
147.00	881.0
148.00	1798.0
149.00	442.0
153.00	495.0
154.00	397.0
155.00	886.0
156.00	1318.0
157.10	316.0
157.90	319.0
160.00	490.0
161.00	739.0
165.00	557.0
166.00	519.0
167.00	3119.0
168.00	1880.0
169.00	319.0
173.00	400.0
174.00	692.0
175.10	1194.0
176.00	312.0
177.00	681.0
179.00	2396.0
180.10	1768.0
181.00	898.0
185.00	1264.0
186.10	9114.0
187.00	2585.0
188.00	362.0
189.00	525.0
192.00	810.0
193.00	835.0
196.00	1802.0
197.10	408.0
198.00	64696.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

199.00	4418.0
200.00	341.0
203.00	467.0
204.10	2348.0
205.10	4068.0
206.10	17048.0
207.10	2327.0
208.00	671.0
211.10	722.0
216.00	349.0
217.00	4628.0
218.00	654.0
221.00	2206.0
221.80	659.0
223.00	911.0
224.10	9423.0
225.10	2341.0
227.00	4014.0
228.00	549.0
229.00	837.0
231.00	341.0
237.00	337.0
242.00	489.0
243.10	528.0
244.10	6885.0
245.10	923.0
246.00	1396.0
249.00	303.0
255.10	36568.0
256.10	5439.0
257.10	410.0
258.00	2198.0
259.00	343.0
265.00	882.0
273.00	975.0
274.00	2731.0
275.10	15364.0
276.10	2107.0
277.10	1397.0
293.00	339.0
296.10	4452.0
297.00	681.0
303.10	466.0
315.00	406.0
323.10	1336.0
334.10	880.0
352.10	419.0
354.10	391.0
365.10	1863.0
366.00	325.0
372.10	655.0
403.00	405.0
421.00	319.0
422.10	332.0
423.10	2413.0
424.10	631.0
441.10	6731.0
442.10	44200.0
443.10	8755.0
444.10	888.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	1143.0
43.00	689.0
45.00	428.0
50.10	3877.0
51.10	15599.0
52.00	789.0
56.00	568.0
57.00	1303.0
60.00	387.0
63.00	667.0
65.00	395.0
68.00	394.0
69.00	20048.0
74.00	2142.0
75.00	3332.0
76.10	1100.0
77.10	23784.0
78.00	1541.0
79.00	1604.0
80.00	1244.0
81.00	1698.0
82.00	438.0
83.00	412.0
85.00	417.0
86.00	505.0
91.00	429.0
92.00	422.0
93.00	2770.0
98.00	2331.0
99.00	1864.0
101.00	977.0
103.00	315.0
104.00	678.0
105.00	622.0
107.00	7948.0
108.00	1198.0
110.00	14906.0
111.00	2183.0
116.00	481.0
117.00	6915.0
118.00	487.0
122.00	549.0
123.00	894.0
124.00	433.0
125.00	406.0
127.00	28776.0
128.00	2240.0
129.00	11165.0
130.00	1037.0
135.00	952.0
136.00	375.0
137.00	570.0
141.00	1485.0
141.90	470.0
142.90	417.0
147.00	776.0
148.00	1750.0
149.10	375.0
153.00	601.0
154.10	346.0
155.10	809.0
156.10	1406.0
160.00	534.0
161.00	824.0
165.00	632.0
166.00	527.0
167.00	3252.0
168.00	1624.0
173.00	437.0
174.00	635.0
175.10	1322.0
176.00	369.0
176.90	563.0
179.00	2295.0
180.00	1909.0
181.00	838.0
185.00	1287.0
186.00	9438.0
187.10	2706.0
188.00	315.0
189.00	619.0
192.00	873.0
193.10	871.0
196.00	1943.0
197.00	375.0
198.00	66200.0
199.00	4375.0
200.00	373.0
203.00	418.0
204.00	2364.0
205.10	4231.0
206.10	18312.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

207.10	2328.0
208.00	621.0
211.00	745.0
216.00	376.0
217.00	4897.0
218.00	644.0
221.00	2478.0
221.90	672.0
223.00	1067.0
224.10	9996.0
225.10	2571.0
227.00	4463.0
228.10	596.0
229.00	928.0
231.00	355.0
237.00	378.0
242.00	556.0
243.00	637.0
244.10	7614.0
245.10	991.0
246.00	1549.0
247.10	314.0
254.10	319.0
255.10	39576.0
256.00	5593.0
257.10	465.0
258.00	2226.0
259.00	368.0
265.00	957.0
273.00	1144.0
274.10	3050.0
275.10	17648.0
276.00	2347.0
277.00	1556.0
293.00	358.0
296.10	5223.0
297.00	740.0
303.10	567.0
315.00	599.0
323.10	1580.0
327.10	313.0
334.00	1018.0
346.00	323.0
352.10	474.0
354.10	521.0
365.10	2210.0
372.00	794.0
402.00	315.0
403.10	497.0
421.10	400.0
422.10	430.0
423.10	2990.0
424.10	714.0
441.10	8992.0
442.10	57328.0
443.10	11138.0
444.10	1029.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	654.0
43.00	735.0
45.00	515.0
50.00	2109.0
51.10	7987.0
52.00	482.0
56.00	306.0
57.00	720.0
60.00	351.0
63.00	381.0
69.00	10489.0
74.00	1065.0
75.00	1782.0
76.00	561.0
77.10	12647.0
78.10	889.0
79.00	951.0
80.00	633.0
81.00	950.0
93.00	1577.0
98.00	1249.0
99.00	1069.0
101.00	578.0
104.00	319.0
105.00	377.0
107.00	4433.0
108.00	660.0
110.00	7958.0
111.00	1207.0
117.00	3506.0
123.00	495.0
127.00	16250.0
128.00	1201.0
129.00	6609.0
130.00	560.0
135.00	533.0
137.00	367.0
141.00	862.0
147.00	482.0
148.00	1057.0
153.00	304.0
155.00	474.0
156.00	791.0
161.00	388.0
165.10	313.0
167.00	2035.0
168.00	1090.0
174.00	355.0
175.00	720.0
176.90	430.0
179.00	1580.0
180.00	1017.0
181.00	475.0
185.10	592.0
186.00	5427.0
187.00	1633.0
189.00	378.0
192.00	432.0
193.00	609.0
196.00	1170.0
198.00	39184.0
199.00	2588.0
203.00	321.0
204.00	1447.0
205.10	2503.0
206.10	10041.0
207.10	1428.0
208.00	429.0
210.90	418.0
217.00	2910.0
218.00	400.0
221.00	1486.0
221.90	390.0
223.00	693.0
224.10	5884.0
225.00	1468.0
227.00	2582.0
227.90	352.0
229.00	507.0
242.10	314.0
243.00	334.0
244.10	4632.0
245.10	578.0
246.10	998.0
255.10	24280.0
256.00	3494.0
257.00	319.0
258.00	1406.0
265.00	646.0
273.00	773.0
274.00	1972.0
275.10	10984.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

276.00	1374.0
277.00	996.0
296.00	3342.0
297.10	366.0
303.10	375.0
315.00	356.0
323.10	1093.0
334.10	717.0
352.00	310.0
354.10	365.0
365.10	1583.0
372.10	664.0
403.10	308.0
423.10	2282.0
424.10	485.0
441.10	6696.0
442.10	44200.0
443.10	8137.0
444.10	752.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60