




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121716.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

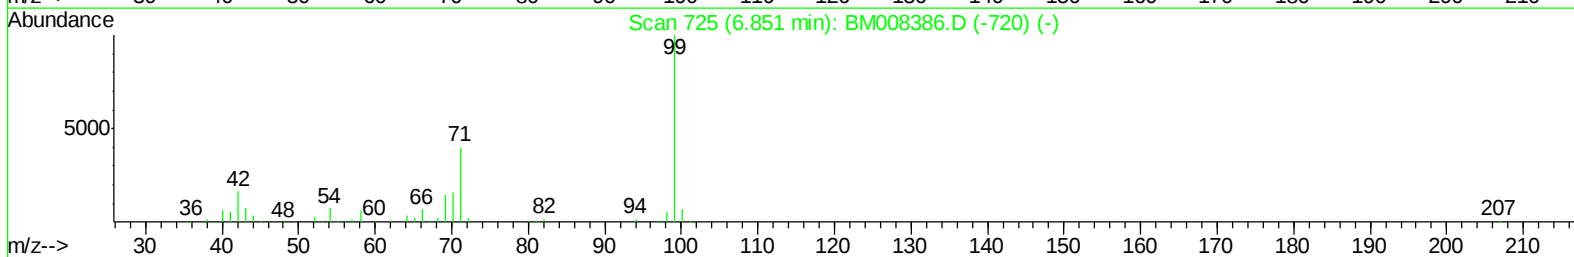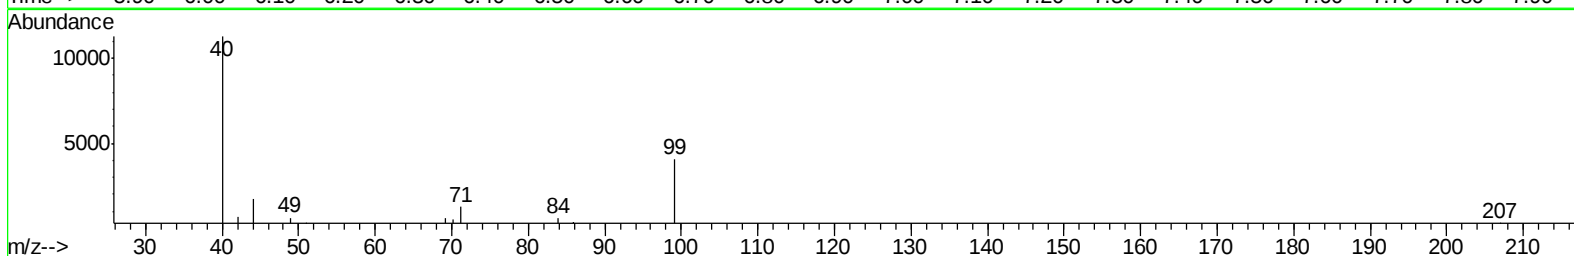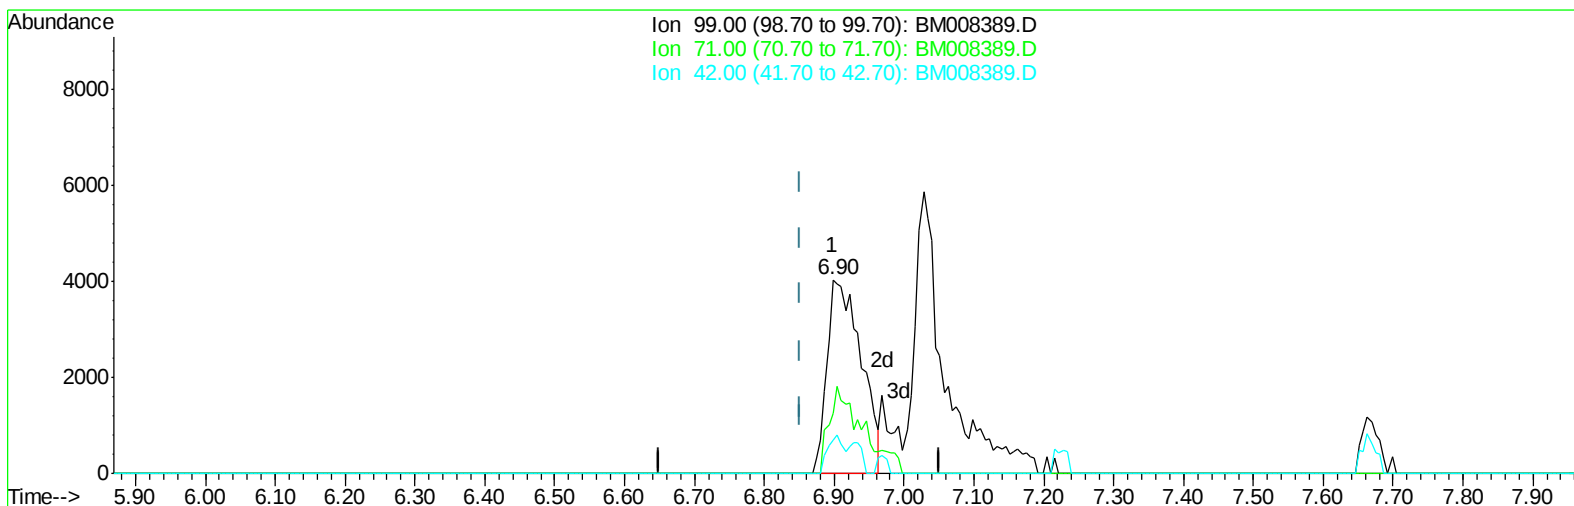

TIC: BM008389.D

(5) Phenol-d5 (S)

6.898min (+0.047) 1.61ng/ul

response 13642

Ion	Exp%	Act%
99.00	100	100
71.00	37.60	30.95
42.00	17.00	17.18
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

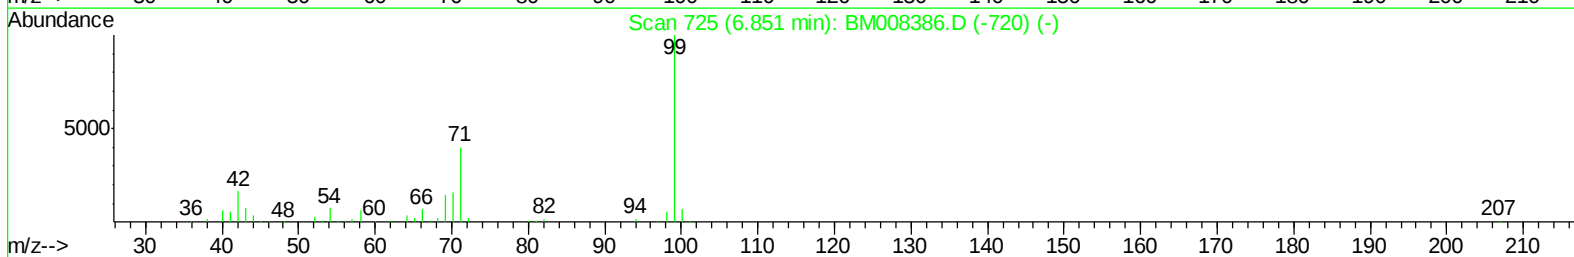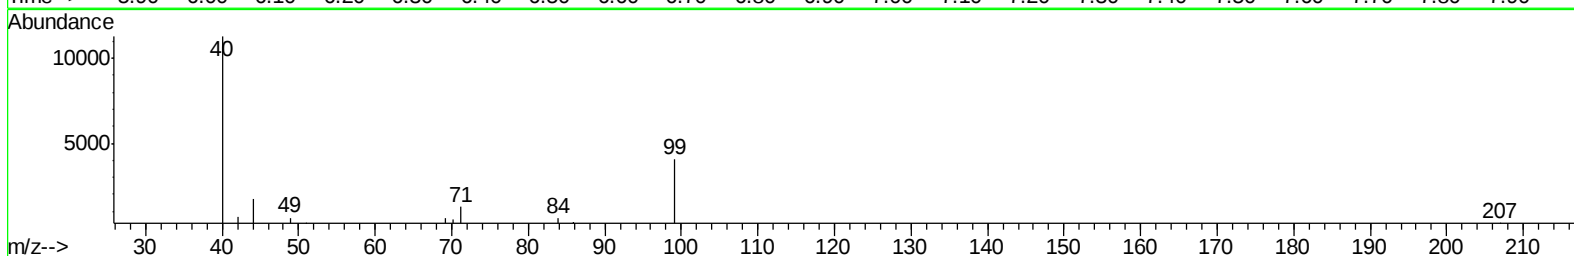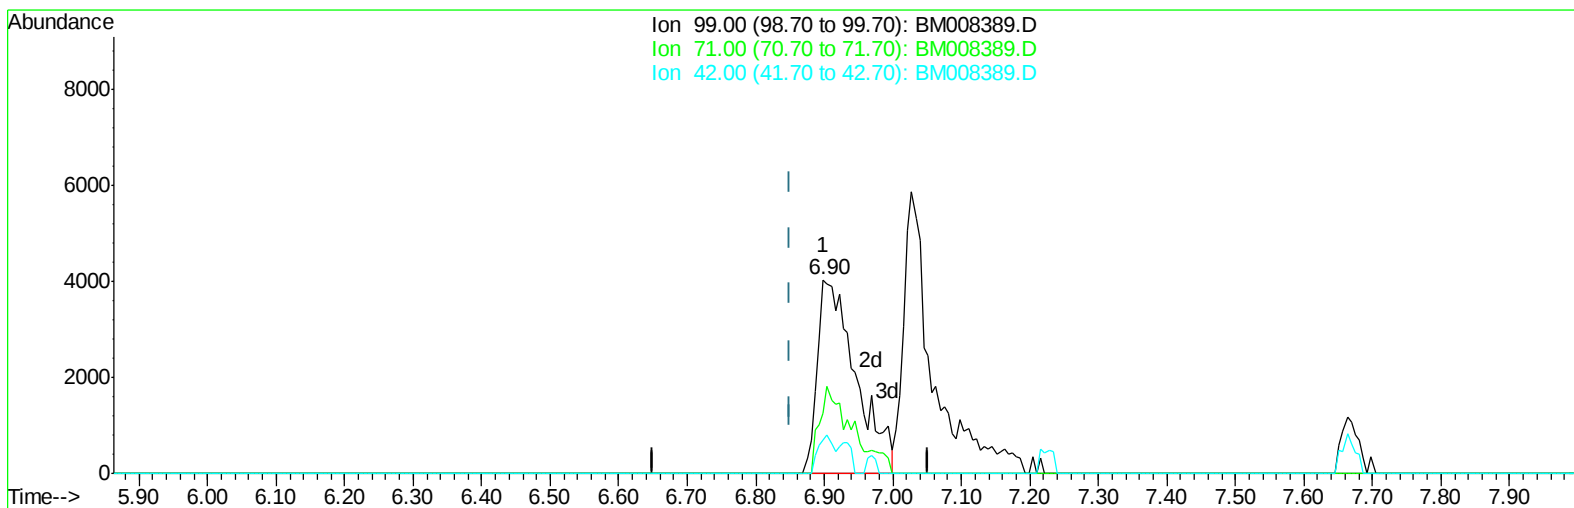

TIC: BM008389.D

(5) Phenol-d5 (S)

6.898min (+0.047) 1.85ng/ul m

response 15634

Ion	Exp%	Act%
99.00	100	100
71.00	37.60	30.95
42.00	17.00	17.18
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

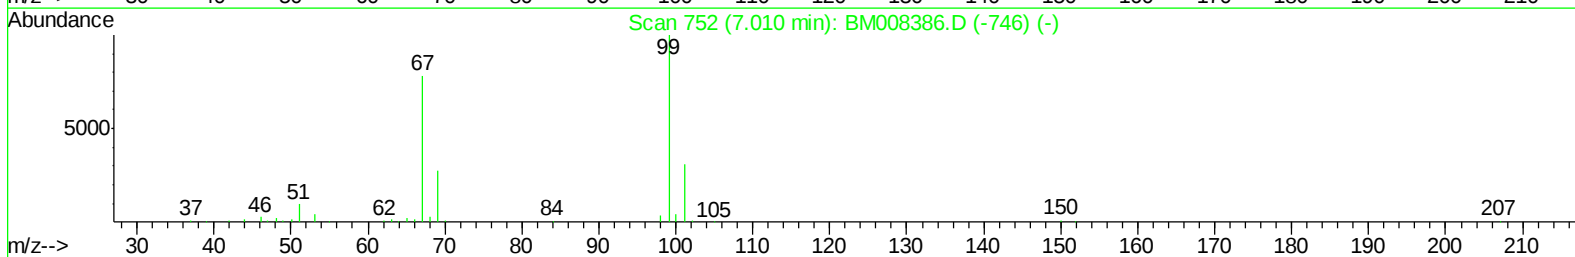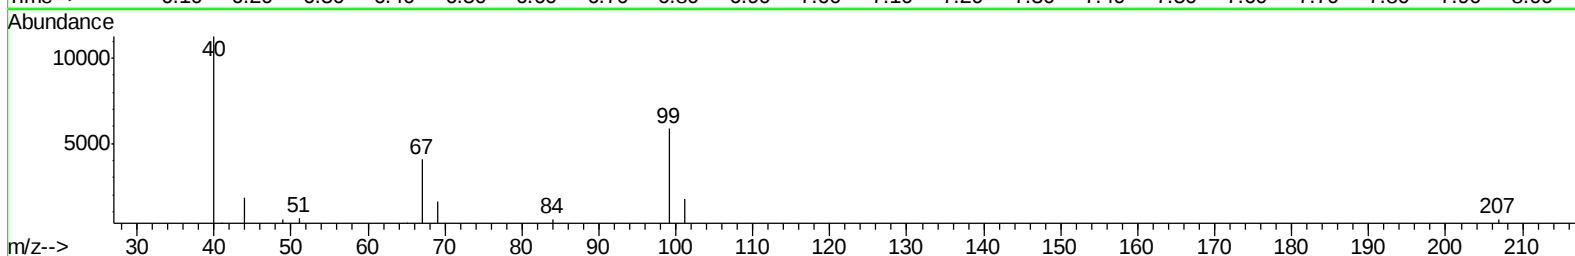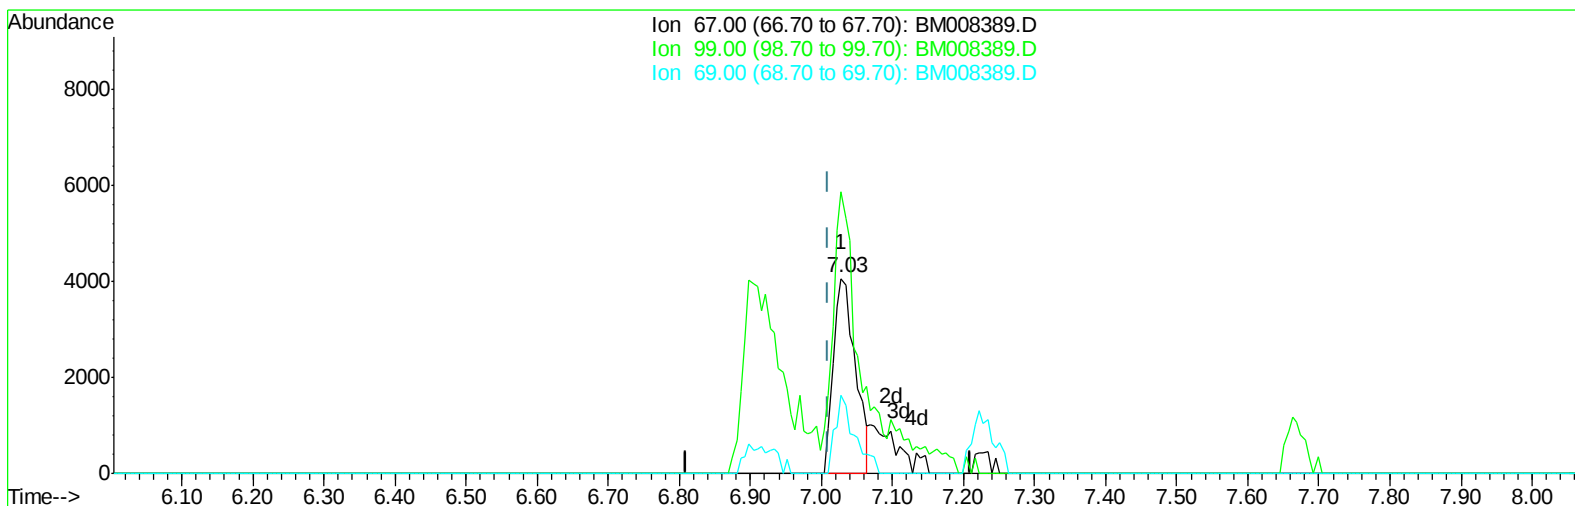

TIC: BM008389.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

7.028min (+0.018) 1.77ng/ul

response 8609

Ion	Exp%	Act%
67.00	100	100
99.00	124.40	144.25
69.00	31.20	39.87#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

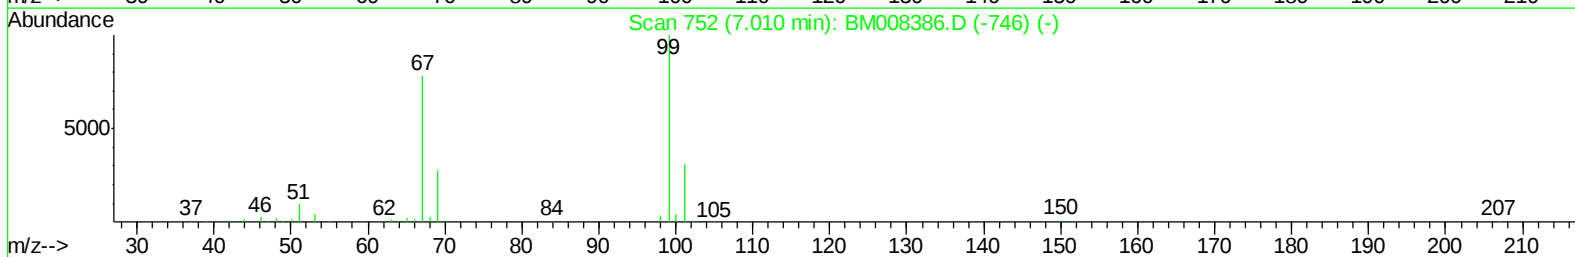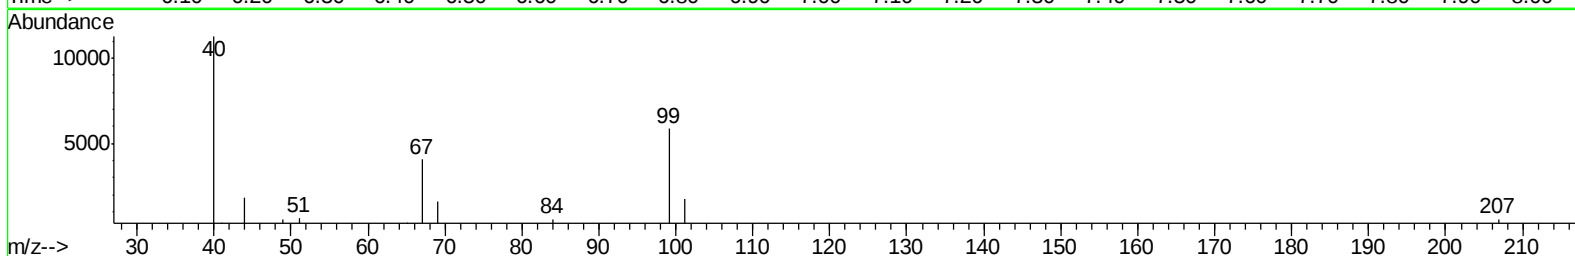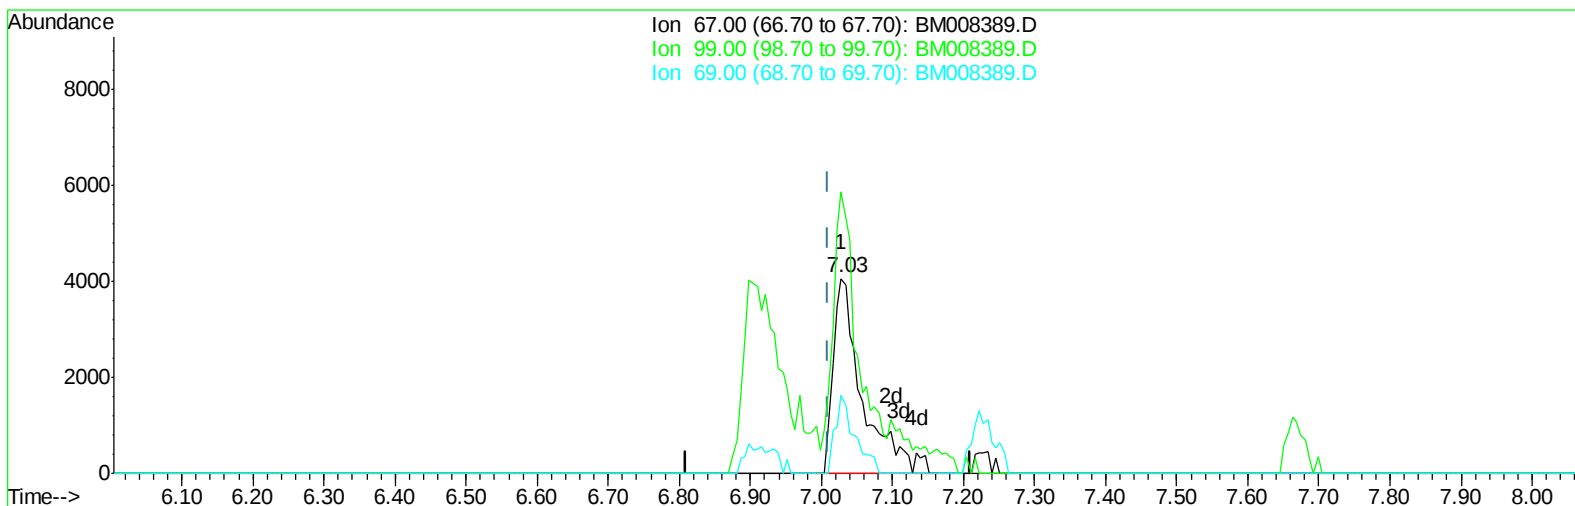

TIC: BM008389.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

7.028min (+0.018) 2.36ng/ul m

response 11483

Ion	Exp%	Act%
67.00	100	100
99.00	124.40	144.25
69.00	31.20	39.87#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

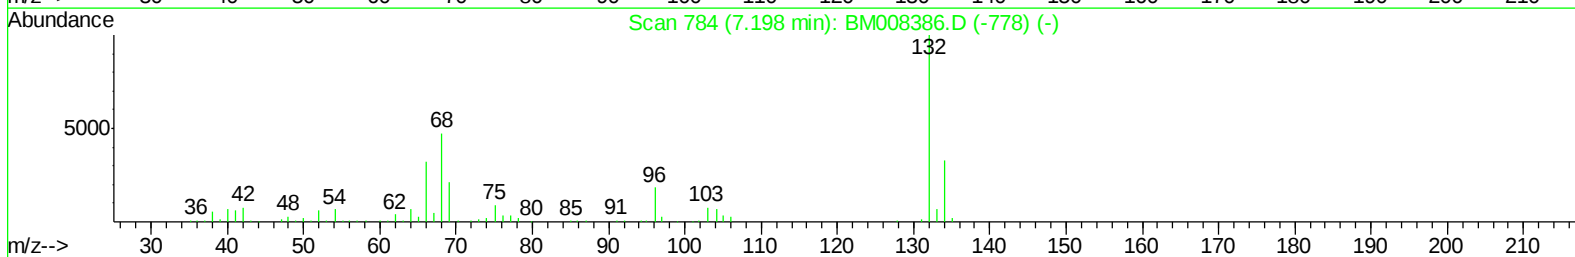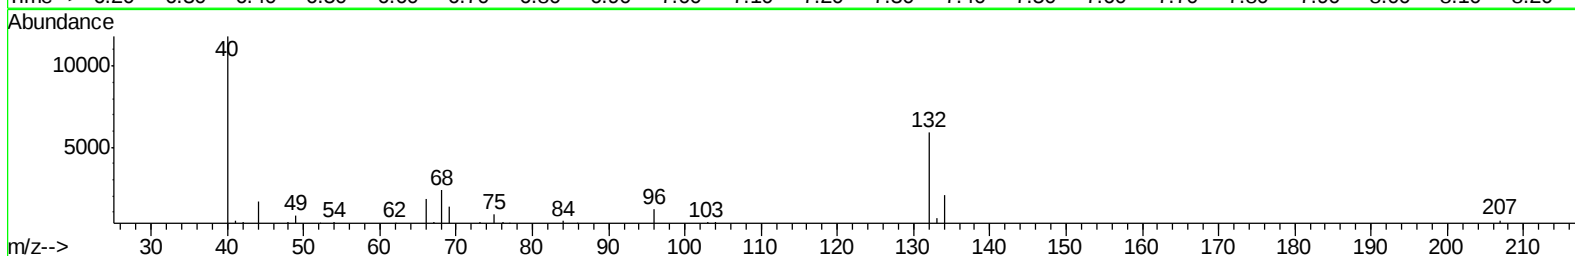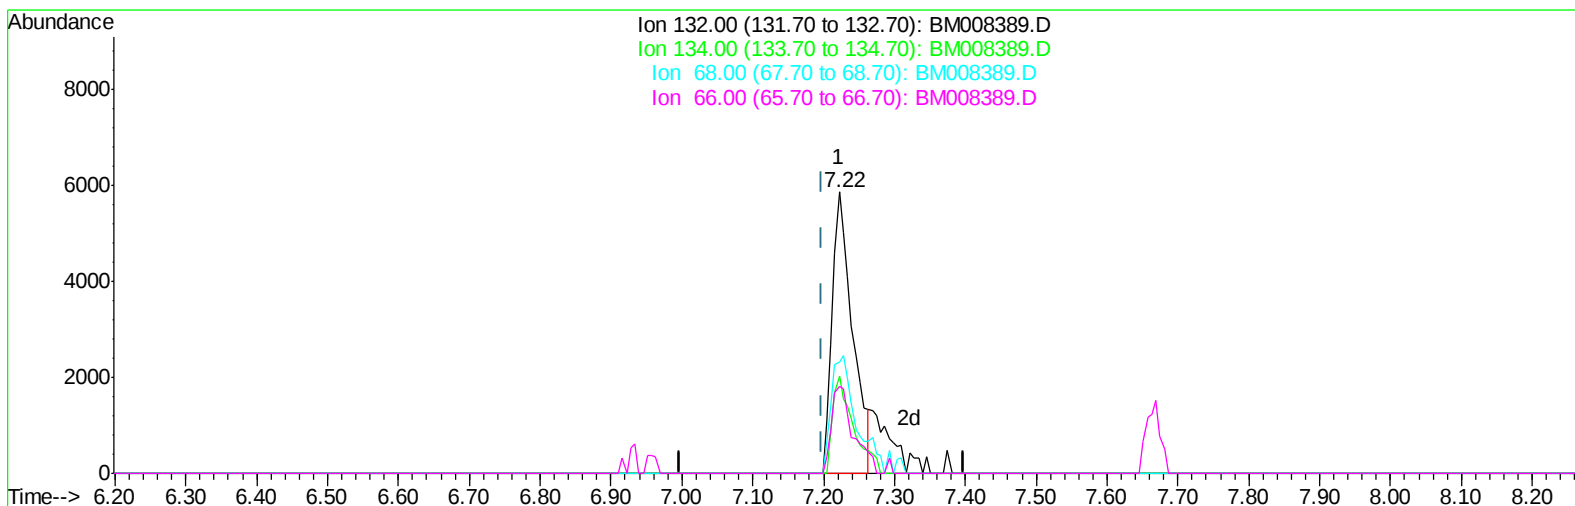

TIC: BM008389.D

(9) 2-Chlorophenol-d4 (S)

7.222min (+0.024) 1.86ng/ul

response 11837

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	34.41
68.00	48.80	39.77
66.00	30.60	30.71




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

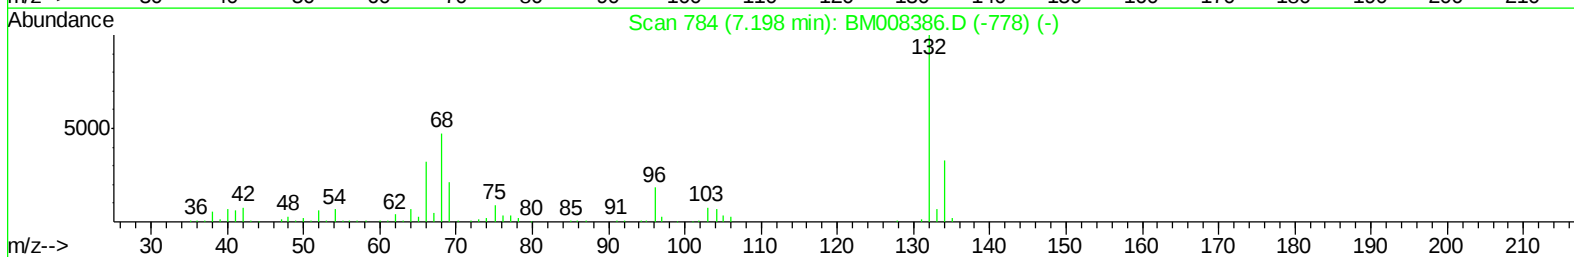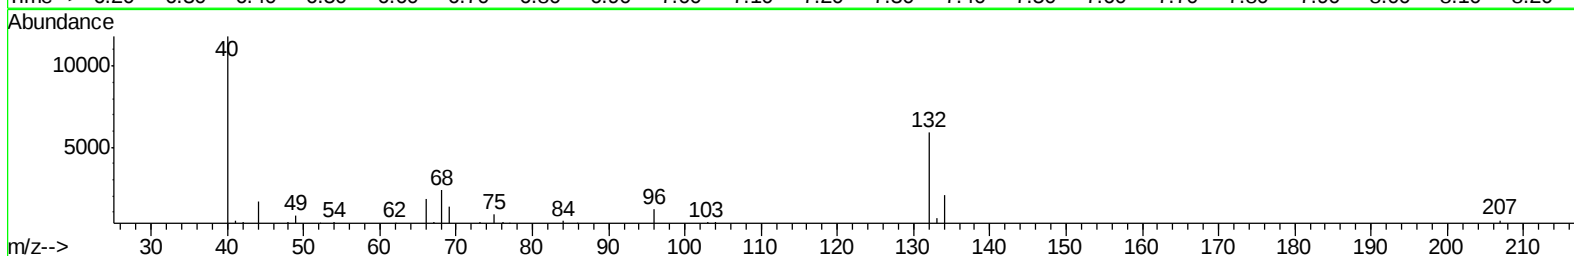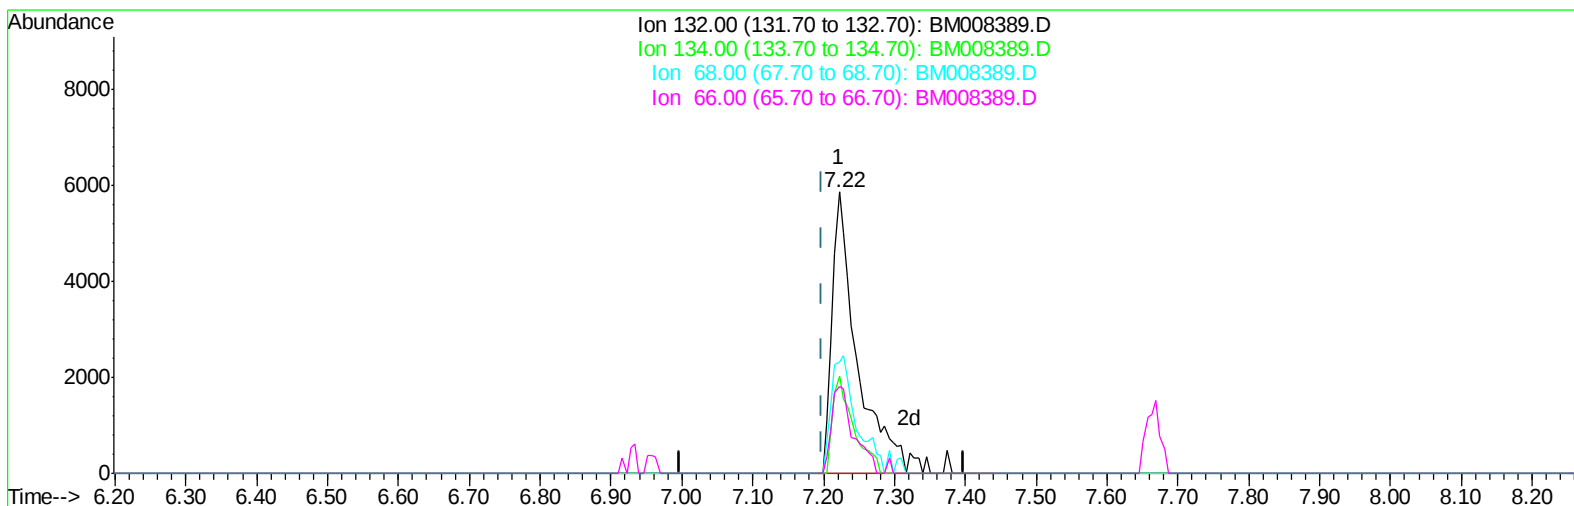

TIC: BM008389.D

(9) 2-Chlorophenol-d4 (S)

7.222min (+0.024) 2.35ng/ul m

response 14940

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	34.41
68.00	48.80	39.77
66.00	30.60	30.71




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

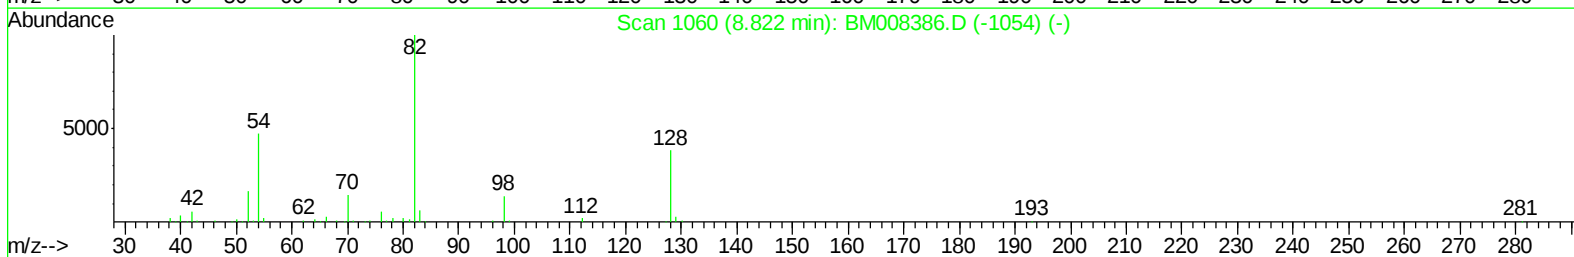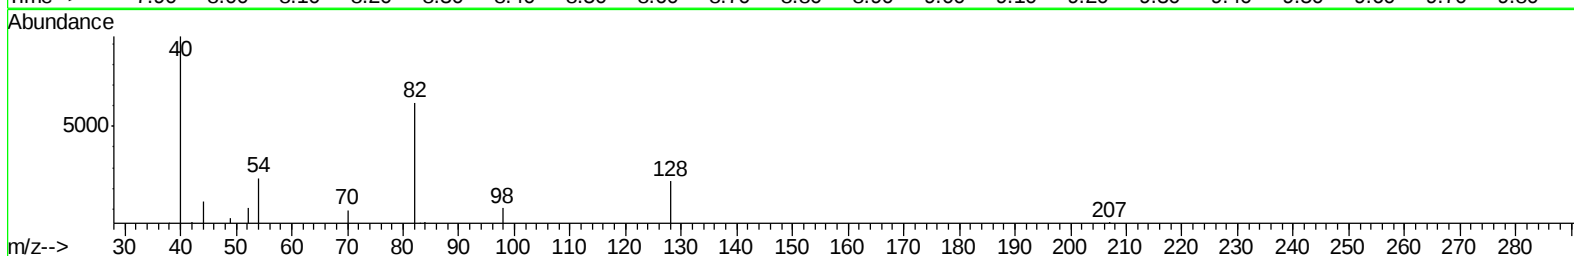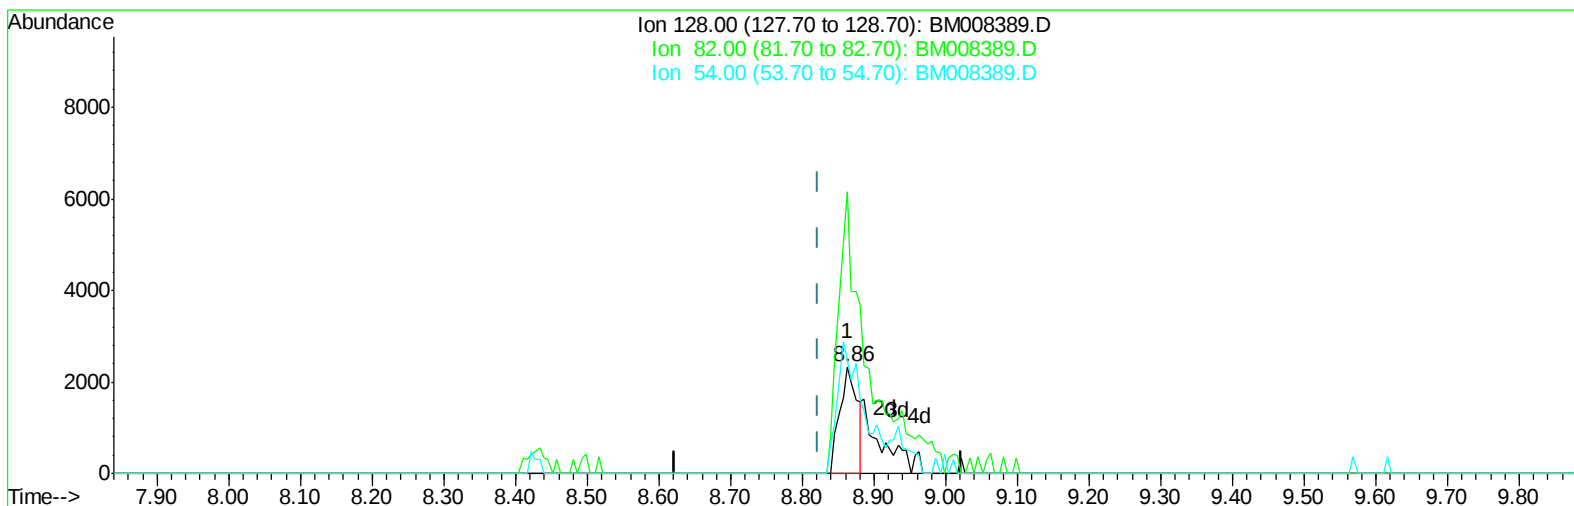

TIC: BM008389.D

(19) Nitrobenzene-d5 (S)

8.863min (+0.041) 1.31ng/ul

response 4003

Ion	Exp%	Act%
128.00	100	100
82.00	250.90	263.44
54.00	119.50	106.59
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

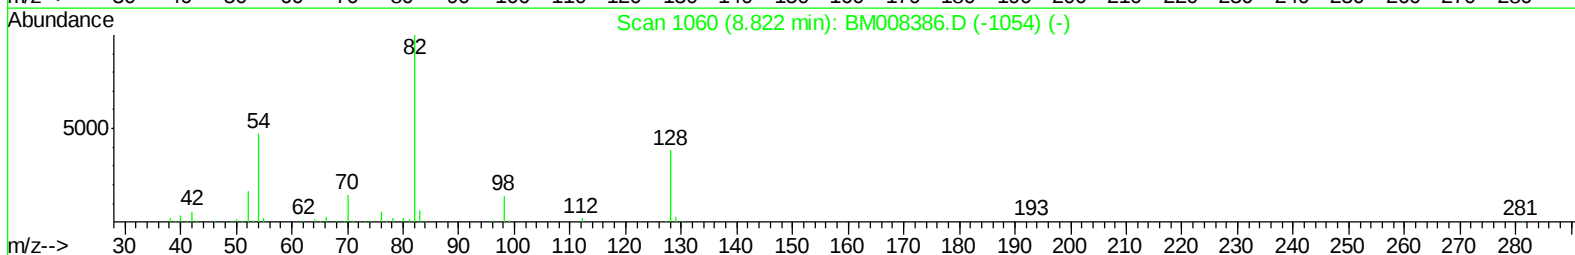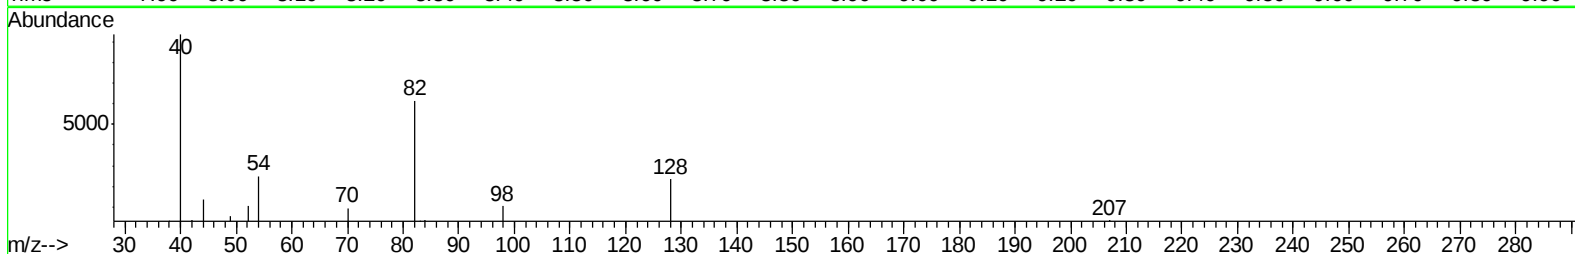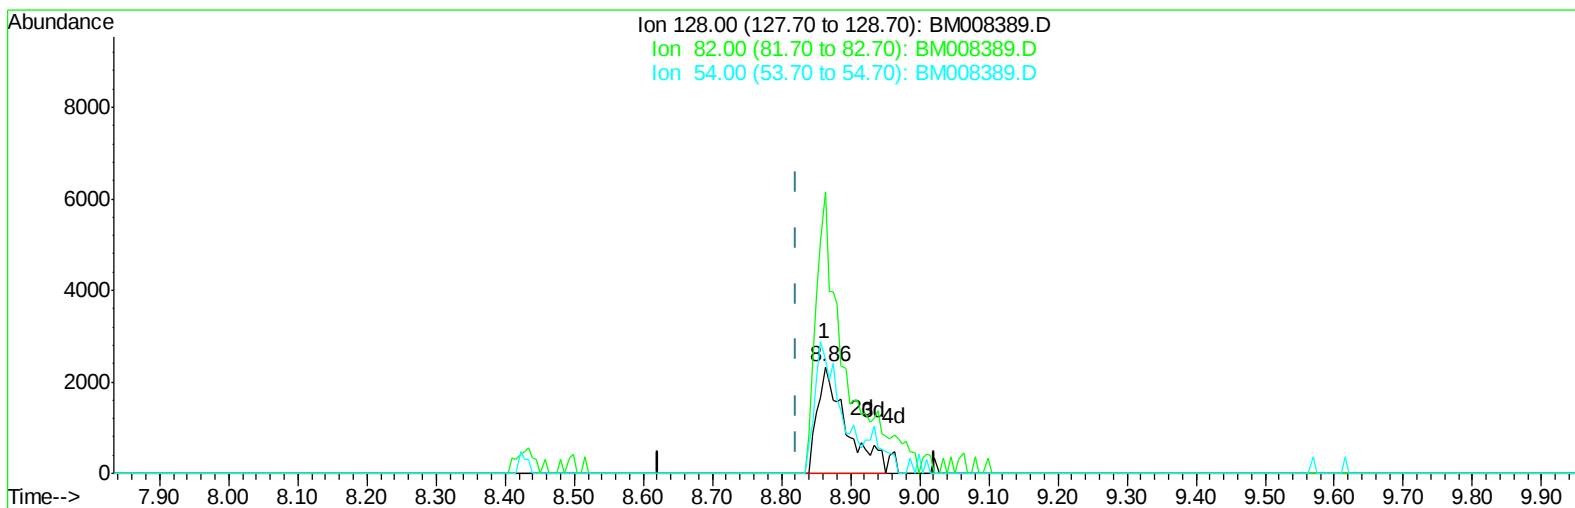

TIC: BM008389.D

(19) Nitrobenzene-d5 (S)

8.863min (+0.041) 2.21ng/ul m

response 6723

Ion	Exp%	Act%
128.00	100	100
82.00	250.90	263.44
54.00	119.50	106.59
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

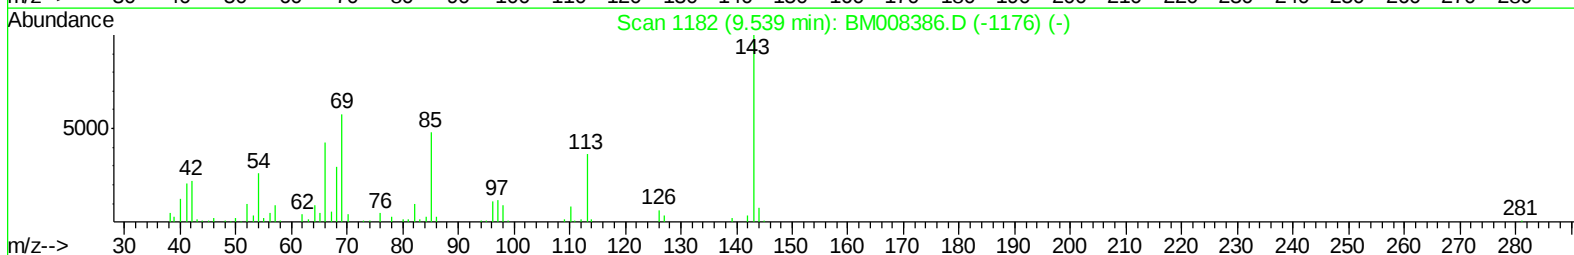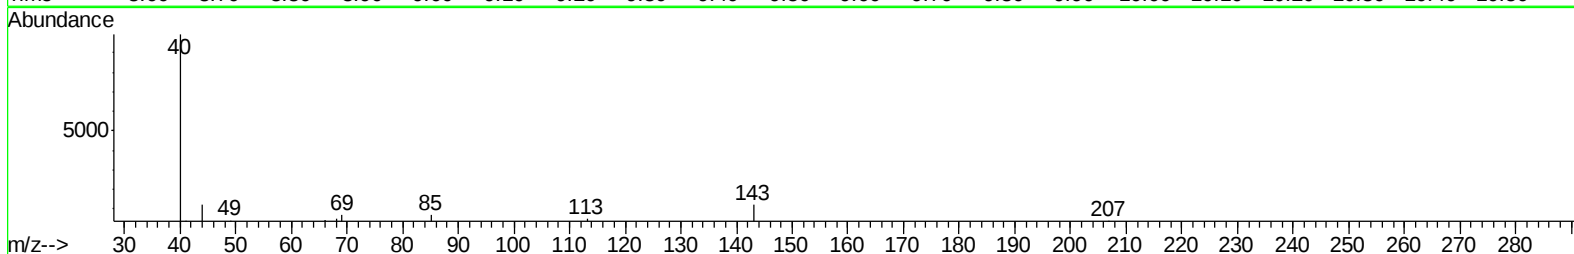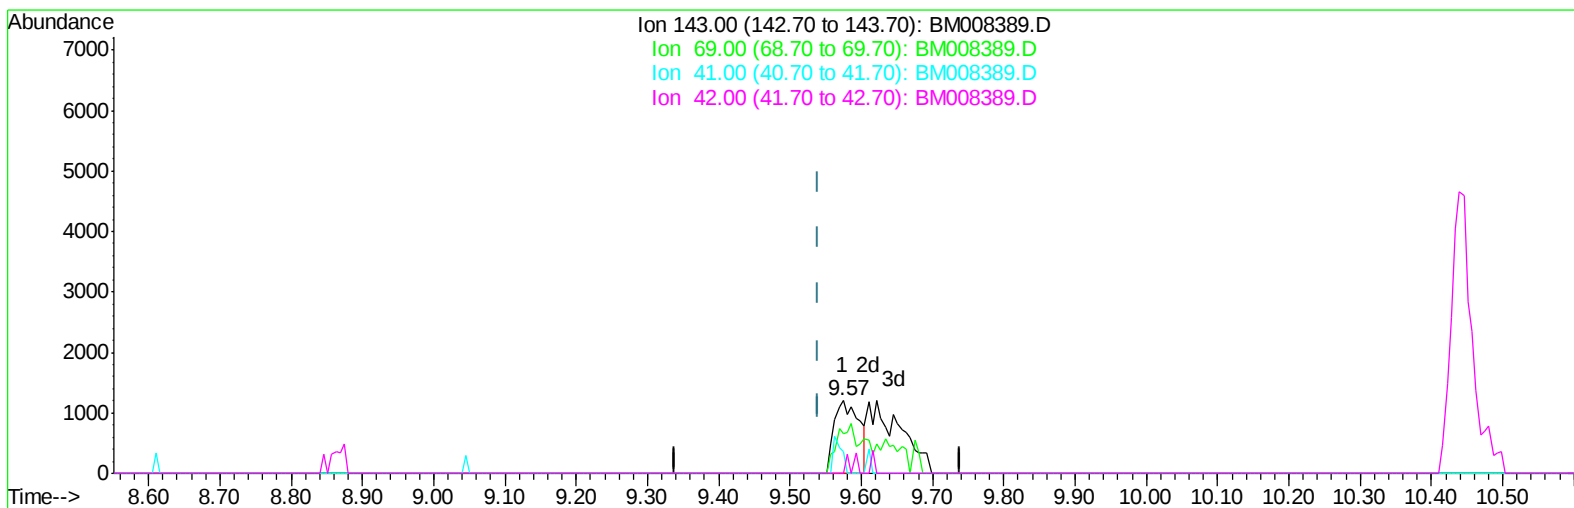

TIC: BM008389.D

(22) 2-Nitrophenol-d4 (S)
9.575min (+0.035) 0.87ng/ul

response 2929

Ion	Exp%	Act%
143.00	100	100
69.00	58.20	55.34
41.00	21.10	30.38#
42.00	24.40	0.00#




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

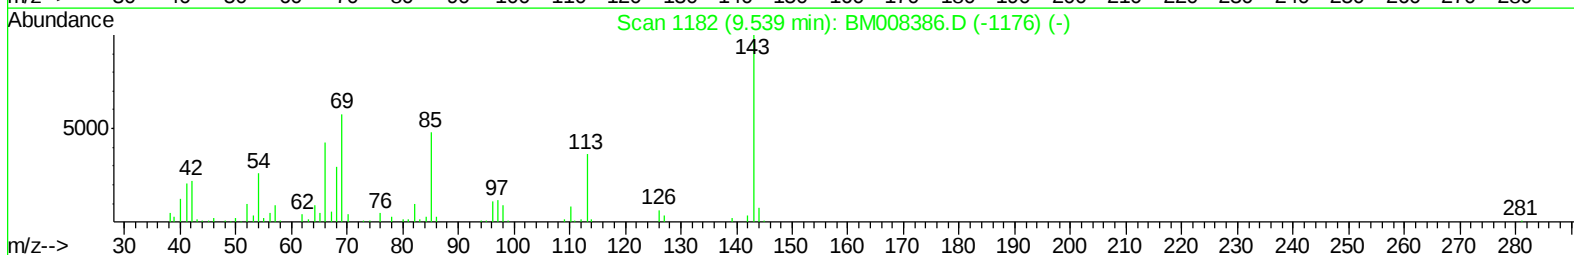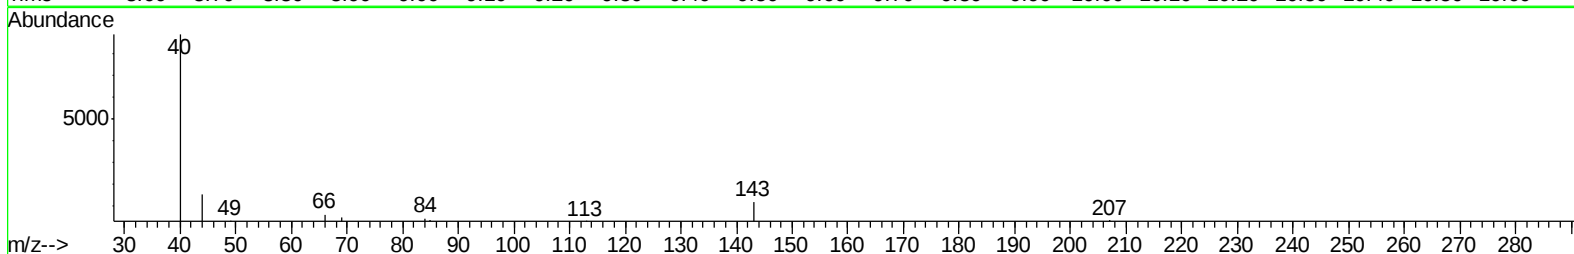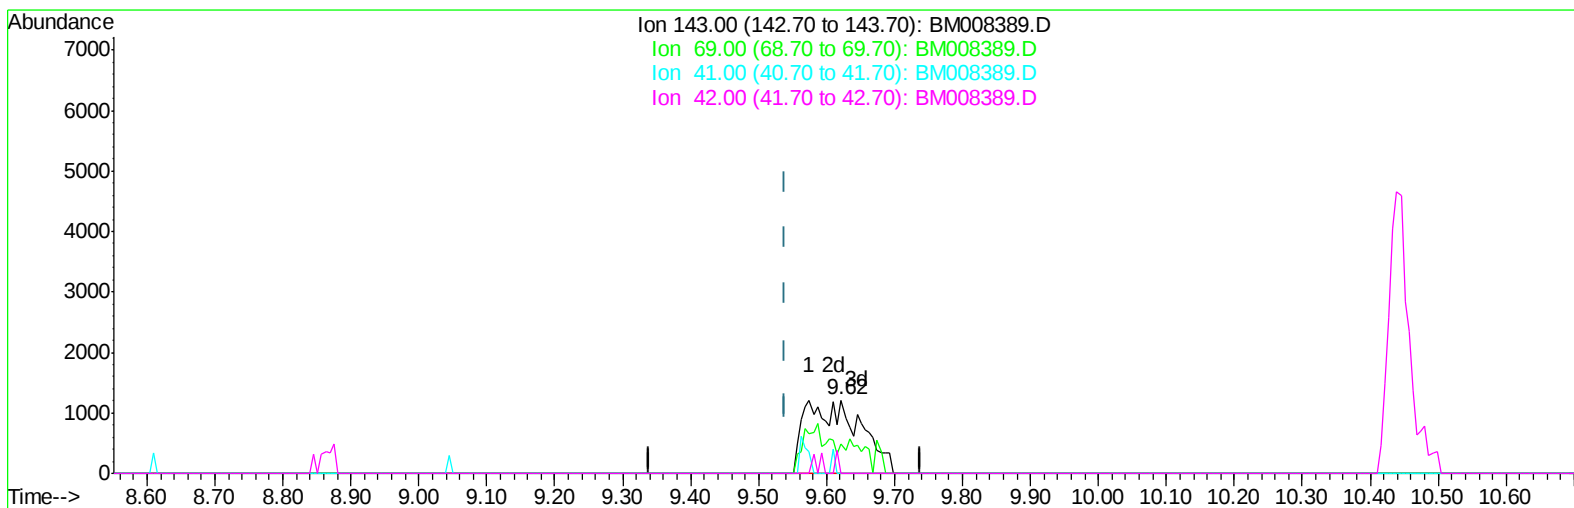

TIC: BM008389.D

(22) 2-Nitrophenol-d4 (S)

9.622min (+0.082) 1.98ng/ul m

response 6687

Ion	Exp%	Act%
143.00	100	100
69.00	58.20	40.05#
41.00	21.10	0.00#
42.00	24.40	0.00#




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

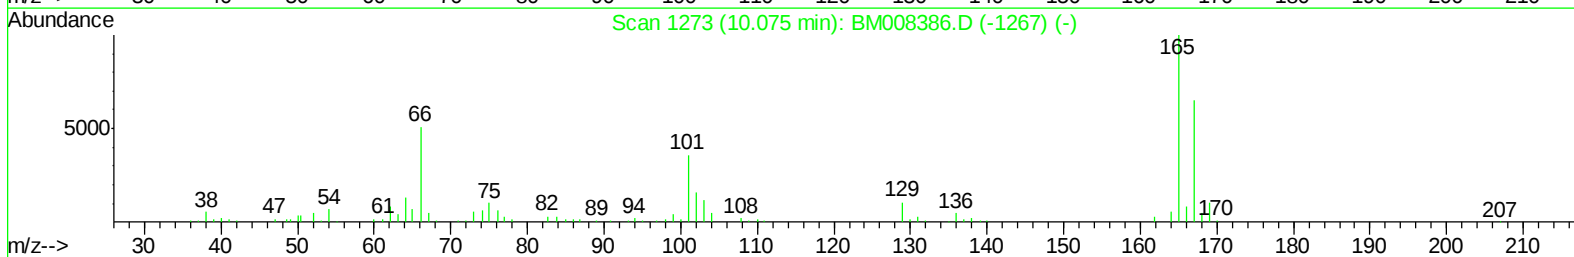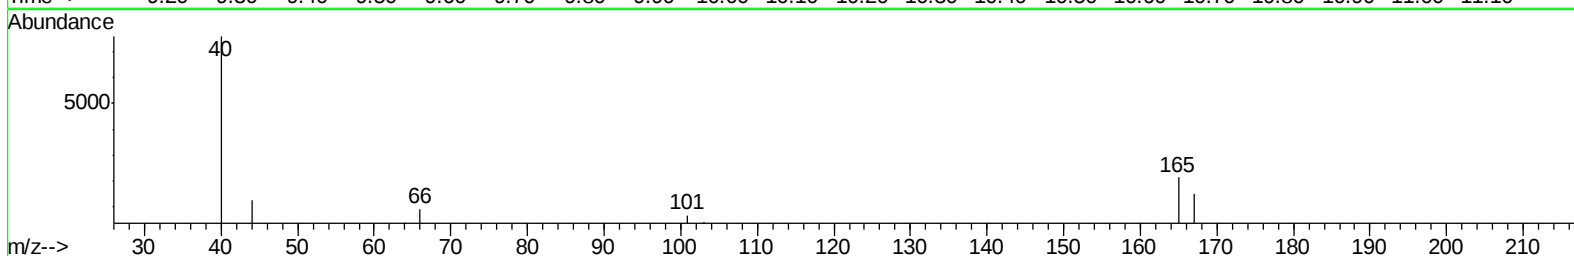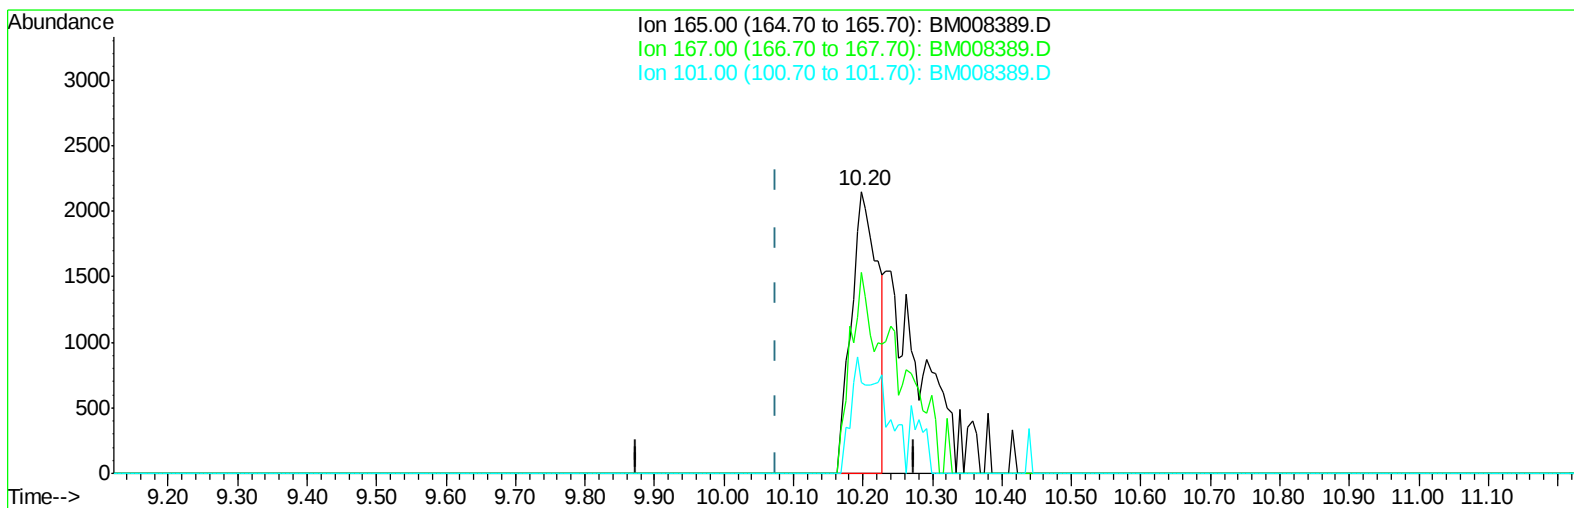

TIC: BM008389.D

(26) 2,4-Dichlorophenol-d3 (S)

10.198min (+0.124) 0.92ng/ul

response 5697

Ion	Exp%	Act%
165.00	100	100
167.00	64.50	71.37
101.00	35.20	32.31
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

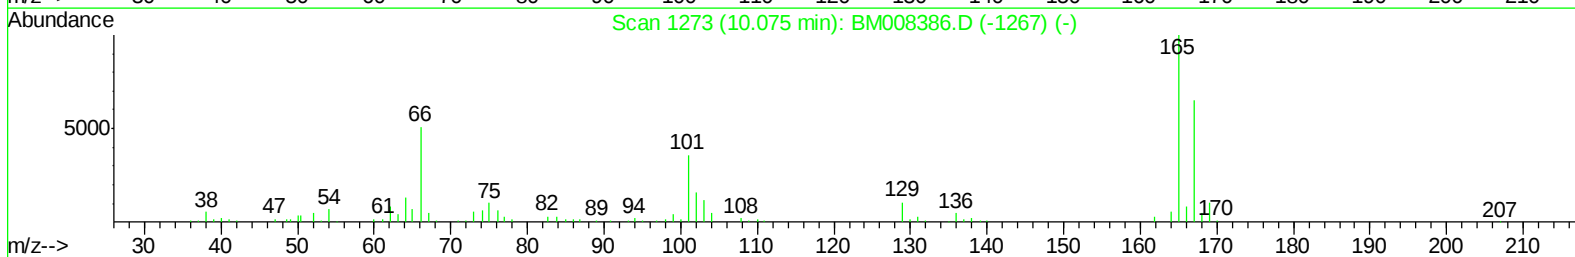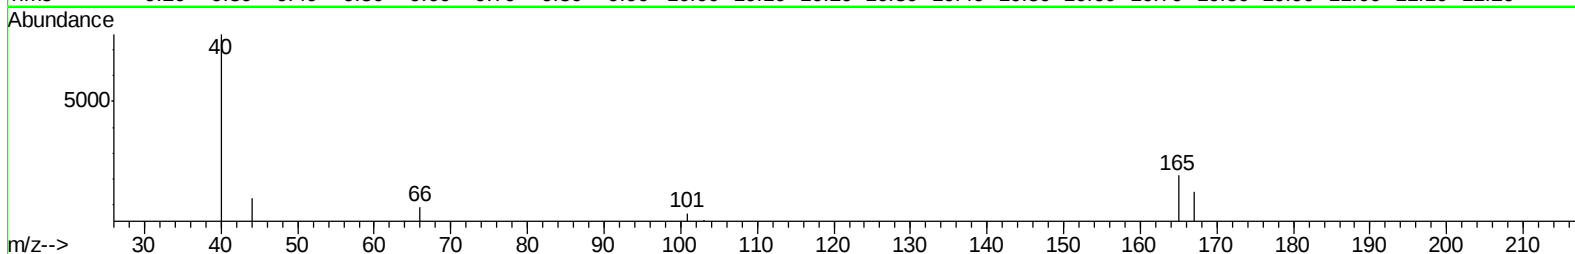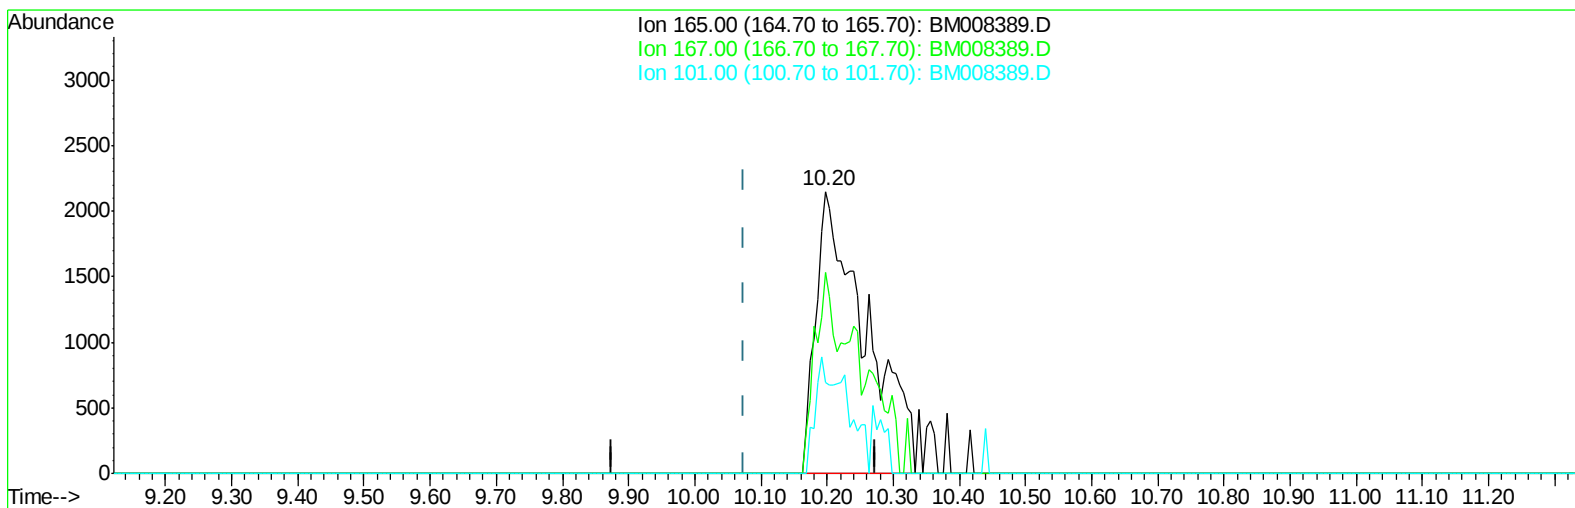

TIC: BM008389.D

(26) 2,4-Dichlorophenol-d3 (S)

10.198min (+0.124) 1.80ng/ul m

response 11113

Ion	Exp%	Act%
165.00	100	100
167.00	64.50	71.37
101.00	35.20	32.31
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

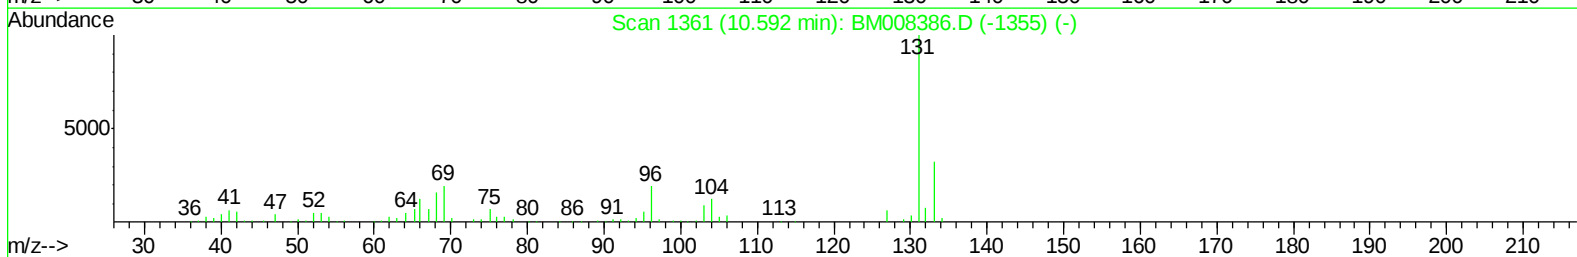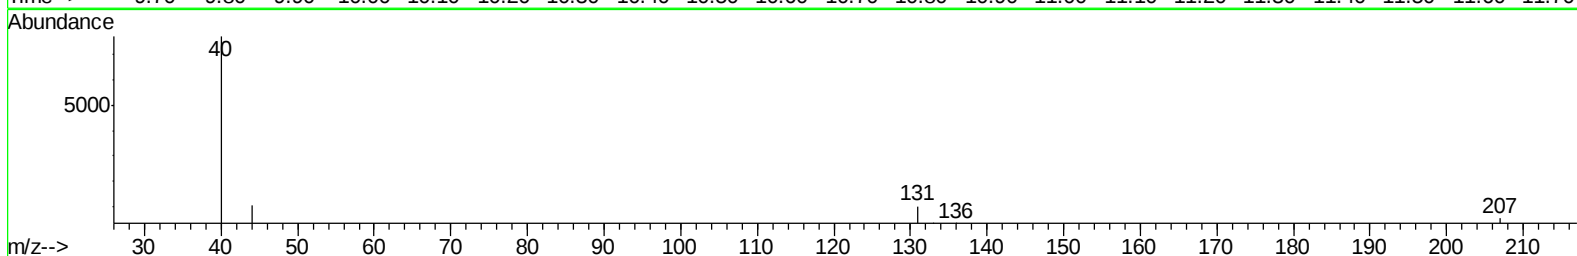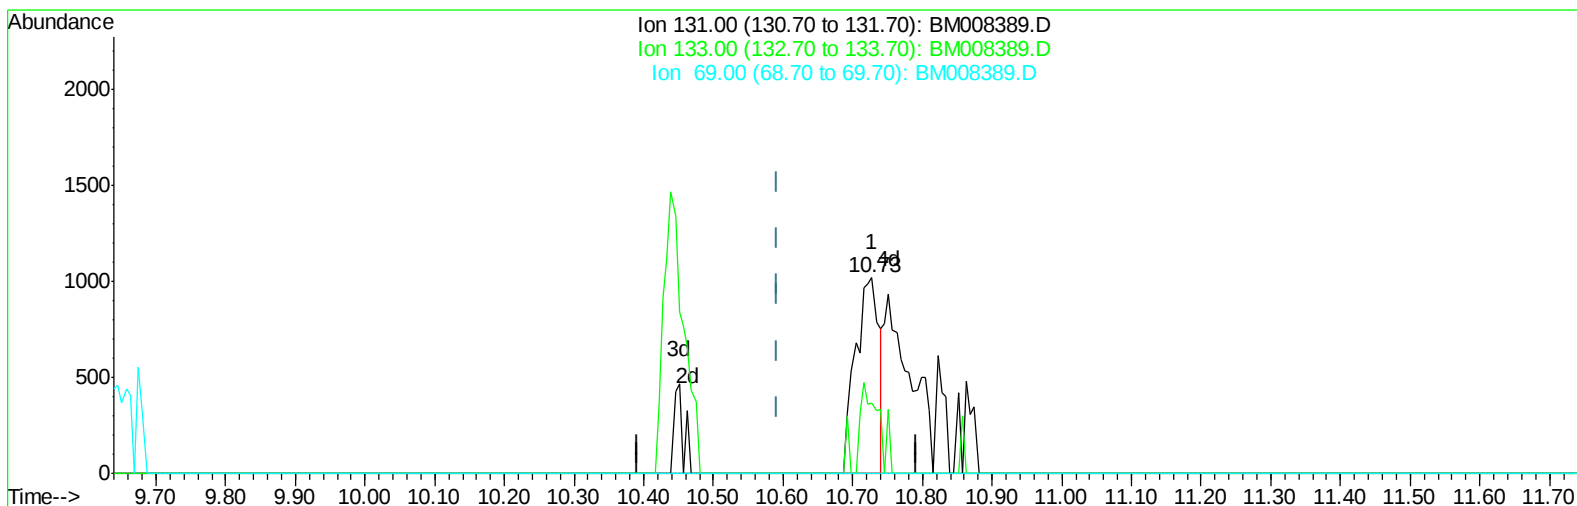

TIC: BM008389.D

(29) 4-Chloroaniline-d4 (S)
10.728min (+0.135) 0.33ng/ul
response 2351

Ion	Exp%	Act%
131.00	100	100
133.00	34.20	36.09
69.00	21.70	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

Quant Time: Dec 17 03:23:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

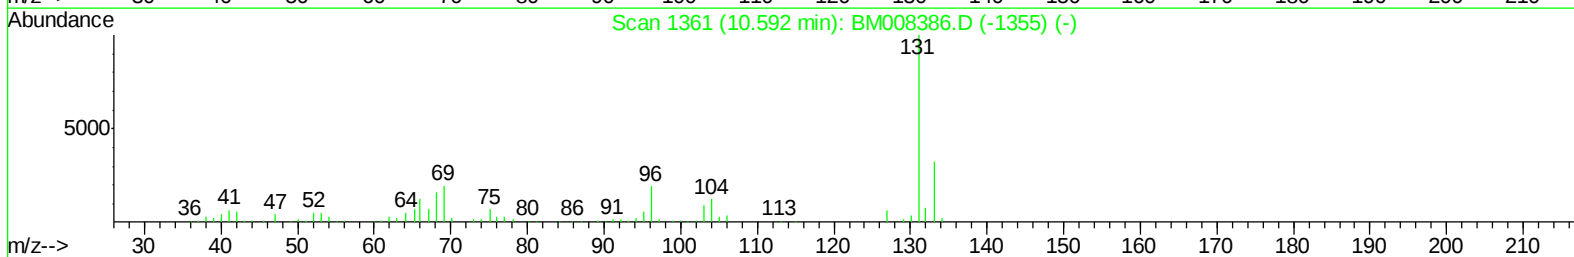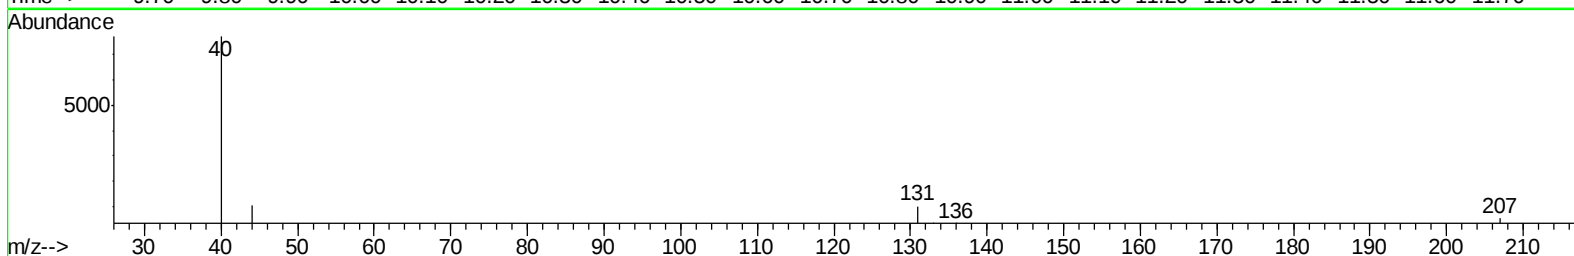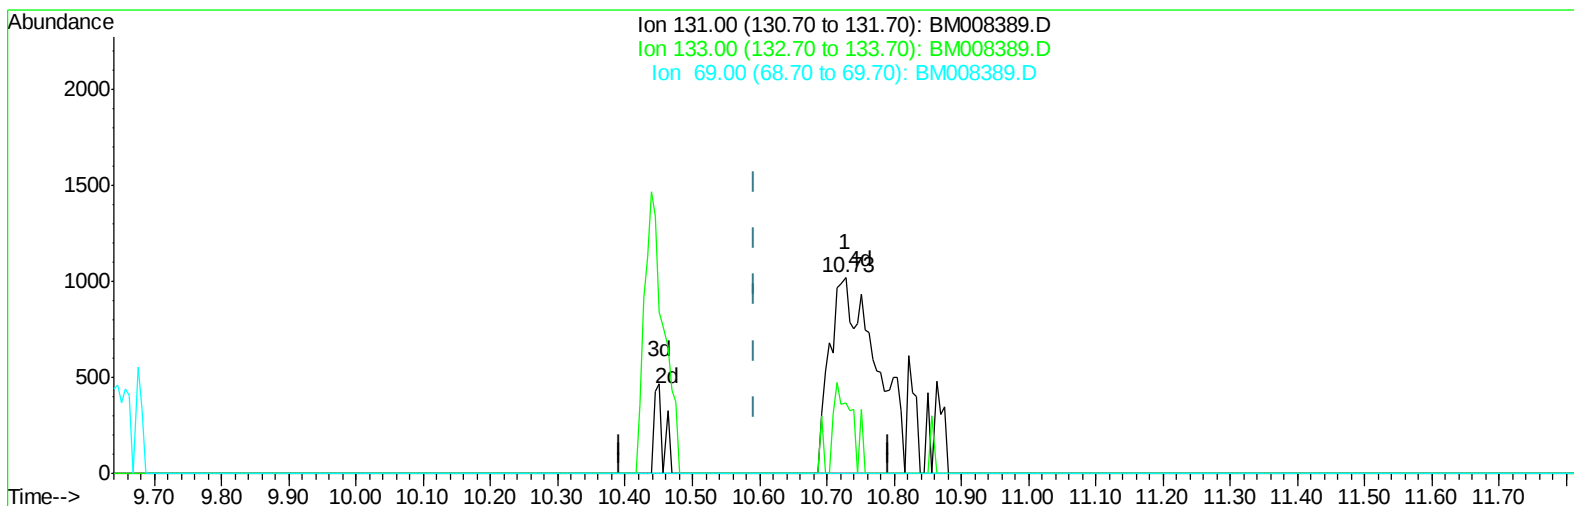

TIC: BM008389.D

(29) 4-Chloroaniline-d4 (S)

10.728min (+0.135) 0.68ng/ul m

response 4835

Ion	Exp%	Act%
131.00	100	100
133.00	34.20	36.09
69.00	21.70	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:48:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

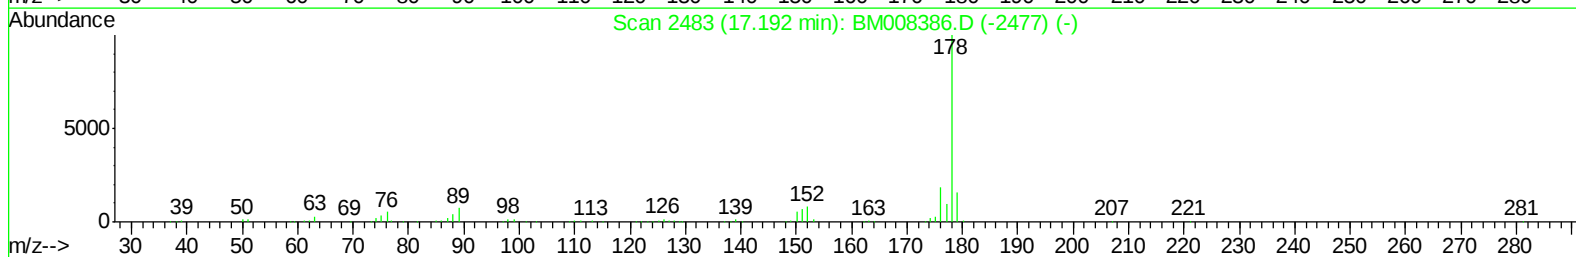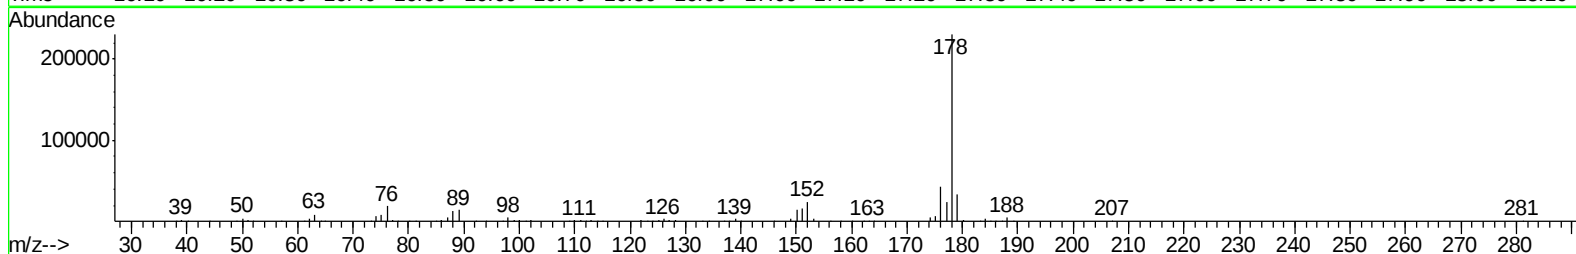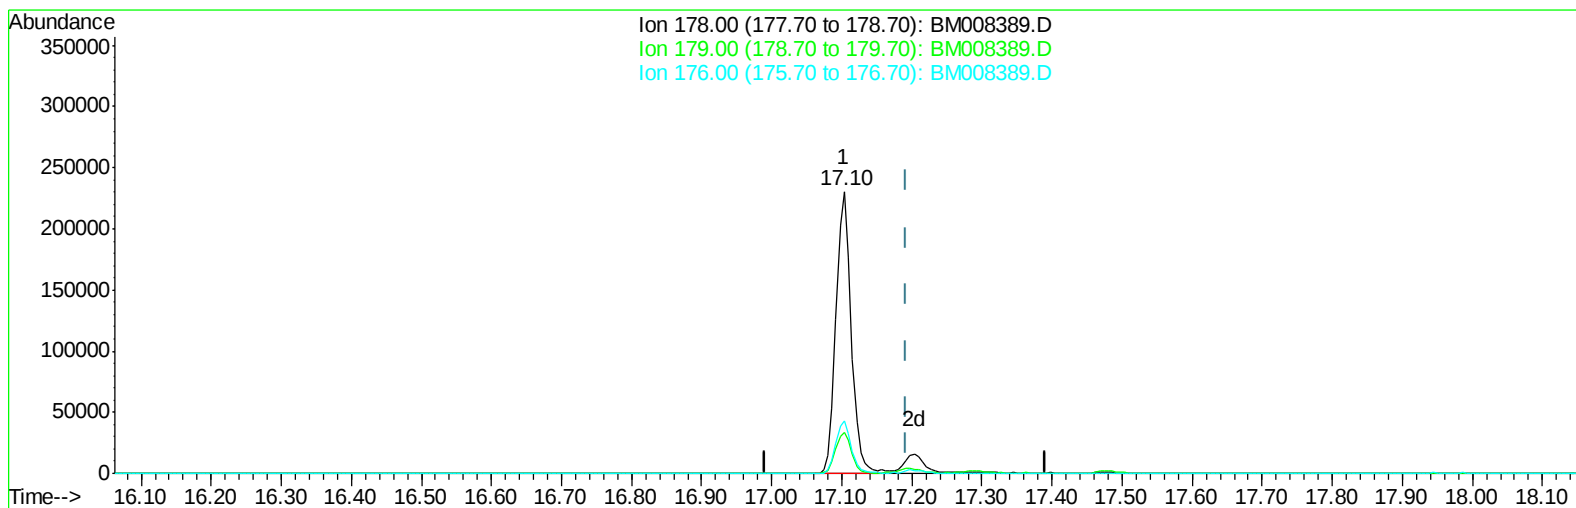

TIC: BM008389.D

(71) Anthracene

17.104min (-0.088) 12.29ng/ul

response 345232

Ion	Exp%	Act%
178.00	100	100
179.00	15.10	14.50
176.00	17.90	18.83
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:48:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

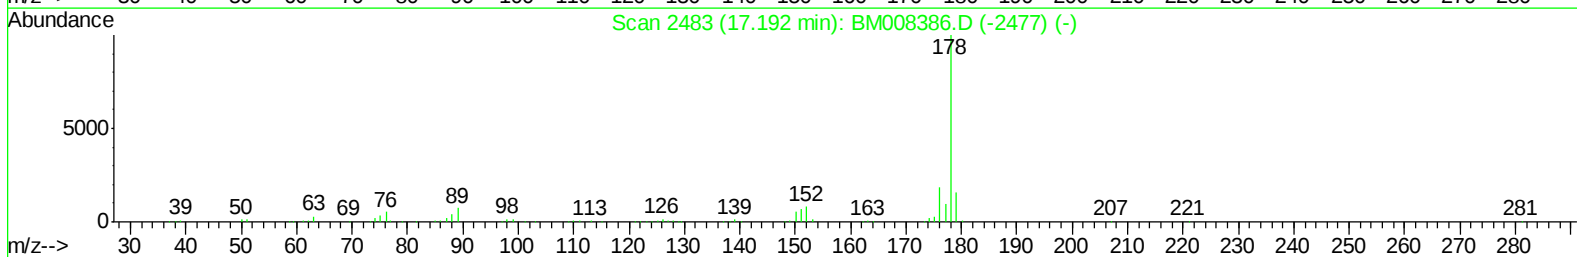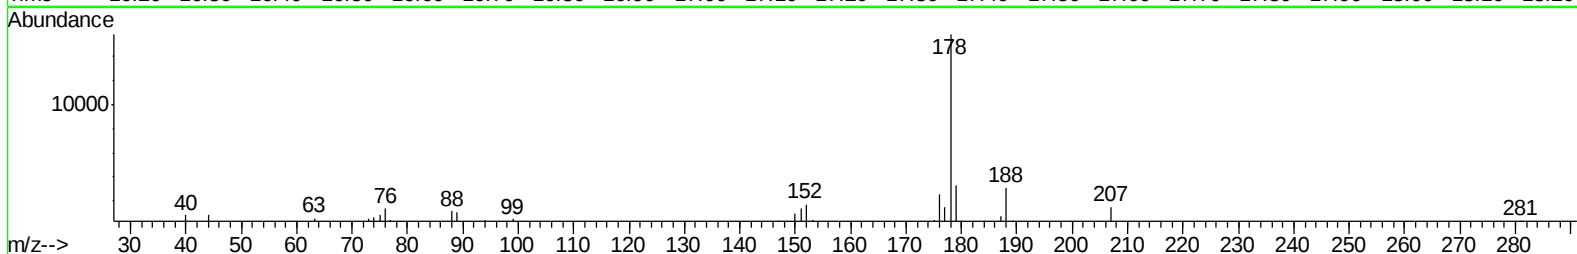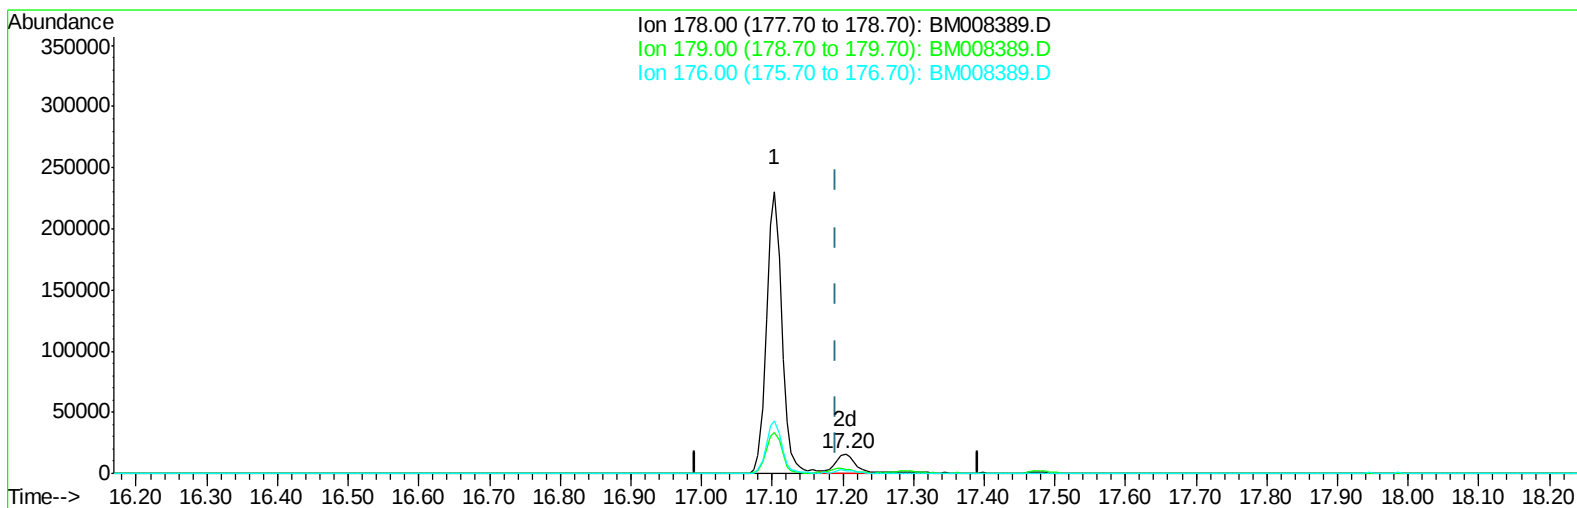

TIC: BM008389.D

(71) Anthracene

17.204min (+0.012) 1.08ng/ul m

response 30250

Ion	Exp%	Act%
178.00	100	100
179.00	15.10	21.00#
176.00	17.90	16.05
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:48:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

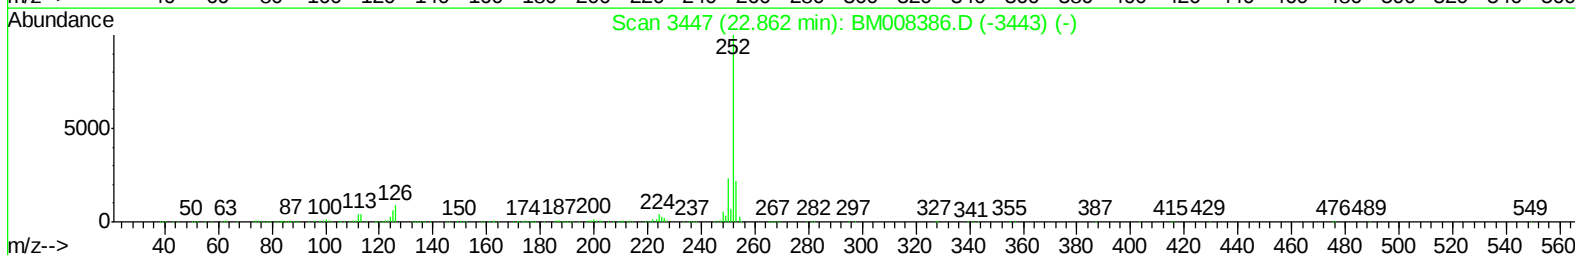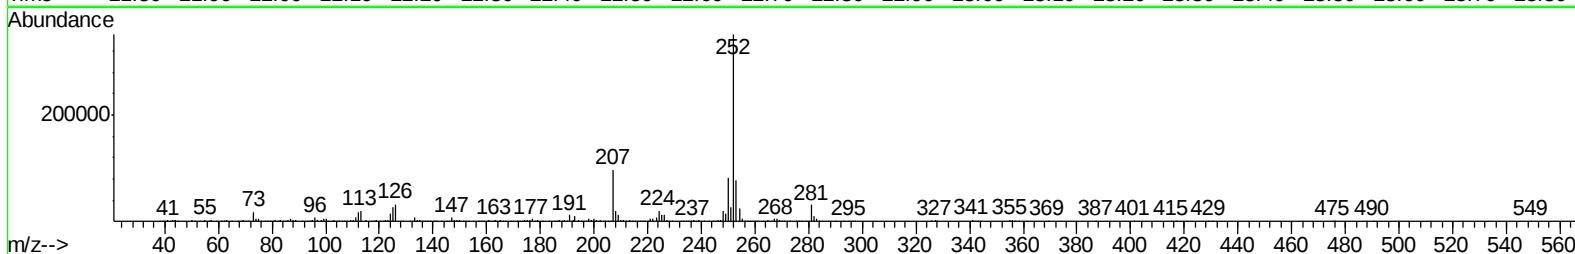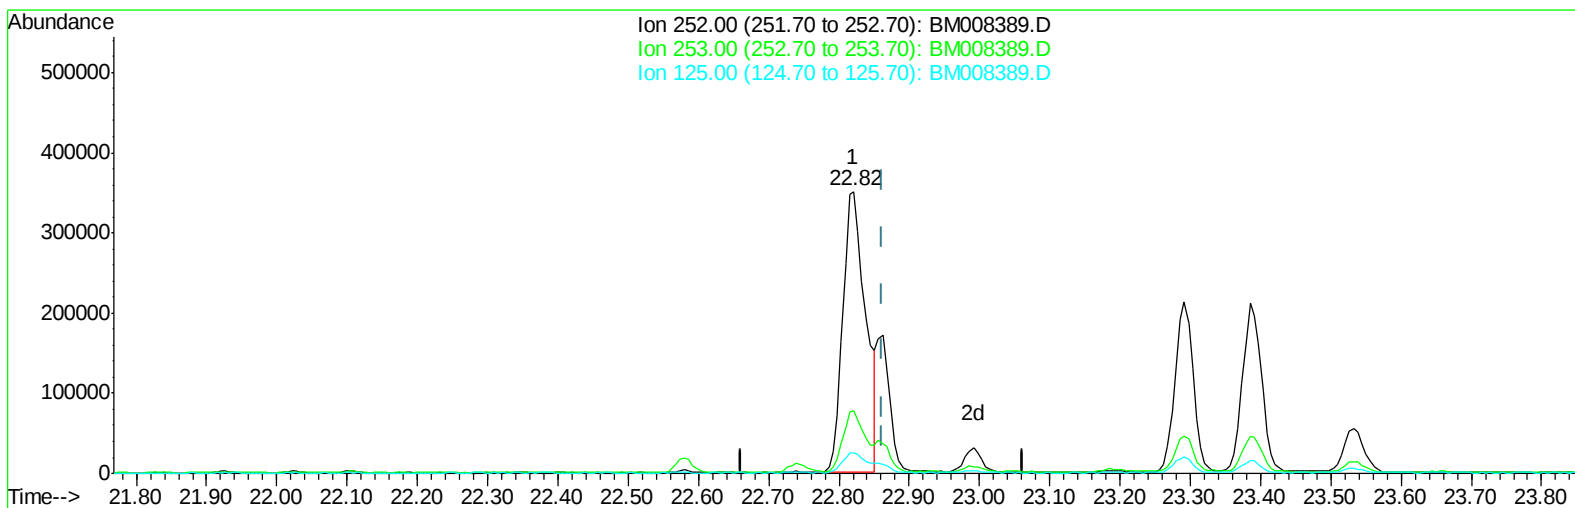

TIC: BM008389.D

(86) Benzo(k)fluoranthene

22.821min (-0.041) 20.06ng/ul

response 799691

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	22.23
125.00	7.20	7.35
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Quant Time: Dec 17 03:48:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM12
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

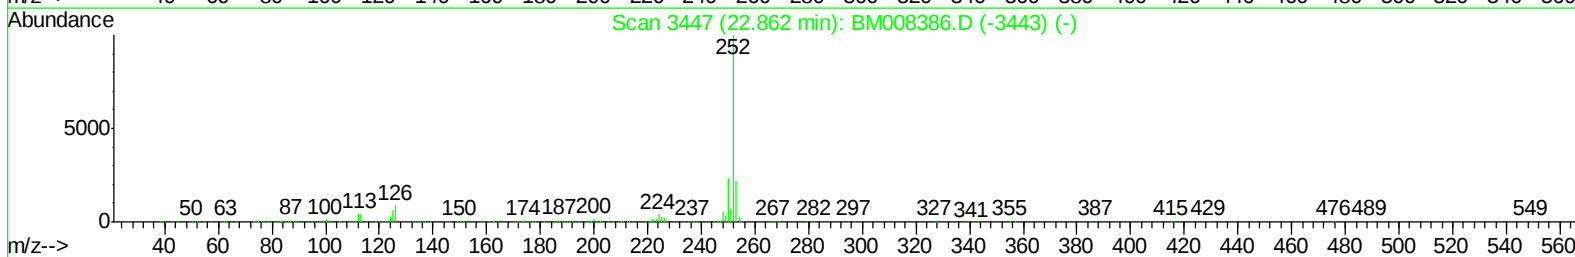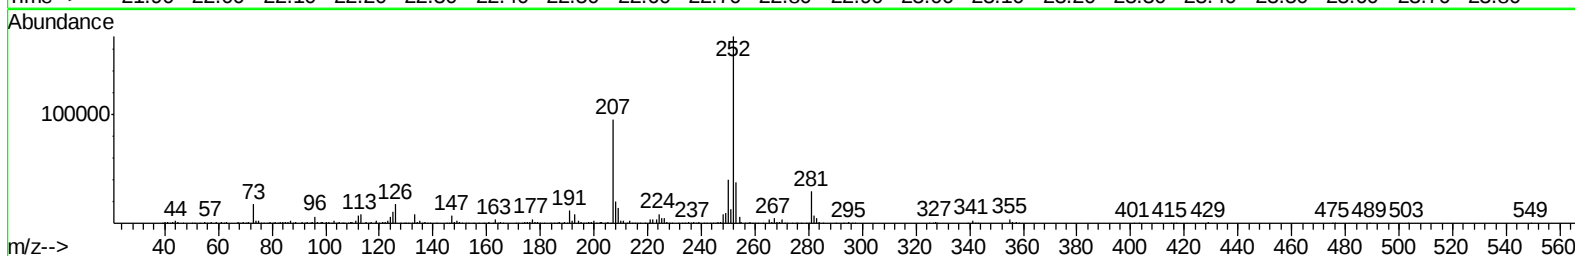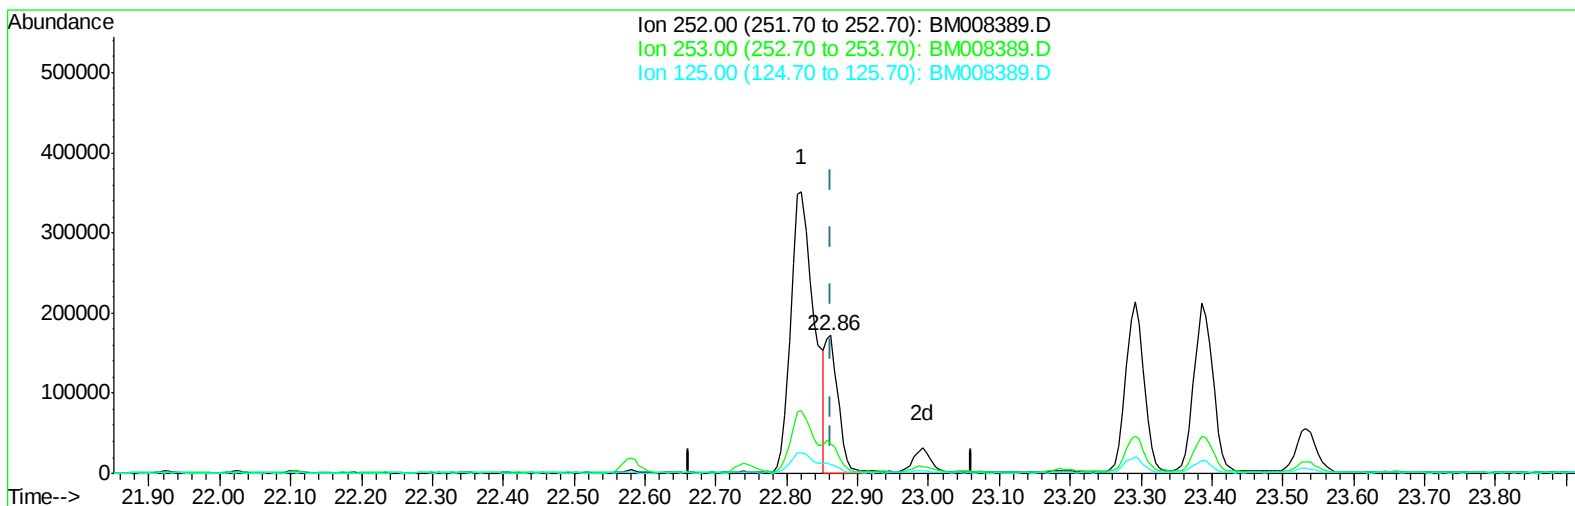

TIC: BM008389.D

(86) Benzo(k)fluoranthene

22.862min (+0.000) 5.53ng/ul m

response 220334

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	21.76
125.00	7.20	6.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
 Data File : BM008389.D
 Acq On : 17 Dec 2016 00:39
 Operator : UM/SJ
 Sample : H5937-13DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 DA8G5DL

Manual Integrations
 APPROVED

umangi
 12/20/2016 10:43:27 AM

Quant Time: Dec 17 03:49:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 17 03:19:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	109064	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	421723	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	267493	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	540011	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	727783	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	771692	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	968	0.42	ng/uL	0.00
5) Phenol-d5	6.90	99	15634m	1.85	ng/ul	0.05
7) Bis-(2-Chloroethyl)ether-d	7.03	67	11483m	2.36	ng/ul	0.02
9) 2-Chlorophenol-d4	7.22	132	14940m	2.35	ng/ul	0.02
13) 4-Methylphenol-d8	8.43	113	5016	0.77	ng/ul	0.05
19) Nitrobenzene-d5	8.86	128	6723m	2.21	ng/ul	0.04
22) 2-Nitrophenol-d4	9.62	143	6687m	1.98	ng/ul	0.08
26) 2,4-Dichlorophenol-d3	10.20	165	11113m	1.80	ng/ul	0.12
29) 4-Chloroaniline-d4	10.73	131	4835m	0.68	ng/ul	0.14
43) Dimethylphthalate-d6	13.74	166	46406	2.61	ng/ul	0.02
46) Acenaphthylene-d8	14.00	160	59144	2.81	ng/ul	0.01
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.32	176	46494	3.01	ng/ul	0.02
62) 4,6-Dinitro-2-methylphenol	15.52	200	1686	0.52	ng/ul	0.06
70) Anthracene-d10	17.16	188	72539	3.08	ng/ul	0.00
76) Pyrene-d10	19.46	212	91855	3.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	103212	3.19	ng/ul	0.00

Target Compounds

						Qvalue
69) Phenanthrene	17.10	178	345232	12.48	ng/ul	99
71) Anthracene	17.20	178	30250m	1.08	ng/ul	
72) Carbazole	17.49	167	59379	2.40	ng/ul	98
74) Fluoranthene	19.12	202	1068340	31.43	ng/ul	99
77) Pyrene	19.49	202	892731	24.98	ng/ul	99
80) Benzo(a)anthracene	21.24	228	361948	9.62	ng/ul	98
82) Chrysene	21.29	228	544327	15.05	ng/ul	98
85) Benzo(b)fluoranthene	22.82	252	799691	19.20	ng/ul	98
86) Benzo(k)fluoranthene	22.86	252	220334m	5.53	ng/ul	
88) Benzo(a)pyrene	23.39	252	392289	9.77	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.71	276	403547	8.28	ng/ul	97
90) Dibenzo(a,h)anthracene	25.71	278	92200	2.25	ng/ul#	83
91) Benzo(g,h,i)perylene	26.40	276	405442	9.95	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121716\
Data File : BM008389.D
Acq On : 17 Dec 2016 00:39
Operator : UM/SJ
Sample : H5937-13DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8G5DL

Manual Integrations
APPROVED

umangi
12/20/2016 10:43:27 AM

Quant Time: Dec 17 03:49:47 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121716.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 17 03:19:37 2016
Response via : Initial Calibration

