

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
 Data File : BM024127.D
 Acq On : 17 Dec 2019 18:34
 Operator : JU
 Sample : PB125268BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 18 00:21:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 17 15:54:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	265749	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	1256361	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.12	164	850741	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	1851693	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	1832245	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	2224123	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.01	96	51364	8.54	ng/uL	0.00
5) Phenol-d5	6.65	99	856810	34.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	583753	38.68	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	665542	37.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	720230	35.01	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	348353	38.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	385799	38.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	666141	34.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	1032796	44.07	ng/ul	0.00
44) Dimethylphthalate-d6	13.54	166	2477197	39.38	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	2843359	37.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	345476	30.59	ng/ul	0.00
58) Fluorene-d10	15.12	176	2126667	38.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	335954	29.74	ng/ul	0.00
71) Anthracene-d10	16.97	188	3328681	39.51	ng/ul	0.00
79) Pyrene-d10	19.27	212	3632575	41.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	4414539	39.96	ng/ul	0.00
Target Compounds						
15) N-Nitroso-di-n-propylamine	8.17	70	18892	1.102	ng/ul#	1
46) 2,6-Dinitrotoluene	13.54	165	16325	1.268	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
Data File : BM024127.D
Acq On : 17 Dec 2019 18:34
Operator : JU
Sample : PB125268BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 18 00:21:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 17 15:54:50 2019
Response via : Initial Calibration

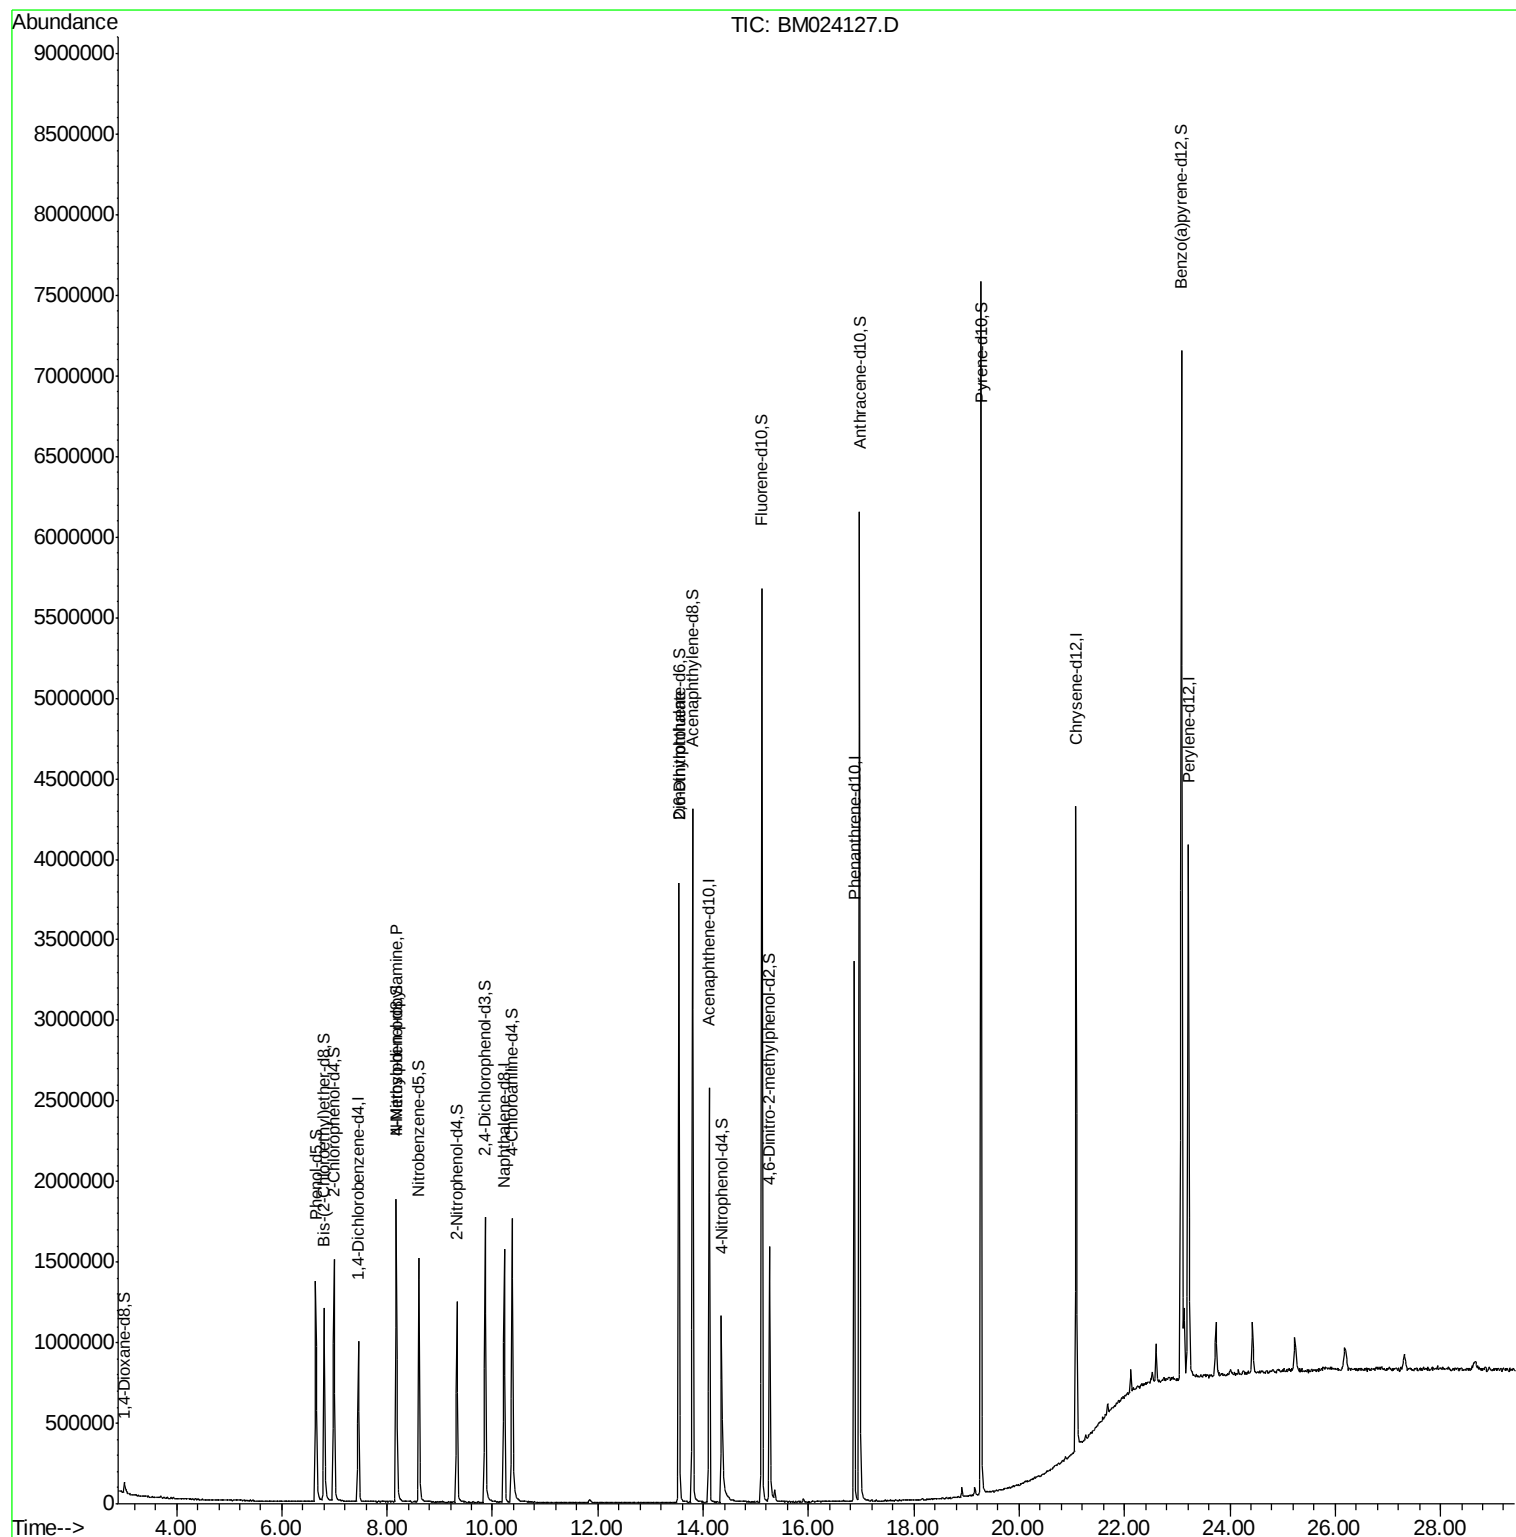

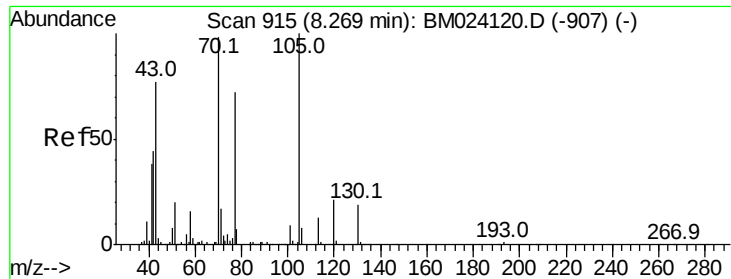

#15

N-Nitroso-di-n-propylamine

Concen: 1.102 ng/ul

RT: 8.17 min Scan# 899

Delta R.T. -0.09 min

Lab File: BM024127.D

Acq: 17 Dec 2019 18:34

Instrument :

BNA_M

ClientSampled :

Tot Ion: 70 Resp: 18892


Ion Ratio Lower Upper

70 100

42 312.9 36.2 54.4#

101 0.0 7.7 11.5#

130 0.0 15.3 22.9#



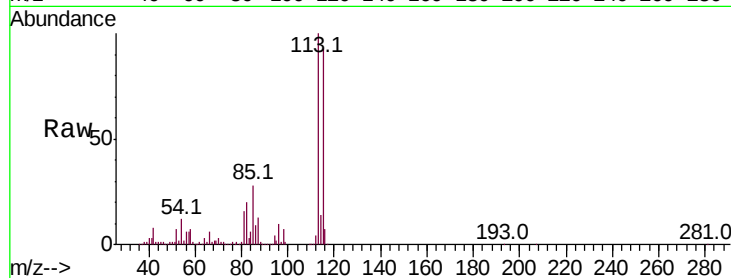


Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

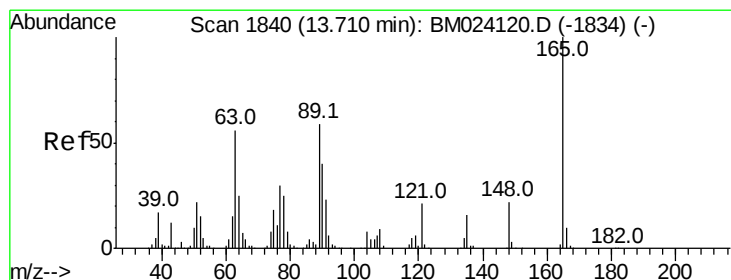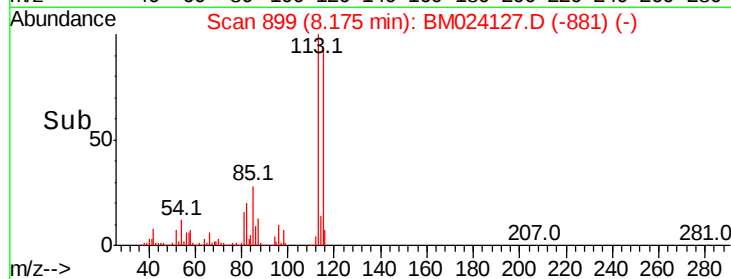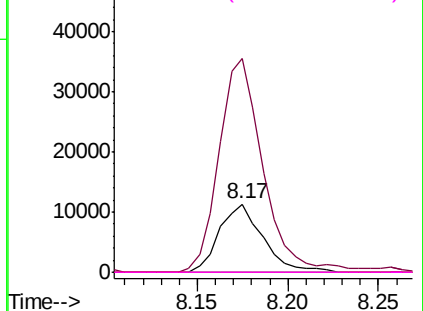

#46

2,6-Dinitrotoluene

Concen: 1.268 ng/ul

RT: 13.54 min Scan# 1811

Delta R.T. -0.17 min

Lab File: BM024127.D

Acq: 17 Dec 2019 18:34


Tgt Ion:165 Resp: 16325

Ion Ratio Lower Upper

165 100

89 0.0 47.0 70.4#

121 38.9 17.1 25.7#

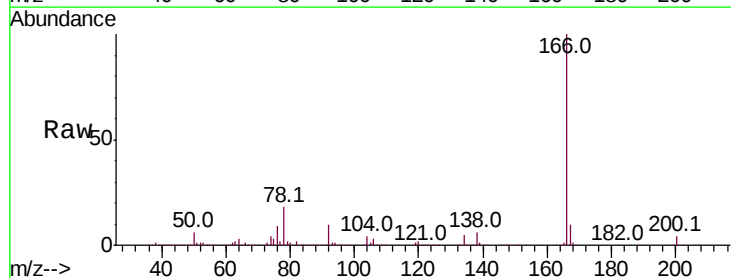

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

