

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
 Data File : BM024132.D
 Acq On : 17 Dec 2019 21:34
 Operator : JU
 Sample : K6132-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQR4

Quant Time: Dec 18 00:22:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 17 15:54:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	423455	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	2021471	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	1320966	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	2835055	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	2504636	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	2367054	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.01	96	47355	4.94	ng/uL	0.00
5) Phenol-d5	6.65	99	213643	5.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	499108	20.76	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	538964	18.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	415395	12.67	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	324699	22.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	374166	23.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	707098	22.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	285887	7.58	ng/ul	0.00
44) Dimethylphthalate-d6	13.54	166	2449169	25.07	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	2831307	24.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	83614	4.77	ng/ul	0.01
58) Fluorene-d10	15.12	176	2132454	24.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	389572	22.53	ng/ul	0.00
71) Anthracene-d10	16.97	188	3342471	25.91	ng/ul	0.00
79) Pyrene-d10	19.27	212	3542525	29.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	3123678	26.57	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.59	163	186276	1.835	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
Data File : BM024132.D
Acq On : 17 Dec 2019 21:34
Operator : JU
Sample : K6132-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQR4

Quant Time: Dec 18 00:22:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 17 15:54:50 2019
Response via : Initial Calibration

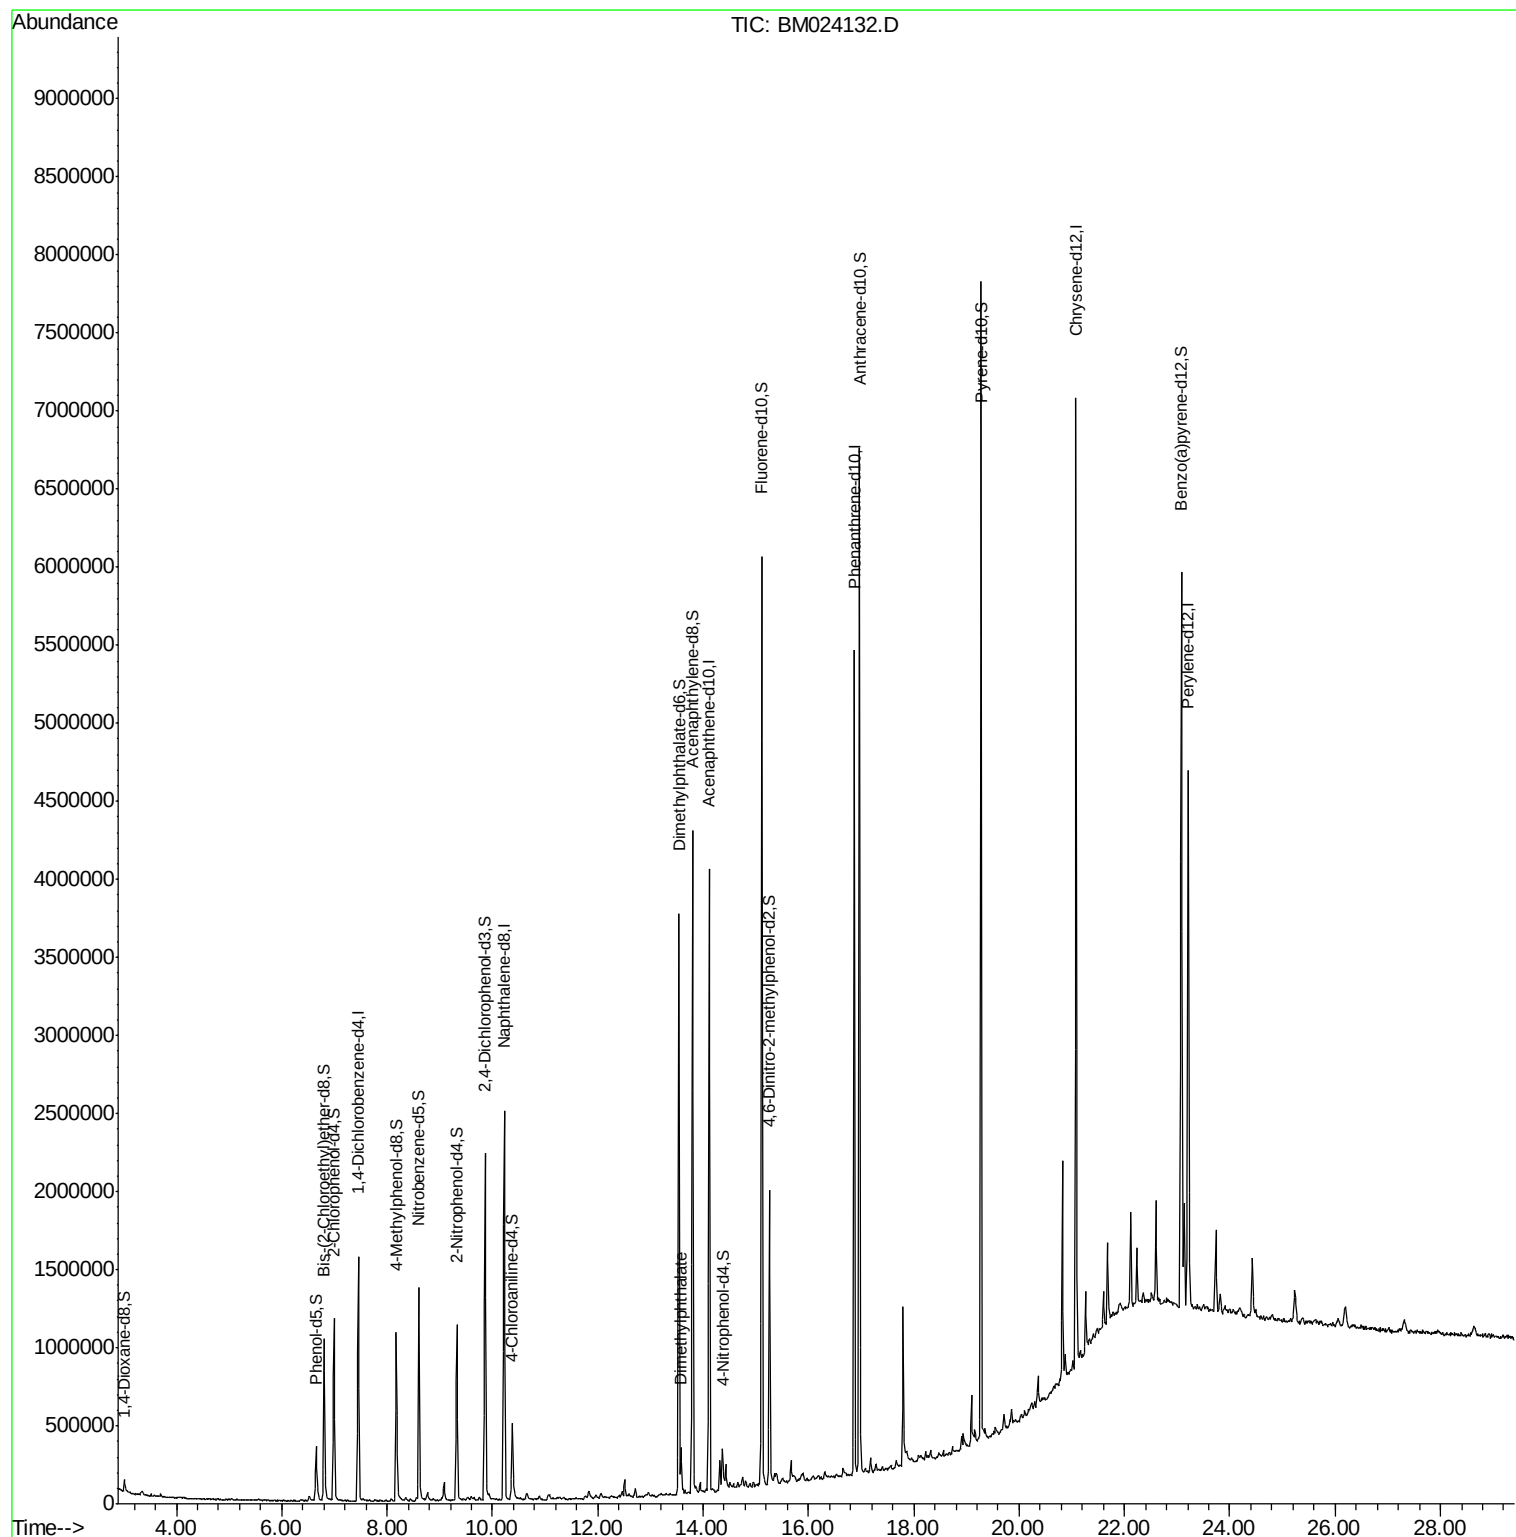

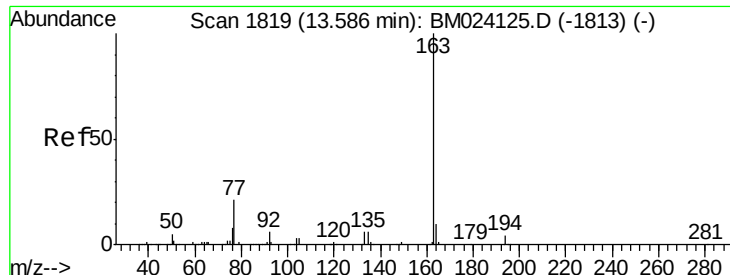

#45

Dimethylphthalate

Concen: 1.835 ng/ul

RT: 13.59 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM024132.D

Acq: 17 Dec 2019 21:34

Instrument :

BNA_M

ClientSampleId :

BFQR4


Tot Ion:163 Resp: 186276

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.1 7.8 11.6

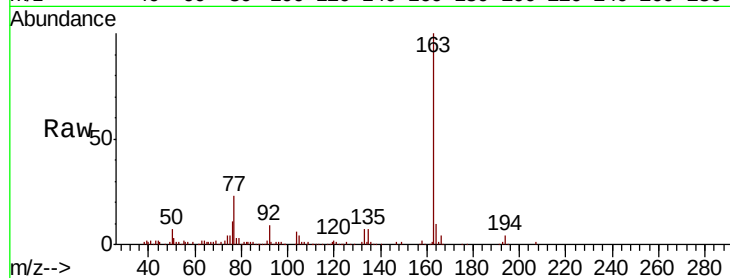

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

