

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
 Data File : BM024134.D
 Acq On : 17 Dec 2019 22:45
 Operator : JU
 Sample : K6132-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQX5

Quant Time: Dec 18 00:22:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 17 15:54:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	383364	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	1847190	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	1214411	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	2581020	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	2399144	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	2370514	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.01	96	50919	5.87	ng/uL	0.00
5) Phenol-d5	6.65	99	219477	6.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	589249	27.07	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	602113	23.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	417954	14.09	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	383626	28.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	441778	30.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	735911	25.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	48730	1.41	ng/ul	0.02
44) Dimethylphthalate-d6	13.54	166	2702132	30.09	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	3234771	30.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	69058	4.28	ng/ul	0.01
58) Fluorene-d10	15.12	176	2429790	30.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	446603	28.36	ng/ul	0.00
71) Anthracene-d10	16.97	188	4232748	36.04	ng/ul	0.00
79) Pyrene-d10	19.27	212	4578778	40.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	4355698	36.99	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.59	163	156188	1.674	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
Data File : BM024134.D
Acq On : 17 Dec 2019 22:45
Operator : JU
Sample : K6132-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQX5

Quant Time: Dec 18 00:22:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 17 15:54:50 2019
Response via : Initial Calibration

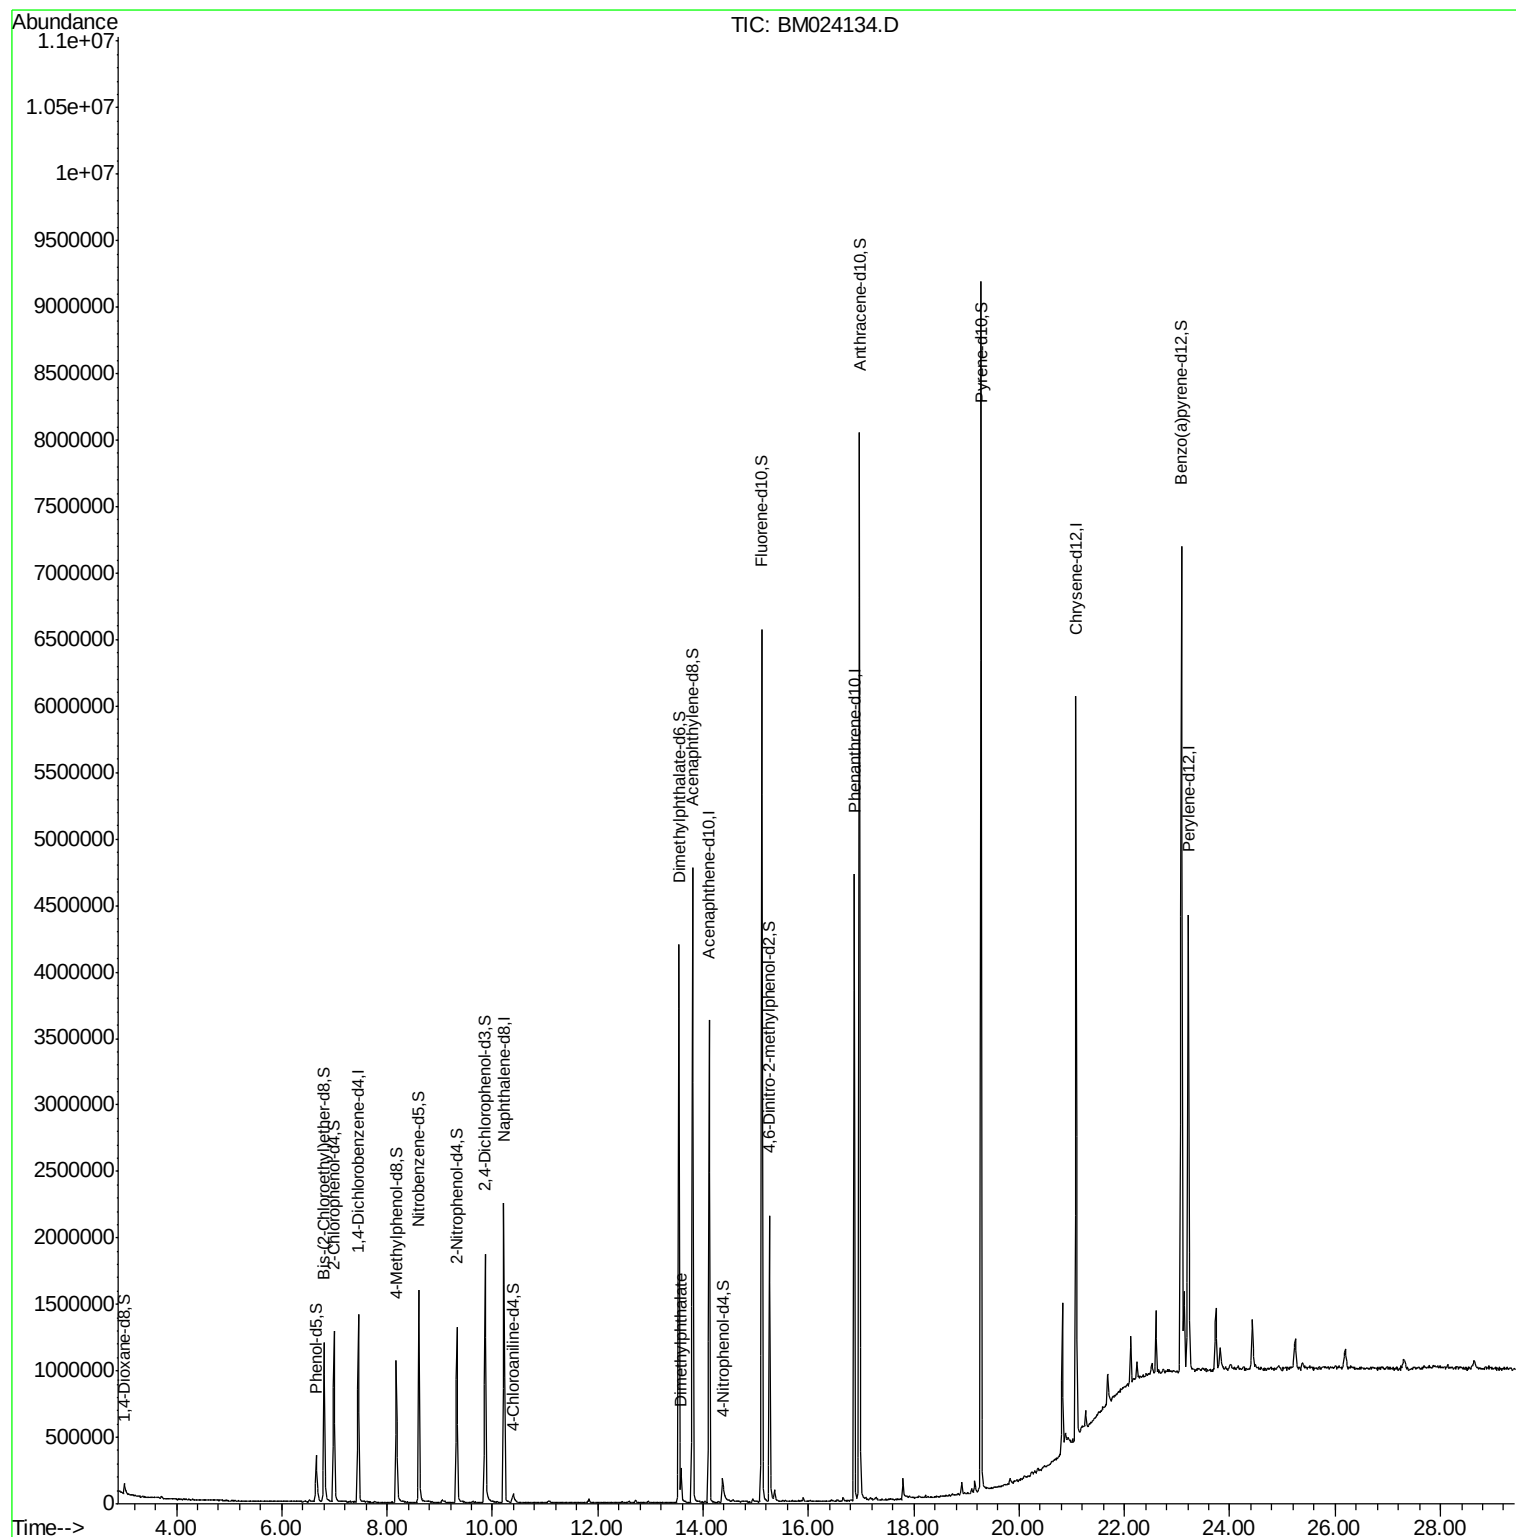

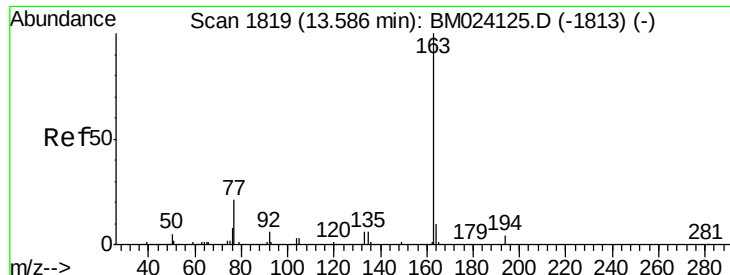

#45

Dimethylphthalate

Concen: 1.674 ng/ul

RT: 13.59 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM024134.D

Acq: 17 Dec 2019 22:45

Instrument :

BNA_M

ClientSampleId :

BFQX5


Tot Ion:163 Resp: 156188

Ion Ratio Lower Upper

163 100

194 4.6 3.2 4.8

164 10.7 7.8 11.6

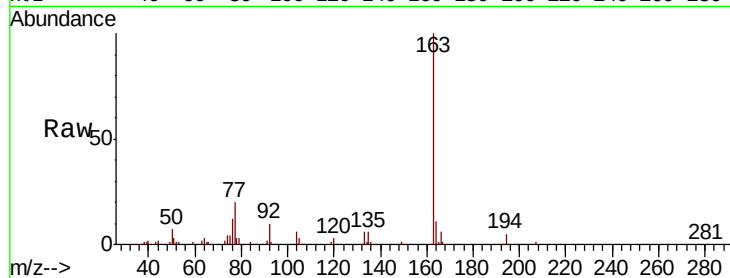

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

