

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
 Data File : BM024136.D
 Acq On : 17 Dec 2019 23:57
 Operator : JU
 Sample : K6132-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQR6

Quant Time: Dec 18 01:38:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 17 15:54:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	404068	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	1938971	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	1265502	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	2671421	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	2436803	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	2357236	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	44851	4.90	ng/uL	0.00
5) Phenol-d5	6.65	99	281546	7.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	664664	28.97	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	705177	25.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	536156	17.14	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	446089	32.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	503575	32.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	894568	30.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	130891	3.62	ng/ul	0.00
44) Dimethylphthalate-d6	13.54	166	2983829	31.88	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	3652878	32.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	89044	5.30	ng/ul	0.01
58) Fluorene-d10	15.12	176	2606528	31.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	430957	26.44	ng/ul	0.00
71) Anthracene-d10	16.97	188	4001510	32.92	ng/ul	0.00
79) Pyrene-d10	19.27	212	4246270	36.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	3938152	33.63	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.59	163	313532	3.224	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
Data File : BM024136.D
Acq On : 17 Dec 2019 23:57
Operator : JU
Sample : K6132-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQR6

Quant Time: Dec 18 01:38:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 17 15:54:50 2019
Response via : Initial Calibration

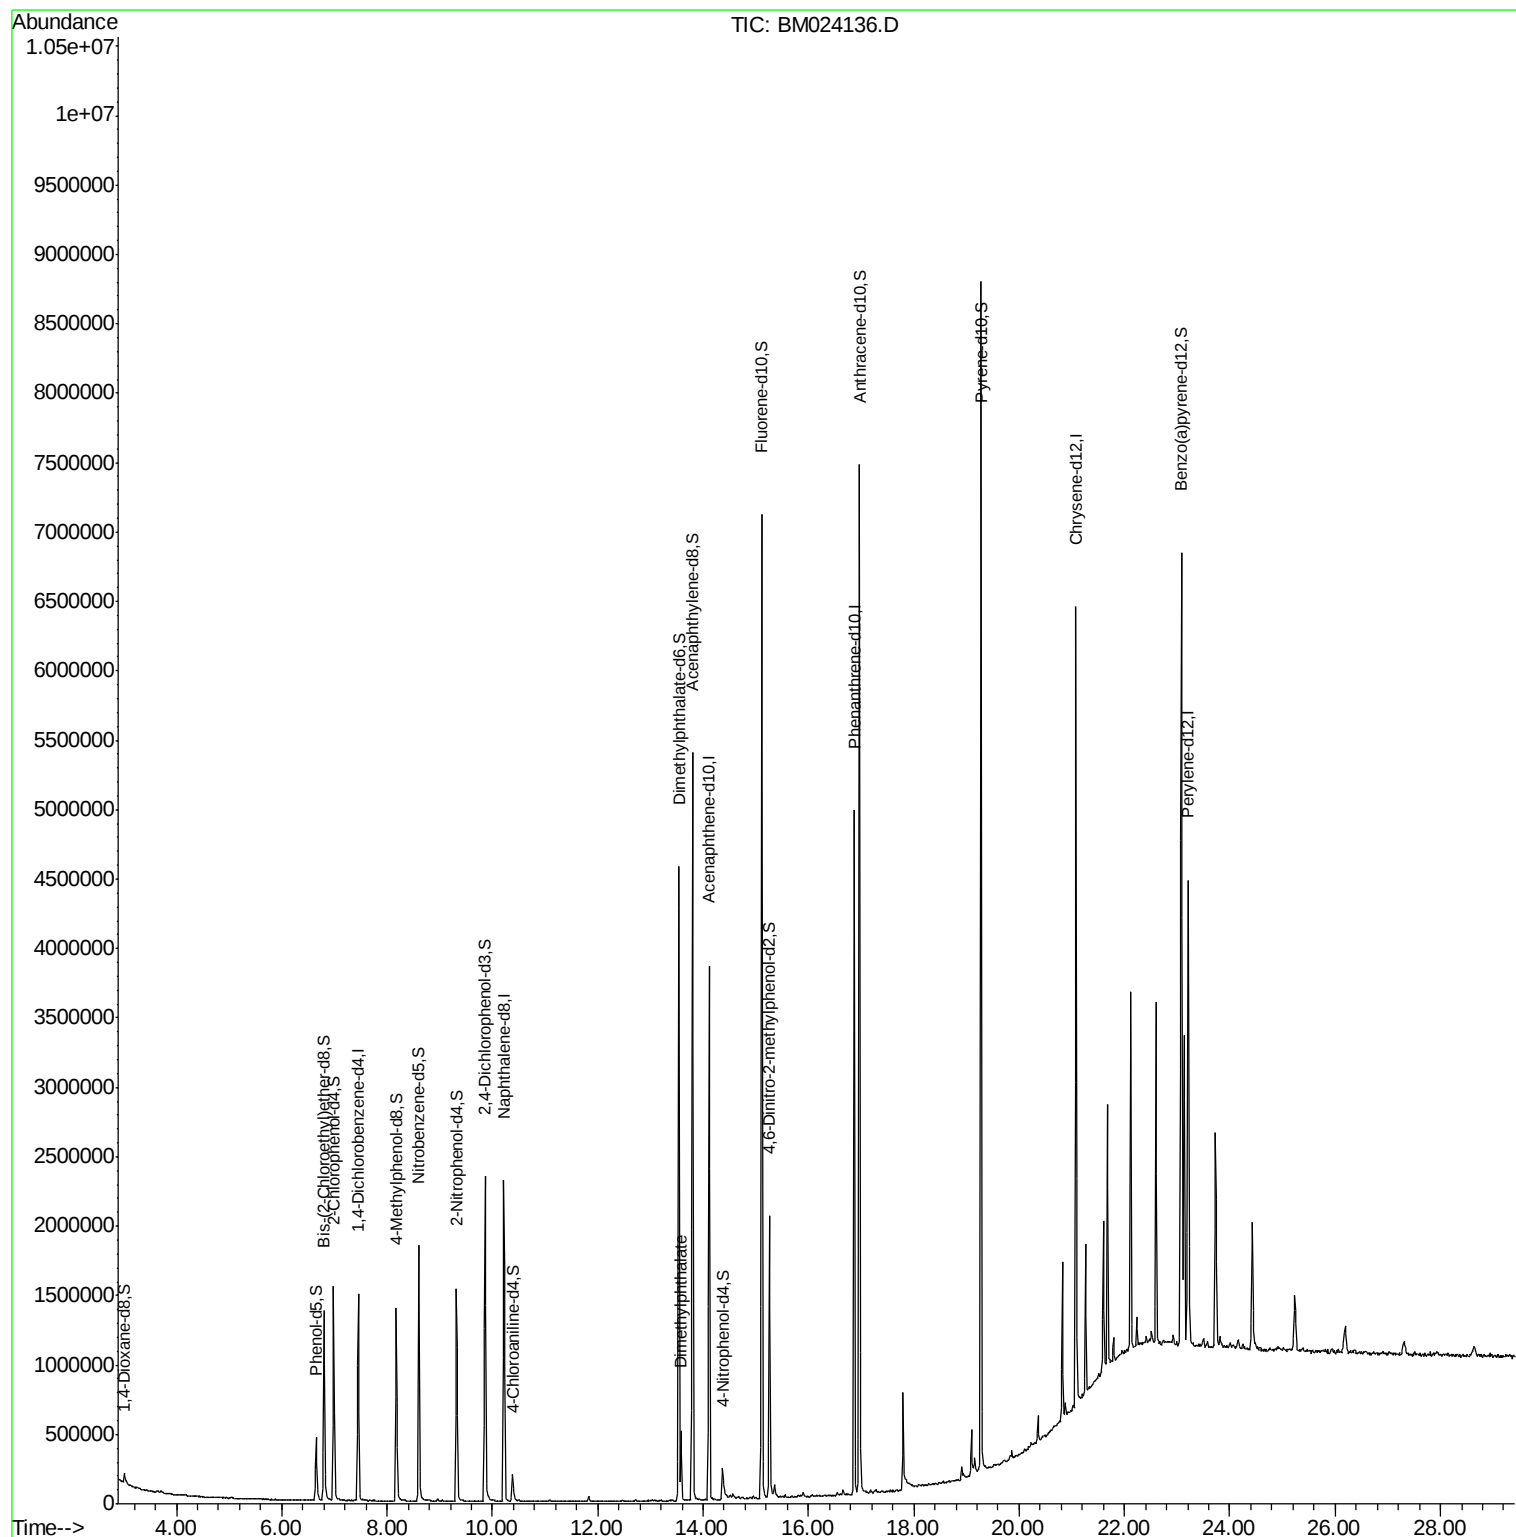

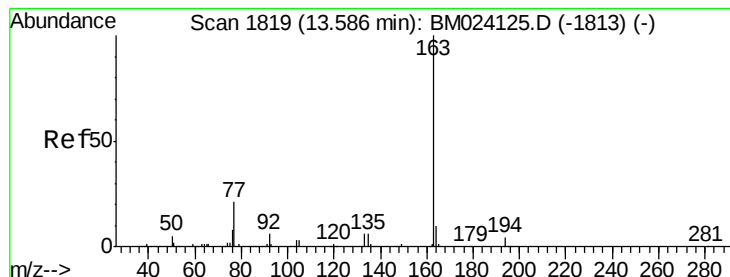

#45

Dimethylphthalate

Concen: 3.224 ng/ul

RT: 13.59 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BM024136.D

Acq: 17 Dec 2019 23:57

Instrument :

BNA_M

ClientSampleId :

BFQR6



Tot Ion:163 Resp: 313532

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.4 7.8 11.6

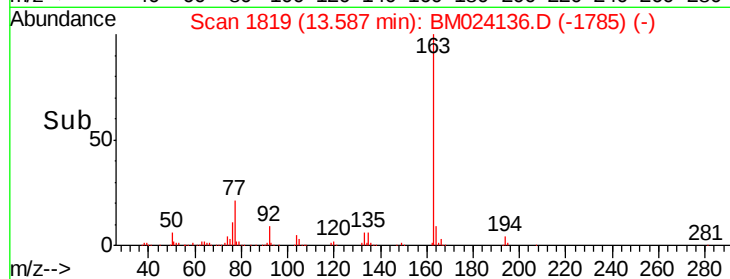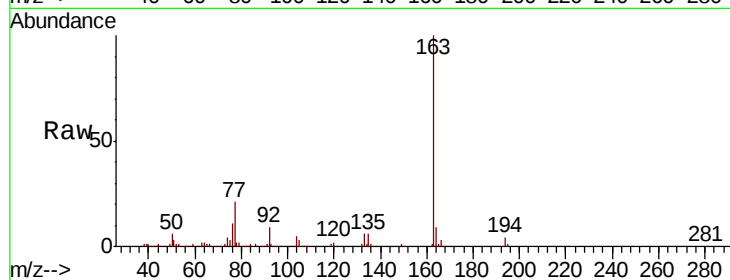

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

