

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
 Data File : BM024137.D
 Acq On : 18 Dec 2019 00:33
 Operator : JU
 Sample : K6132-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQR7

Quant Time: Dec 18 01:38:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 17 15:54:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	401460	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	1915380	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	1242595	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	2641868	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	2491262	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	2394423	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.01	96	49236	5.42	ng/uL	0.00
5) Phenol-d5	6.65	99	266213	7.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	679544	29.81	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	699589	25.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	520880	16.76	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	443975	32.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	509925	33.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	880718	29.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	82623	2.31	ng/ul	0.01
44) Dimethylphthalate-d6	13.54	166	3043248	33.12	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	3693101	33.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	81624	4.95	ng/ul	0.02
58) Fluorene-d10	15.12	176	2637856	32.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	439810	27.29	ng/ul	0.00
71) Anthracene-d10	16.97	188	4071958	33.87	ng/ul	0.00
79) Pyrene-d10	19.27	212	4392002	37.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	4154803	34.93	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.59	163	250853	2.627	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121719\
Data File : BM024137.D
Acq On : 18 Dec 2019 00:33
Operator : JU
Sample : K6132-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQR7

Quant Time: Dec 18 01:38:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 17 15:54:50 2019
Response via : Initial Calibration

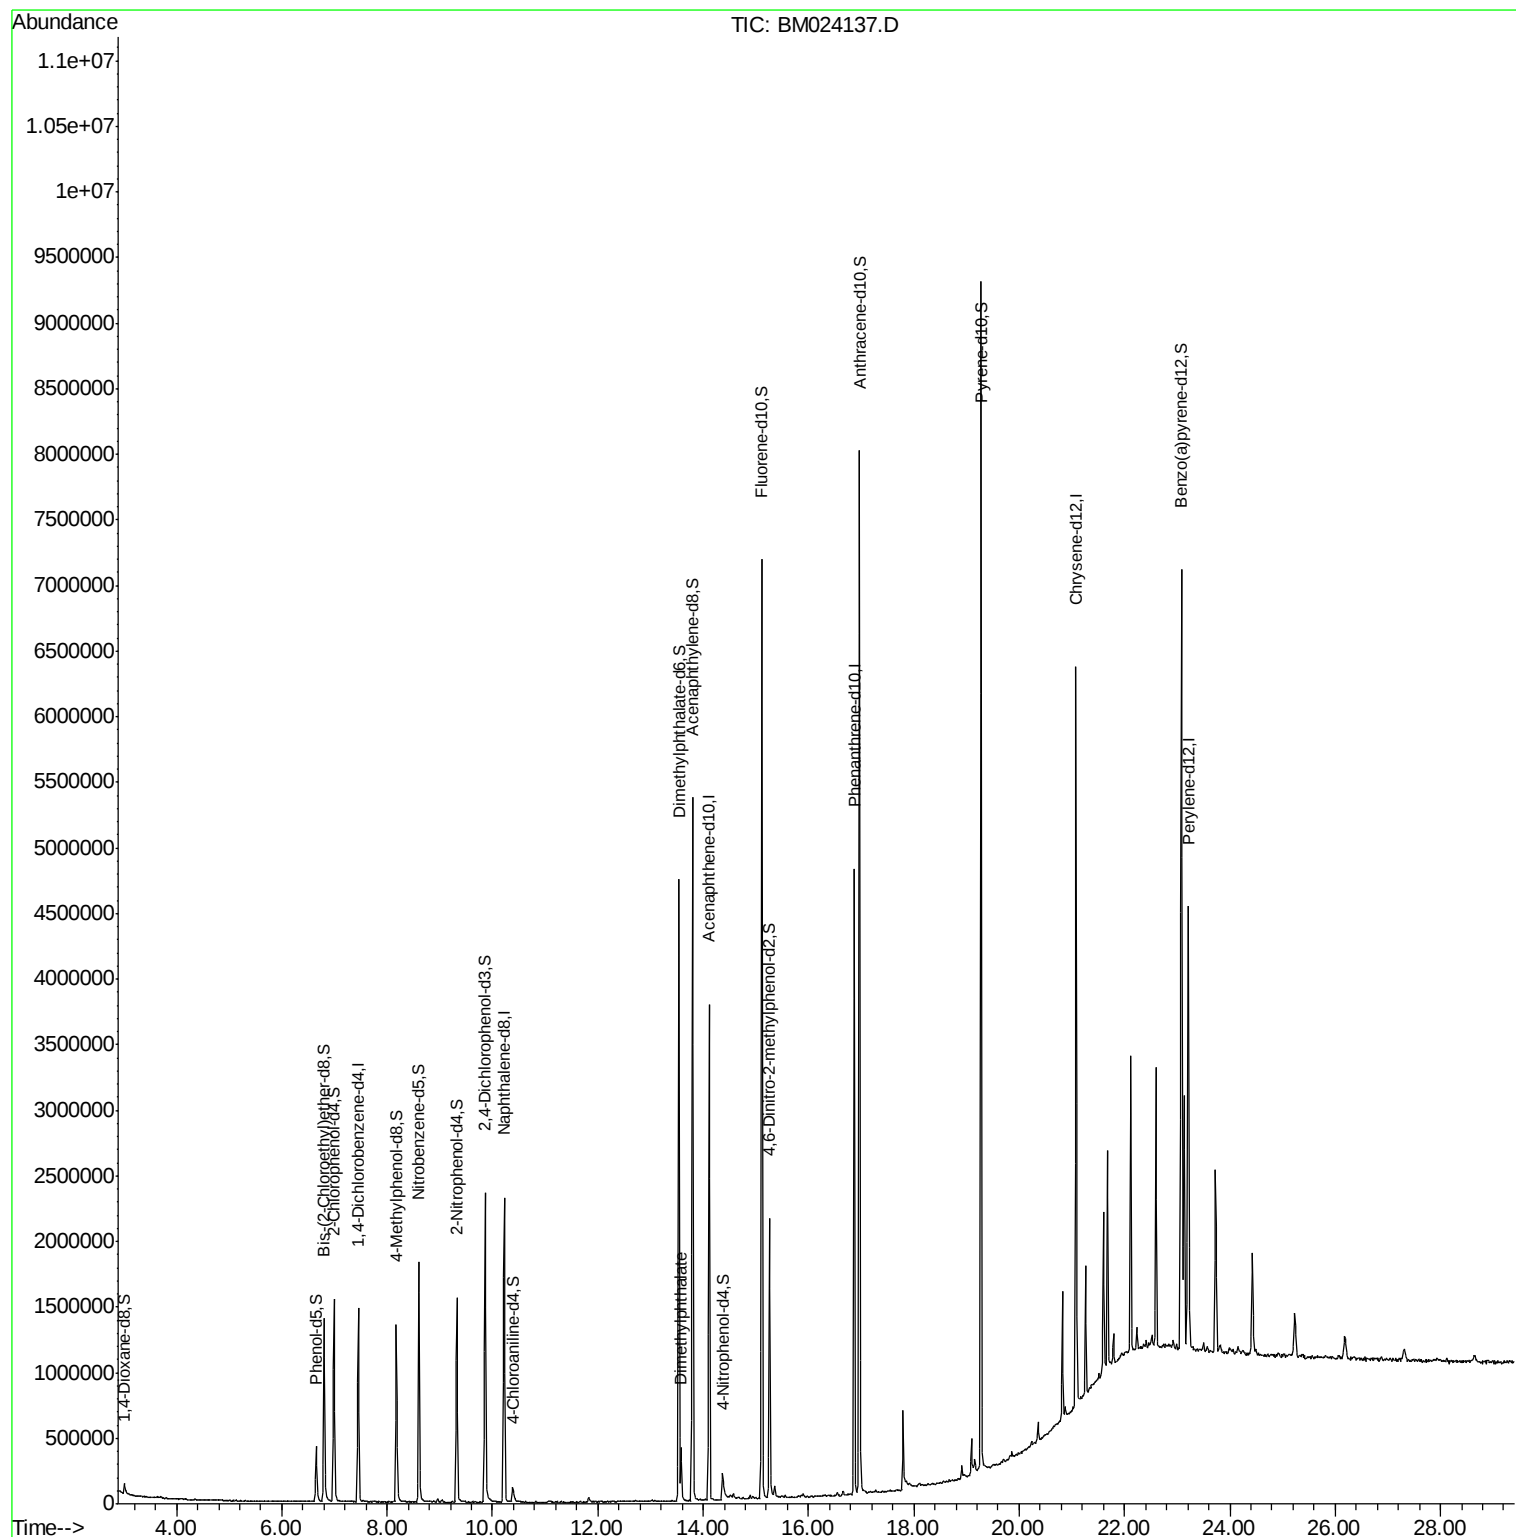

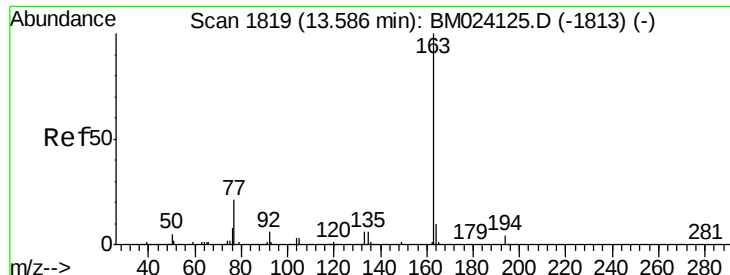

#45

Dimethylphthalate

Concen: 2.627 ng/ul

RT: 13.59 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM024137.D

Acq: 18 Dec 2019 00:33

Instrument :

BNA_M

ClientSampleId :

BFQR7


Tot Ion:163 Resp: 250853

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.2 7.8 11.6

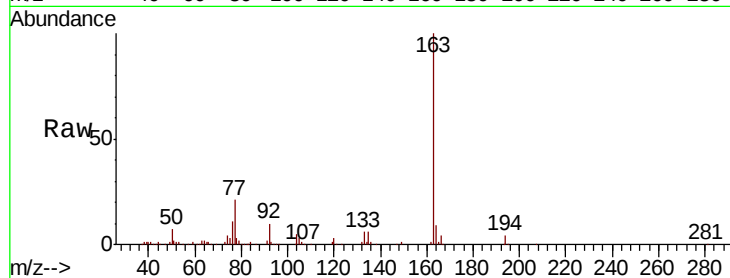

Abundance Ion 163.00 (162.70 to 163.70): E

250000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

