

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121724\
 Data File : BM049020.D
 Acq On : 17 Dec 2024 14:03
 Operator : RC/JU
 Sample : P5228-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/18/2024
 Supervised By :mohammad ahmed 12/18/2024

Quant Time: Dec 17 14:59:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 17 10:03:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	8425	0.400	ng/ul	0.00
4) Naphthalene-d8	10.332	136	26349	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.206	164	14979	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.951	188	29847m	0.400	ng/ul	0.00
17) Chrysene-d12	21.149	240	15919m	0.400	ng/ul	0.00
23) Perylene-d12	23.308	264	13277m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	24288	2.467	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.932	152	13920	0.414	ng/ul	0.00
18) Fluoranthene-d10	18.984	212	23909	0.503	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.381	128	1503	0.022	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121724\
Data File : BM049020.D
Acq On : 17 Dec 2024 14:03
Operator : RC/JU
Sample : P5228-03
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E2AT0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/18/2024


Quant Time: Dec 17 14:59:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 17 10:03:27 2024
Response via : Initial Calibration

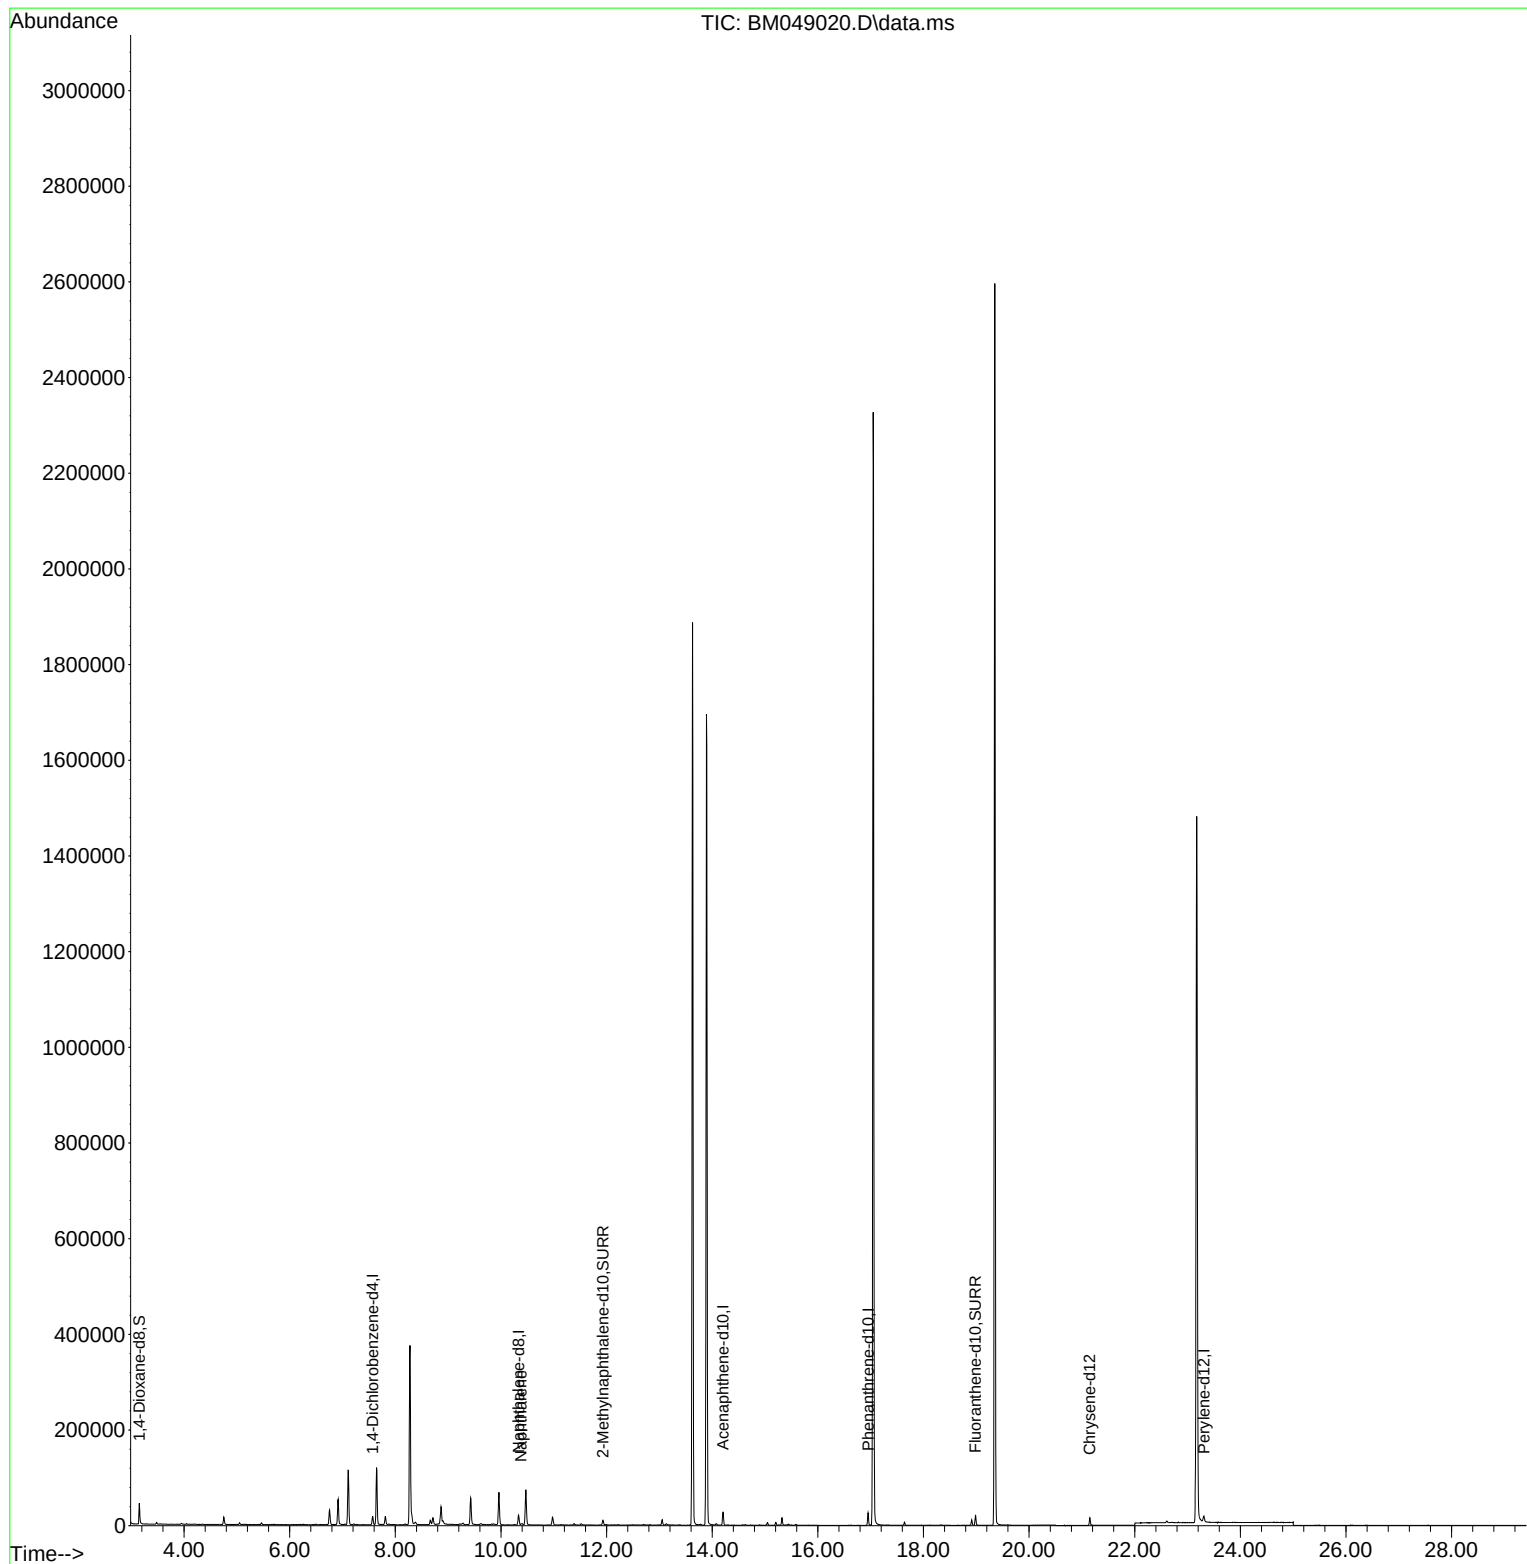

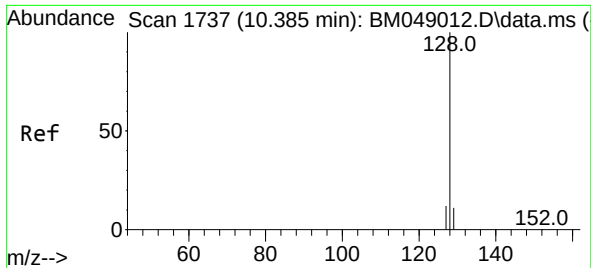

#5
Naphthalene
Concen: 0.022 ng/ul
RT: 10.381 min Scan# 1736
Delta R.T. -0.004 min
Lab File: BM049020.D
Acq: 17 Dec 2024 14:03

Instrument :
BNA_M
ClientSampleId :
E2AT0

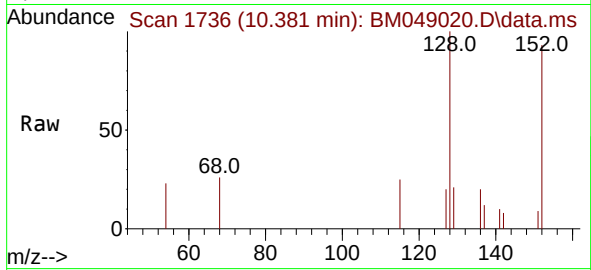

Tgt Ion:128 Resp: 1500
Ion Ratio Lower Upper
128 100
129 20.9 9.4 14.2
127 19.7 10.6 16.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/18/2024

