
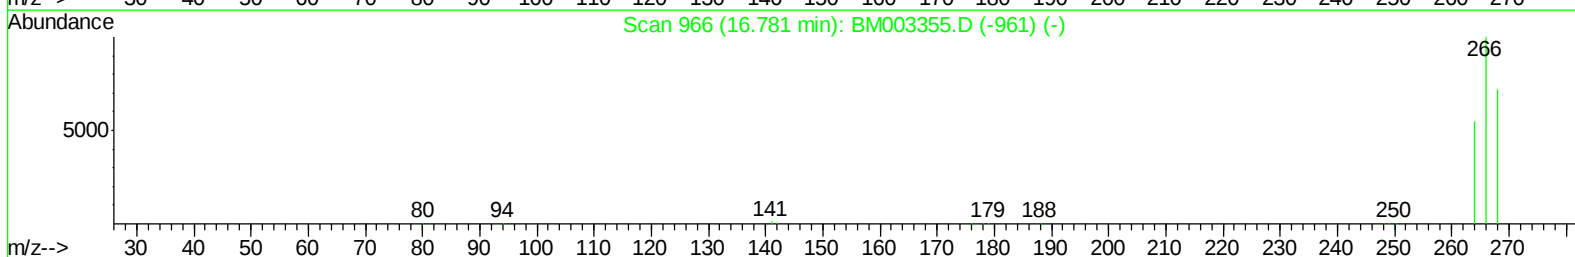
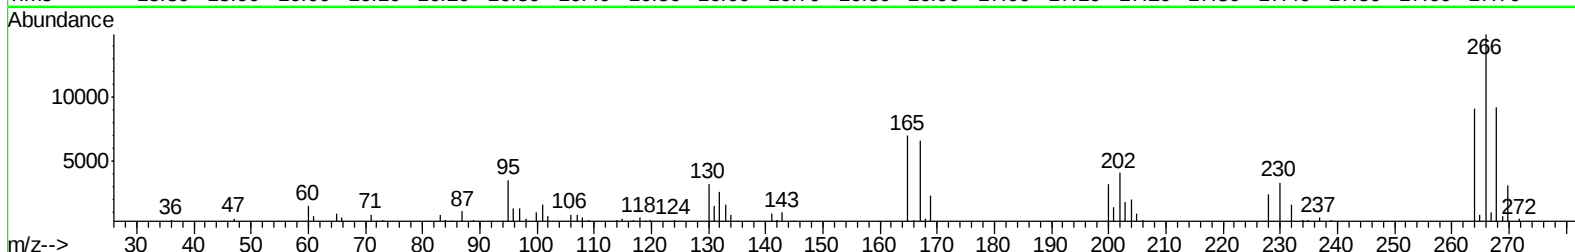


Data Path : Z:\HPCHEM1\BNA M\Data\BM121815\
Data File : BM003609.D
Acq On : 18 Dec 2015 09:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 09:56:19 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 16:19:00 2015
Response via : Initial Calibration

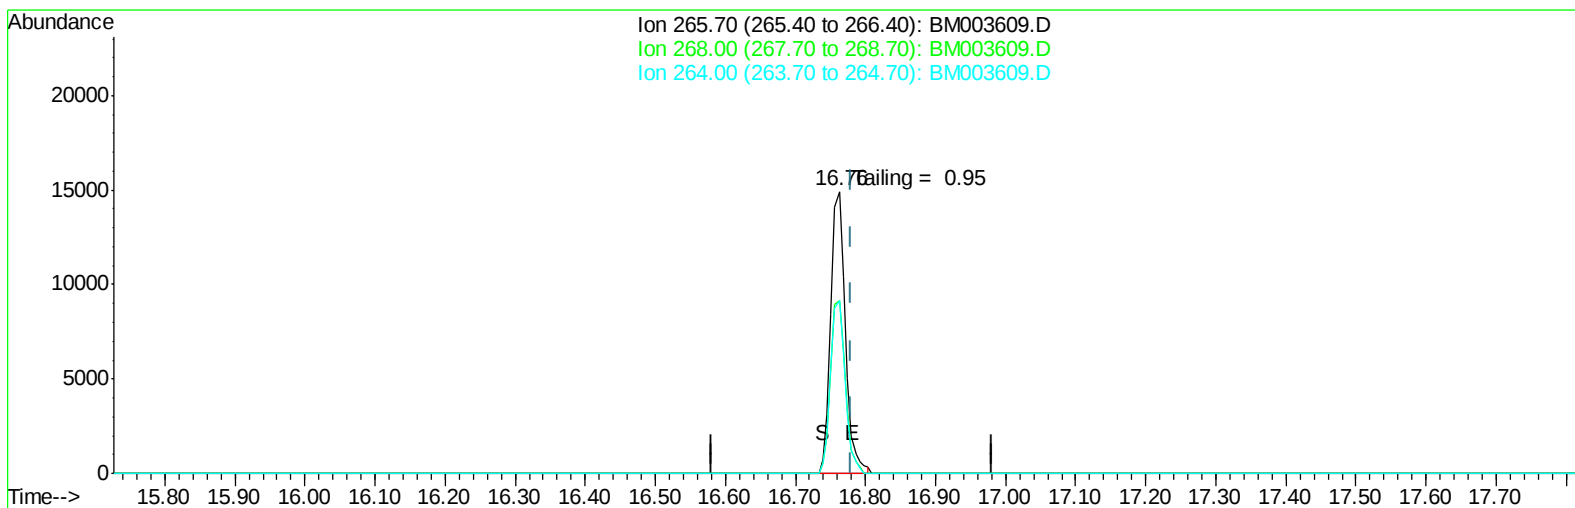

TIC: BM003609.D

(22) Pentachlorophenol




16.762min (-0.019) 0.00ng

response 21561

Ion	Exp%	Act%
265.70	100	100
268.00	57.30	61.59
264.00	70.90	61.19
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA M\Data\BM121815\  
Data File : BM003609.D  
Acq On    : 18 Dec 2015  09:15  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Dec 21 09:56:19 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 16:19:00 2015
Response via : Initial Calibration

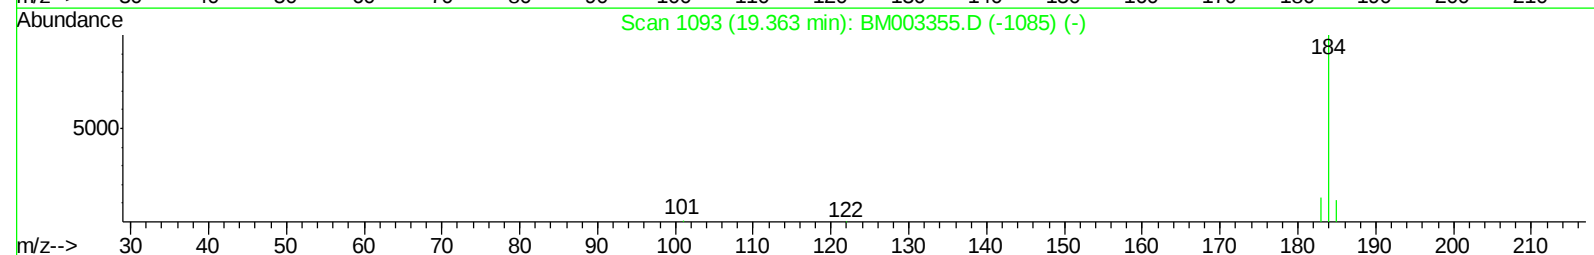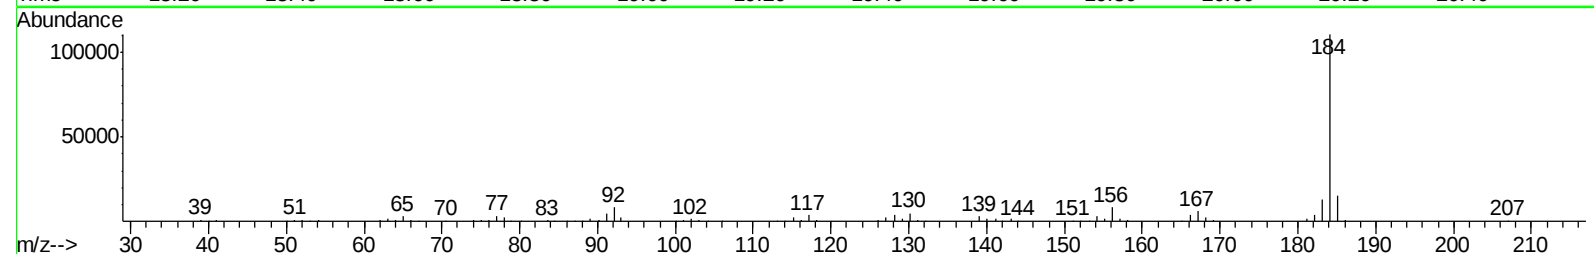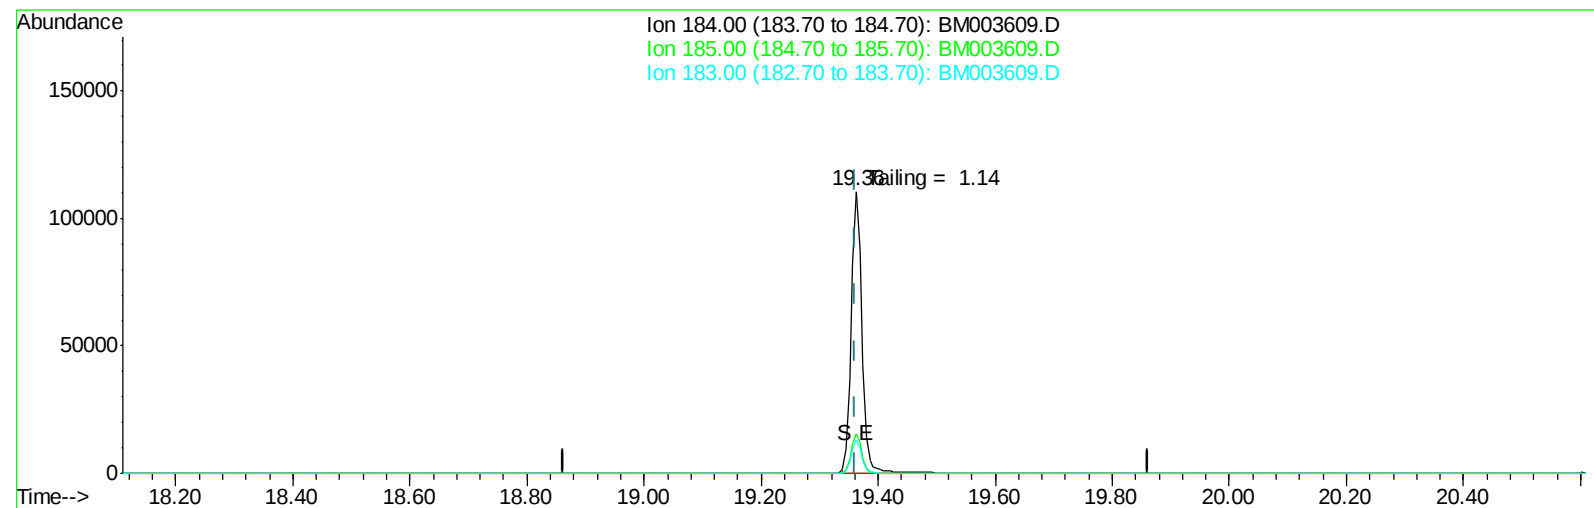

TIC: BM003609.D

(27) Benzidine

19.362min (+0.000) 10187.83ng

response 142604

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.03
183.00	10.80	11.66
0.00	0.00	0.00