


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121815\
Data File : BM003609.D
Acq On : 18 Dec 2015 09:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM120215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 02 16:19:00 2015

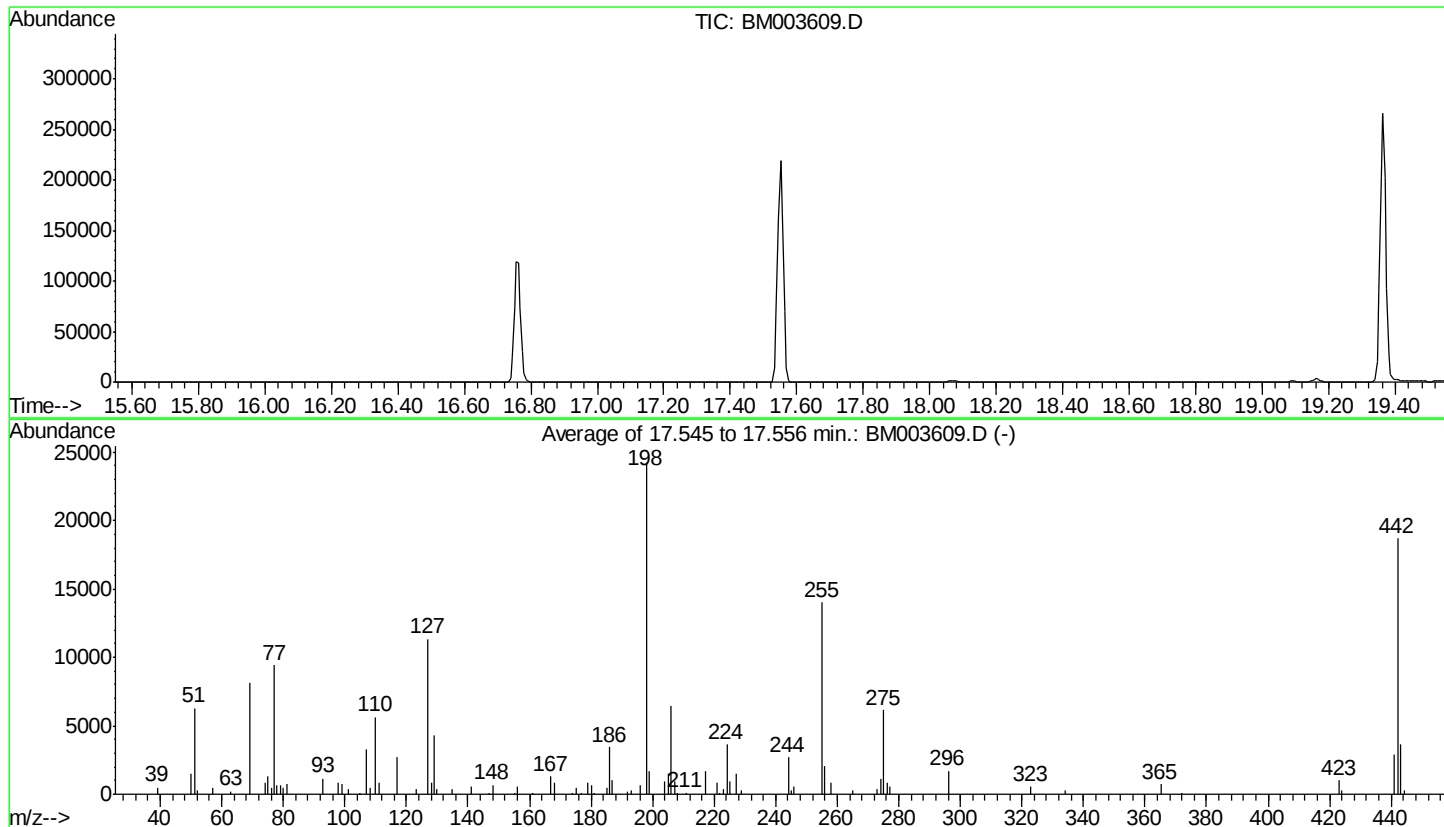

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	6282	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.5	8125	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	11336	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24221	PASS
199	198	5	9	6.9	1665	PASS
275	198	10	60	25.3	6131	PASS
365	198	1	100	3.1	739	PASS
441	442	0.01	24	15.5	2896	PASS
442	198	50	100	77.0	18657	PASS
443	442	15	24	19.4	3615	PASS