

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121816\
 Data File : BM008437.D
 Acq On : 18 Dec 2016 14:35
 Operator : UM/SJ
 Sample : H6067-10DL 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7G1DL

Quant Time: Dec 19 01:25:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-2016\SOM02.2-EPA-BM121416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 01:22:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	122399	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	485952	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	323152	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	643454	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	811080	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	856274	20.00	ng/ul	0.00


System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	2773	1.07	ng/uL	0.01
5) Phenol-d5	6.87	99	40111	4.22	ng/ul	0.03
7) Bis-(2-Chloroethyl)ether-d	7.02	67	27489	5.04	ng/ul	0.01
9) 2-Chlorophenol-d4	7.21	132	35409	4.96	ng/ul	0.01
13) 4-Methylphenol-d8	8.40	113	28600	3.89	ng/ul	0.03
19) Nitrobenzene-d5	8.84	128	16200	4.61	ng/ul	0.02
22) 2-Nitrophenol-d4	9.56	143	16466	4.23	ng/ul	0.03
26) 2,4-Dichlorophenol-d3	10.13	165	18605	2.61	ng/ul	0.06
29) 4-Chloroaniline-d4	10.65	131	6129	0.75	ng/ul	0.06
43) Dimethylphthalate-d6	13.73	166	132259	6.16	ng/ul	0.01
46) Acenaphthylene-d8	13.99	160	157506	6.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	1246	0.39	ng/ul	0.15
57) Fluorene-d10	15.31	176	114511	6.13	ng/ul	0.01
62) 4,6-Dinitro-2-methylphenol	15.49	200	7721	2.02	ng/ul	0.04
70) Anthracene-d10	17.16	188	176943	6.31	ng/ul	0.00
76) Pyrene-d10	19.46	212	213502	6.82	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	224634	6.25	ng/ul	0.00

Target Compounds

						Qvalue
6) Phenol	6.90	94	9980	1.01	ng/ul#	83
44) Dimethylphthalate	13.77	163	34460	1.64	ng/ul	96
47) Acenaphthylene	14.03	152	33935	1.31	ng/ul	99
71) Anthracene	17.20	178	42665	1.27	ng/ul	96
77) Pyrene	19.49	202	49136	1.23	ng/ul	98
80) Benzo(a)anthracene	21.29	228	157802	3.76	ng/ul	92
81) Bis(2-ethylhexyl)phthalate	21.16	149	692184	33.09	ng/ul	99
82) Chrysene	21.29	228	157802	3.91	ng/ul	95
85) Benzo(b)fluoranthene	22.81	252	452938	9.80	ng/ul	97
86) Benzo(k)fluoranthene	22.81	252	452938	10.24	ng/ul	99
88) Benzo(a)pyrene	23.39	252	311485	6.99	ng/ul	96
89) Indeno(1,2,3-cd)pyrene	25.71	276	324926	6.01	ng/ul	97
90) Dibenzo(a,h)anthracene	25.71	278	86750	1.91	ng/ul	92
91) Benzo(g,h,i)perylene	26.40	276	293535	6.49	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

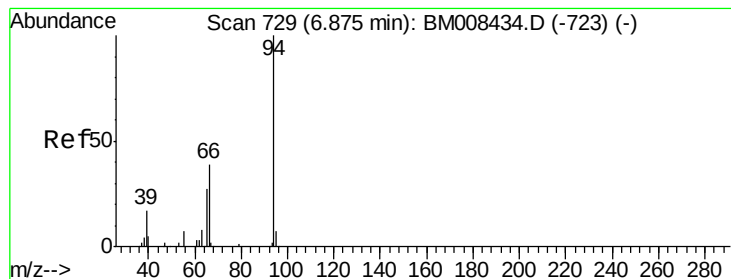

#6

Phenol

Concen: 1.01 ng/ul

RT: 6.90 min Scan# 734

Delta R.T. 0.03 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35

Instrument :

BNA_M

ClientSampleId :

DA7G1DL


Tgt Ion: 94 Resp: 9980

Ion Ratio Lower Upper

94 100

65 29.5 22.6 34.0

66 62.0 35.8 53.8#



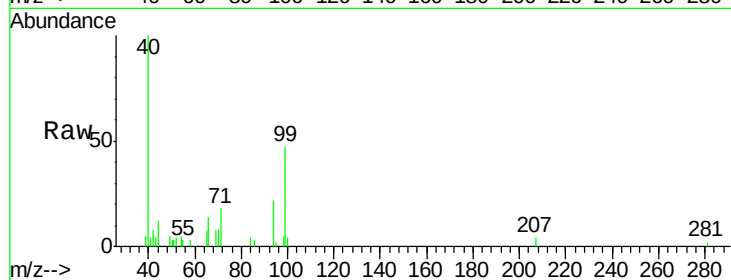


Abundance Ion 94.00 (93.70 to 94.70): BM008437.D (-695) (-)

Ion 65.00 (64.70 to 65.70): BM008437.D (-695) (-)

Ion 66.00 (65.70 to 66.70): BM008437.D (-695) (-)

Time-->

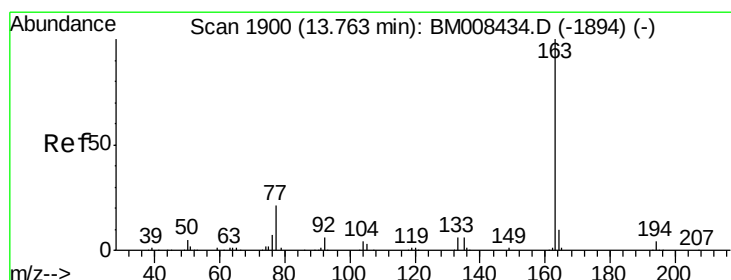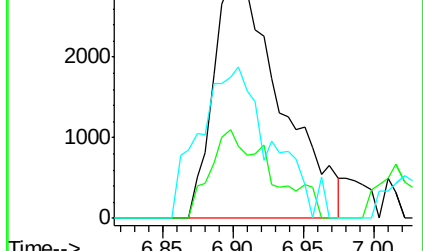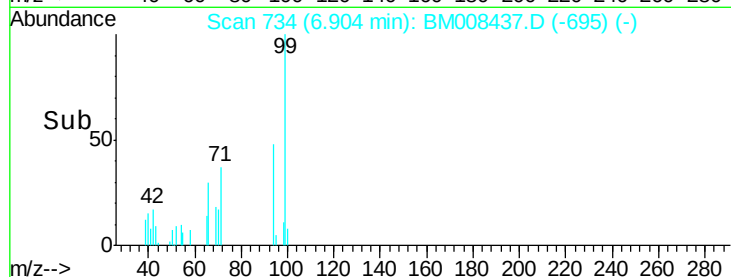

#44

Dimethylphthalate

Concen: 1.64 ng/ul

RT: 13.77 min Scan# 1902

Delta R.T. 0.01 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35


Tgt Ion: 163 Resp: 34460

Ion Ratio Lower Upper

163 100

194 3.9 3.5 5.3

164 11.6 7.8 11.8


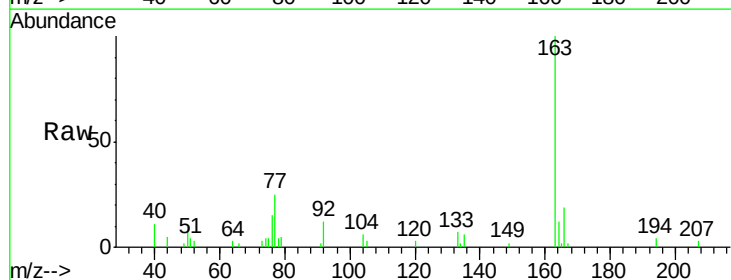



Abundance Ion 163.00 (162.70 to 163.70): BM008437.D (-1866) (-)

Ion 194.00 (193.70 to 194.70): BM008437.D (-1866) (-)

Ion 164.00 (163.70 to 164.70): BM008437.D (-1866) (-)

Time-->



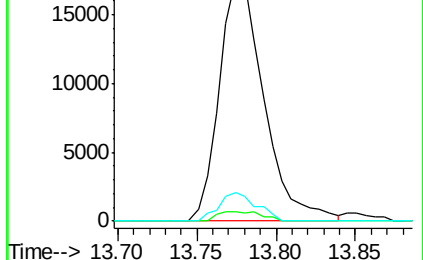
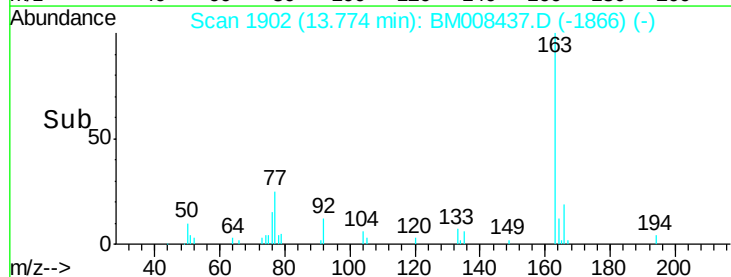


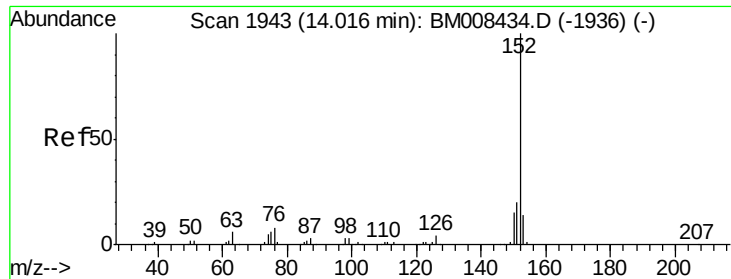

#47
 Acenaphthylene
 Concen: 1.31 ng/ul
 RT: 14.03 min Scan# 1945
 Delta R.T. 0.01 min
 Lab File: BM008437.D
 Acq: 18 Dec 2016 14:35




Instrument :
 BNA_M
 ClientSampleId :
 DA7G1DL


Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.5	15.3	22.9
153	11.7	9.9	14.9

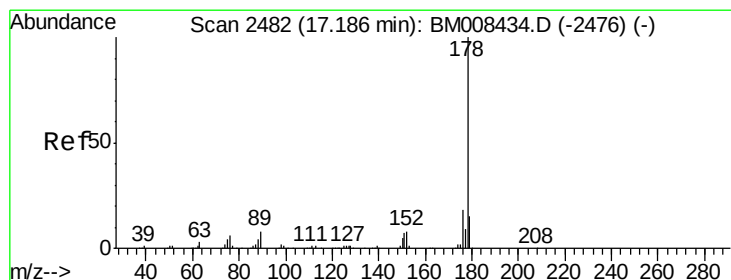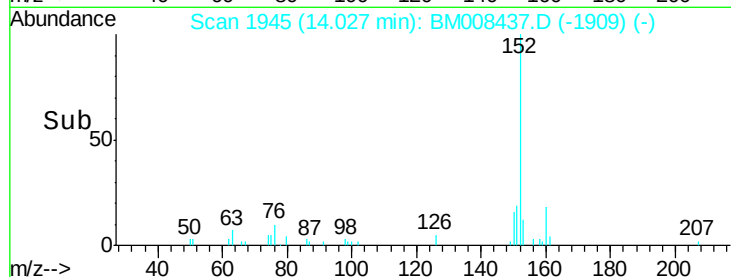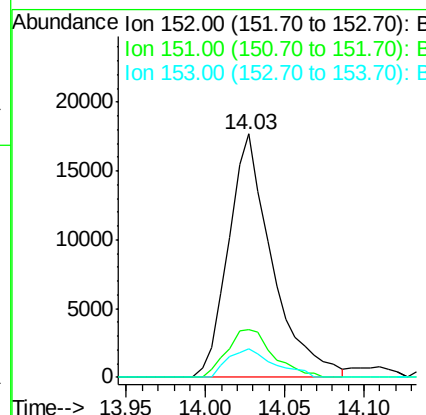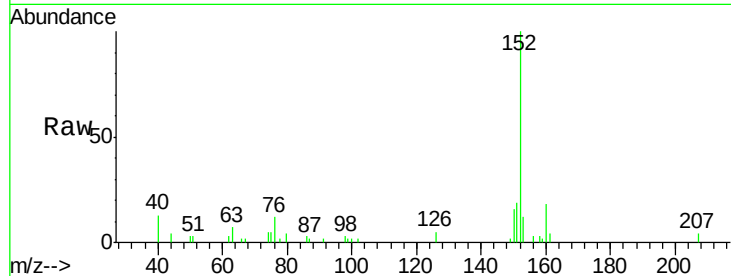

#71
 Anthracene
 Concen: 1.27 ng/ul
 RT: 17.20 min Scan# 2484
 Delta R.T. 0.01 min
 Lab File: BM008437.D
 Acq: 18 Dec 2016 14:35

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.7	12.1	18.1
176	16.2	14.3	21.5

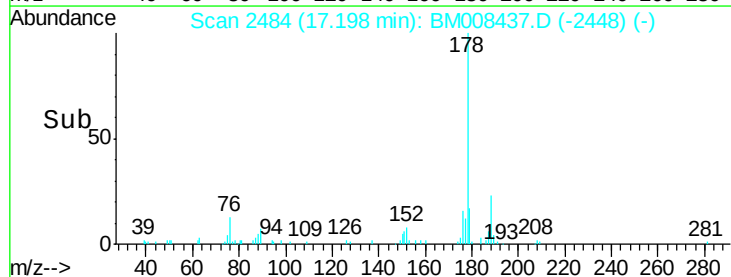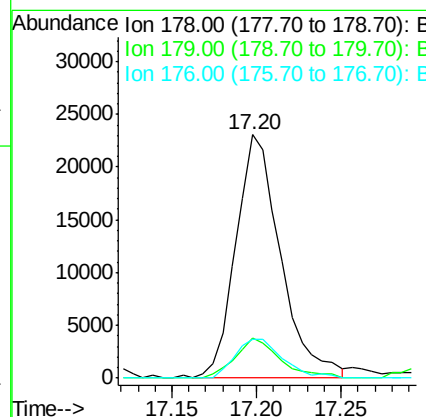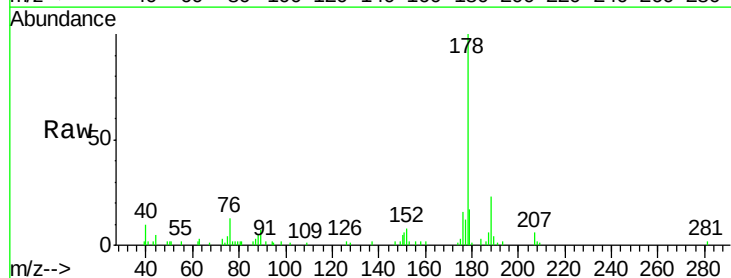

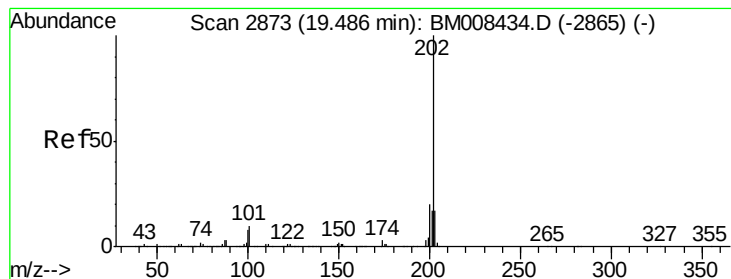

#77

Pyrene

Concen: 1.23 ng/ul

RT: 19.49 min Scan# 2873

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35

Instrument :

BNA_M

ClientSampleId :

DA7G1DL


Tgt Ion:202 Resp: 49136

Ion Ratio Lower Upper

202 100

101 11.0 8.2 12.4




100 9.8 7.0 10.6

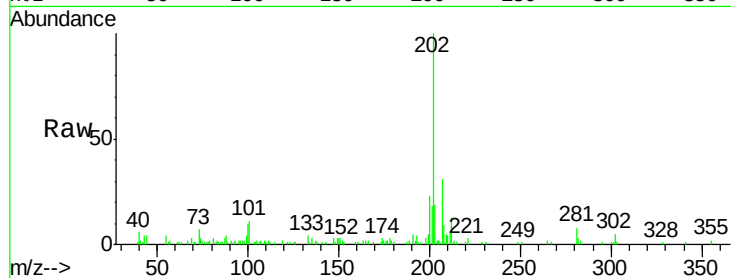

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

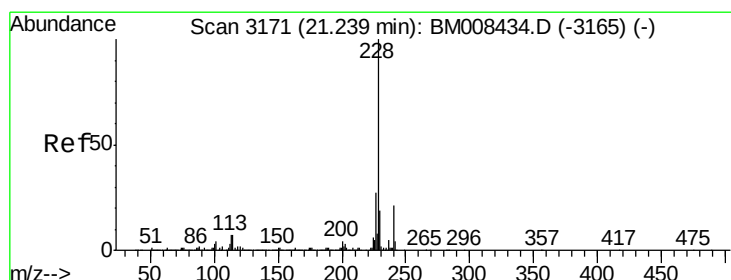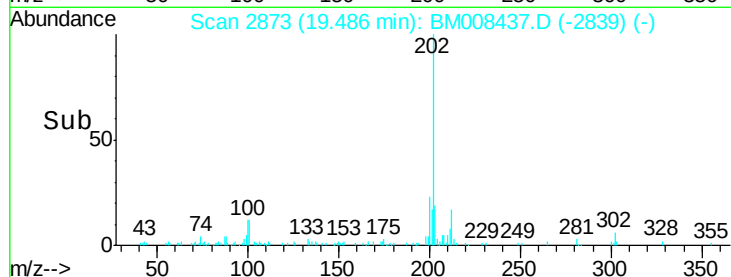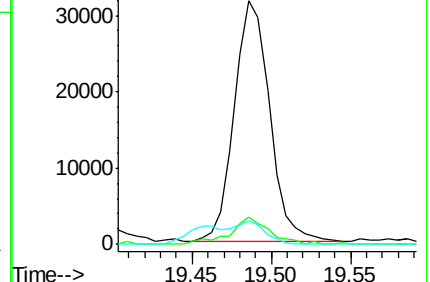

#80

Benzo(a)anthracene

Concen: 3.76 ng/ul

RT: 21.29 min Scan# 3180

Delta R.T. 0.05 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35


Tgt Ion:228 Resp: 157802

Ion Ratio Lower Upper

228 100

229 22.5 15.4 23.2



226 30.7 21.2 31.8

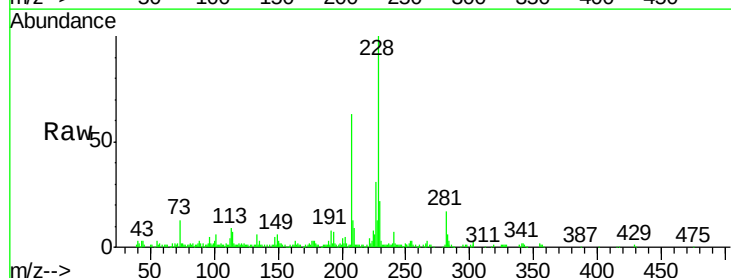


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

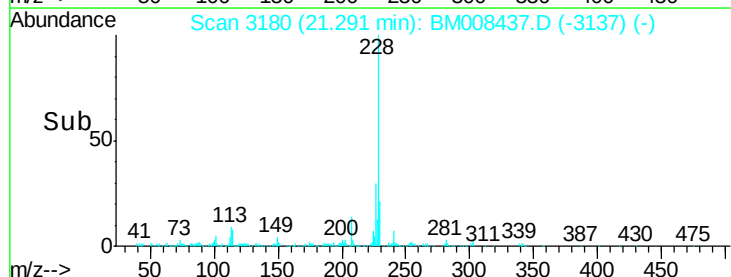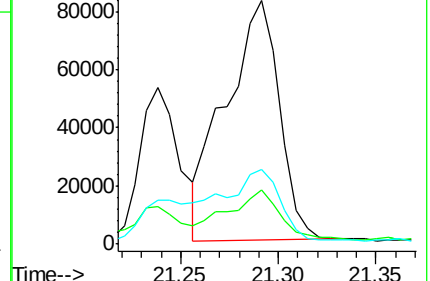

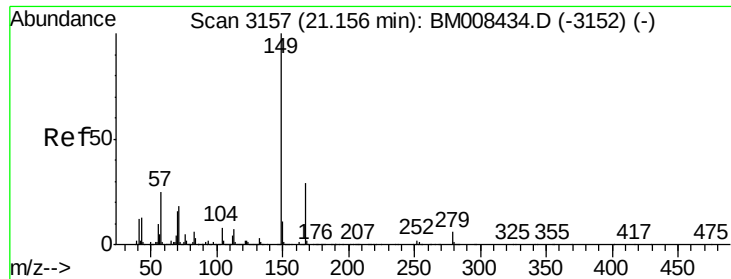

#81

Bis(2-ethylhexyl)phthalate

Concen: 33.09 ng/ul

RT: 21.16 min Scan# 3157

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35

Instrument :

BNA_M

ClientSampleId :

DA7G1DL


Tgt Ion:149 Resp: 692184

Ion Ratio Lower Upper

149 100

167 29.1 22.6 34.0




279 5.3 4.2 6.4

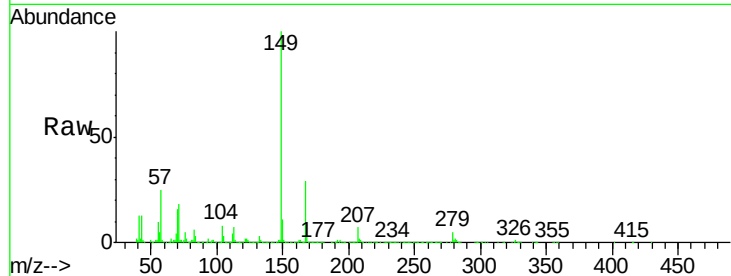

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

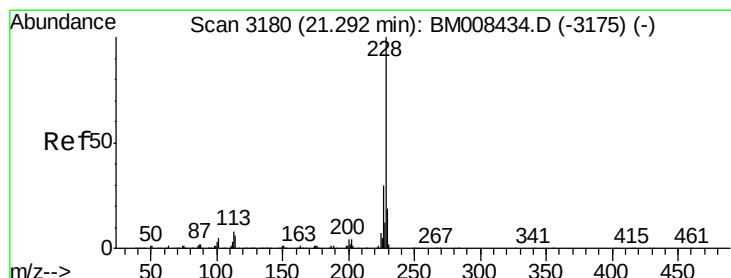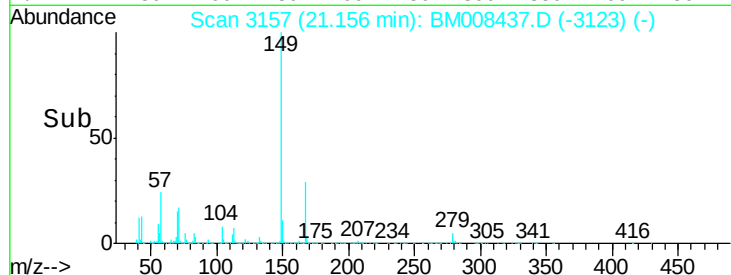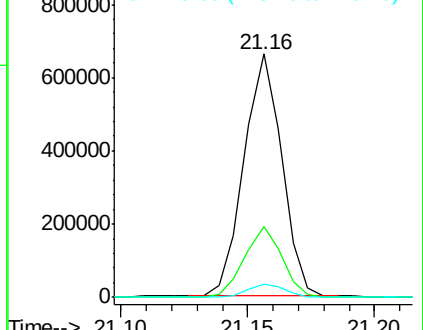

#82

Chrysene

Concen: 3.91 ng/ul

RT: 21.29 min Scan# 3180

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35


Tgt Ion:228 Resp: 157802

Ion Ratio Lower Upper

228 100

226 30.7 23.1 34.7



229 22.5 15.4 23.2

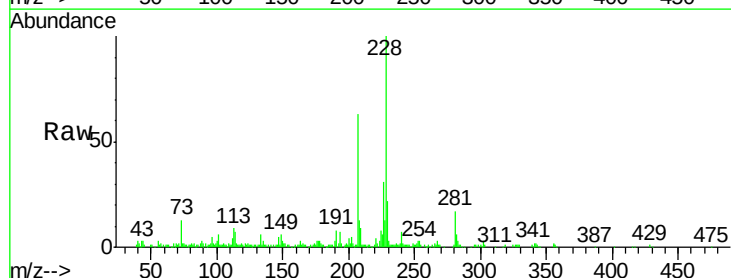


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

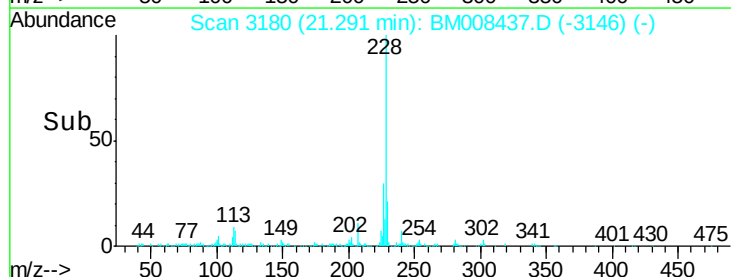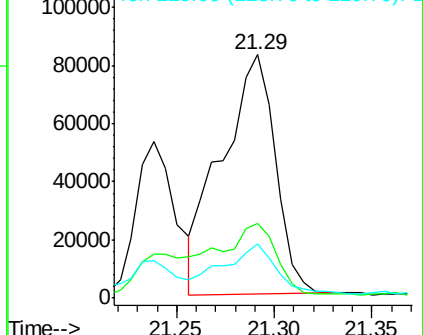

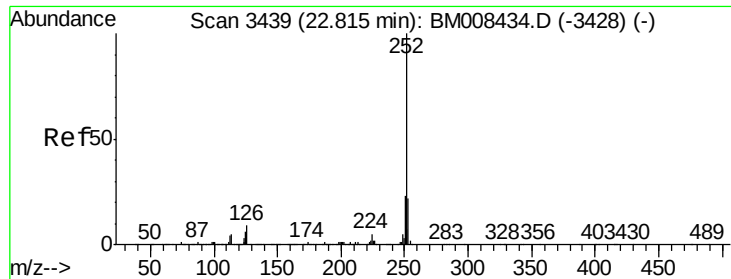

#85

Benzo(b)fluoranthene

Concen: 9.80 ng/ul

RT: 22.81 min Scan# 3439

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35

Instrument :

BNA_M

ClientSampleId :

DA7G1DL


Tgt Ion:252 Resp: 452938

Ion Ratio Lower Upper




252 100

253 22.8 17.1 25.7

125 7.5 5.4 8.2

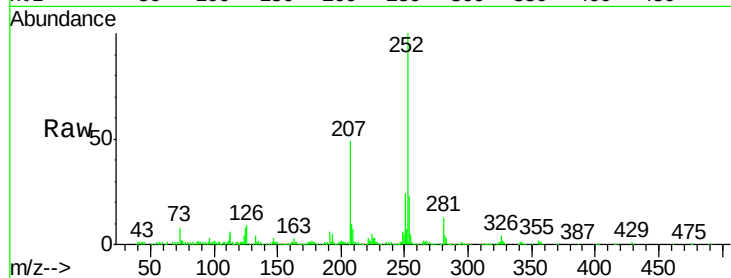

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

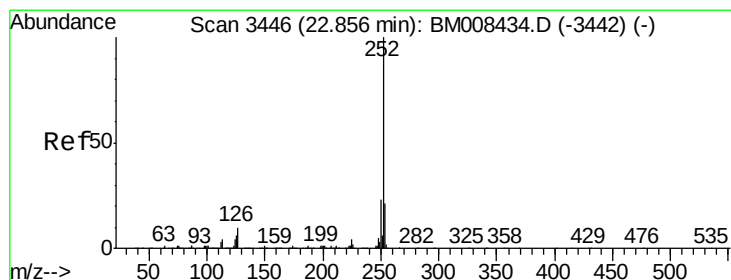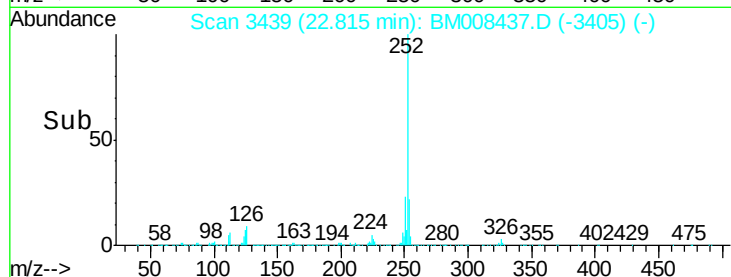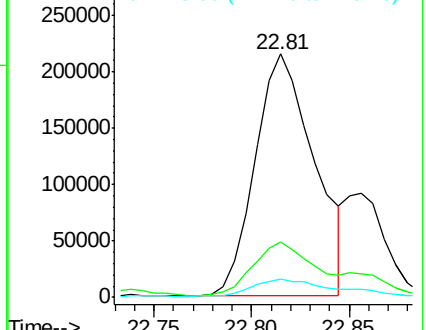

#86

Benzo(k)fluoranthene

Concen: 10.24 ng/ul

RT: 22.81 min Scan# 3439

Delta R.T. -0.04 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35


Tgt Ion:252 Resp: 452938

Ion Ratio Lower Upper



252 100


253 22.8 17.6 26.4

125 7.5 5.8 8.6

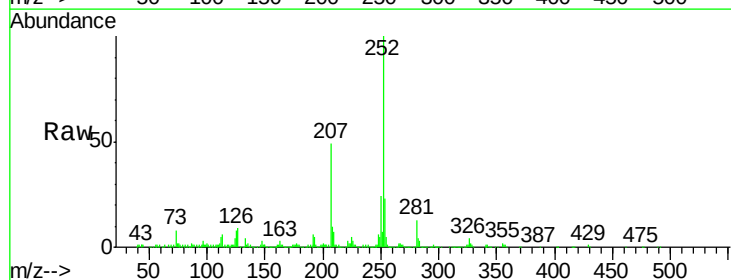

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

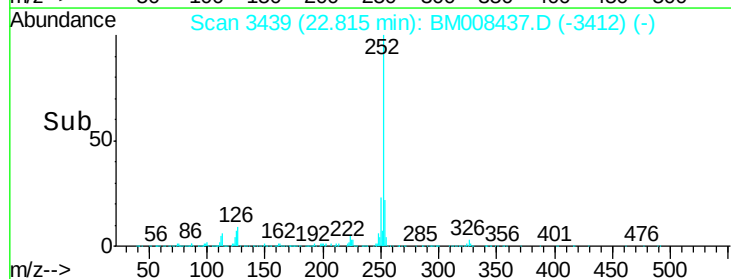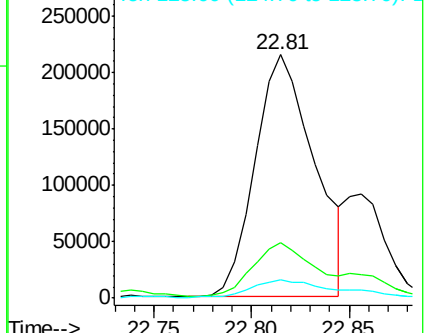

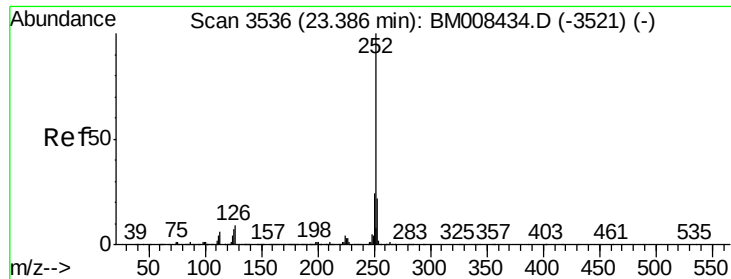

#88

Benzo(a)pyrene

Concen: 6.99 ng/ul

RT: 23.39 min Scan# 3536

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35

Instrument :

BNA_M

ClientSampleId :

DA7G1DL





Tgt Ion:252 Resp: 311485

Ion Ratio Lower Upper

252 100

253 24.1 17.4 26.2

125 7.3 6.6 9.8

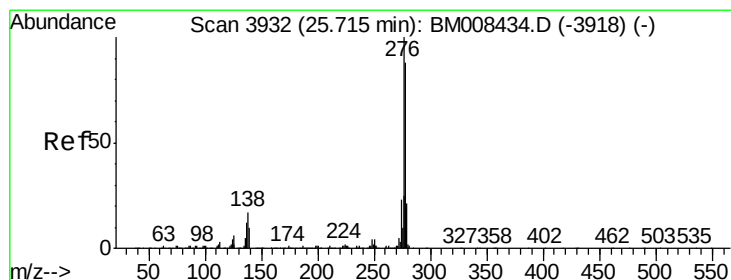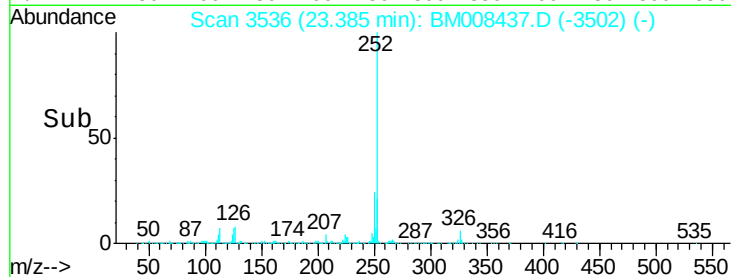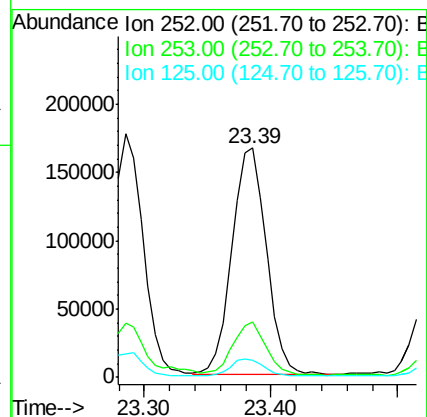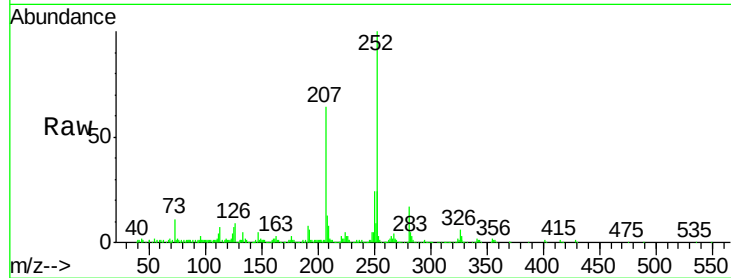

#89

Indeno(1,2,3-cd)pyrene

Concen: 6.01 ng/ul

RT: 25.71 min Scan# 3932

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35




Tgt Ion:276 Resp: 324926


Ion Ratio Lower Upper

276 100

138 14.3 13.4 20.2

277 24.2 19.7 29.5

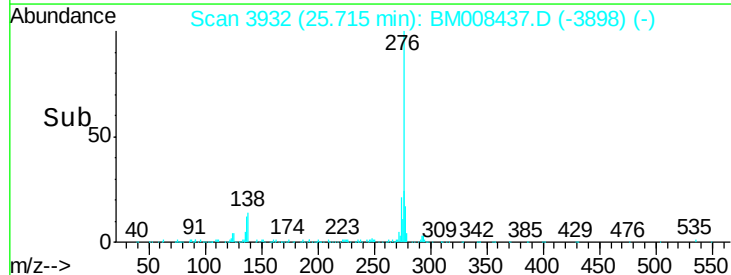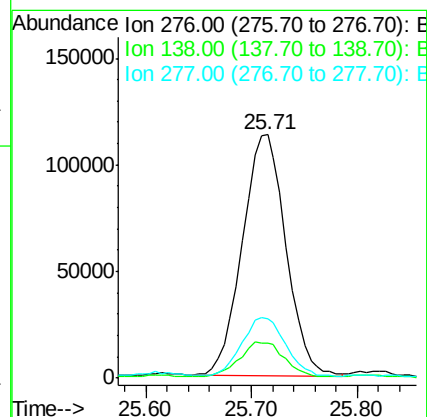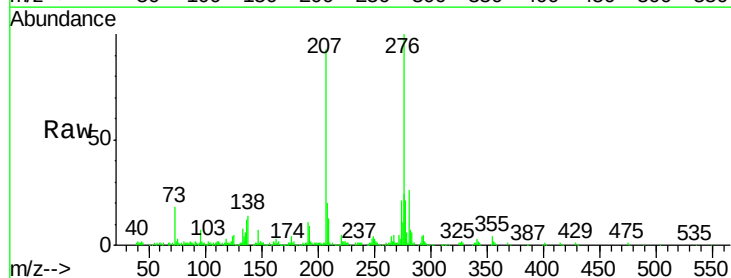

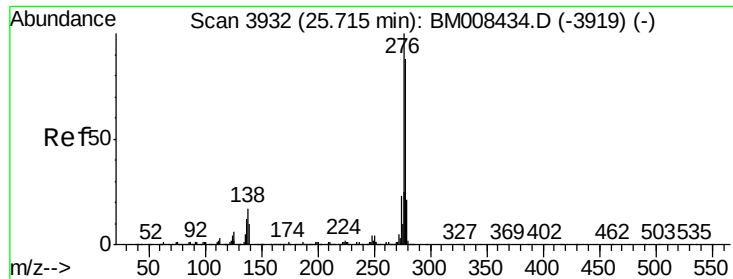

#90

Dibenzo(a,h)anthracene

Concen: 1.91 ng/ul

RT: 25.71 min Scan# 3931

Delta R.T. -0.01 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35

Instrument :

BNA_M

ClientSampleId :

DA7G1DL


Tgt Ion:278 Resp: 86750

Ion Ratio Lower Upper

278 100

139 13.9 9.4 14.0




279 27.6 18.6 28.0

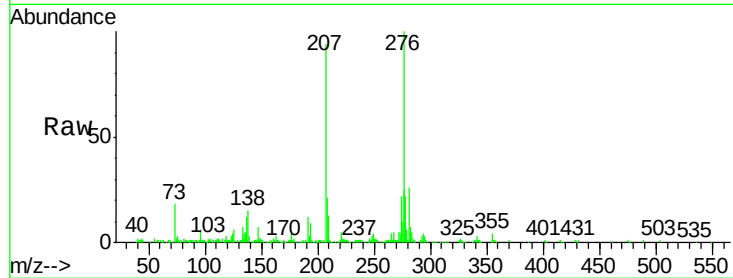

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

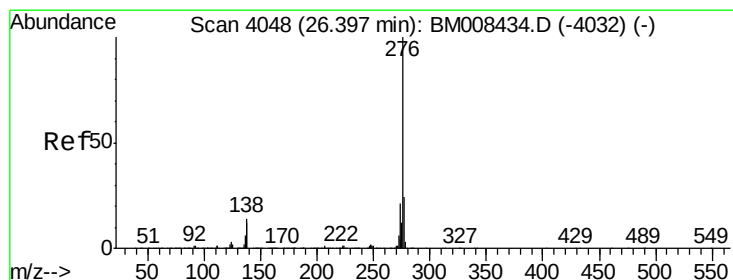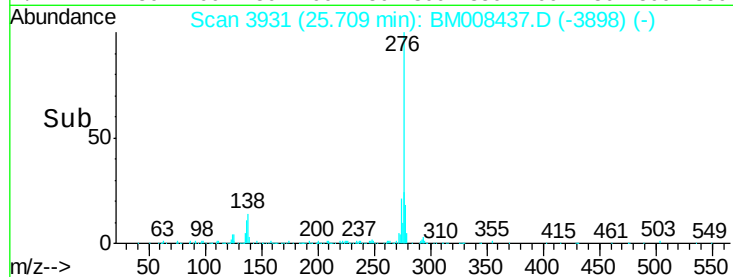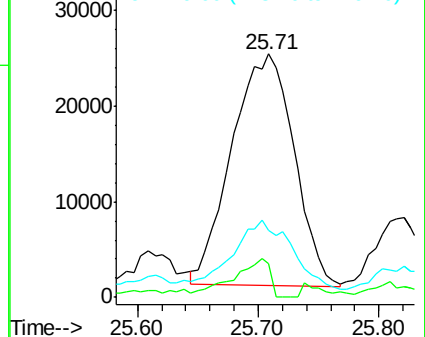

#91

Benzo(g,h,i)perylene

Concen: 6.49 ng/ul

RT: 26.40 min Scan# 4048

Delta R.T. -0.00 min

Lab File: BM008437.D

Acq: 18 Dec 2016 14:35


Tgt Ion:276 Resp: 293535

Ion Ratio Lower Upper

276 100

138 14.7 12.0 18.0

277 24.2 19.4 29.0

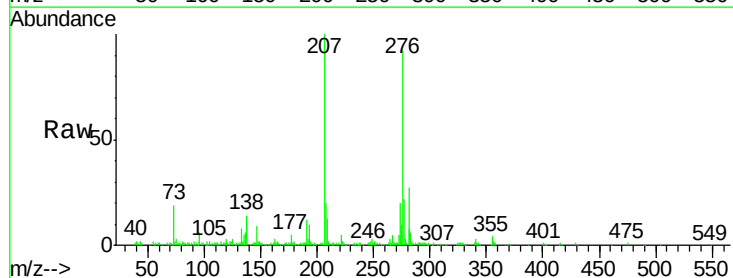

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

