
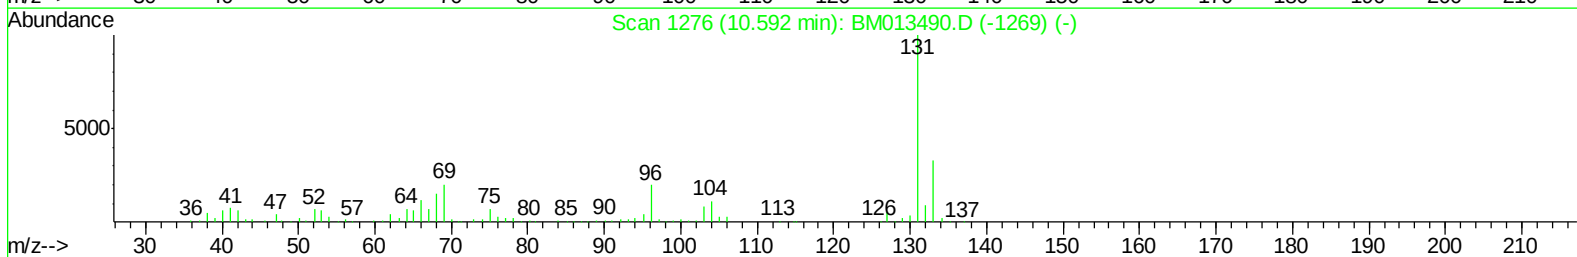
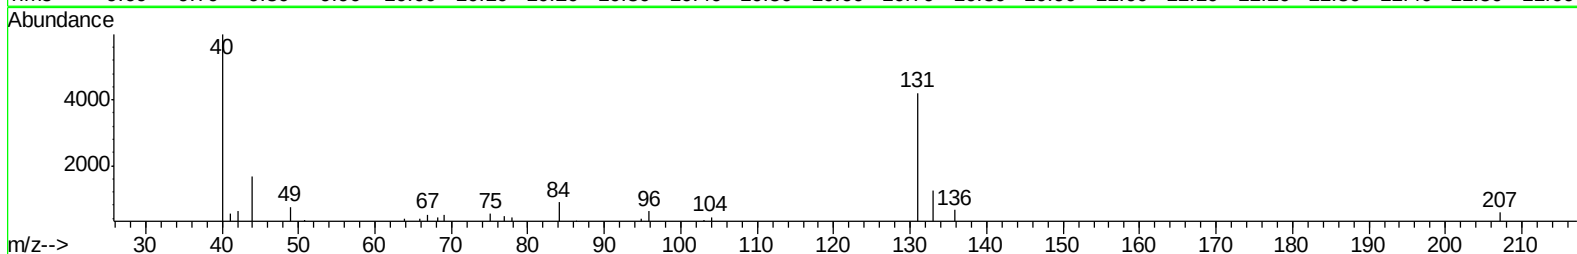


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
Data File : BM013504.D
Acq On : 18 Dec 2017 18:24
Operator : SJ/JU
Sample : I6776-04MEDL2 30X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 03:14:34 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 19 00:41:55 2017
Response via : Initial Calibration

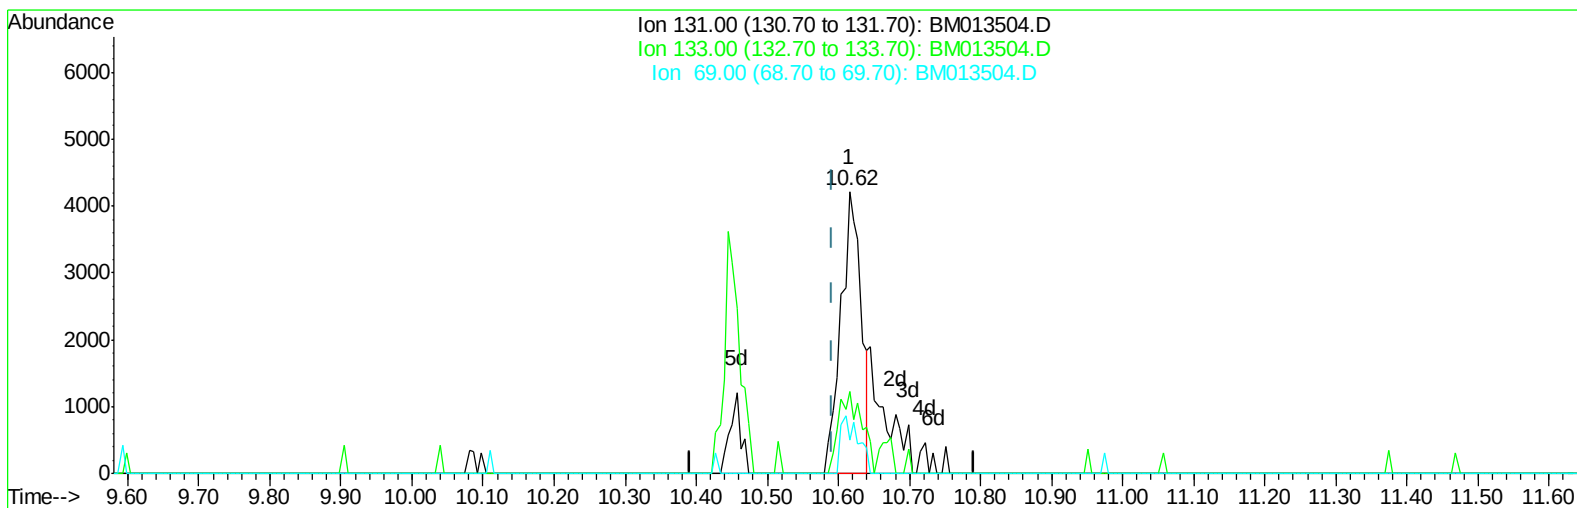

TIC: BM013504.D

(29) 4-Chloroaniline-d4 (S)
10.616min (+0.023) 0.65ng/ul
response 8324

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	29.08
69.00	24.30	11.87#
0.00	0.00	0.00