


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
 Data File : BM013497.D
 Acq On : 18 Dec 2017 14:13
 Operator : SJ/JU
 Sample : I6776-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:57:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 00:41:55 2017
 Response via : Initial Calibration

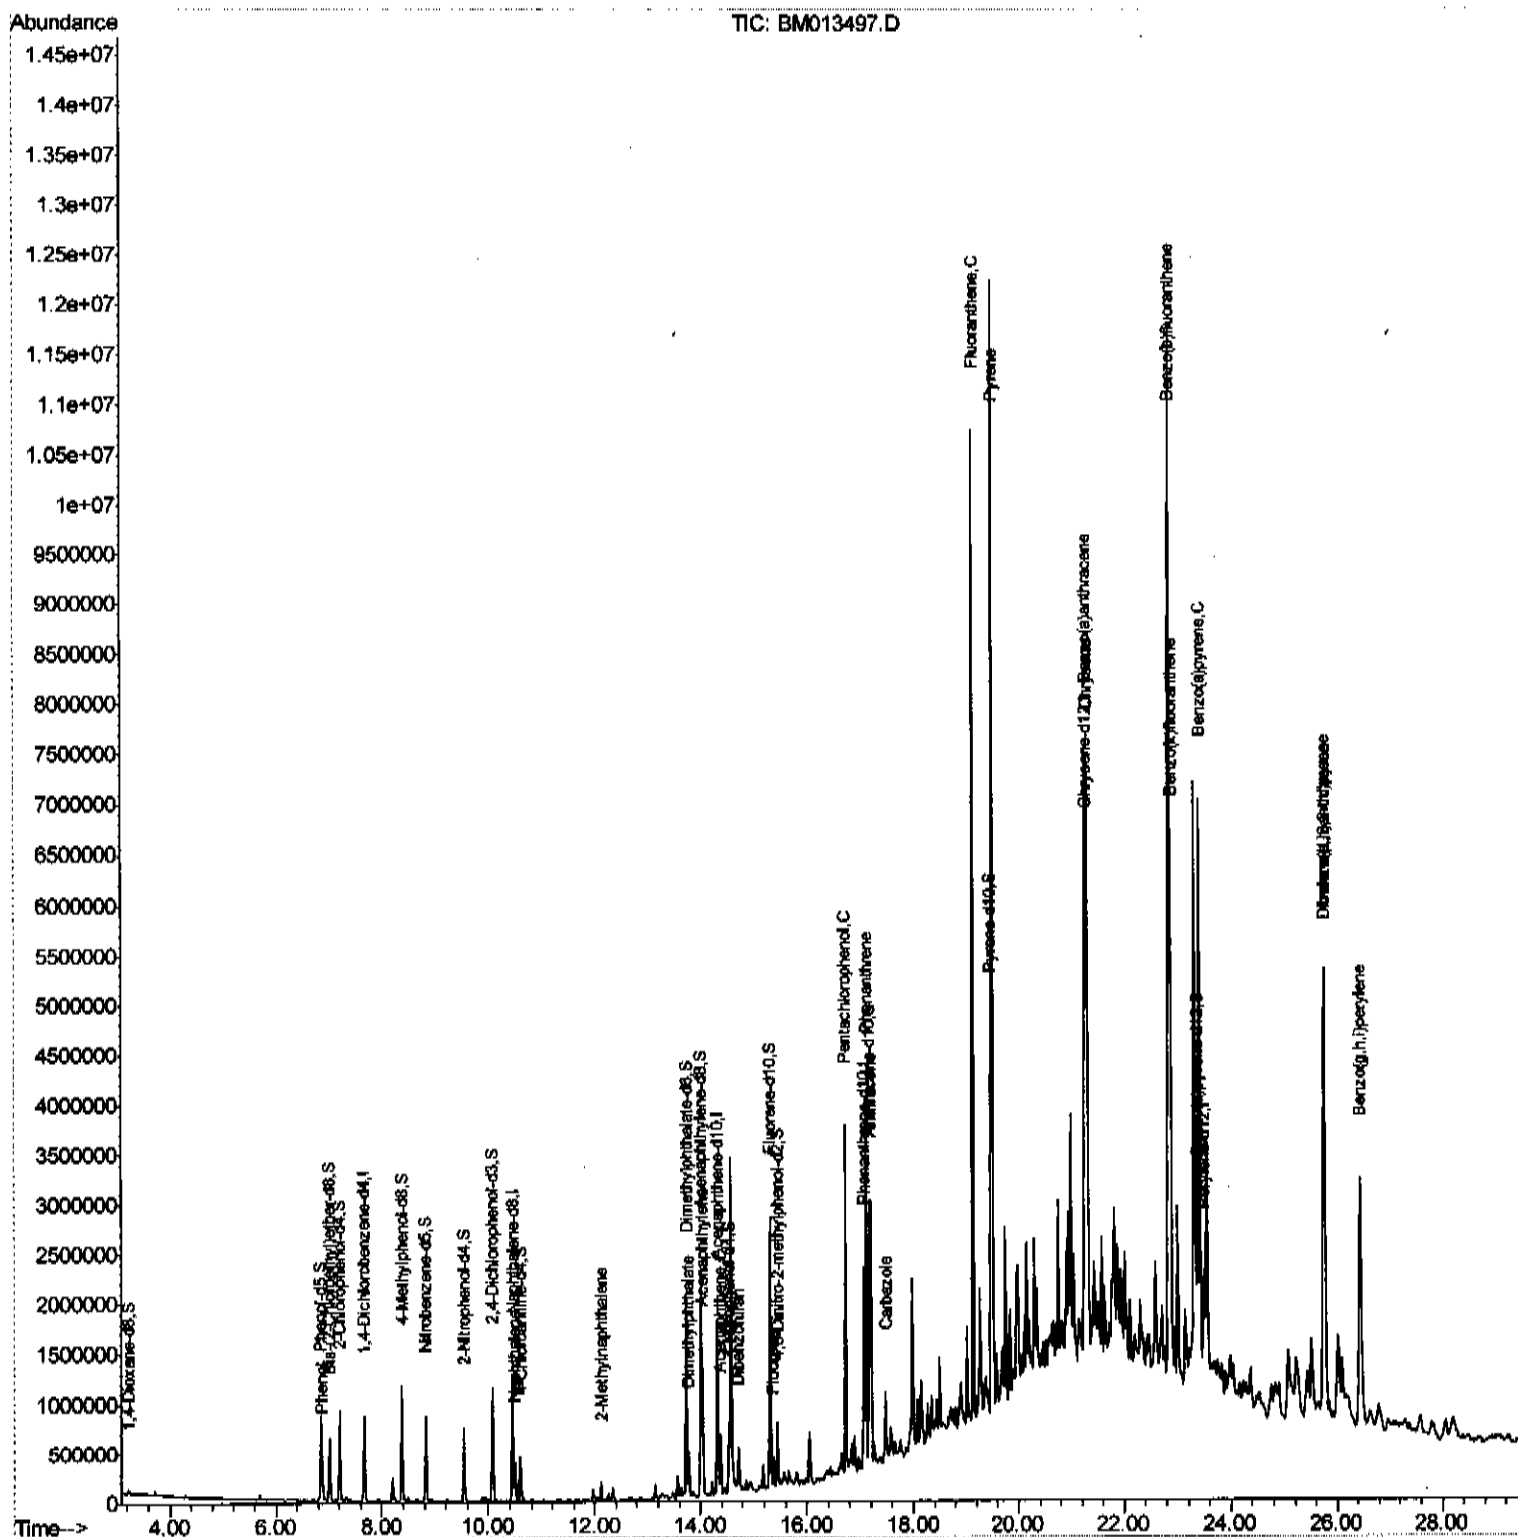


Data Path : Z:\HPCHEM1\BNA M\Data\BM121817\
 Data File : BM013496.D
 Acq On : 18 Dec 2017 13:37
 Operator : SJ/JU
 Sample : I6778-13ME
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 18 17:38:40 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 18 14:36:05 2017
 Response via : Initial Calibration

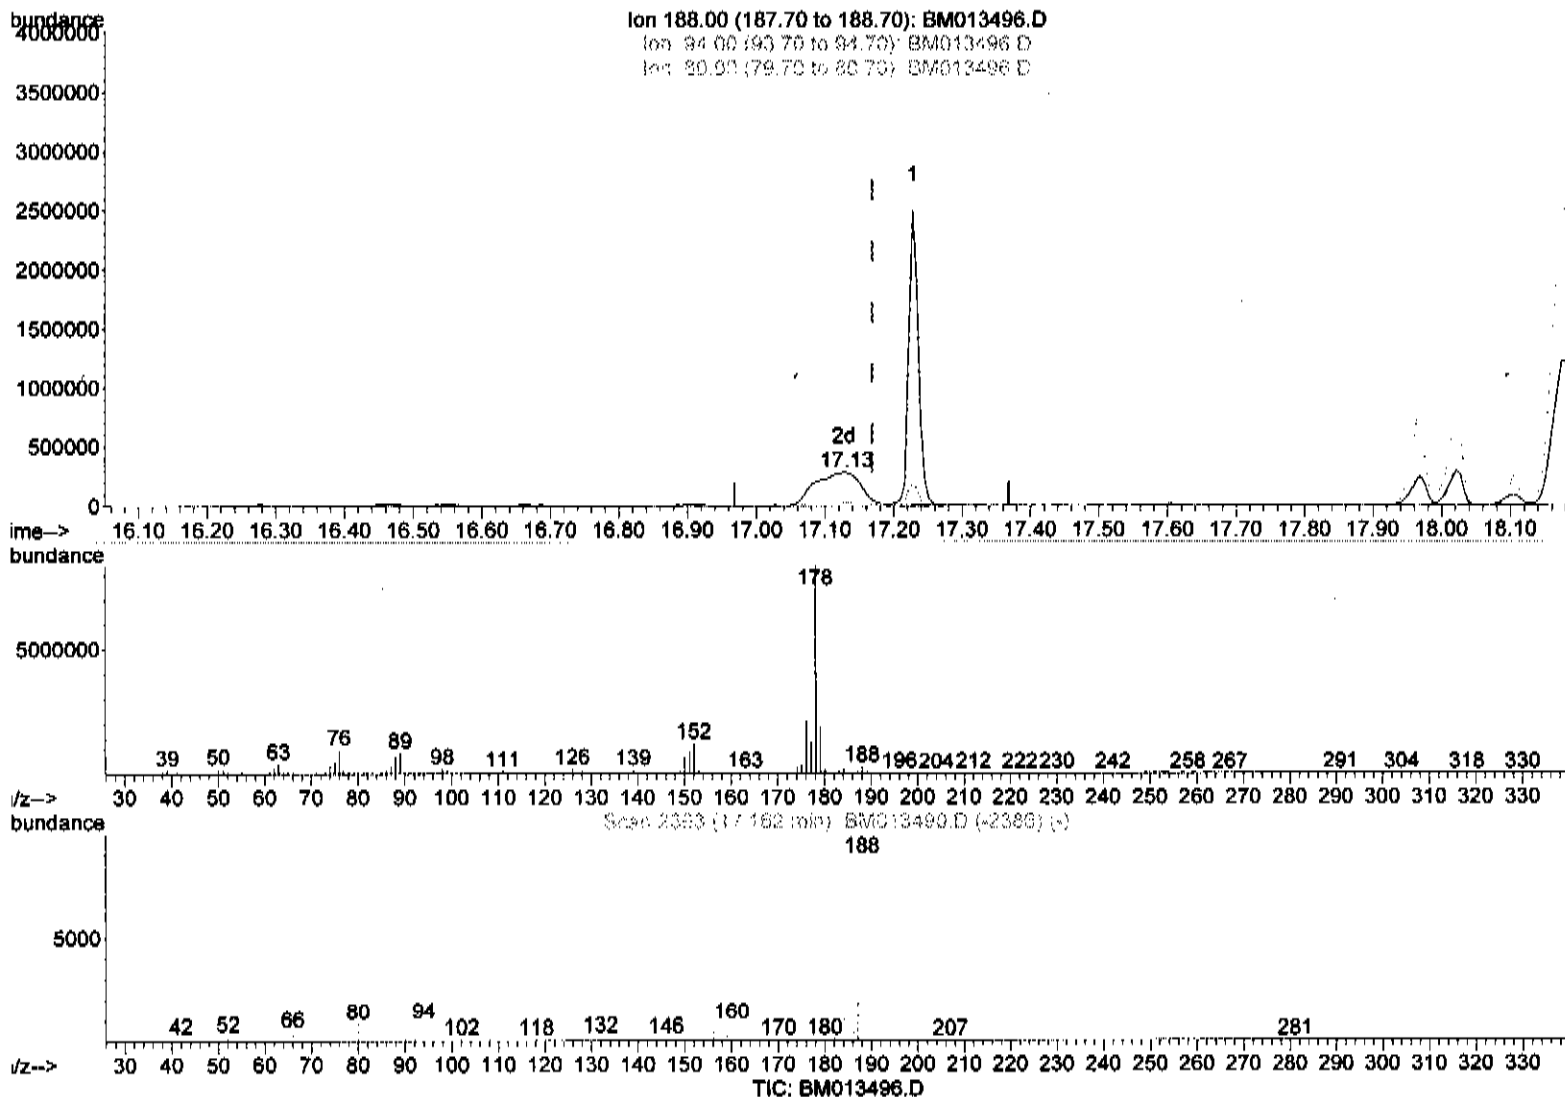

(70) Anthracene-d10 (S)

17.127min (-0.041) 20.18ng/ul m

SJ 12/19/17

response 1287278

Ion	Exp%	Act%
188.00	100	100
94.00	5.70	8.44#
80.00	5.90	10.17#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM121817\
 Data File : BM013496.D
 Acq On : 18 Dec 2017 13:37
 Operator : SJ/JU
 Sample : I6778-13ME
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 18 17:38:40 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 18 14:36:05 2017
 Response via : Initial Calibration

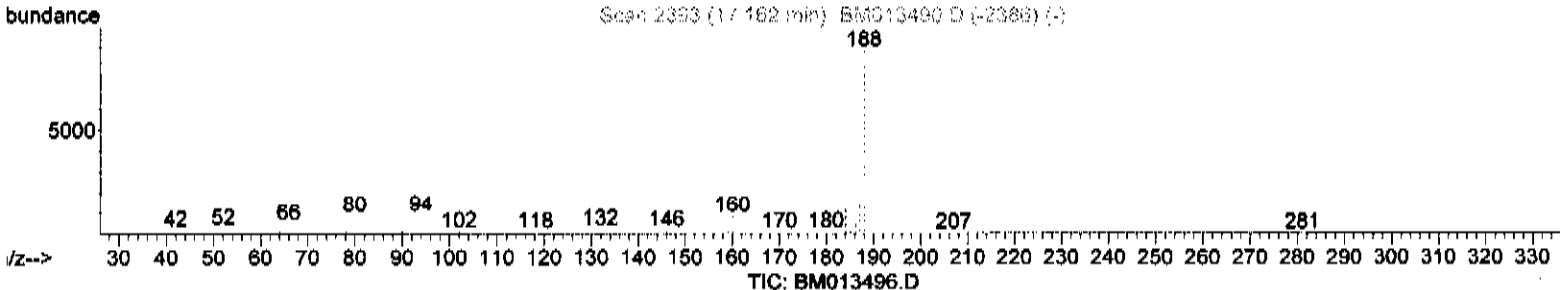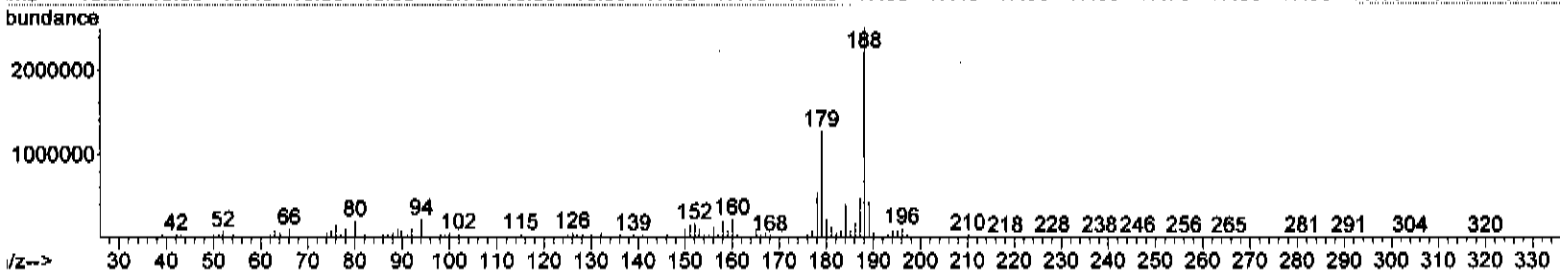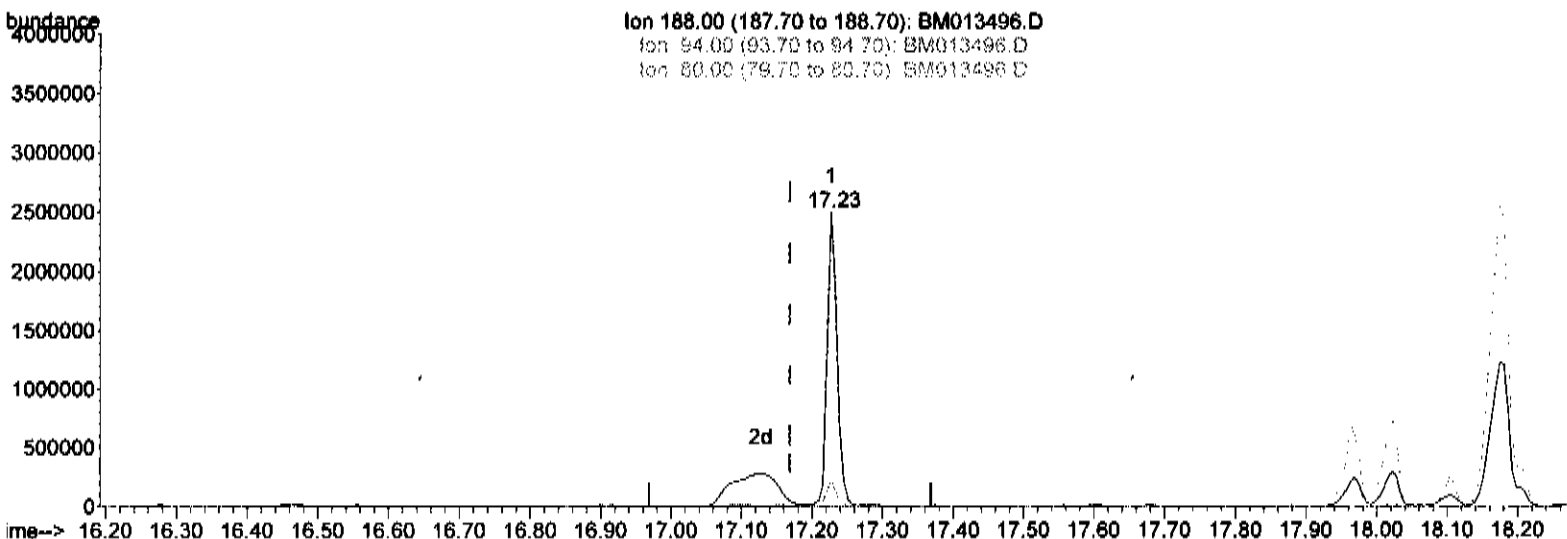

(70) Anthracene-d10 (S)

17.227min (+0.059) 38.90ng/ul m

SJ 12/19/17

response 2481714

Ion	Exp%	Act%
188.00	100	100
94.00	5.70	8.62%
80.00	5.90	7.98%
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
 Data File : BM013497.D
 Acq On : 18 Dec 2017 14:13
 Operator : SJ/JU
 Sample : I6776-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:42:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 00:41:55 2017
 Response via : Initial Calibration

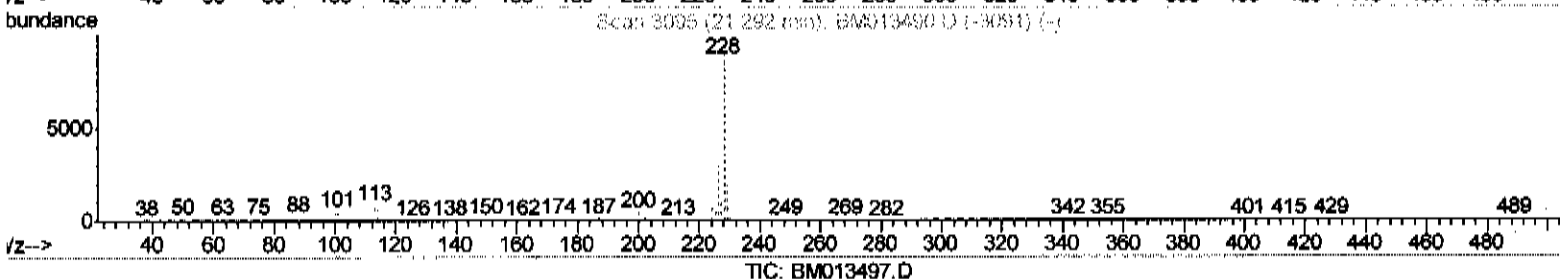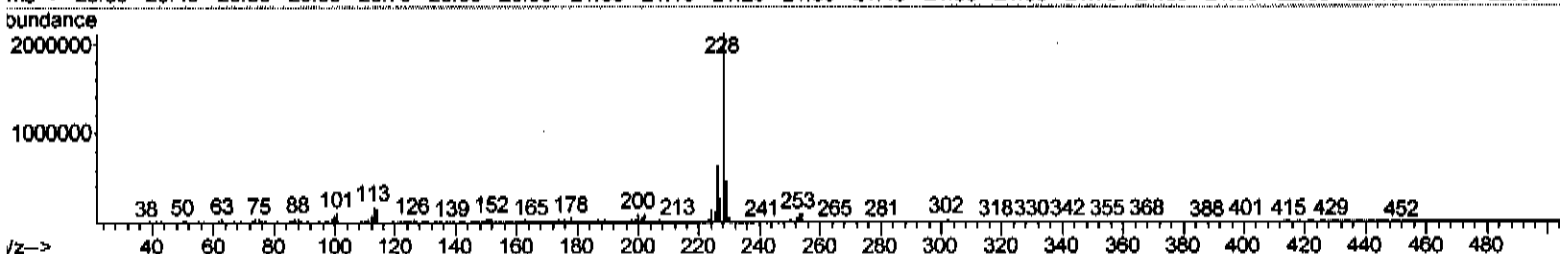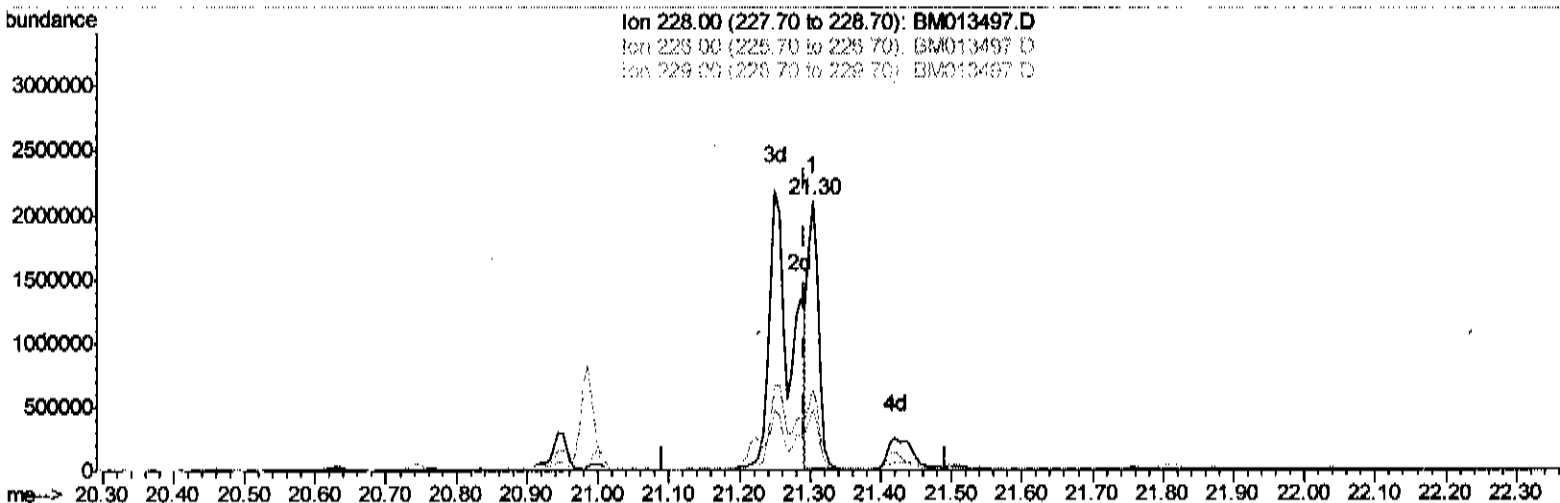

(82) Chrysene

21.303min (+0.012) 44.01ng/ul

response 2234971

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	30.16
229.00	19.40	22.11
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
 Data File : BM013497.D
 Acq On : 18 Dec 2017 14:13
 Operator : SJ/JU
 Sample : I6776-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:42:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 00:41:55 2017
 Response via : Initial Calibration

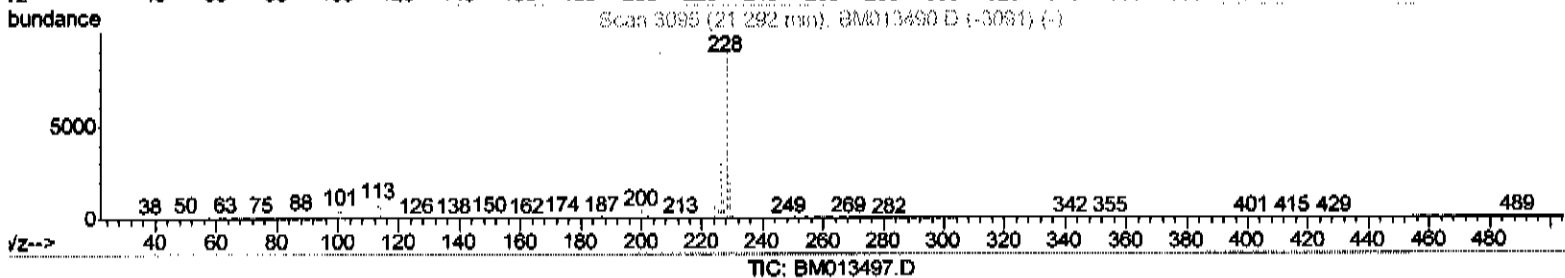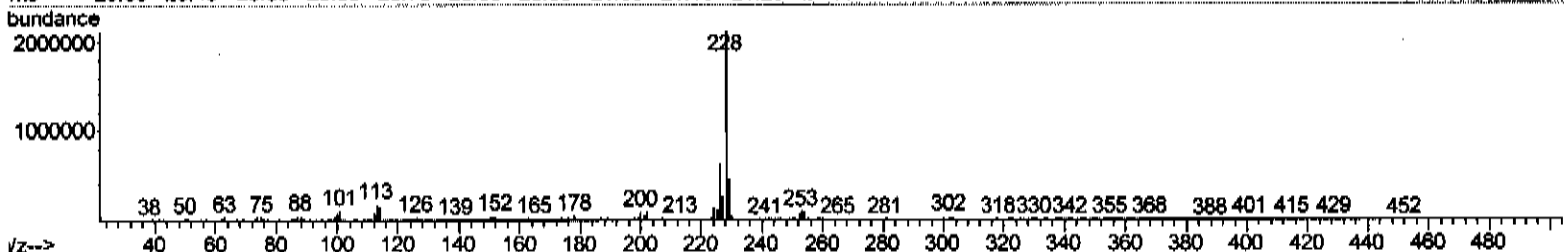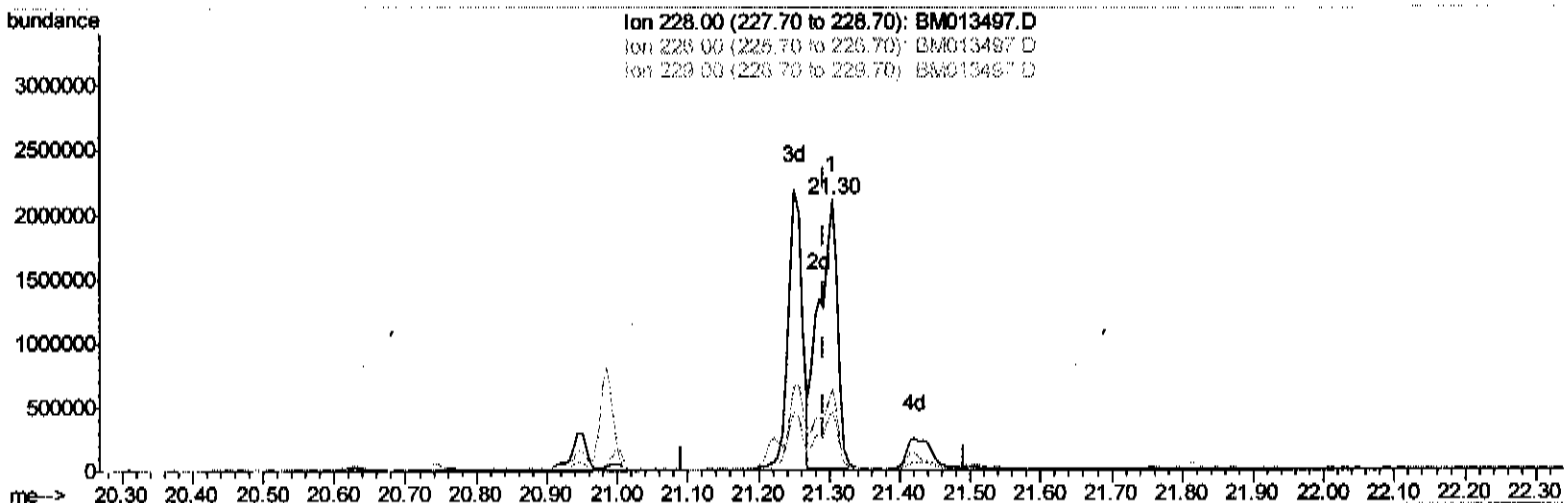

(82) Chrysene

21.303min (+0.012) 75.05ng/ul m

SD 12/19/17

response 3810741

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	30.16
229.00	19.40	22.11
0.00	0.00	0.00



Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
 Data File : BM013497.D
 Acq On : 18 Dec 2017 14:13
 Operator : SJ/JU
 Sample : I6776-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:42:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 00:41:55 2017
 Response via : Initial Calibration

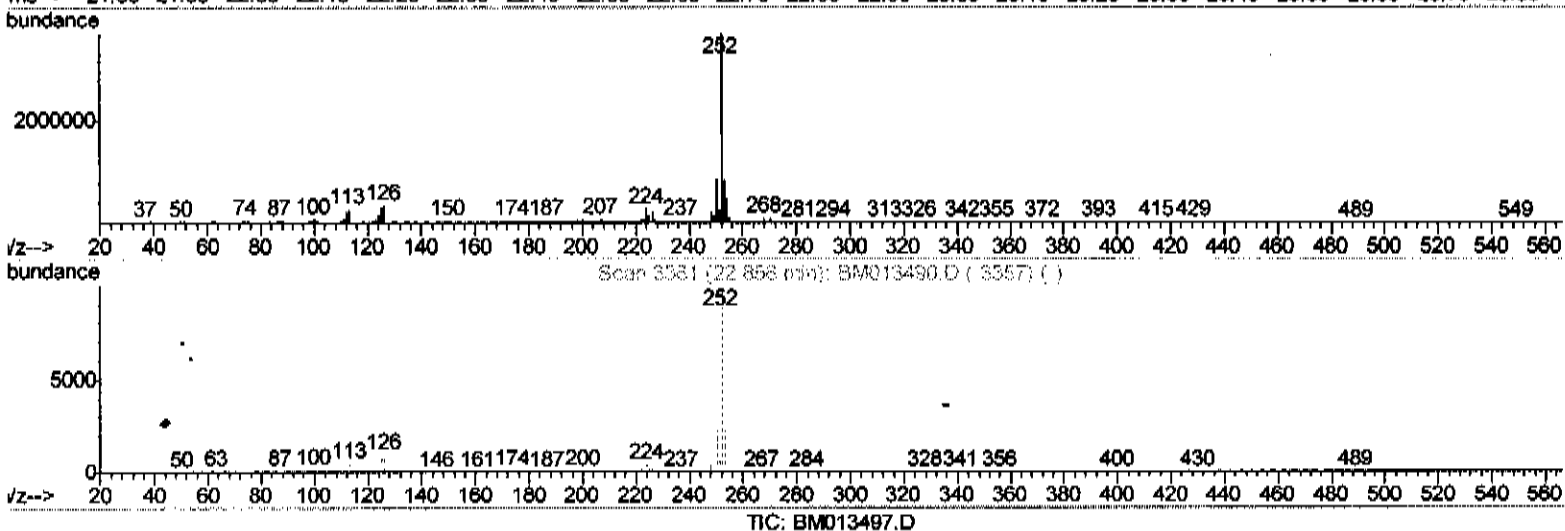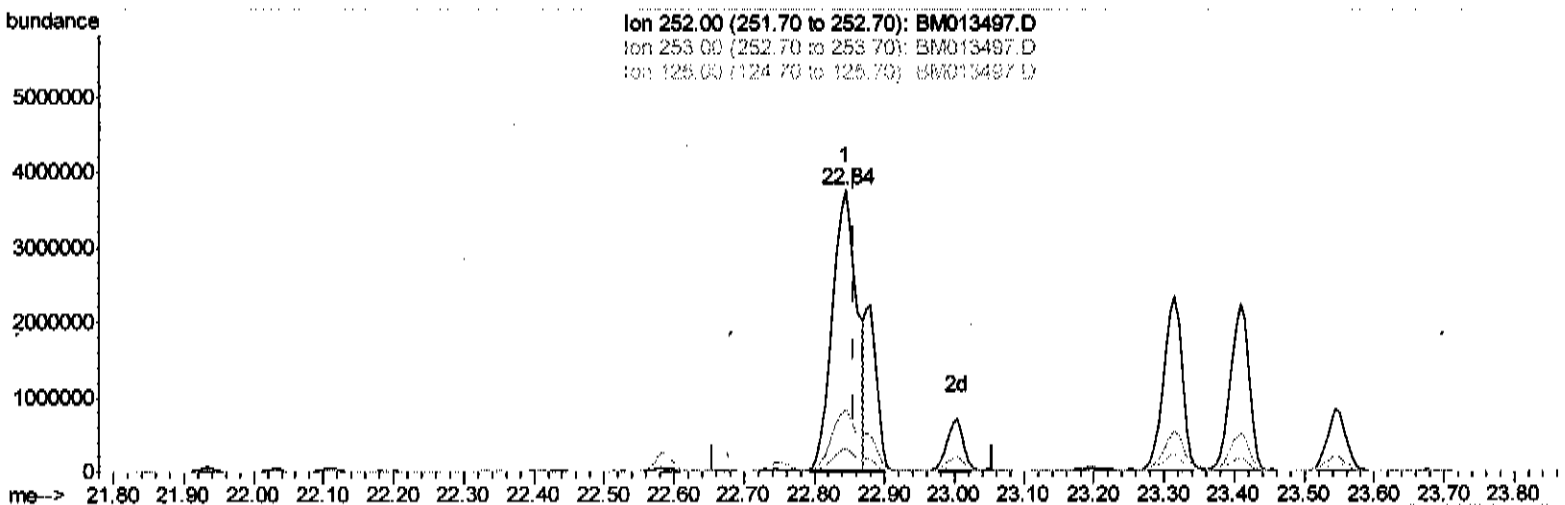

(86) Benzo(k)fluoranthene

22.844min (-0.012) 183.24ng/ul

response 9036588

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.41
125.00	4.30	7.98#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
 Data File : BM013497.D
 Acq On : 18 Dec 2017 14:13
 Operator : SJ/JU
 Sample : I6776-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:42:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 00:41:55 2017
 Response via : Initial Calibration

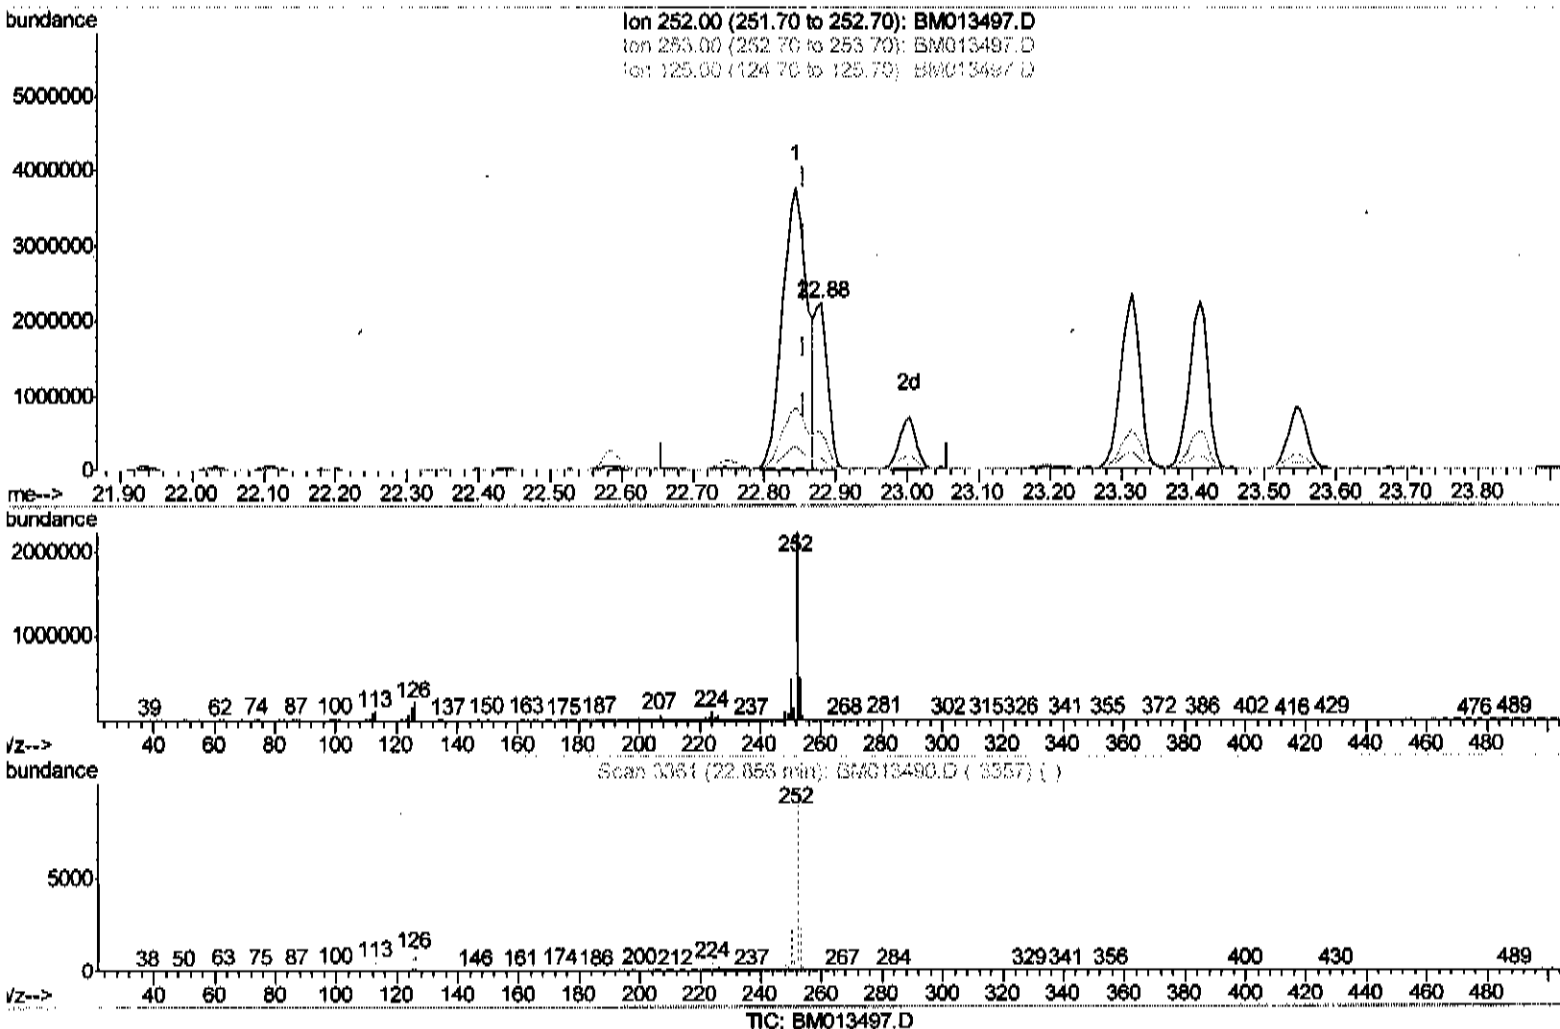

(86) Benzo(k)fluoranthene

22.880min (+0.024) 52.26ng/ul m

response 2577273

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.45
125.00	4.30	7.09#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
 Data File : BM013497.D
 Acq On : 18 Dec 2017 14:13
 Operator : SJ/JU
 Sample : I6776-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A60

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:57:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 OLast Update : Tue Dec 19 00:41:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	226268	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	978316	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	556068	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1142667	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	862665	20.00	ng/ul	0.01
83) Perylene-d12	23.50	264	777390	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	18413	4.03	ng/uL	0.00
5) Phenol-d5	6.85	99	482019	24.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	262941	23.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	386078	25.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	395281	23.63	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	198327	25.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	223672	26.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	419827	24.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	248519	15.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1241116	25.08	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1592870	26.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	186448	21.69	ng/ul	0.00
57) Fluorene-d10	15.32	176	1068557	25.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	142131	19.77	ng/ul	0.00
70) Anthracene-d10	17.17	188	1479466	25.85	ng/ul	0.00
76) Pyrene-d10	19.47	212	1349085	31.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	974615	24.61	ng/ul	0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	6.88	94	89428	4.621	ng/ul#	86
28) Naphthalene	10.50	128	281019	5.583	ng/ul	98
34) 2-Methylnaphthalene	12.12	142	87709	2.318	ng/ul	85
44) Dimethylphthalate	13.78	163	238725	5.044	ng/ul	98
47) Acenaphthylene	14.04	152	936636	16.575	ng/ul	99
49) Acenaphthene	14.38	153	235475	6.117	ng/ul	97
53) Dibenzofuran	14.72	168	245081	4.313	ng/ul	98
58) Fluorene	15.37	166	144851	3.081	ng/ul#	95
68) Pentachlorophenol	16.73	266	533220	62.237	ng/ul	99
69) Phenanthrene	17.11	178	2177061	33.536	ng/ul	99
71) Anthracene	17.20	178	1628217	24.538	ng/ul	98
72) Carbazole	17.47	167	381702	6.688	ng/ul	99
74) Fluoranthene	19.14	202	6042011	75.948	ng/ul#	93
77) Pyrene	19.50	202	6692439	127.696	ng/ul#	92
80) Benzo(a)anthracene	21.25	228	3040214	55.545	ng/ul	94
82) Chrysene	21.30	228	3810741m	75.045	ng/ul	94
85) Benzo(b)fluoranthene	22.84	252	9036588	172.437	ng/ul#	98
86) Benzo(k)fluoranthene	22.88	252	2577273m	52.260	ng/ul	98
88) Benzo(a)pyrene	23.41	252	4081966	86.711	ng/ul#	98
89) Indeno(1,2,3-cd)pyrene	25.75	276	3611241	77.313	ng/ul#	96
90) Dibenzo(a,h)anthracene	25.74	278	974616	24.505	ng/ul#	91
91) Benzo(g,h,i)perylene	26.44	276	3330212	90.387	ng/ul#	95

SJ 12/19/17
 SJ 12/19/17

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121817\
Data File : BM013497.D
Acq On : 18 Dec 2017 14:13
Operator : SJ/JU
Sample : I6776-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A60

Manual Integrations
APPROVED

Sohil
12/19/2017 4:56:27 PM

Quant Time: Dec 19 00:57:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 19 00:41:55 2017
Response via : Initial Calibration

Internal Standards	R.T.	QI	on	Response	Conc	Units	Dev	(Min)
--------------------	------	----	----	----------	------	-------	-----	-------

(#) = qualifier out of range (m) = manual integration (+) = signals summed