
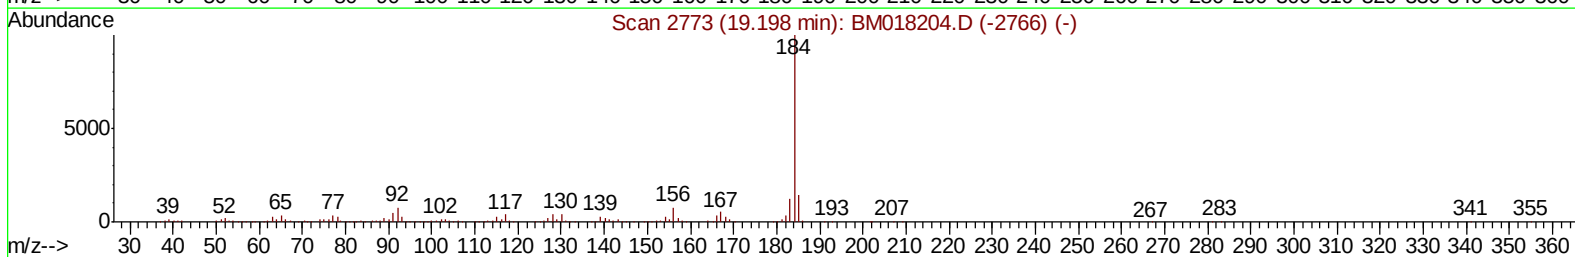
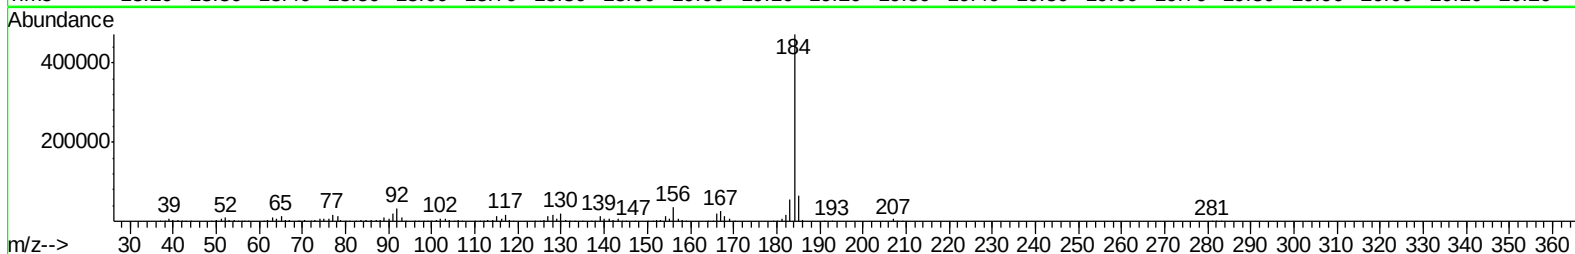


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121818\
Data File : BM018270.D
Acq On : 18 Dec 2018 13:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:17:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

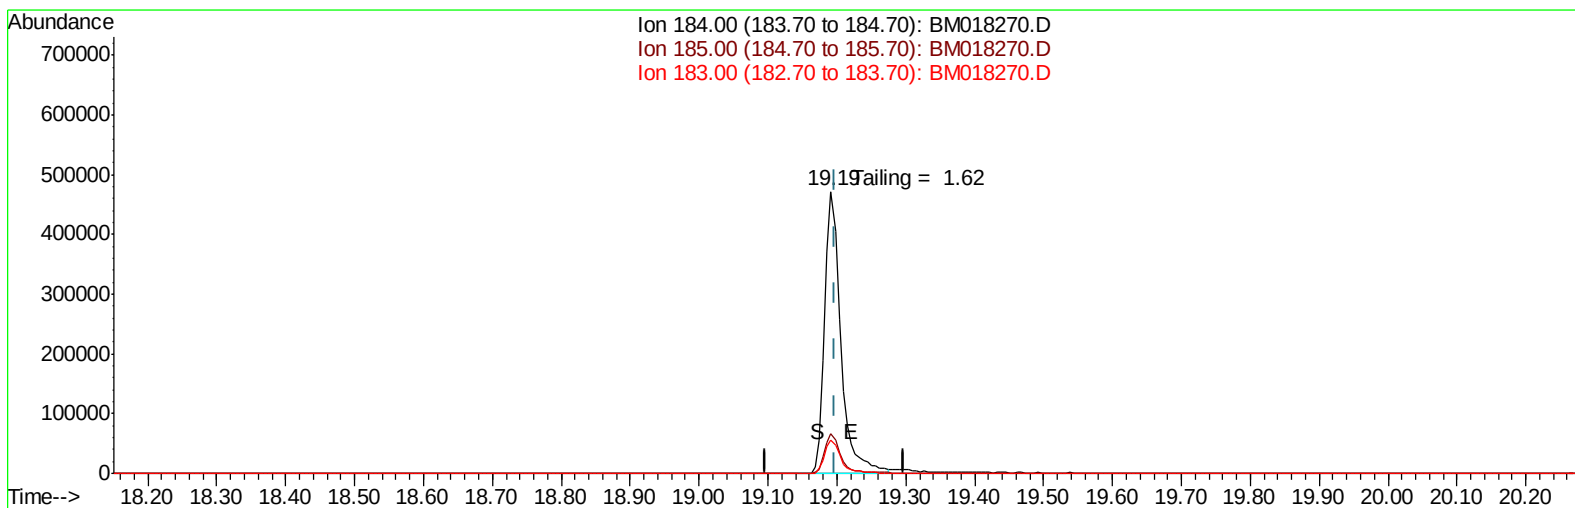

TIC: BM018270.D

(77) Benzidine




19.192min (-0.006) 0.00ng

response 770244

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.05
183.00	12.10	11.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121818\
Data File : BM018270.D
Acq On : 18 Dec 2018 13:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:17:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

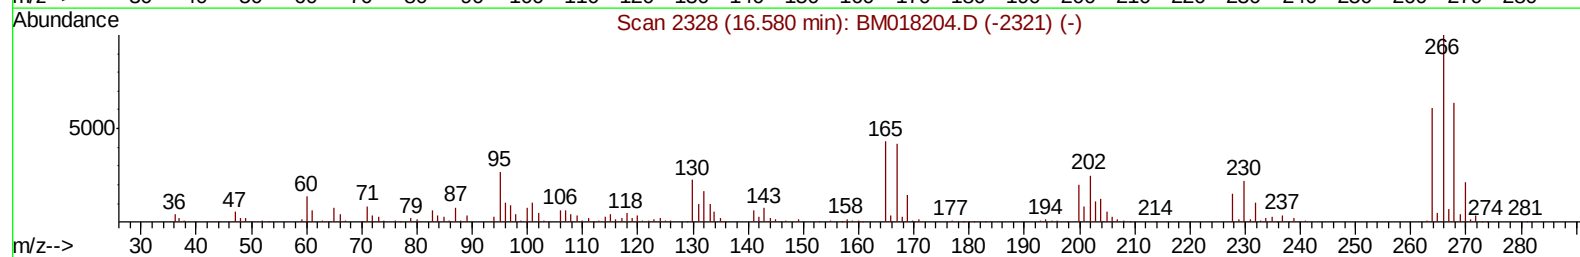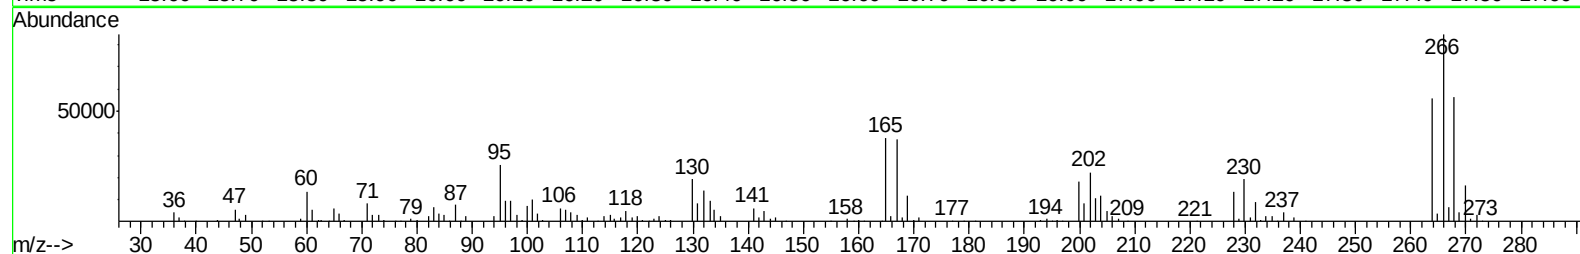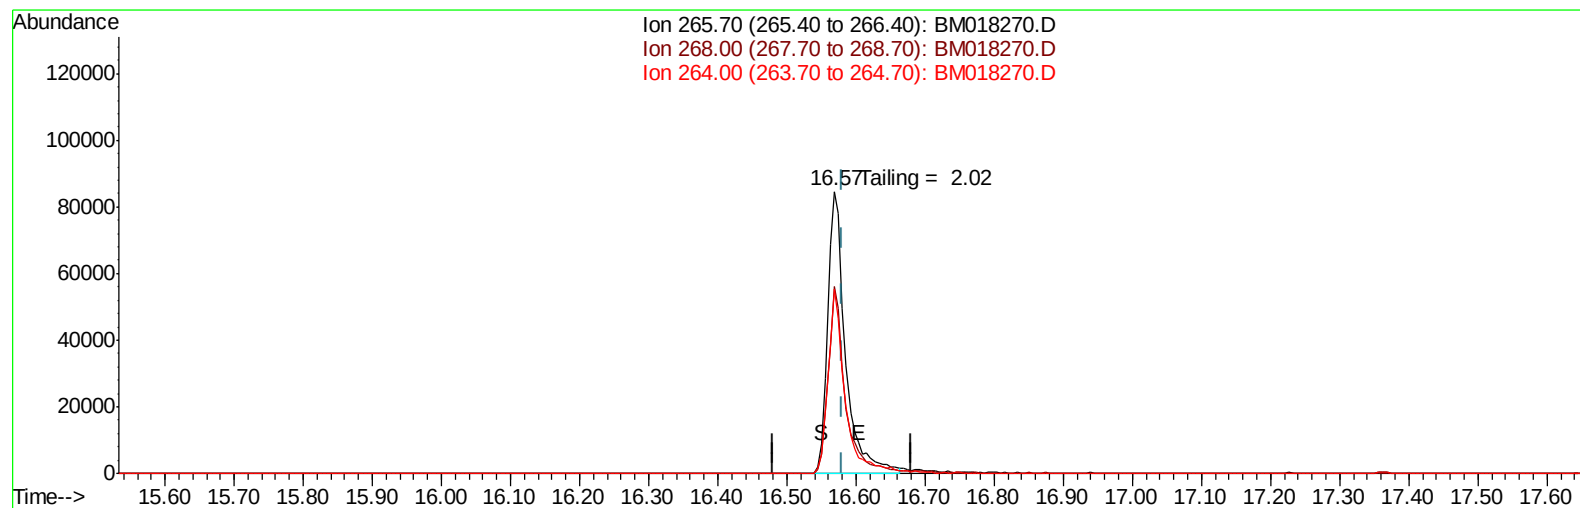

TIC: BM018270.D

(70) Pentachlorophenol (C)

16.568min (-0.012) 0.00ng

response 148976

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.46
264.00	61.20	65.69
0.00	0.00	0.00