

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121818\
 Data File : BM018277.D
 Acq On : 18 Dec 2018 18:47
 Operator : JU/SJ
 Sample : J6340-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-04B

Quant Time: Dec 19 03:41:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	131466	20.00	ng	-0.02
21) Naphthalene-d8	10.25	136	499354	20.00	ng	-0.02
39) Acenaphthene-d10	14.15	164	256674	20.00	ng	-0.02
64) Phenanthrene-d10	16.91	188	474785	20.00	ng	-0.01
76) Chrysene-d12	21.13	240	411648	20.00	ng	-0.01
87) Perylene-d12	23.29	264	456000	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	1156774	146.99	ng	0.00
7) Phenol-d6	6.69	99	1532929	140.14	ng	-0.01
23) Nitrobenzene-d5	8.65	82	985667	101.25	ng	-0.02
42) 2,4,6-Tribromophenol	15.66	330	400738	106.37	ng	-0.01
45) 2-Fluorobiphenyl	12.75	172	1825718	92.13	ng	-0.02
79) Terphenyl-d14	19.56	244	1682458	92.44	ng	-0.01
Target Compounds						
10) Phenol	6.72	94	83778	7.232	ng	94
50) Dimethylphthalate	13.62	163	144304	6.762	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121818\
Data File : BM018277.D
Acq On : 18 Dec 2018 18:47
Operator : JU/SJ
Sample : J6340-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-04B

Quant Time: Dec 19 03:41:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

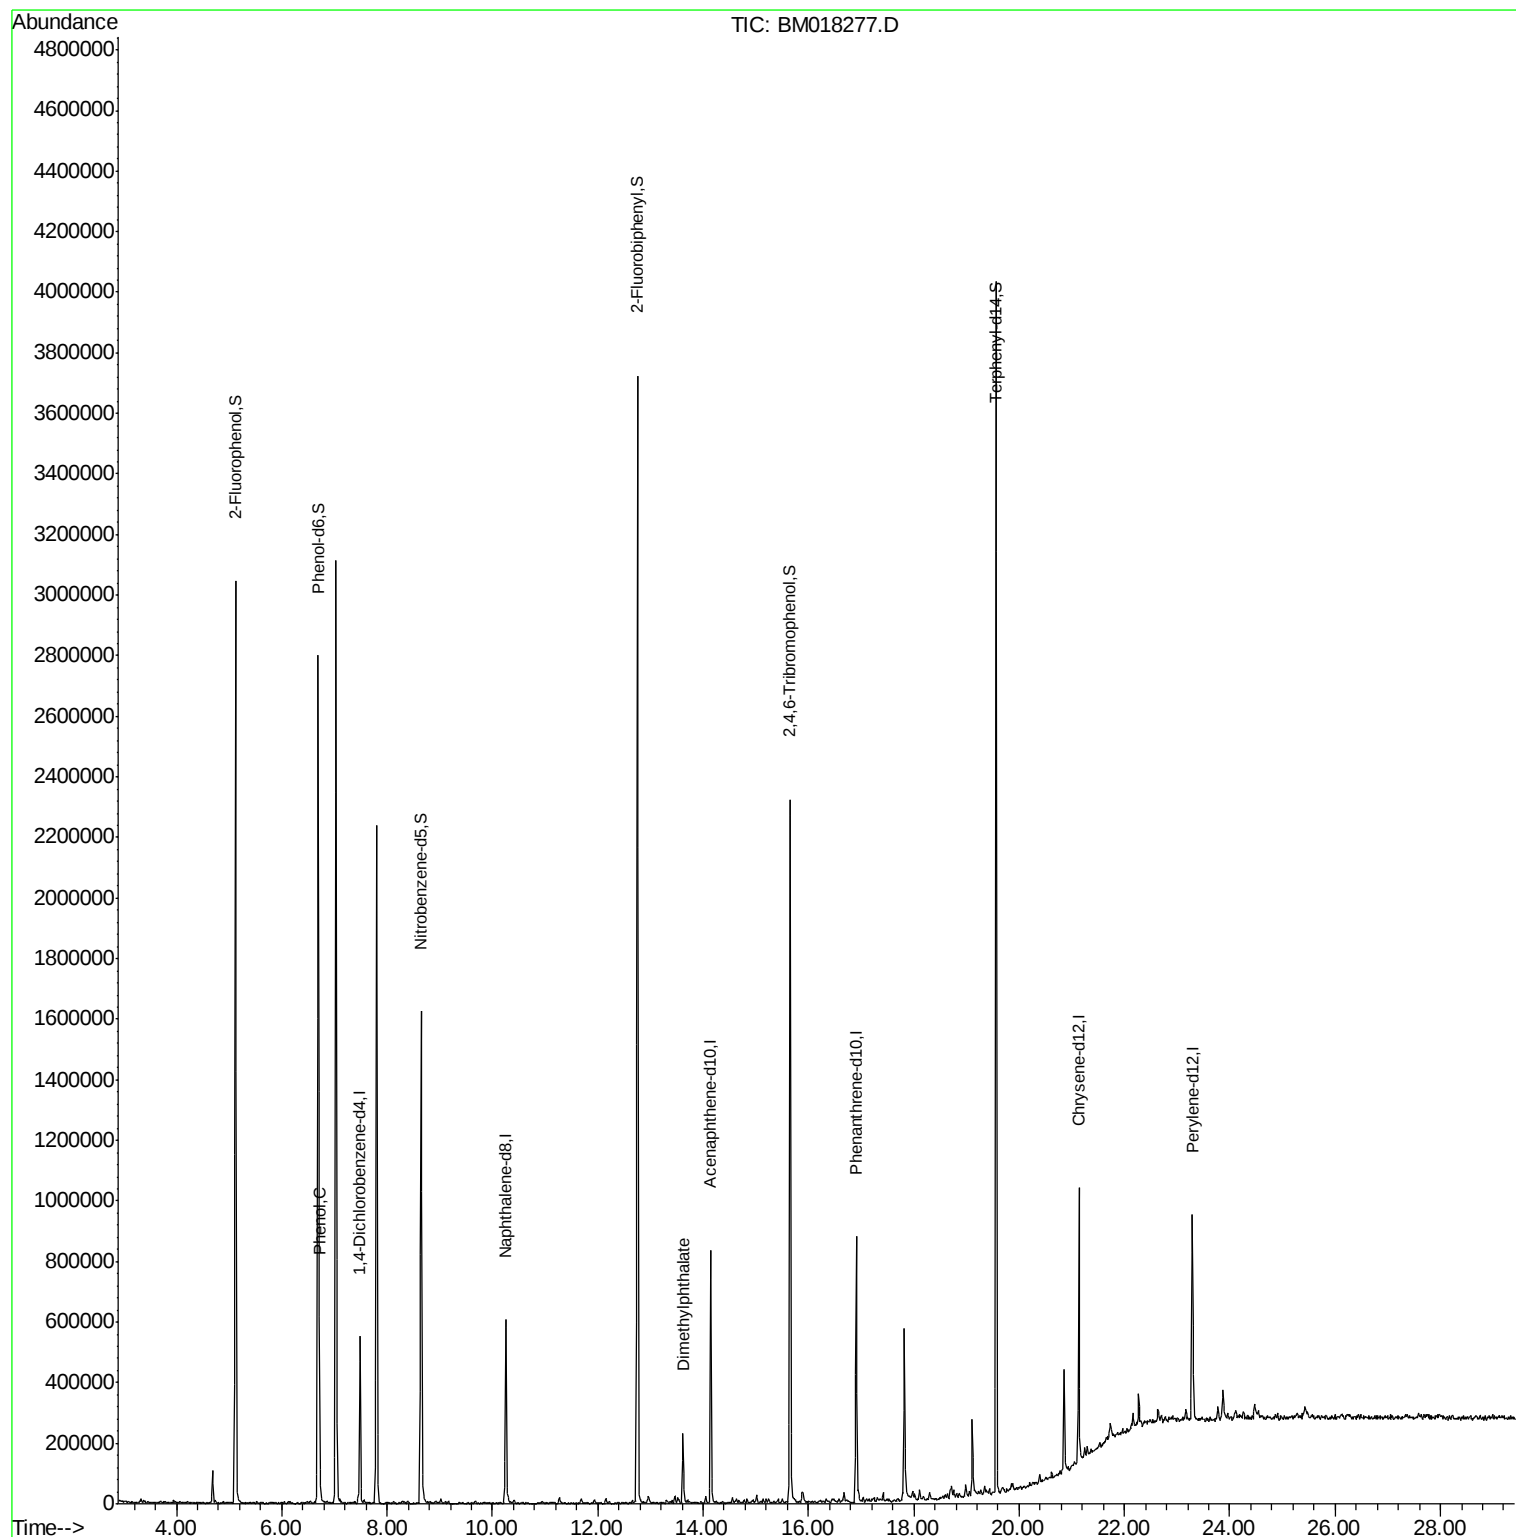

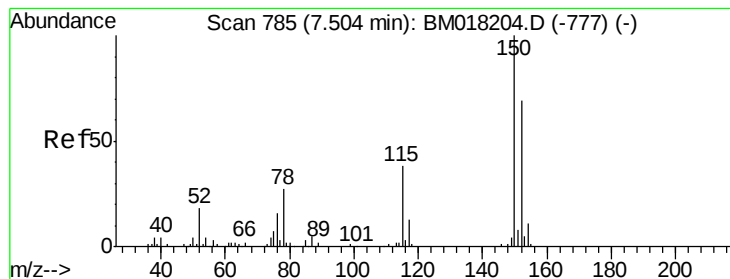


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 782
Delta R.T. -0.02 min
Lab File: BM018277.D
Acq: 18 Dec 2018 18:47

Instrument :
BNA_M
ClientSampleId :
SB-04B

Tot Ion:152 Resp: 131466
Ion Ratio Lower Upper
152 100
150 154.7 116.1 174.1
115 64.7 44.6 67.0

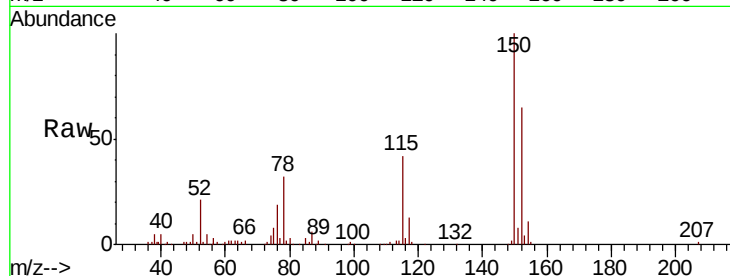


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

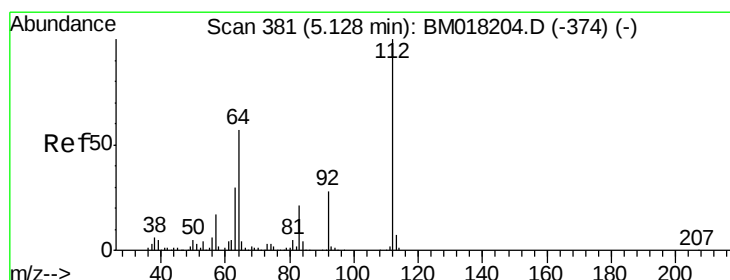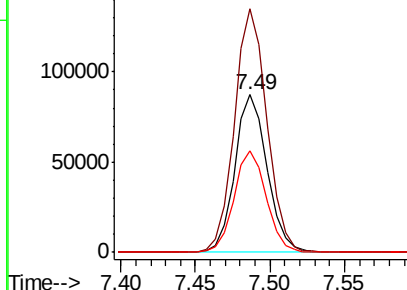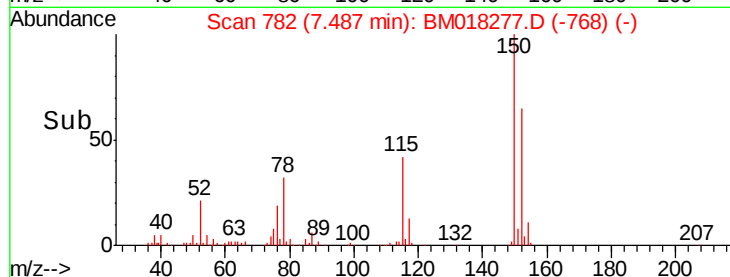



#5

2-Fluorophenol
Concen: 146.987 ng
RT: 5.12 min Scan# 380
Delta R.T. -0.01 min
Lab File: BM018277.D
Acq: 18 Dec 2018 18:47

Tgt Ion:112 Resp: 1156774
Ion Ratio Lower Upper
112 100
64 58.6 45.4 68.2
63 32.7 24.0 36.0

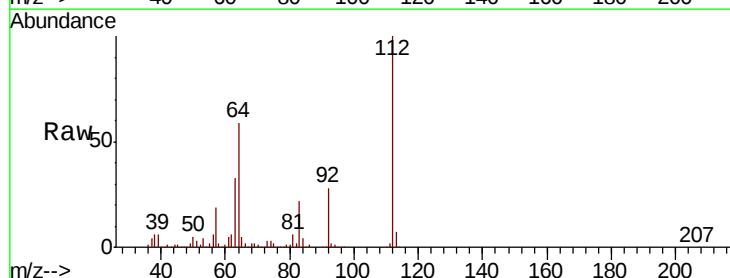

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

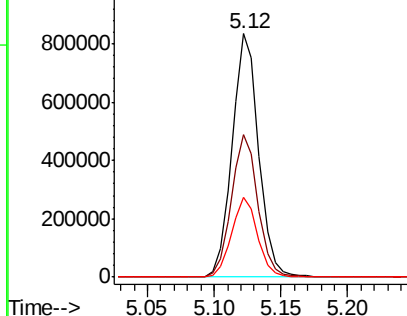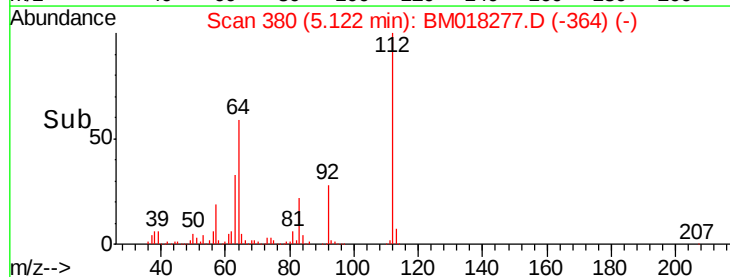



#7

Phenol-d6

Concen: 140.140 ng

RT: 6.69 min Scan# 647

Delta R.T. -0.01 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47

Instrument :

BNA_M

ClientSampled :

SB-04B


Tot Ion: 99 Resp: 1532929

Ion Ratio Lower Upper

99 100

42 16.5 12.3 18.5




71 40.7 30.2 45.2

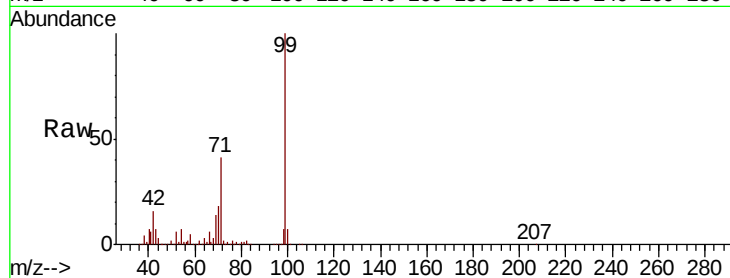

Abundance Ion 99.00 (98.70 to 99.70): BM018277.D (-632) (-)

Ion 42.00 (41.70 to 42.70): BM018277.D (-632) (-)

Ion 71.00 (70.70 to 71.70): BM018277.D (-632) (-)

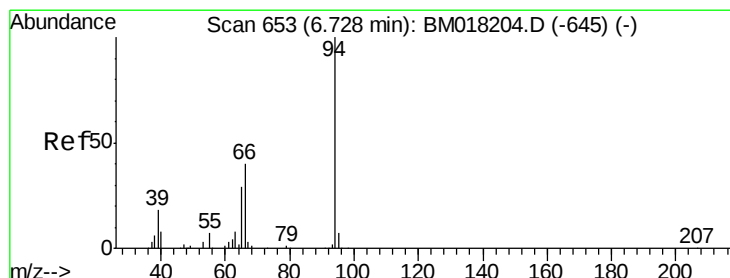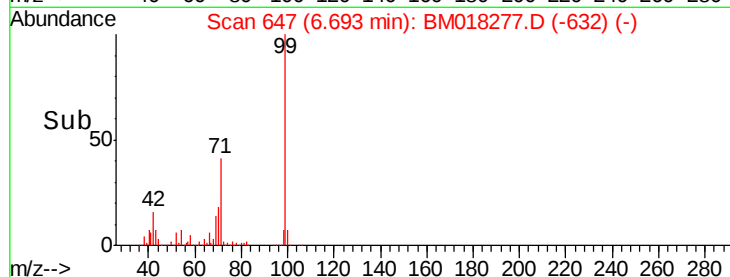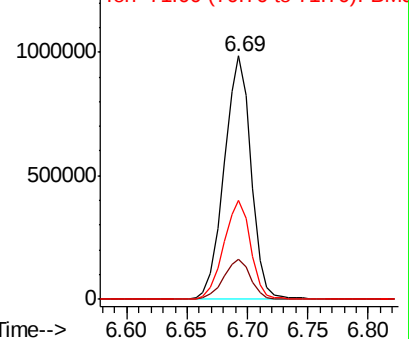

#10

Phenol

Concen: 7.232 ng

RT: 6.72 min Scan# 651

Delta R.T. -0.01 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47


Tgt Ion: 94 Resp: 83778

Ion Ratio Lower Upper

94 100

65 31.9 9.5 49.5



66 45.9 21.3 61.3

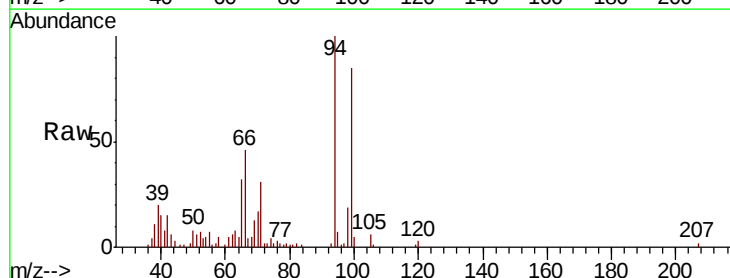


Abundance Ion 94.00 (93.70 to 94.70): BM018277.D (-636) (-)

Ion 65.00 (64.70 to 65.70): BM018277.D (-636) (-)

Ion 66.00 (65.70 to 66.70): BM018277.D (-636) (-)

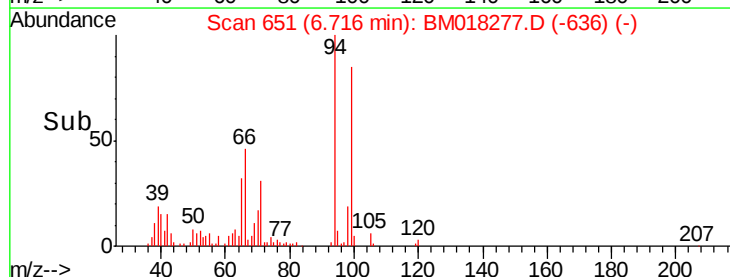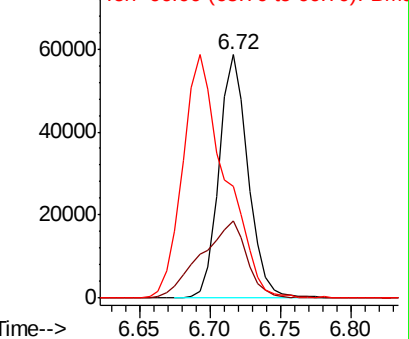

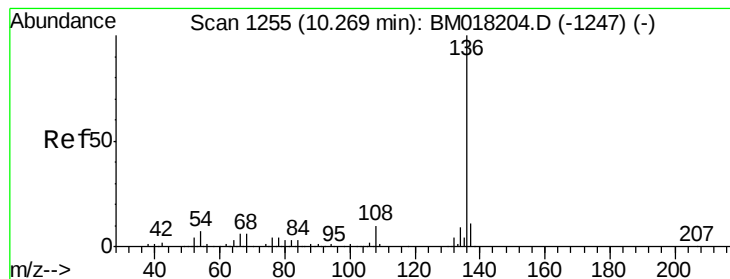

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.25 min Scan# 1252

Delta R.T. -0.02 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47

Instrument :

BNA_M

ClientSampleId :

SB-04B

Tot Ion:136 Resp: 499354


Ion Ratio Lower Upper

136 100

137 10.8 9.2 13.8

54 6.2 5.2 7.8

68 5.7 5.0 7.6



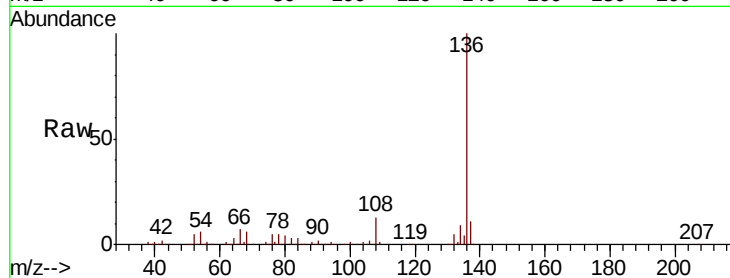


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM

Ion 68.00 (67.70 to 68.70): BM

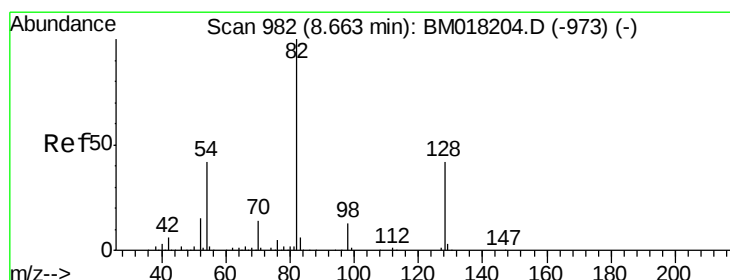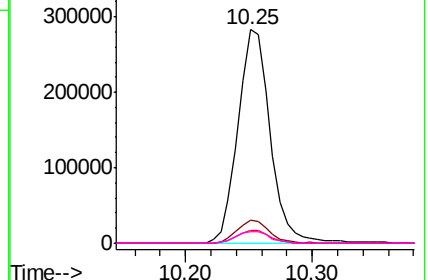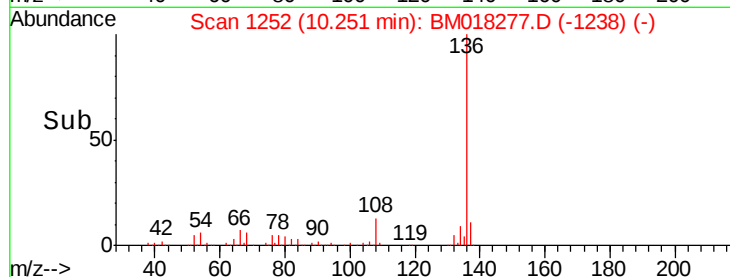

#23

Nitrobenzene-d5

Concen: 101.248 ng

RT: 8.65 min Scan# 979

Delta R.T. -0.02 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47


Tgt Ion: 82 Resp: 985667

Ion Ratio Lower Upper

82 100

128 38.0 33.4 50.2



54 42.7 33.4 50.2

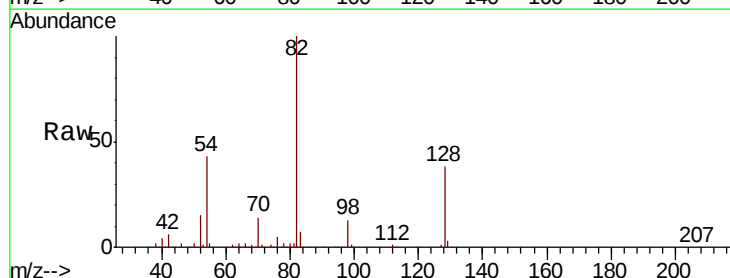


Abundance Ion 82.00 (81.70 to 82.70): BM

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BM

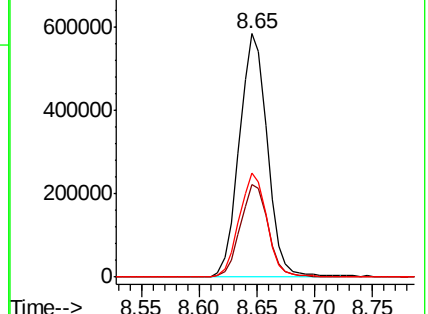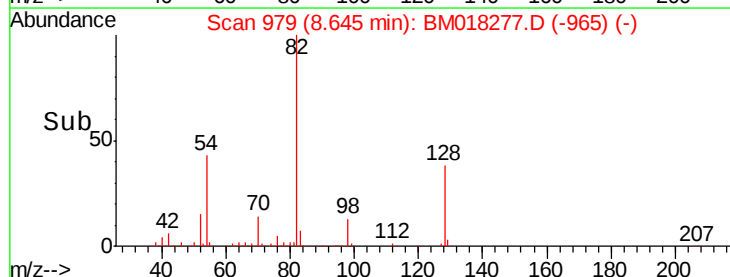

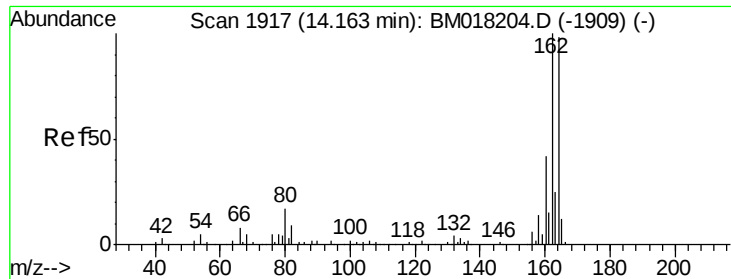

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.15 min Scan# 1914

Delta R.T. -0.02 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47

Instrument :

BNA_M

ClientSampleId :

SB-04B





Tot Ion:164 Resp: 256674

Ion Ratio Lower Upper

164 100

162 102.5 81.8 122.6

160 44.7 34.6 51.8

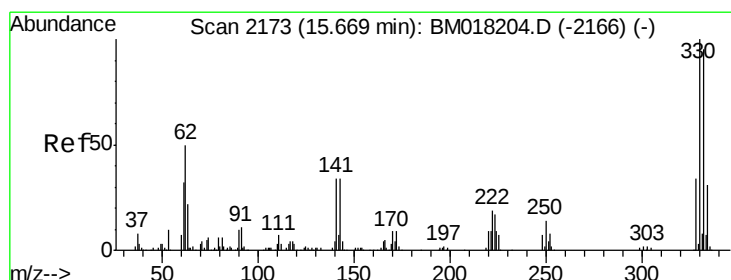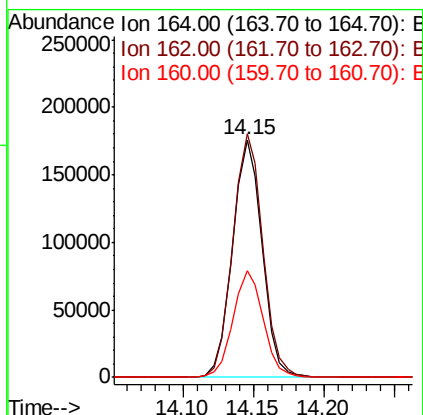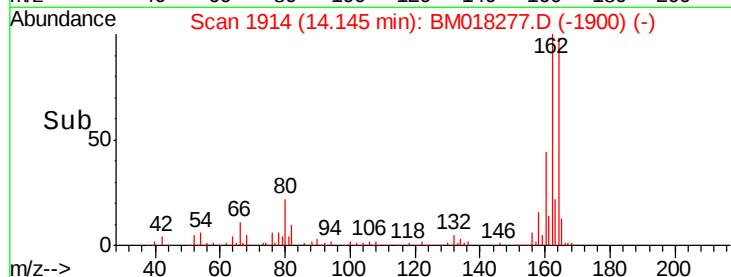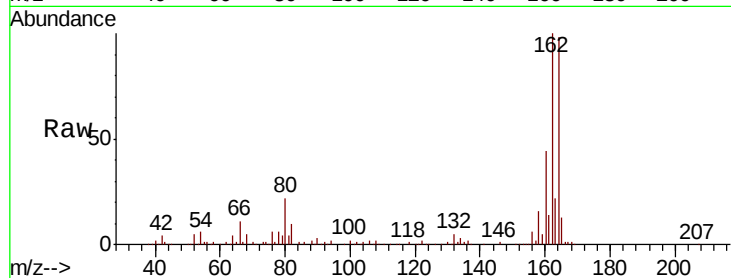

#42

2,4,6-Tribromophenol

Concen: 106.374 ng

RT: 15.66 min Scan# 2171

Delta R.T. -0.01 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47




Tgt Ion:330 Resp: 400738


Ion Ratio Lower Upper

330 100

332 96.7 78.6 118.0

141 39.2 27.1 40.7

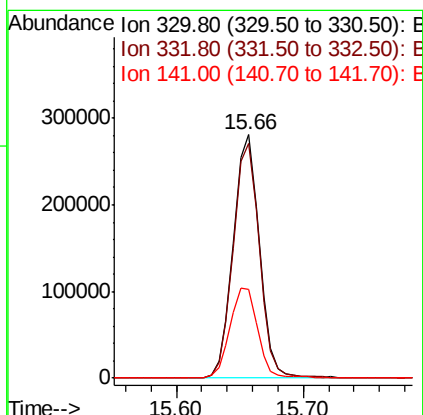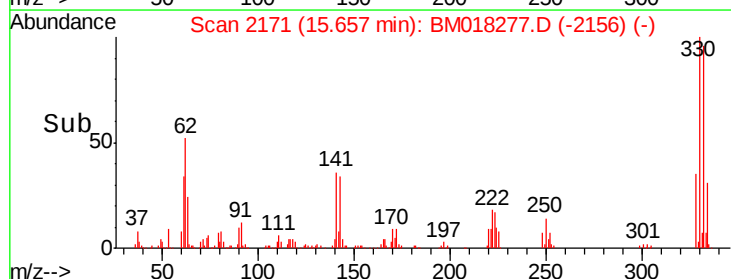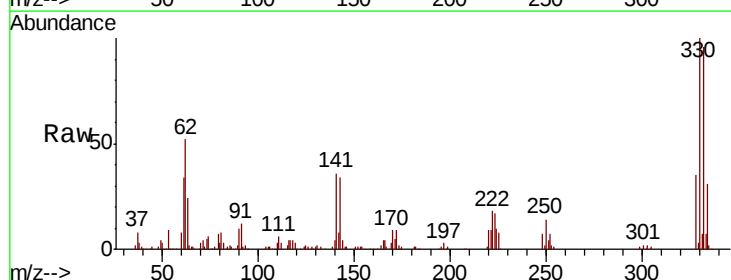




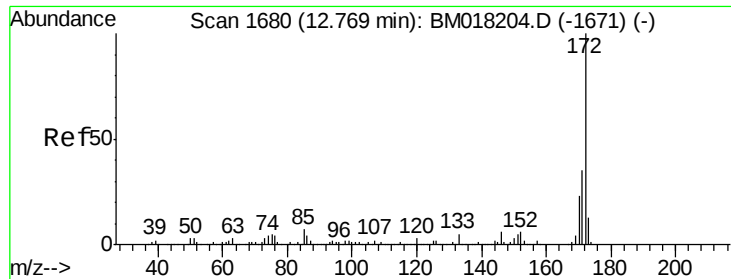


#45
 2-Fluorobiphenyl
 Concen: 92.130 ng
 RT: 12.75 min Scan# 1677
 Delta R.T. -0.02 min
 Lab File: BM018277.D
 Acq: 18 Dec 2018 18:47

Instrument :
 BNA_M
 ClientSampleId :
 SB-04B

Tot Ion:172 Resp: 1825718




Ion	Ratio	Lower	Upper
172	100		
171	34.6	28.3	42.5
170	22.1	18.1	27.1

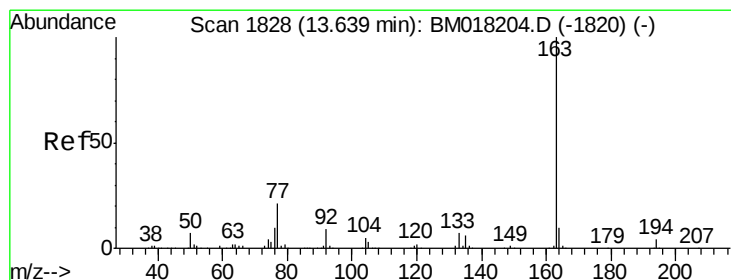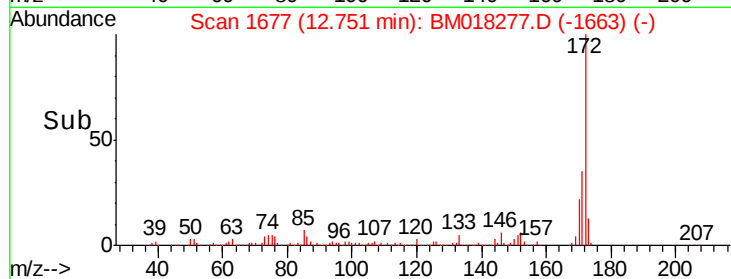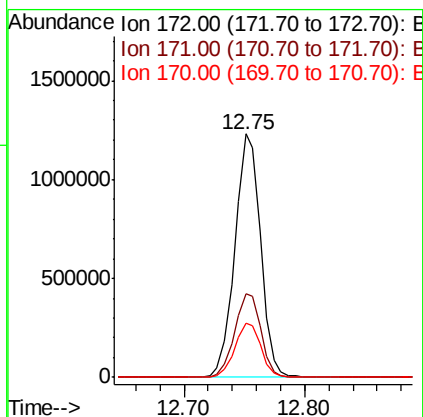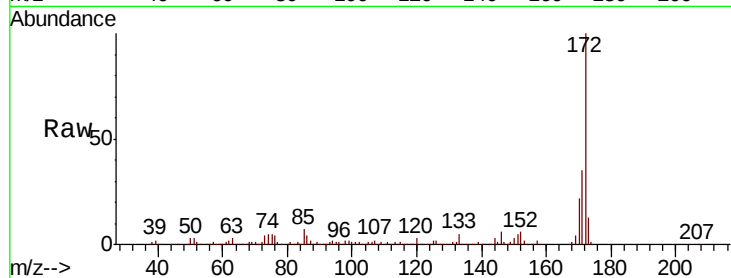


#50
 Dimethylphthalate
 Concen: 6.762 ng
 RT: 13.62 min Scan# 1825
 Delta R.T. -0.02 min
 Lab File: BM018277.D
 Acq: 18 Dec 2018 18:47

Tgt Ion:163 Resp: 144304

Ion	Ratio	Lower	Upper
163	100		
194	5.0	3.1	4.7#
164	10.3	7.9	11.9

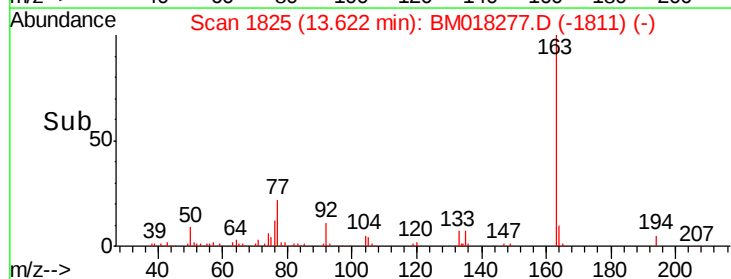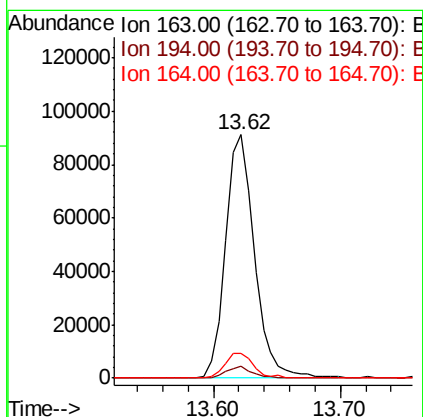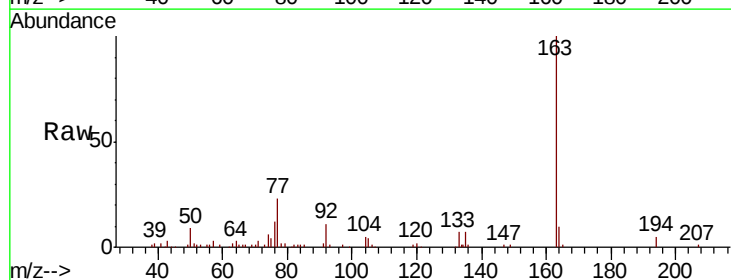

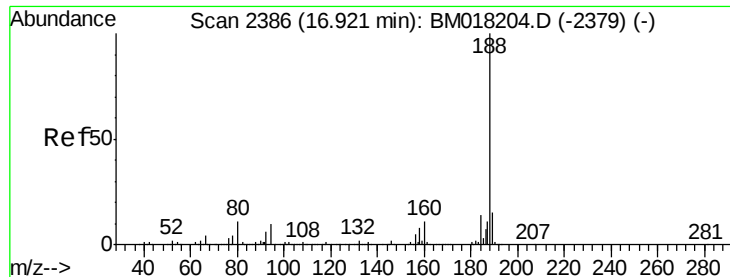

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.91 min Scan# 2384

Delta R.T. -0.01 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47

Instrument :

BNA_M

ClientSampleId :

SB-04B


Tot Ion:188 Resp: 474785

Ion Ratio Lower Upper

188 100

94 8.9 8.0 12.0




80 10.4 9.0 13.6

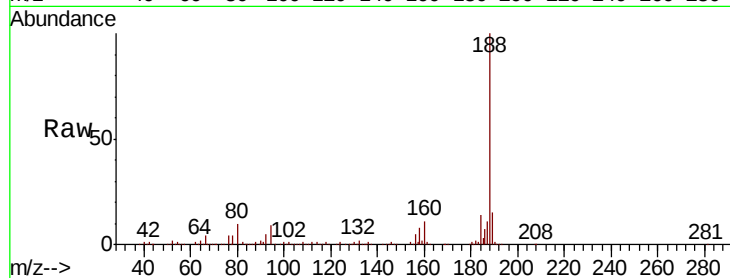

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

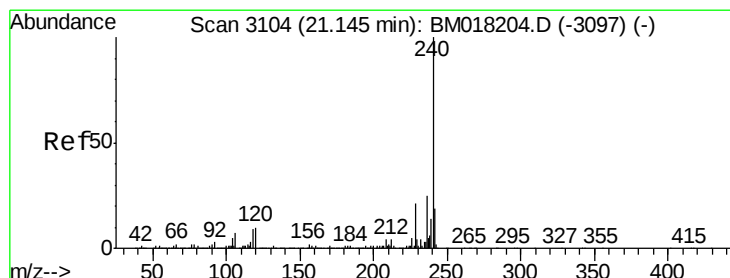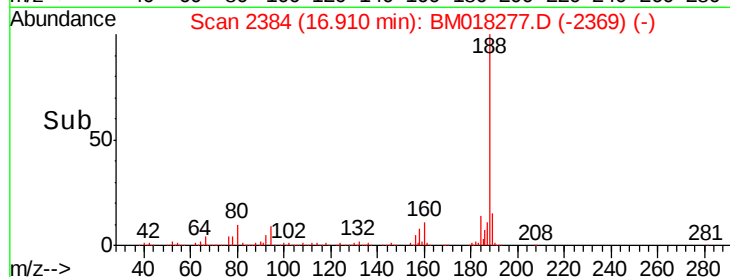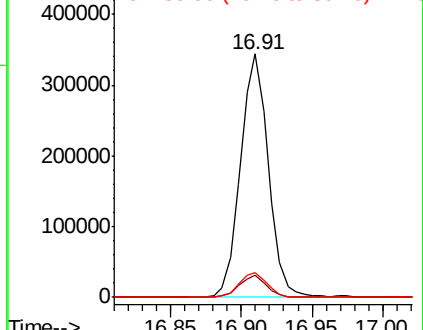

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.13 min Scan# 3102

Delta R.T. -0.01 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47


Tgt Ion:240 Resp: 411648

Ion Ratio Lower Upper

240 100

120 8.4 8.2 12.2



236 25.3 20.3 30.5

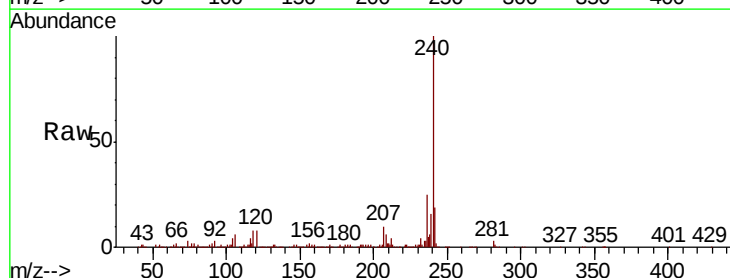


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

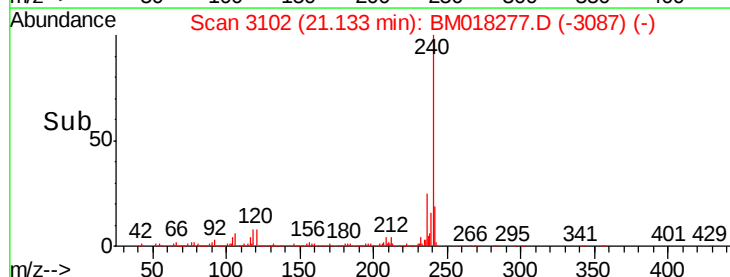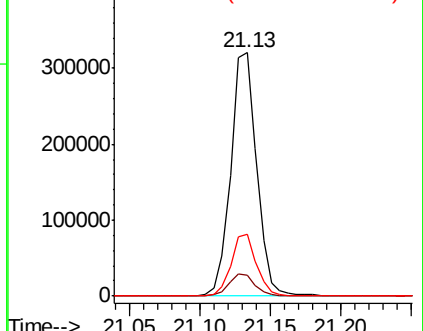

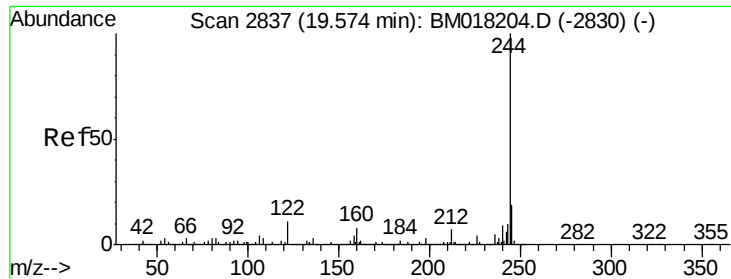

#79

Terphenyl-d14

Concen: 92.436 ng

RT: 19.56 min Scan# 2835

Delta R.T. -0.01 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47

Instrument :

BNA_M

ClientSampleId :

SB-04B


Tot Ion:244 Resp: 1682458

Ion Ratio Lower Upper

244 100

212 7.3 5.8 8.8




122 10.4 9.0 13.6

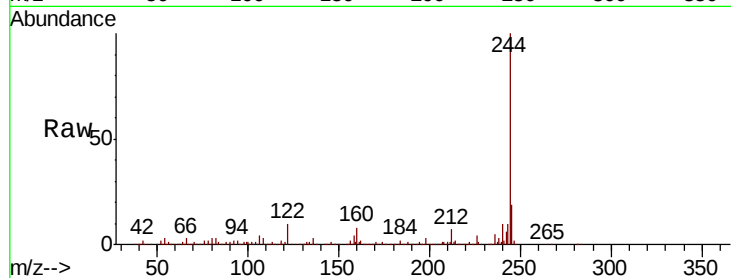

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

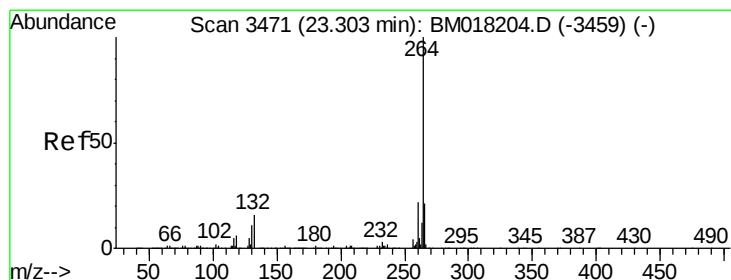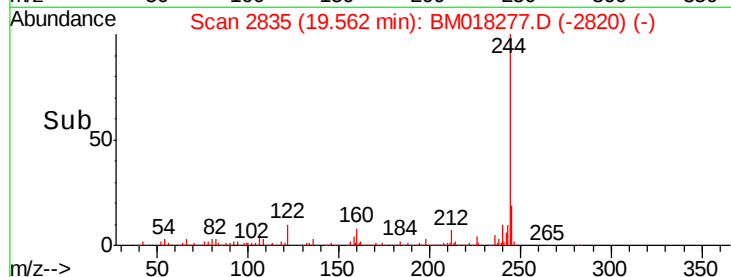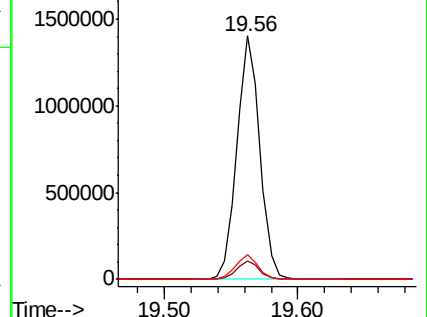

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.29 min Scan# 3468

Delta R.T. -0.02 min

Lab File: BM018277.D

Acq: 18 Dec 2018 18:47


Tgt Ion:264 Resp: 456000

Ion Ratio Lower Upper

264 100

260 23.8 17.5 26.3

265 22.9 17.3 25.9

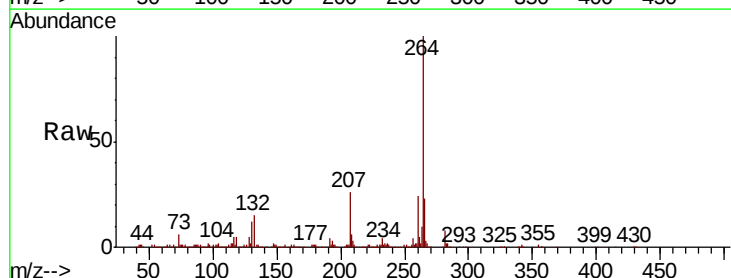

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

