


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121818\
 Data File : BM018270.D
 Acq On : 18 Dec 2018 13:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

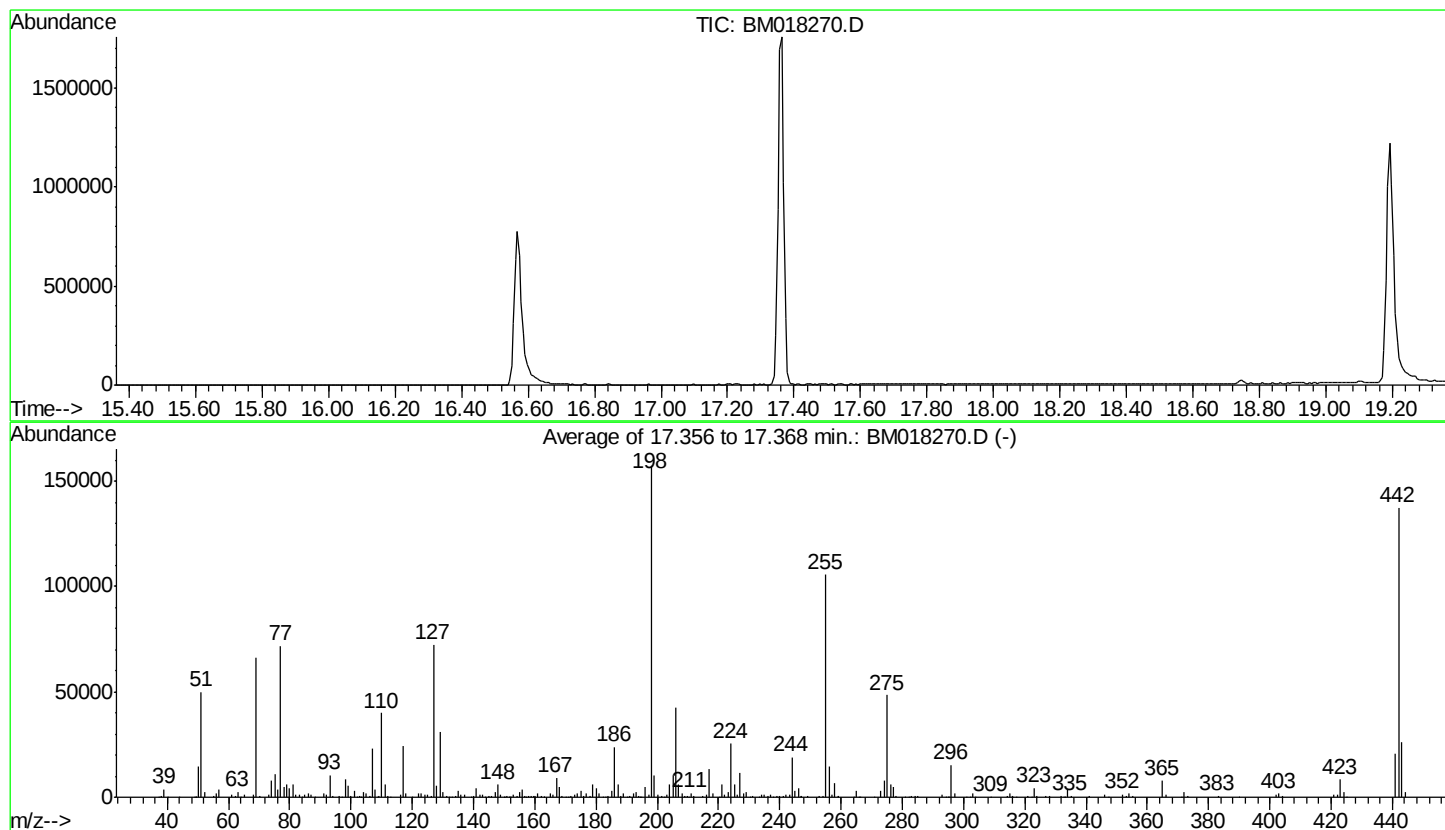

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	50010	PASS
68	69	0.00	2	1.9	1275	PASS
69	198	0.00	100	42.1	66213	PASS
70	69	0.00	2	0.6	391	PASS
127	198	10	80	46.1	72517	PASS
197	198	0.00	2	0.7	1088	PASS
198	198	100	100	100.0	157386	PASS
199	198	5	9	6.7	10525	PASS
275	198	10	60	30.7	48344	PASS
365	198	1	100	4.9	7724	PASS
441	198	0.01	100	13.0	20461	PASS
442	198	50	100	87.2	137309	PASS
443	442	15	24	18.8	25877	PASS