

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
 Data File : BM043408.D
 Acq On : 19 Dec 2023 00:10
 Operator : MA/JU
 Sample : 05807-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AY0

Quant Time: Dec 19 02:02:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 22:09:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.992	152	488982	20.000	ng/ul	0.00
20) Naphthalene-d8	10.798	136	2126928	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.621	164	1094674	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.368	188	1816772	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	1246049	20.000	ng/ul	0.00
88) Perylene-d12	23.968	264	1441893	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	58657	3.899	ng/uL	0.00
4) Pyridine-d5	3.810	84	608090	14.043	ng/ul	0.00
7) Phenol-d5	7.151	99	1105598	19.876	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	782061	22.199	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	911671	21.465	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	909662	21.074	ng/ul	0.00
21) Nitrobenzene-d5	9.163	128	468394	22.761	ng/ul	0.00
24) 2-Nitrophenol-d4	9.886	143	487307	22.919	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	802169	21.372	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	1192326	21.592	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	2176827	22.090	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	2725363	23.314	ng/ul	0.00
54) 4-Nitrophenol-d4	14.821	143	263267	14.115	ng/ul	0.00
60) Fluorene-d10	15.615	176	1822906	22.371	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	197218	16.414	ng/ul	0.00
73) Anthracene-d10	17.462	188	2384842	23.406	ng/ul	0.00
81) Pyrene-d10	19.750	212	2174165	22.101	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.809	264	2028109	22.793	ng/ul	0.00
Target Compounds						
12) 2-Chlorophenol	7.551	128	207700	4.801	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043408.D
Acq On : 19 Dec 2023 00:10
Operator : MA/JU
Sample : 05807-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AY0

Quant Time: Dec 19 02:02:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 22:09:25 2023
Response via : Initial Calibration

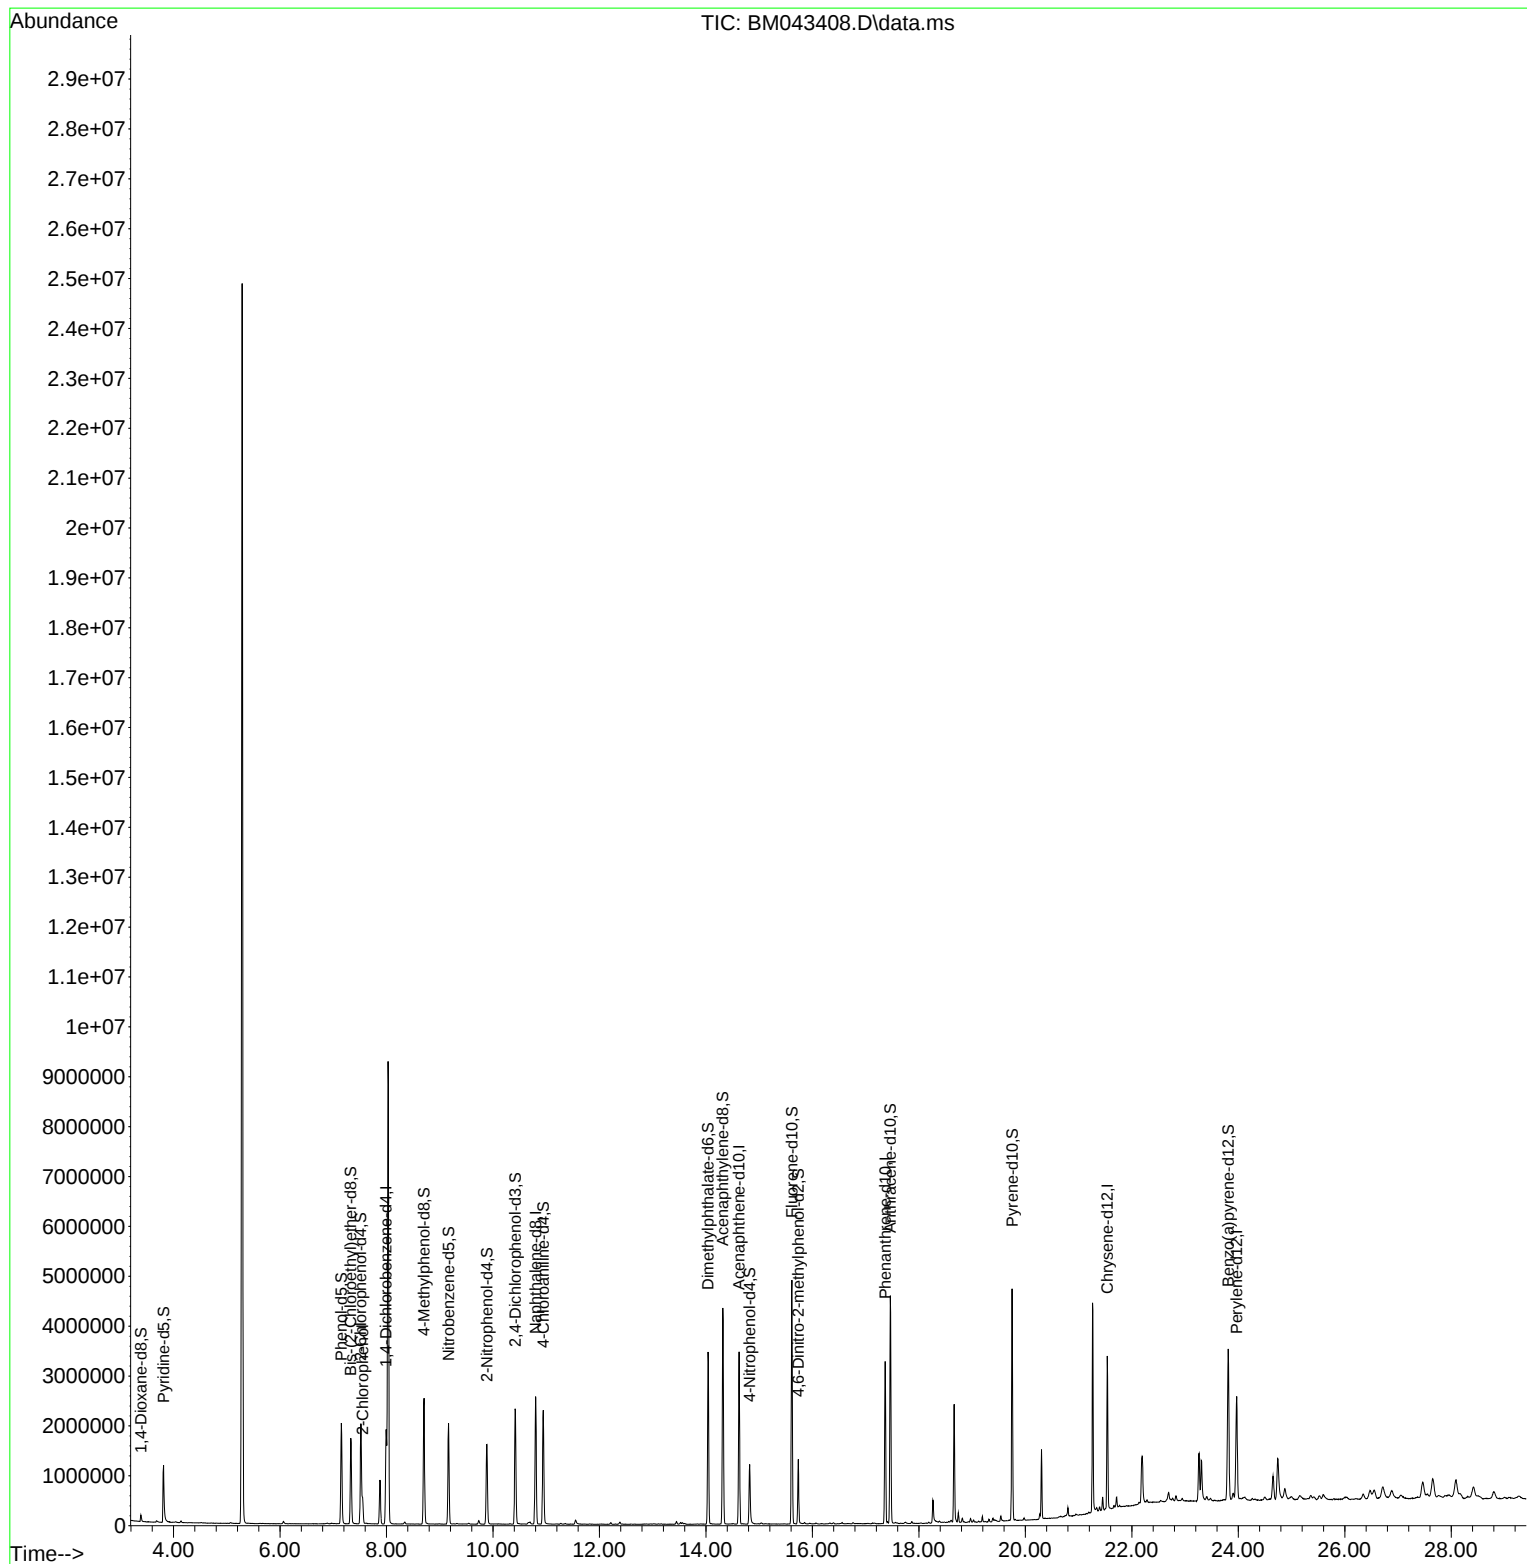

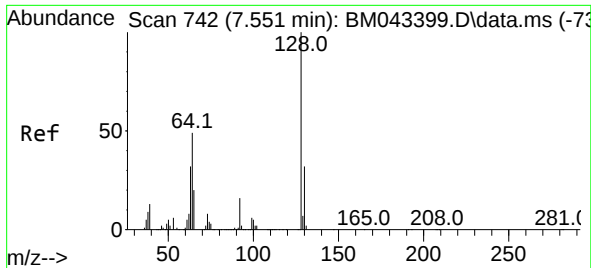

#12
 2-Chlorophenol
 Concen: 4.801 ng/ul
 RT: 7.551 min Scan# 742
 Delta R.T. 0.000 min
 Lab File: BM043408.D
 Acq: 19 Dec 2023 00:10

Instrument :
 BNA_M
 ClientSampleId :
 C0AY0

Tgt Ion:128 Resp: 207700

Ion	Ratio	Lower	Upper
128	100		
64	48.5	40.5	60.7
130	32.7	25.6	38.4

