

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
 Data File : BM043418.D
 Acq On : 19 Dec 2023 06:47
 Operator : MA/JU
 Sample : 05807-15
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B00

Quant Time: Dec 19 07:19:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 22:09:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.992	152	435702	20.000	ng/u1	0.00
20) Naphthalene-d8	10.798	136	1805701	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.621	164	929636	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.362	188	1629353	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1244370	20.000	ng/u1	0.00
88) Perylene-d12	23.968	264	1413112	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	48230	3.598	ng/uL	0.00
4) Pyridine-d5	3.810	84	418434	10.845	ng/u1	0.00
7) Phenol-d5	7.151	99	914909	18.459	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	680668	21.684	ng/u1	0.00
11) 2-Chlorophenol-d4	7.516	132	792959	20.953	ng/u1	0.00
15) 4-Methylphenol-d8	8.704	113	779381	20.264	ng/u1	0.00
21) Nitrobenzene-d5	9.163	128	403464	23.094	ng/u1	0.00
24) 2-Nitrophenol-d4	9.886	143	425745	23.585	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	692815	21.742	ng/u1	0.00
31) 4-Chloroaniline-d4	10.945	131	713127	15.212	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	1868678	22.329	ng/u1	0.00
49) Acenaphthylene-d8	14.316	160	2371835	23.892	ng/u1	0.00
54) 4-Nitrophenol-d4	14.821	143	203889	12.872	ng/u1	0.00
60) Fluorene-d10	15.615	176	1592203	23.008	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	175309	16.268	ng/u1	0.00
73) Anthracene-d10	17.462	188	2193897	24.009	ng/u1	0.00
81) Pyrene-d10	19.750	212	2154354	21.929	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.809	264	2059368	23.616	ng/u1	0.00
Target Compounds						
12) 2-Chlorophenol	7.551	128	48784	1.265	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043418.D
Acq On : 19 Dec 2023 06:47
Operator : MA/JU
Sample : 05807-15
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B00

Quant Time: Dec 19 07:19:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 22:09:25 2023
Response via : Initial Calibration

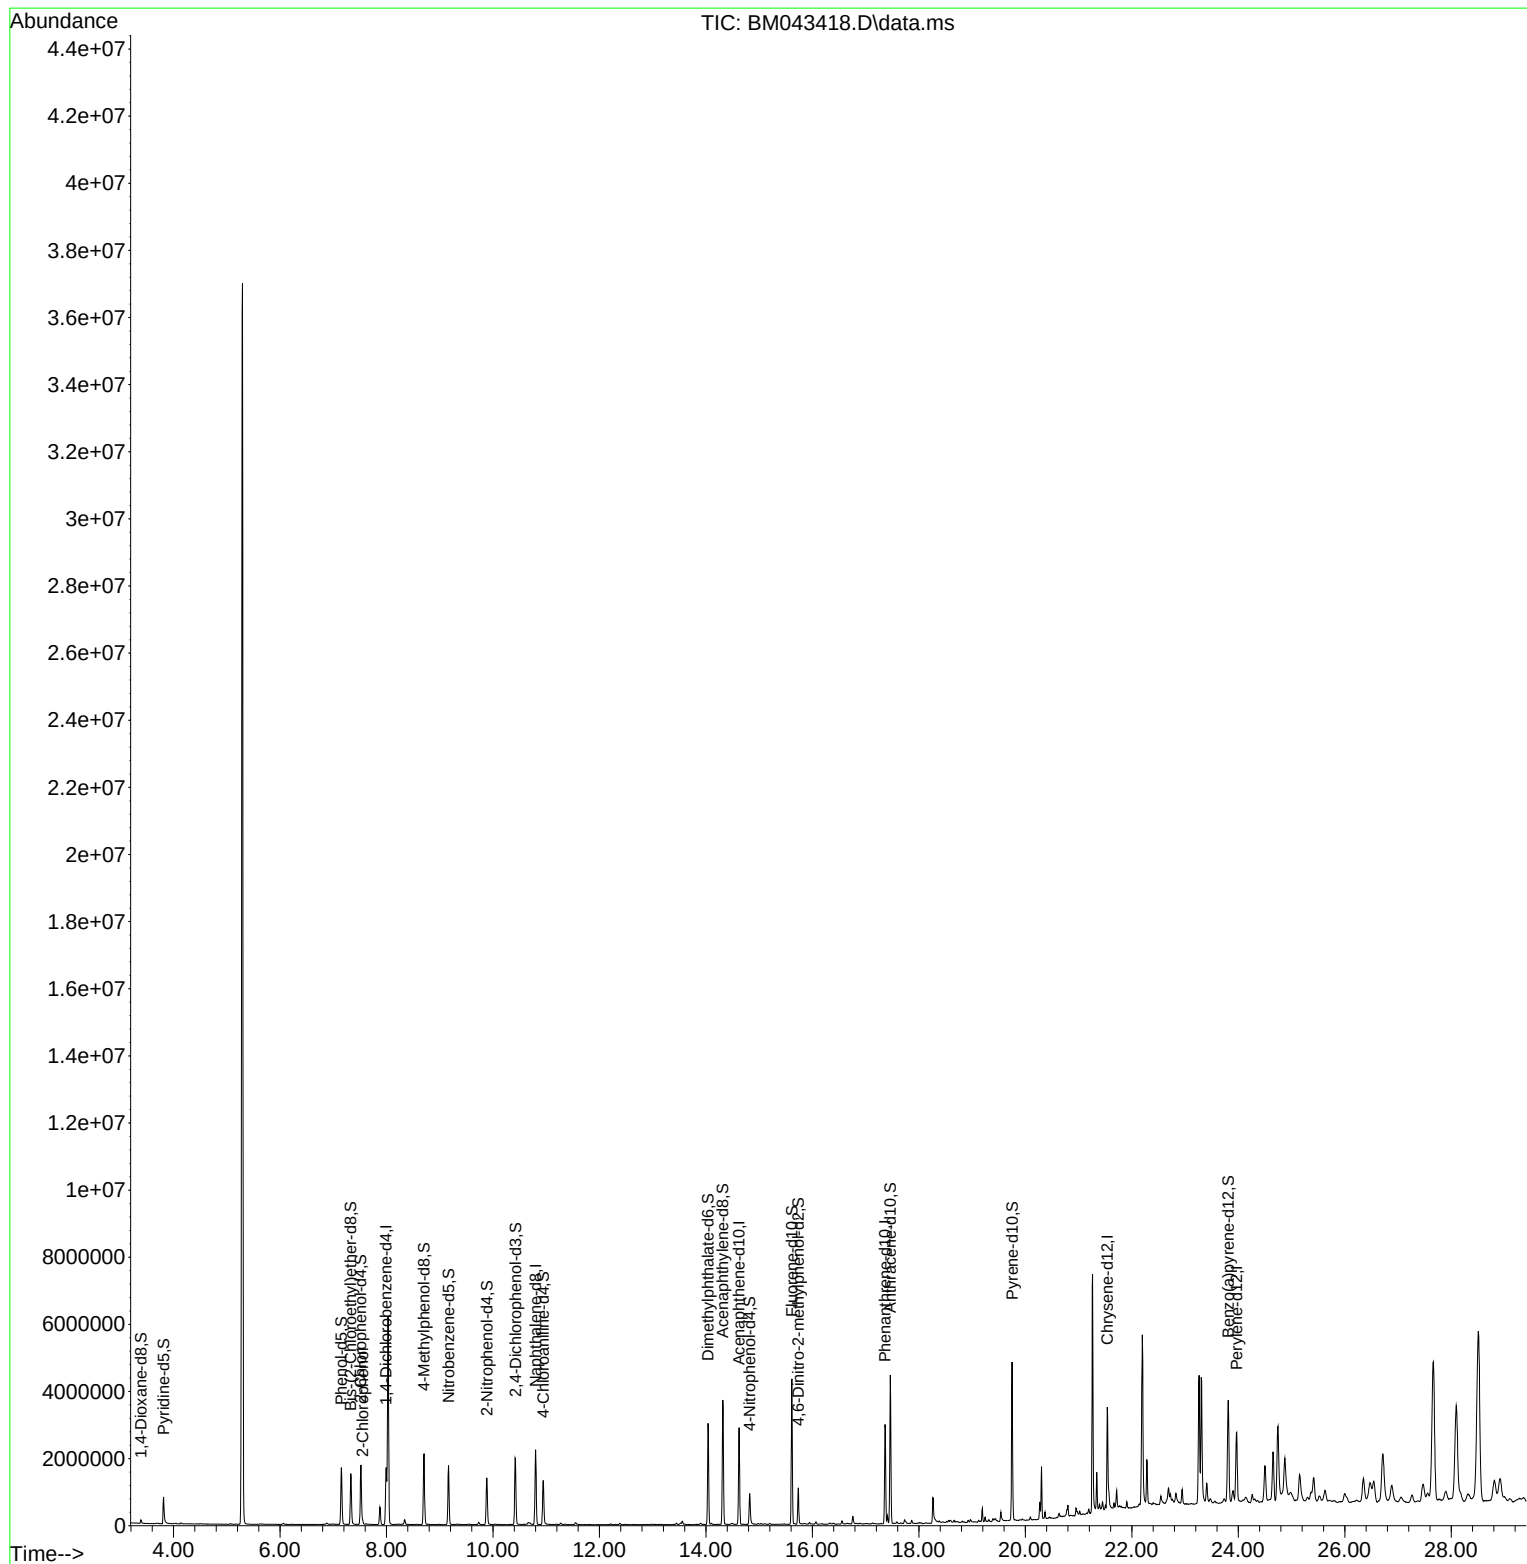

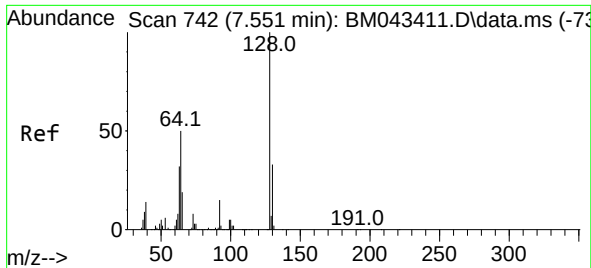

#12
 2-Chlorophenol
 Concen: 1.265 ng/ul
 RT: 7.551 min Scan# 74
 Delta R.T. -0.000 min
 Lab File: BM043418.D
 Acq: 19 Dec 2023 06:47

Instrument :
 BNA_M
 ClientSampleId :
 C0B00

Tgt Ion:128 Resp: 48784
 Ion Ratio Lower Upper
 128 100
 64 49.0 40.5 60.7
 130 31.0 25.6 38.4

