

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
 Data File : BM043422.D
 Acq On : 19 Dec 2023 09:11
 Operator : MA/JU
 Sample : 05807-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B20

Quant Time: Dec 19 23:10:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 15 22:09:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.992	152	525173	20.000	ng/u1	0.00
20) Naphthalene-d8	10.798	136	2227234	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.621	164	1127551	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.368	188	1874511	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1373551	20.000	ng/u1	0.00
88) Perylene-d12	23.968	264	1547165	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	78241	4.842	ng/uL	0.00
4) Pyridine-d5	3.810	84	1121373	24.112	ng/u1	0.00
7) Phenol-d5	7.151	99	1677230	28.074	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	1056391	27.920	ng/u1	0.00
11) 2-Chlorophenol-d4	7.522	132	1272620	27.899	ng/u1	0.00
15) 4-Methylphenol-d8	8.704	113	1321828	28.512	ng/u1	0.00
21) Nitrobenzene-d5	9.163	128	655378	30.414	ng/u1	0.00
24) 2-Nitrophenol-d4	9.886	143	692767	31.114	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	1157742	29.456	ng/u1	0.00
31) 4-Chloroaniline-d4	10.945	131	1659791	28.704	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	3139214	30.927	ng/u1	0.00
49) Acenaphthylene-d8	14.321	160	3877642	32.204	ng/u1	0.00
54) 4-Nitrophenol-d4	14.821	143	506805	26.381	ng/u1	0.00
60) Fluorene-d10	15.615	176	2598218	30.955	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	310074	25.011	ng/u1	0.00
73) Anthracene-d10	17.462	188	3435001	32.675	ng/u1	0.00
81) Pyrene-d10	19.750	212	3269757	30.152	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.809	264	3123993	32.720	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.181	94	63562	1.081	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043422.D
Acq On : 19 Dec 2023 09:11
Operator : MA/JU
Sample : 05807-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B20

Quant Time: Dec 19 23:10:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 15 22:09:25 2023
Response via : Initial Calibration

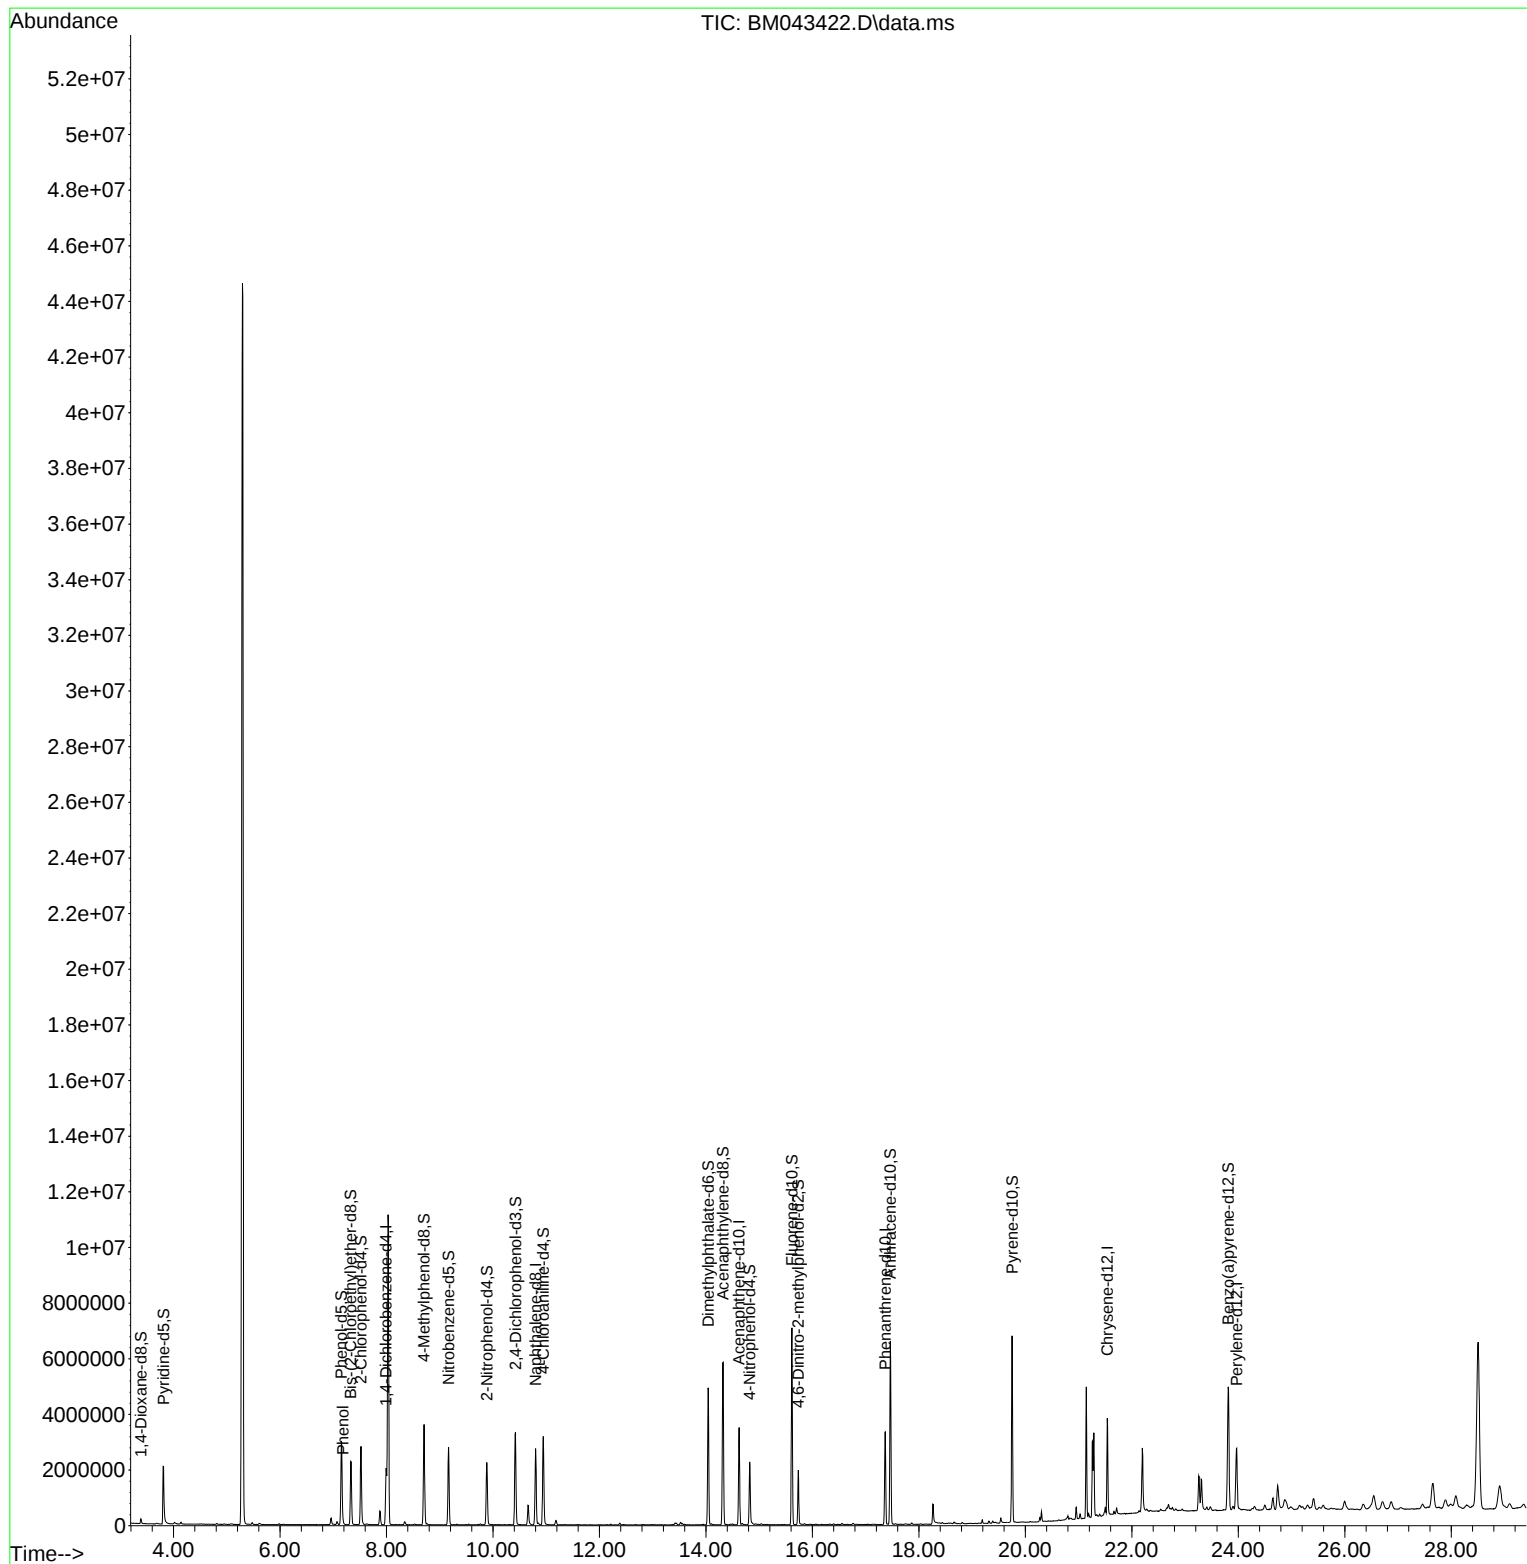

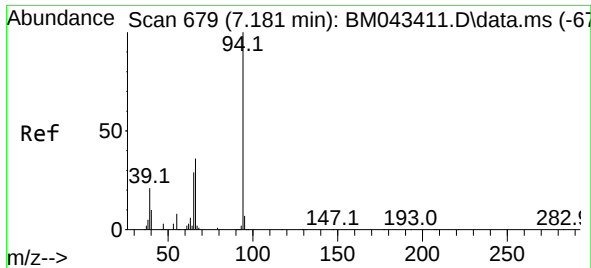

#8
Phenol
Concen: 1.081 ng/ul
RT: 7.181 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM043422.D
Acq: 19 Dec 2023 09:11

Instrument :
BNA_M
ClientSampleId :
C0B20

Tgt Ion: 94 Resp: 63562
Ion Ratio Lower Upper
94 100
65 33.8 23.7 35.5
66 43.1 30.2 45.4

