

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
 Data File : BM043385.D
 Acq On : 18 Dec 2023 10:13
 Operator : MA/JU
 Sample : PB157781BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK781

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	43	rVB	137878	184689	2.37%	0.182%
2	3.805	102	105	125	rBV	1652419	2579399	33.13%	2.547%
3	4.140	157	162	172	rVB	93826	136436	1.75%	0.135%
4	7.151	666	674	685	rBV	2015197	3122797	40.11%	3.084%
5	7.328	697	704	716	rBV	1596317	2498205	32.09%	2.467%
6	7.516	729	736	748	rBV	1883693	3010650	38.67%	2.973%
7	7.993	809	817	830	rBV	1698783	2673198	34.34%	2.640%
8	8.698	930	937	950	rBV	2238162	3717460	47.75%	3.671%
9	9.163	1008	1016	1027	rBV	1876231	3089187	39.68%	3.051%
10	9.887	1131	1139	1147	rBV	1479988	2480255	31.86%	2.449%
11	10.416	1220	1229	1242	rBV	2125466	3585504	46.06%	3.541%
12	10.798	1286	1294	1305	rBV	2389435	4050444	52.03%	4.000%
13	10.945	1309	1319	1334	rBV	2350892	4089676	52.53%	4.039%
14	12.386	1557	1564	1571	rBV	36826	66080	0.85%	0.065%
15	12.604	1595	1601	1604	rVB8	4872	7936	0.10%	0.008%
16	13.522	1751	1757	1763	rVB2	40844	66757	0.86%	0.066%
17	13.604	1765	1771	1778	rVB9	7996	16260	0.21%	0.016%
18	14.039	1837	1845	1859	rBV	3951637	5434002	69.80%	5.366%
19	14.316	1885	1892	1902	rBV	4298751	6506588	83.58%	6.425%
20	14.622	1936	1944	1955	rBV	3668555	5207532	66.89%	5.142%
21	14.722	1958	1961	1966	rBV6	6245	9695	0.12%	0.010%
22	14.822	1970	1978	1994	rBV	1986201	2943036	37.81%	2.906%
23	15.045	2012	2016	2021	rVB8	8979	15212	0.20%	0.015%
24	15.616	2106	2113	2126	rBV	5349185	7658571	98.38%	7.563%
25	15.733	2126	2133	2149	rBV	1736985	2376304	30.53%	2.347%
26	15.851	2149	2153	2162	rVB5	28002	47119	0.61%	0.047%
27	16.174	2204	2208	2213	rBV7	4542	8778	0.11%	0.009%
28	16.316	2227	2232	2237	rVV7	8039	15603	0.20%	0.015%
29	16.398	2240	2246	2251	rBV3	19309	29551	0.38%	0.029%
30	16.710	2294	2299	2302	rBV6	8876	11522	0.15%	0.011%
31	16.763	2303	2308	2312	rVB8	6312	8791	0.11%	0.009%
32	17.045	2352	2356	2360	rBV6	9090	13736	0.18%	0.014%
33	17.157	2370	2375	2380	rBV4	7704	16048	0.21%	0.016%
34	17.368	2404	2411	2421	rBV	3841838	5542406	71.20%	5.473%
35	17.468	2421	2428	2441	rVV	5374827	7784699	100.00%	7.687%
36	17.563	2442	2444	2448	rVB4	8558	9716	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043385.D
Acq On : 18 Dec 2023 10:13
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	17.751	2470	2476	2477	rBV6	9016	14440	0.19%	0.014%
38	19.321	2738	2743	2748	rBV2	51312	77867	1.00%	0.077%
39	19.386	2750	2754	2760	rVV	46697	66256	0.85%	0.065%
40	19.751	2810	2816	2824	rBV	5512052	7344314	94.34%	7.253%
41	20.762	2985	2988	2991	rVB4	29567	31871	0.41%	0.031%
42	21.545	3115	3121	3128	rBV	3323354	4339620	55.75%	4.285%
43	23.815	3499	3507	3518	rVB2	3161770	6178911	79.37%	6.102%
44	23.974	3526	3534	3544	rVB	1974275	4197706	53.92%	4.145%




Sum of corrected areas: 101264827

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043385.D
Acq On : 18 Dec 2023 10:13
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

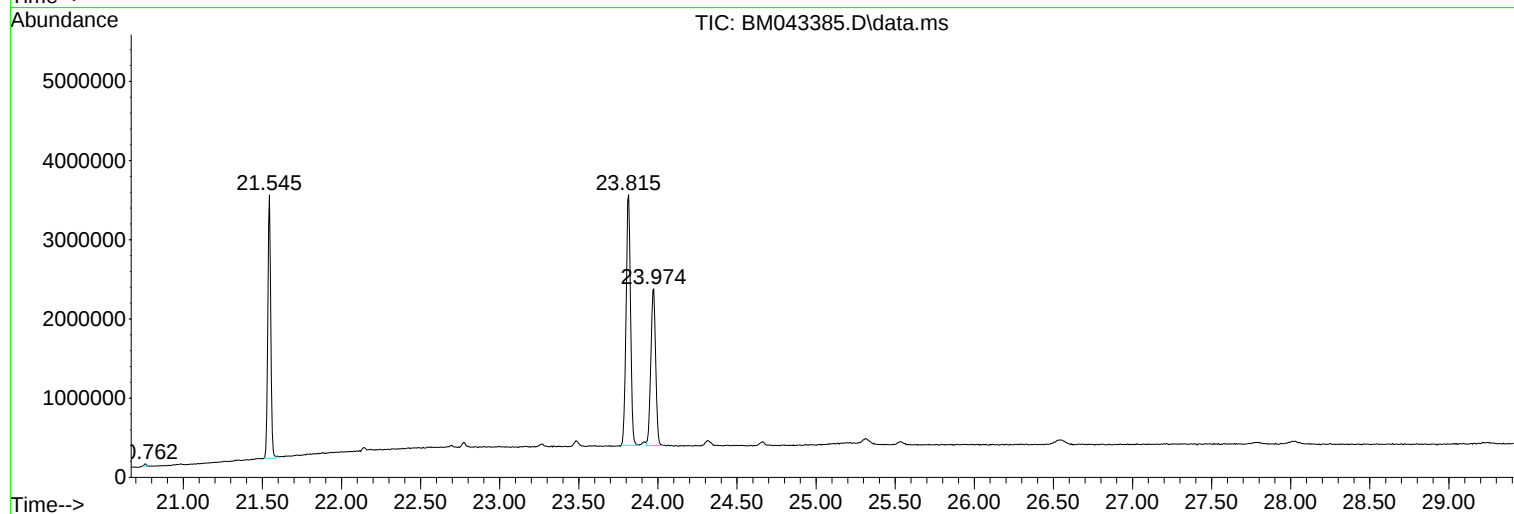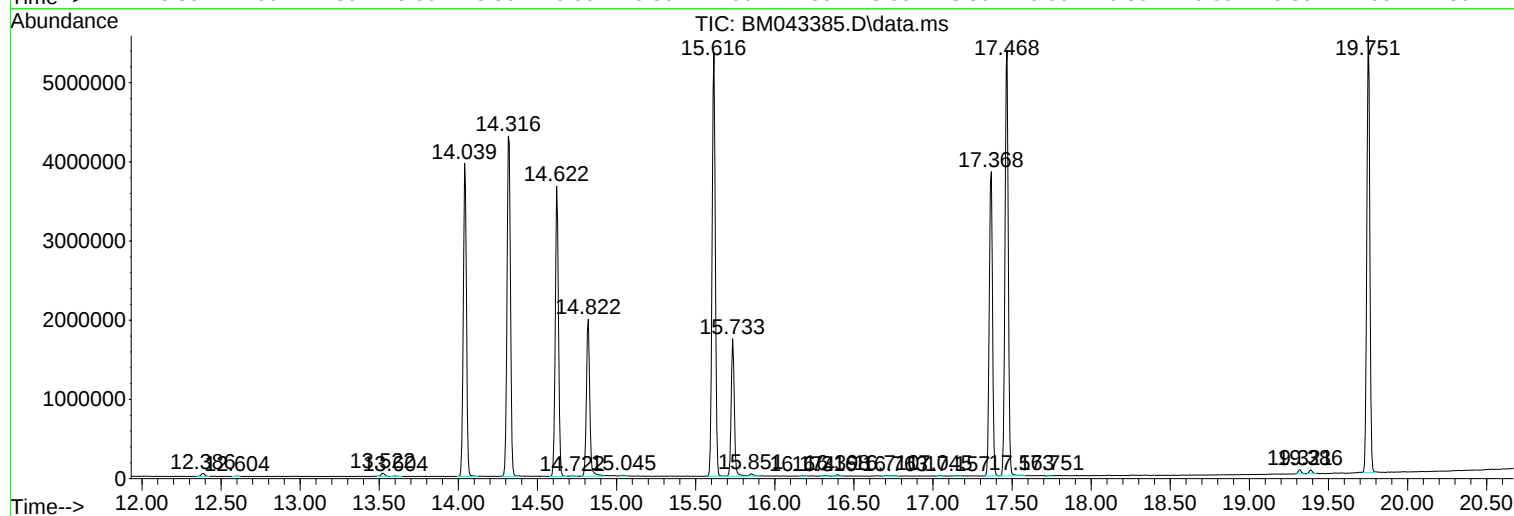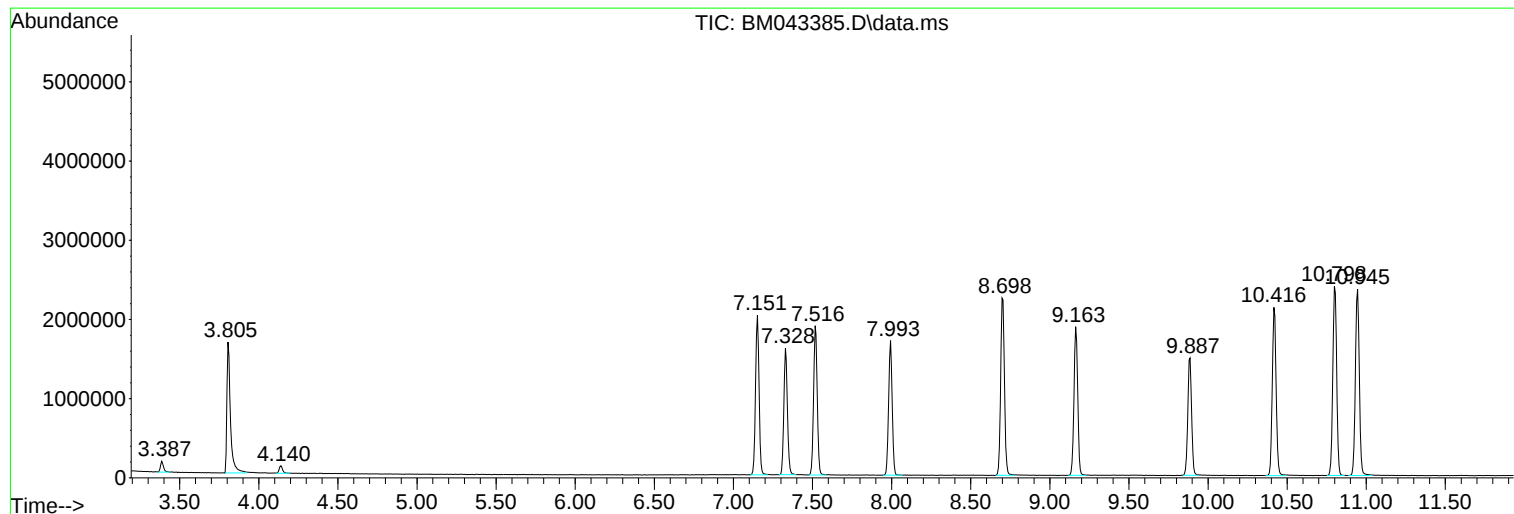

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043385.D
Acq On : 18 Dec 2023 10:13
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121823\
Data File : BM043385.D
Acq On : 18 Dec 2023 10:13
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
